

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006313.D
Acq On : 07 Jul 2016 11:12
Operator : UM/SJ
Sample : PB91937BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Manual Integration

Quant Time: Jul 08 01:51:36 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:14:08 2016
Response via : Initial Calibration

APPROVED
umangi
7/8/2016 7:12:35 PM

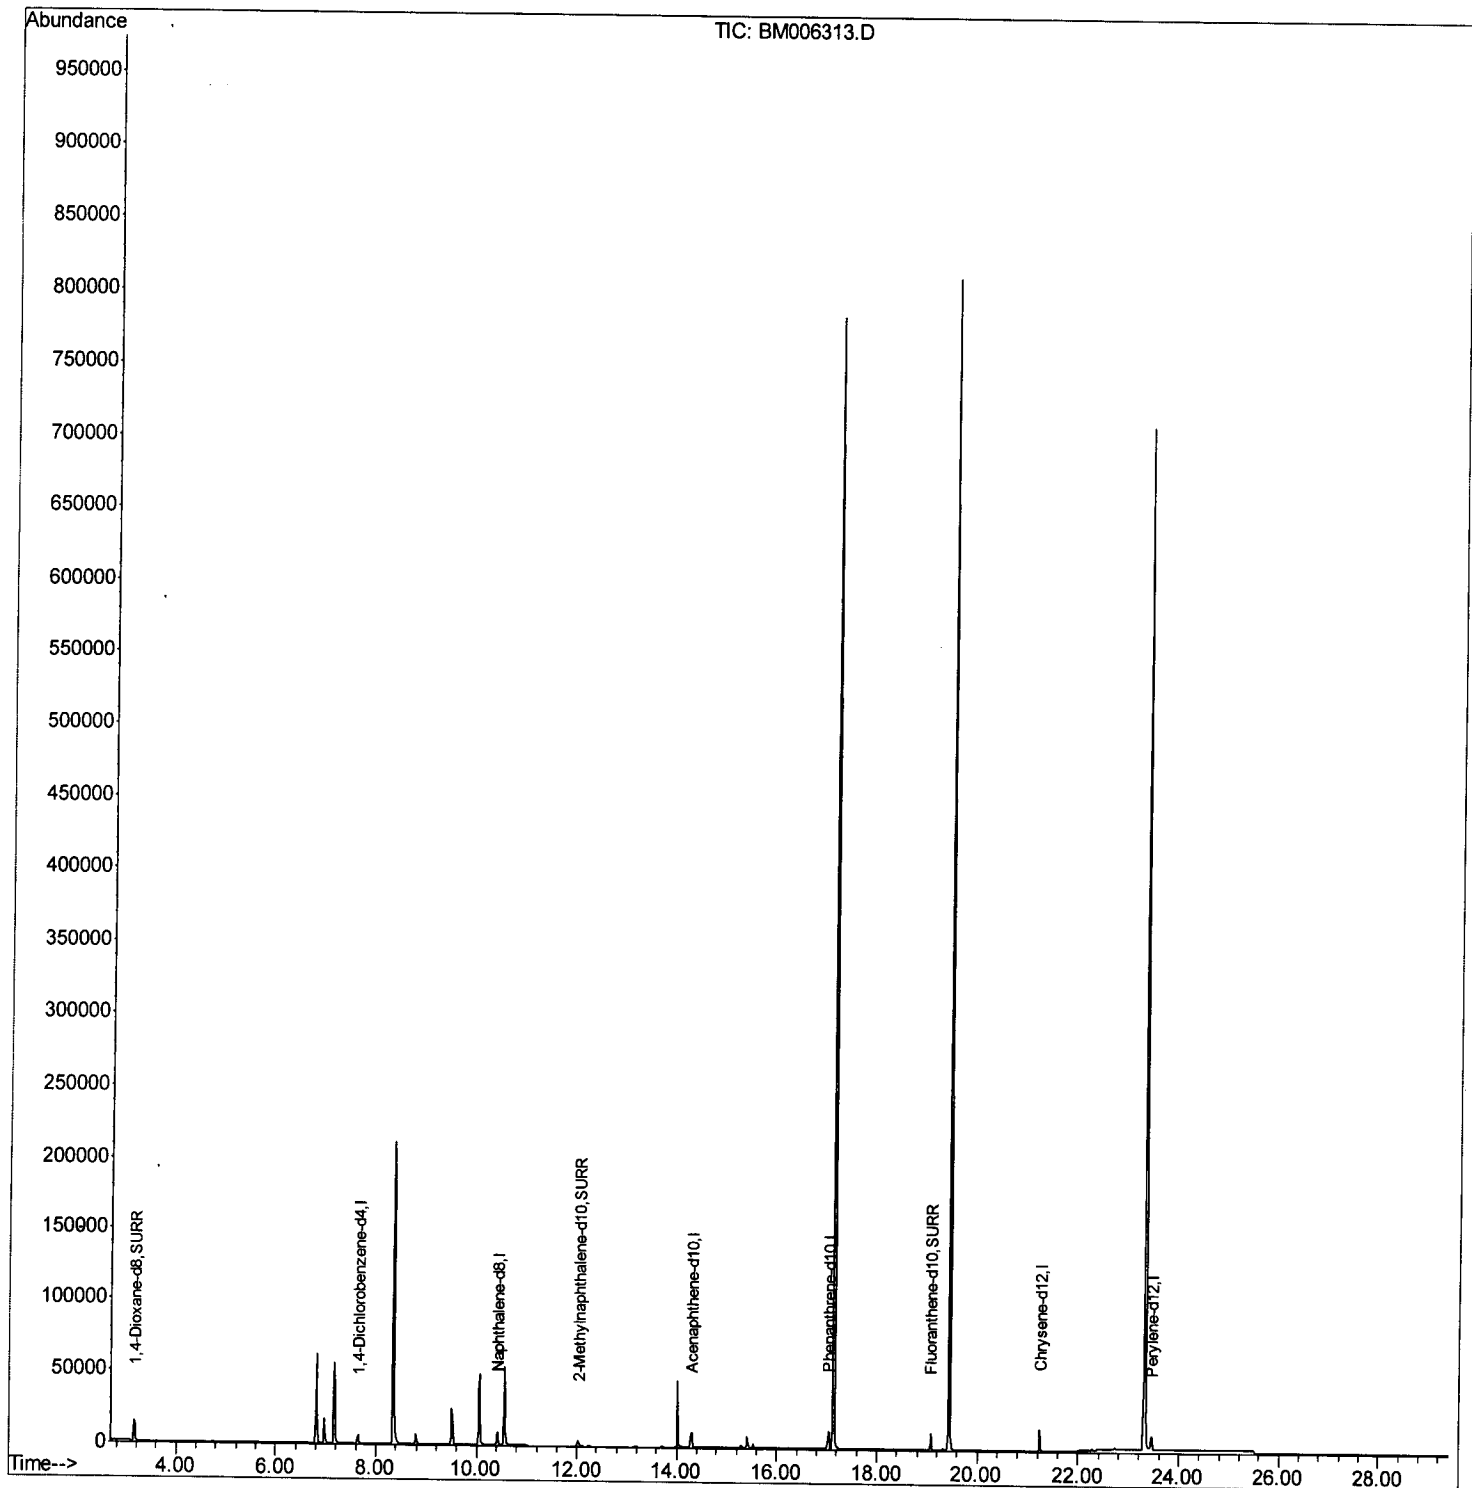

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006313.D
 Acq On : 07 Jul 2016 11:12
 Operator : UM/SJ
 Sample : PB91937BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Manual Integration

umangi
 7/8/2016 7:12:35 PM

Quant Time: Jul 08 01:32:19 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:14:08 2016
 Response via : Initial Calibration

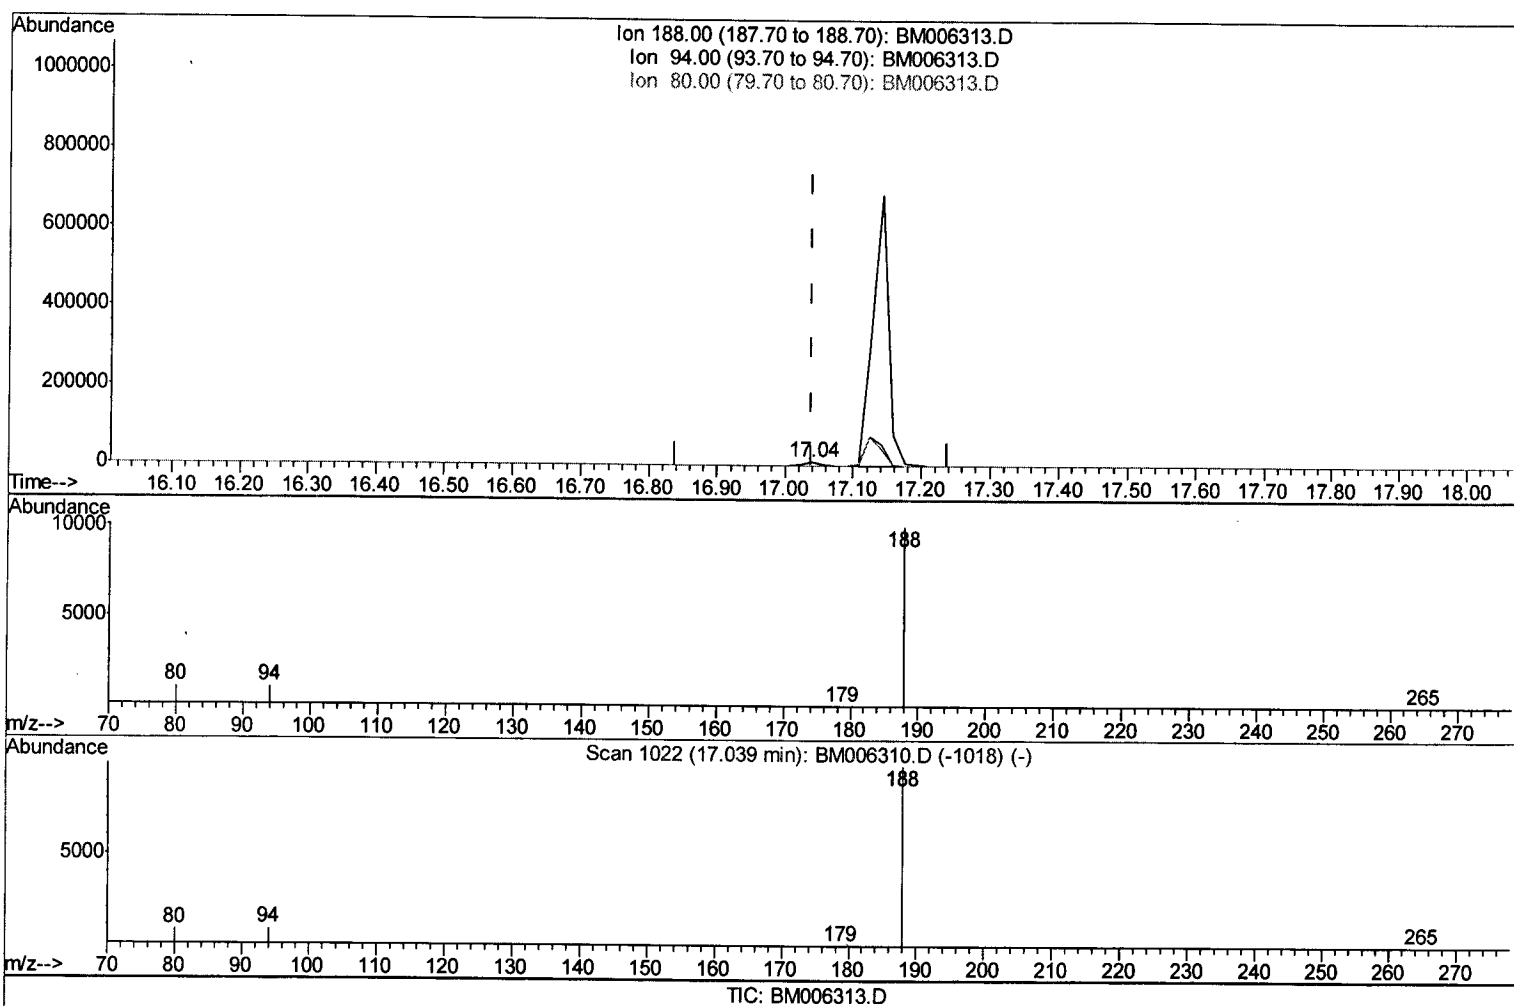

(12) Phenanthrene-d10 (I)

17.039min (-0.000) 0.40ng/ul m

response 14679

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	10.33
80.00	11.90	10.22
0.00	0.00	0.00

U.M
 07/12/16




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006313.D
Acq On : 07 Jul 2016 11:12
Operator : UM/SJ
Sample : PB91937BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Manual Integration

umangi
7/8/2016 7:12:35 PM

Quant Time: Jul 08 01:32:19 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:14:08 2016
Response via : Initial Calibration

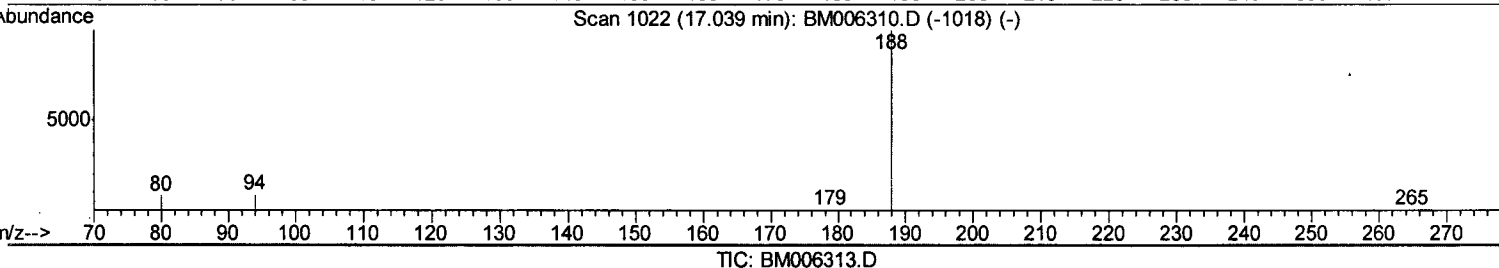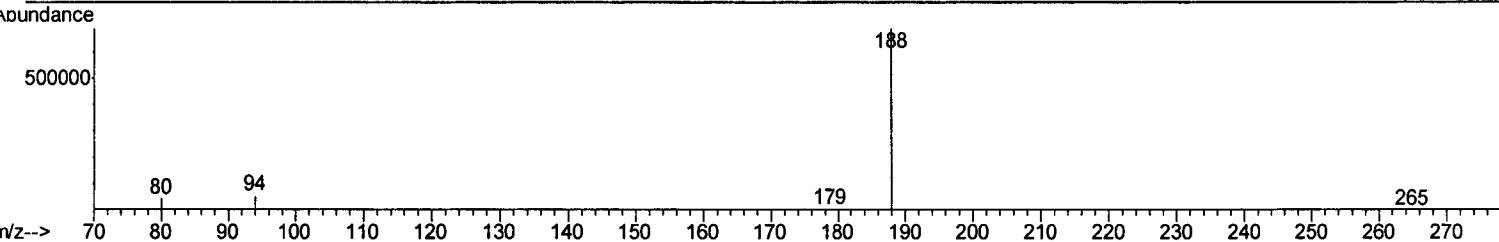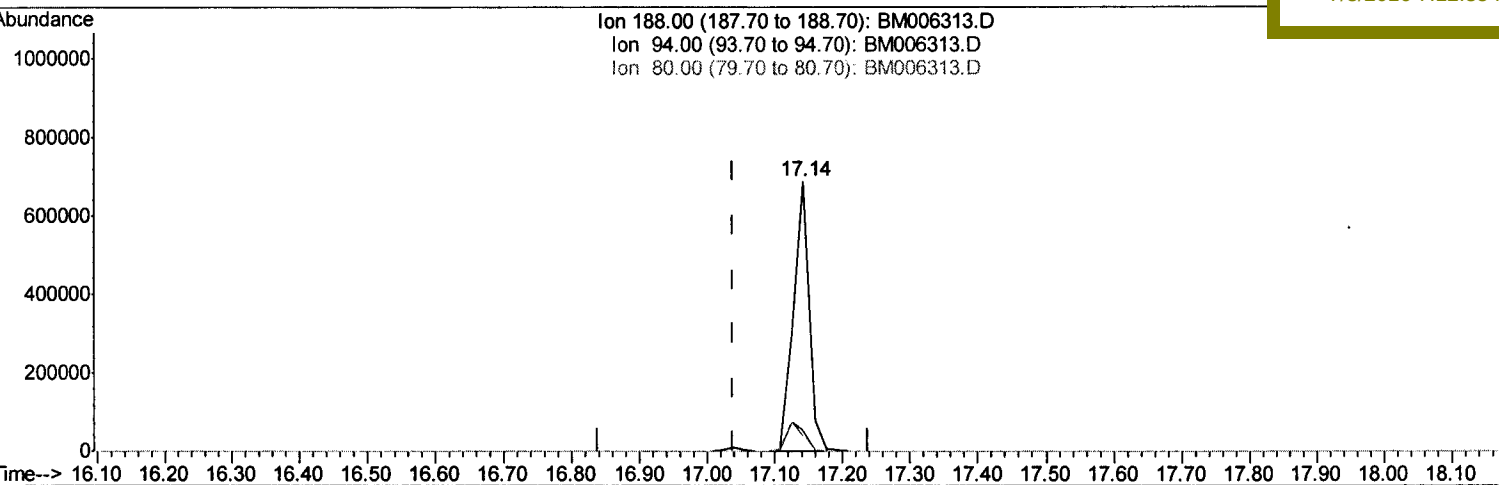

(12) Phenanthrene-d10 (I)

17.142min (+0.103) 0.40ng/ul

response 1108216

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.87#
80.00	11.90	6.13#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006313.D
 Acq On : 07 Jul 2016 11:12
 Operator : UM/SJ
 Sample : PB91937BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Manual Integration

umangi
 7/8/2016 7:12:35 PM

Quant Time: Jul 08 01:50:19 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:14:08 2016
 Response via : Initial Calibration

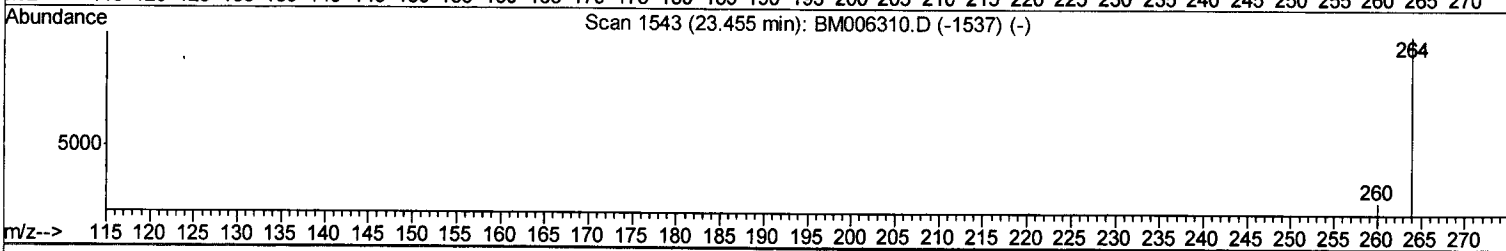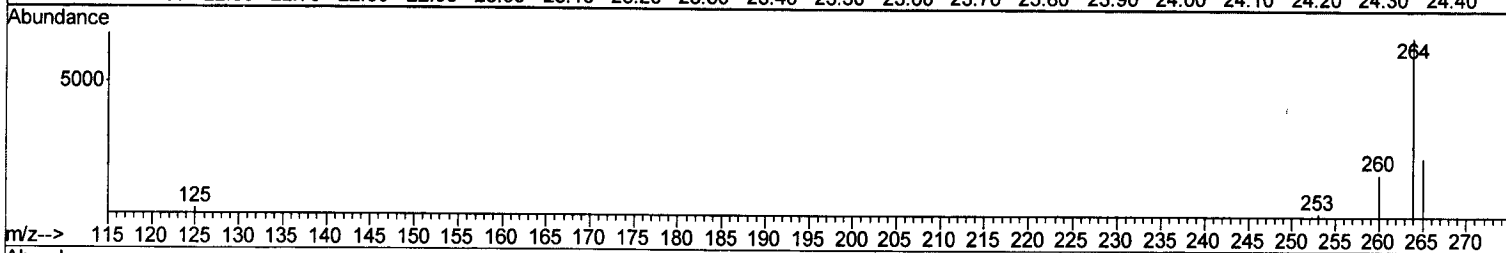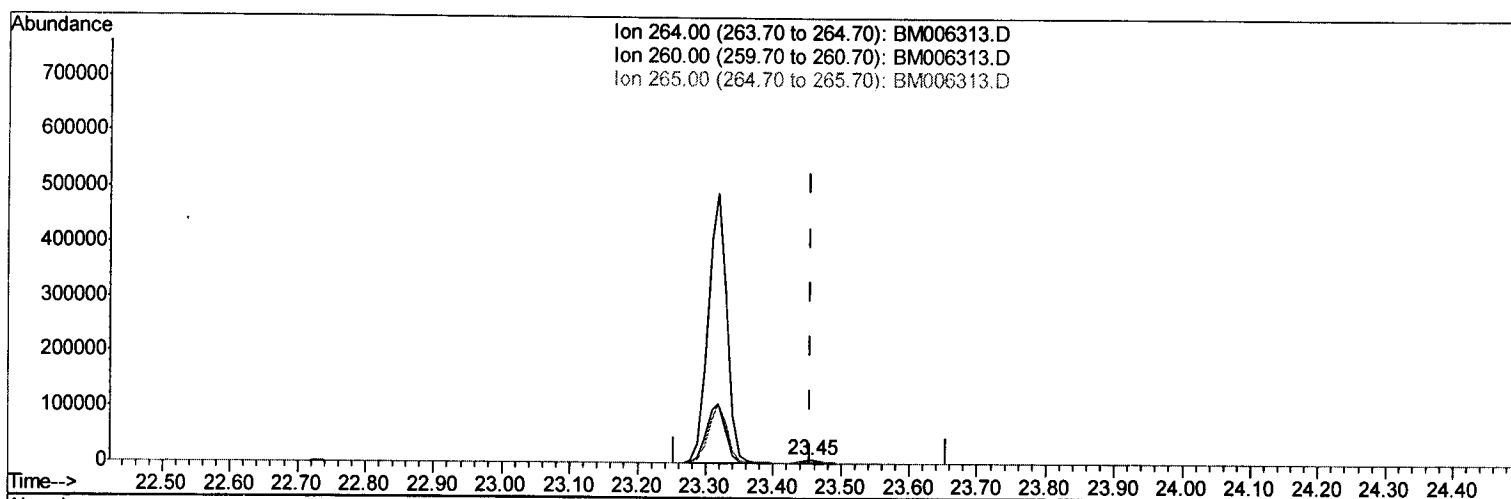

(22) Perylene-d12 (I)

23.455min (-0.000) 0.40ng/ul m

response 10708

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.37
265.00	38.20	35.46
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006313.D
 Acq On : 07 Jul 2016 11:12
 Operator : UM/SJ
 Sample : PB91937BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Quant Time: Jul 08 01:50:19 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:14:08 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/8/2016 7:12:35 PM

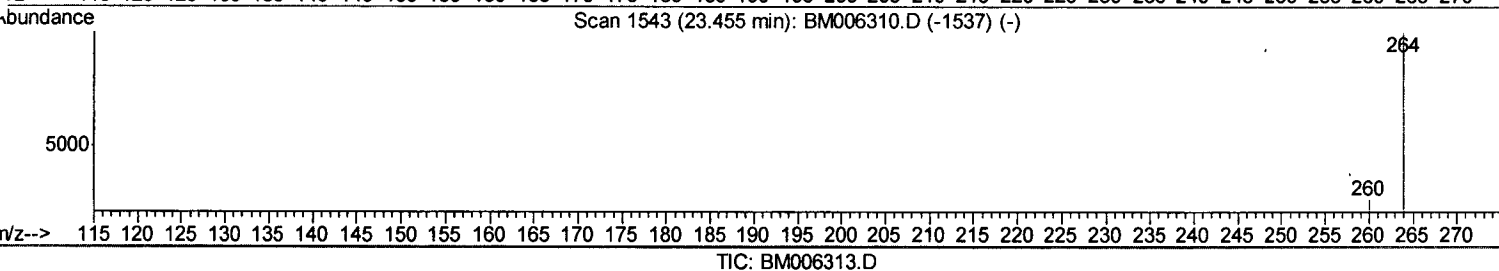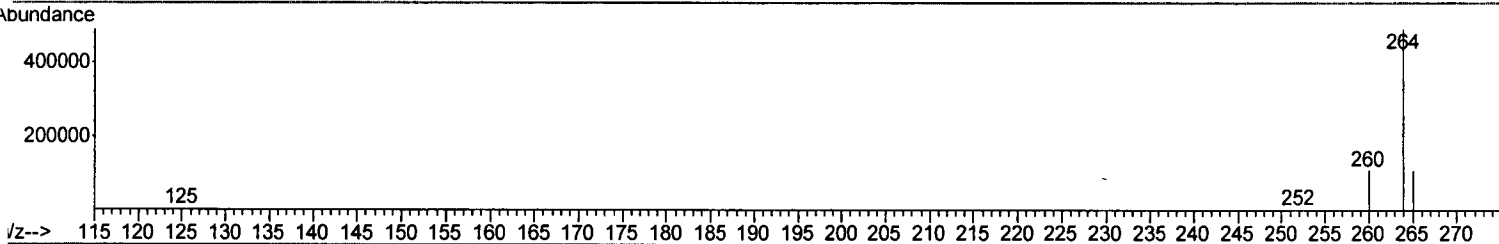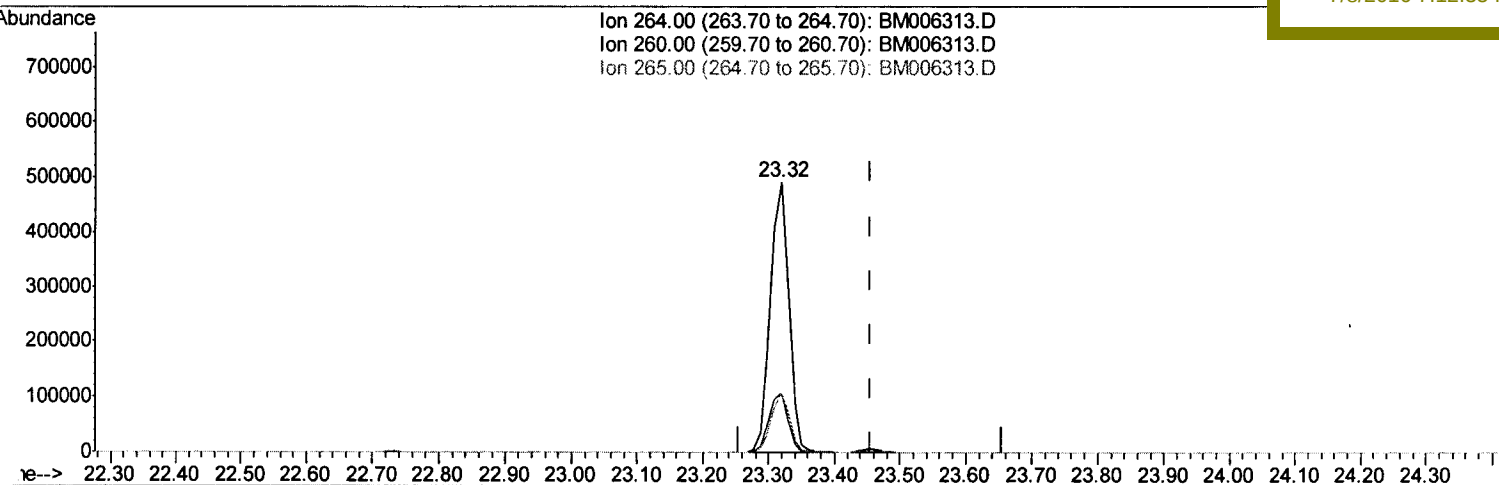

(22) Perylene-d12 (I)

23.319min (-0.136) 0.40ng/ul

response 945548

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	21.95
265.00	38.20	21.87#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006313.D
 Acq On : 07 Jul 2016 11:12
 Operator : UM/SJ
 Sample : PB91937BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Quant Time: Jul 08 01:51:36 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:14:08 2016
 Response via : Initial Calibration

Manual Integration

APPROVED
 umangi
 7/8/2016 7:12:35 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	3470	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	13288	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	7291	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.04	188	14679m	0.40	ng/ul	0.00
18) Chrysene-d12	21.24	240	13774	0.40	ng/ul	0.00
22) Perylene-d12	23.45	264	10708m	0.40	ng/ul	0.00

u.m
 07/12/16

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	10743	7.32	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.03	152	6696	0.43	ng/ul	0.01
16) Fluoranthene-d10	19.08	212	13387	0.43	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed