

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 08 04:35:16 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/8/2016 7:13:05 PM

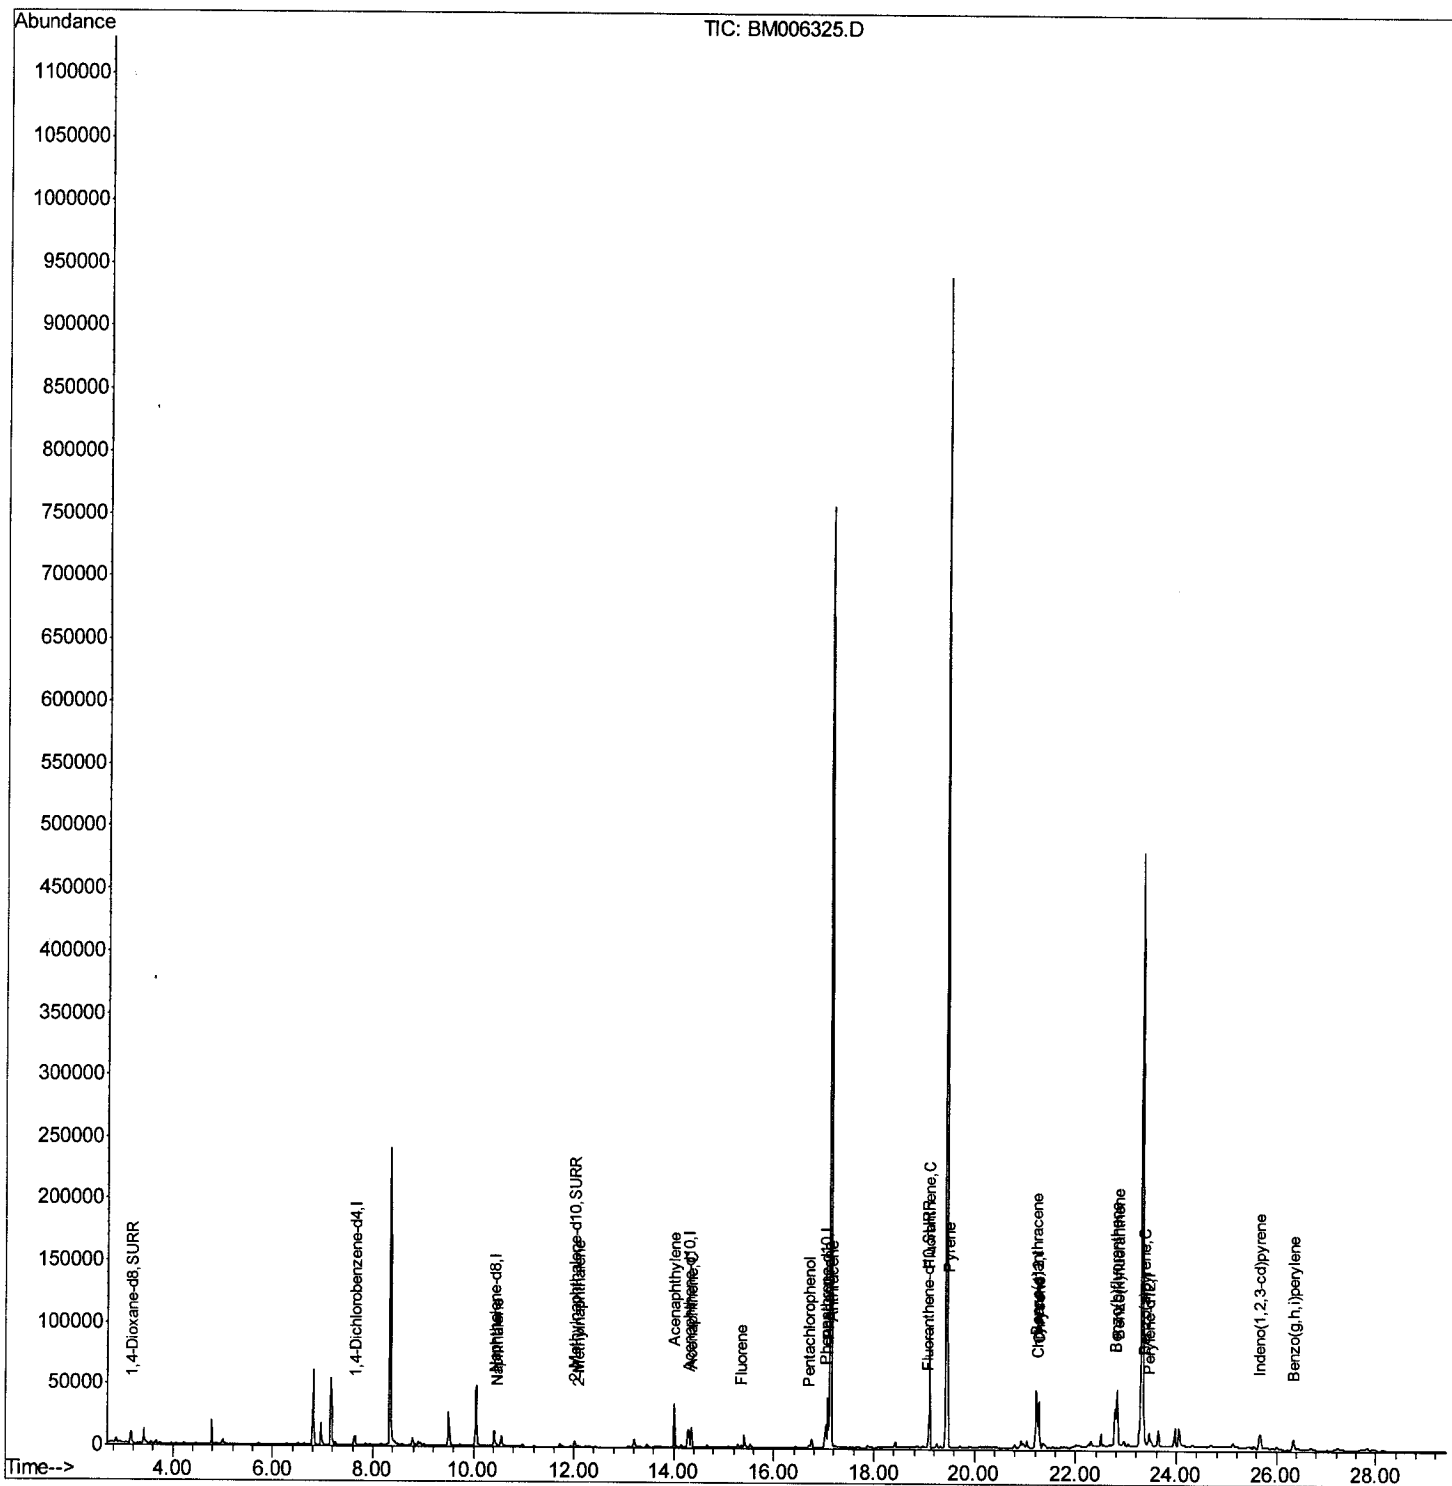

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 A4TV6MSD

Manual Integration

Quant Time: Jul 08 03:46:20 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

umangi
 7/8/2016 7:13:05 PM

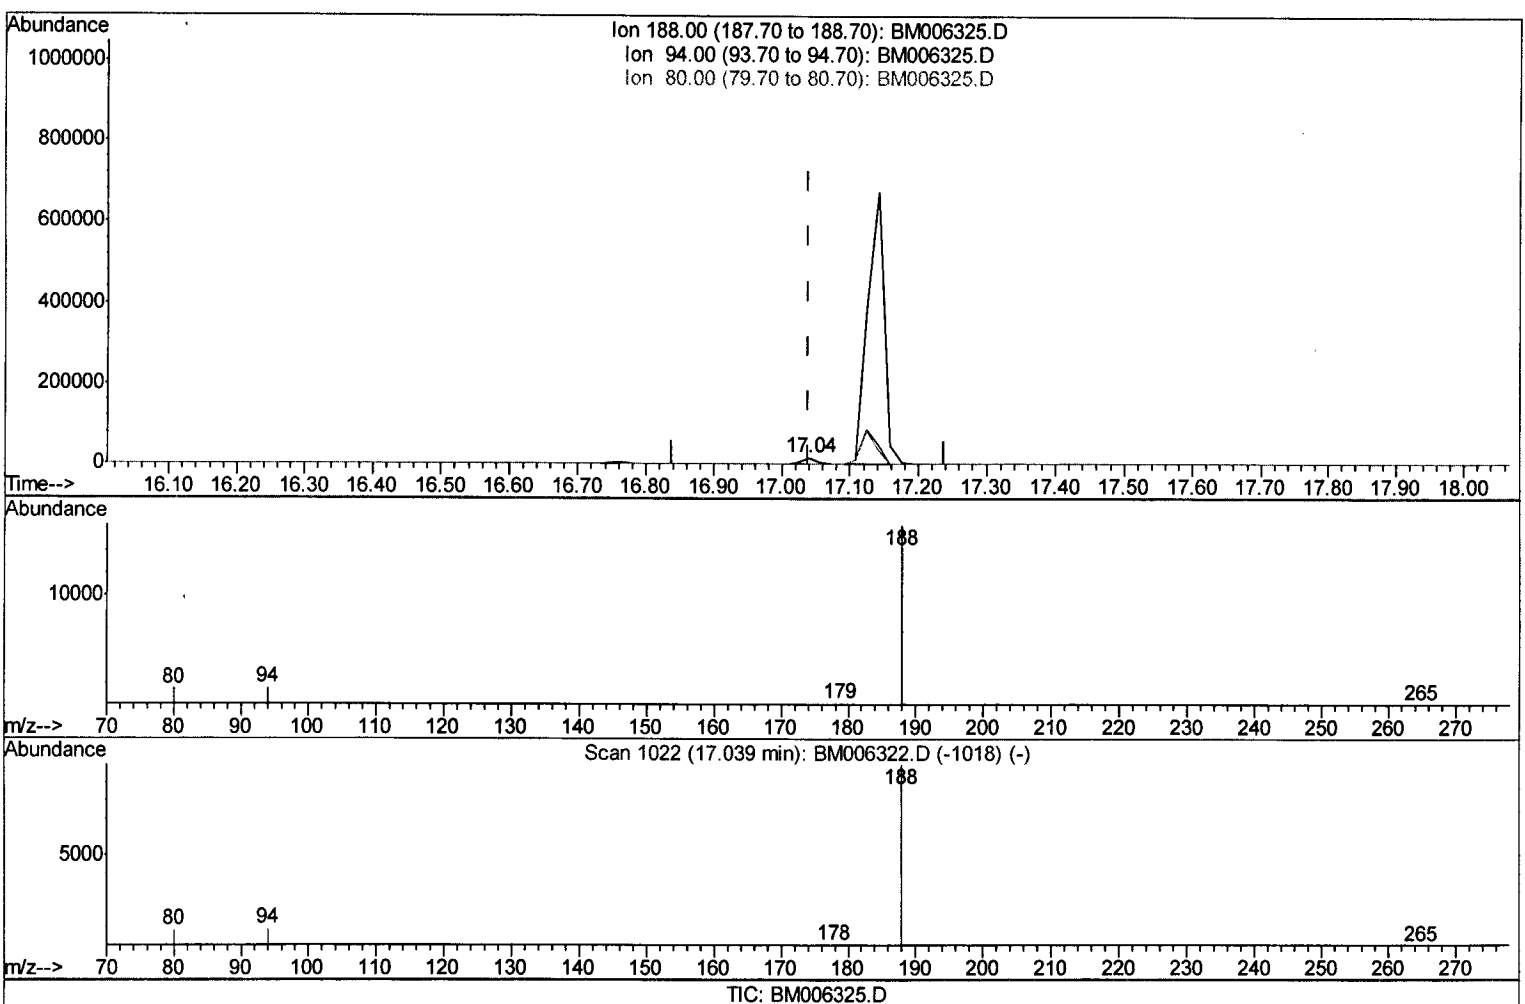

(12) Phenanthrene-d10 (I)

17.039min (-0.000) 0.40ng/ul m

response 23858

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	9.29#
80.00	11.90	8.92#
0.00	0.00	0.00

U.M.
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

APPROVED
 umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 03:46:20 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

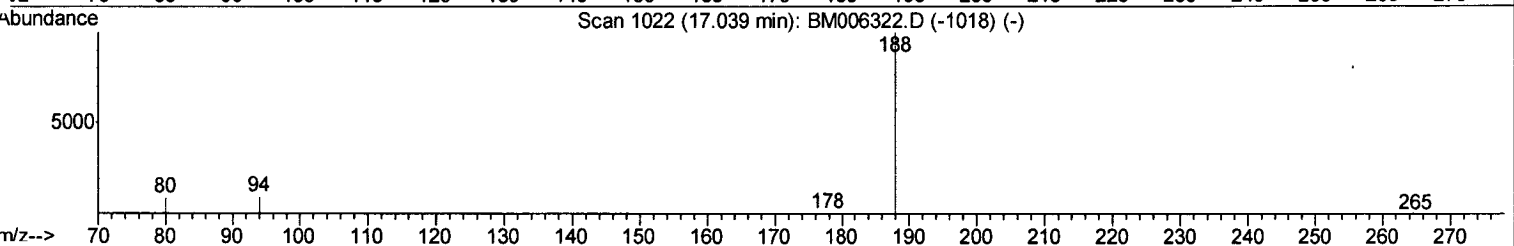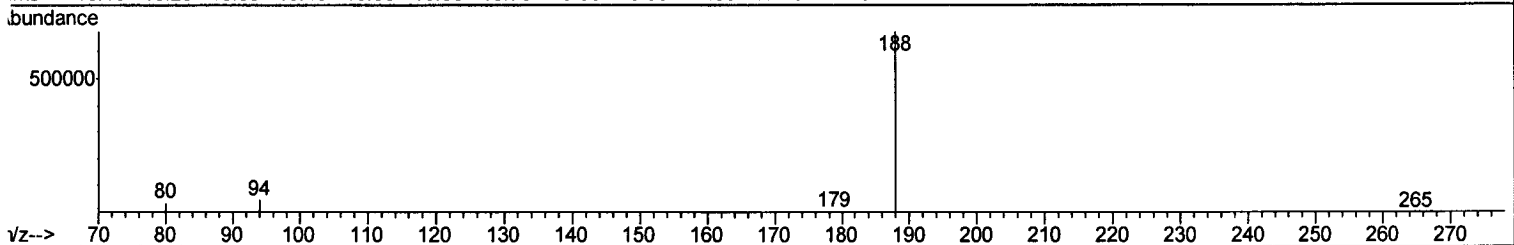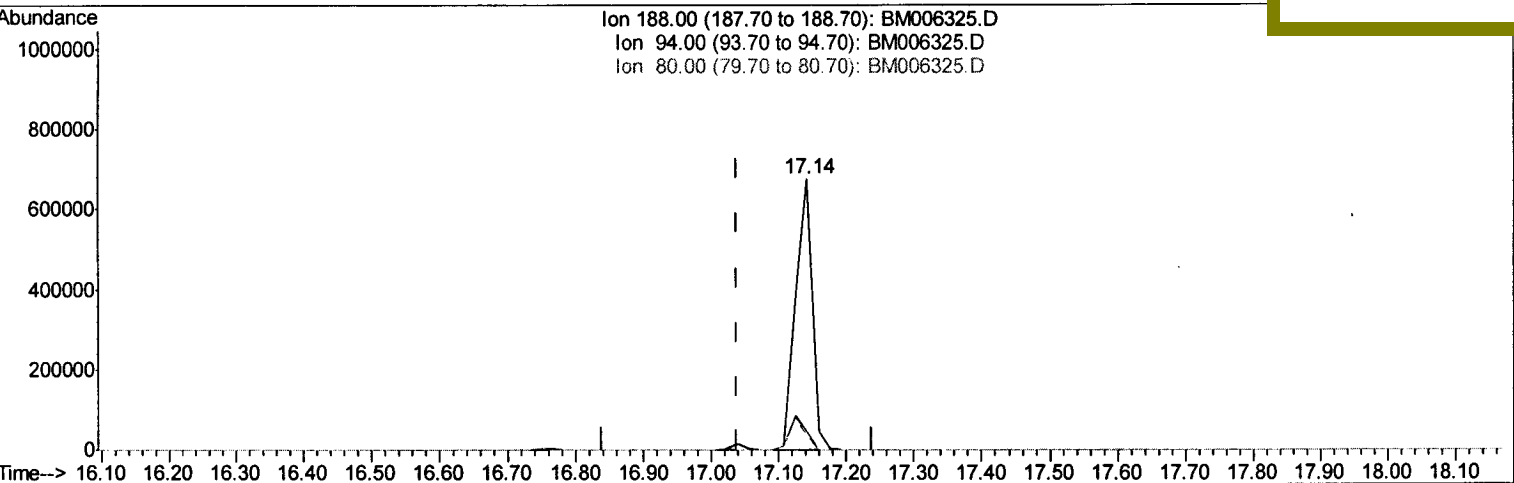

TIC: BM006325.D

(12) Phenanthrene-d10 (I)

17.142min (+0.103) 0.40ng/ul

response 1148485

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	6.86#
80.00	11.90	5.03#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4TV6MSD

Manual Integration

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:29:44 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

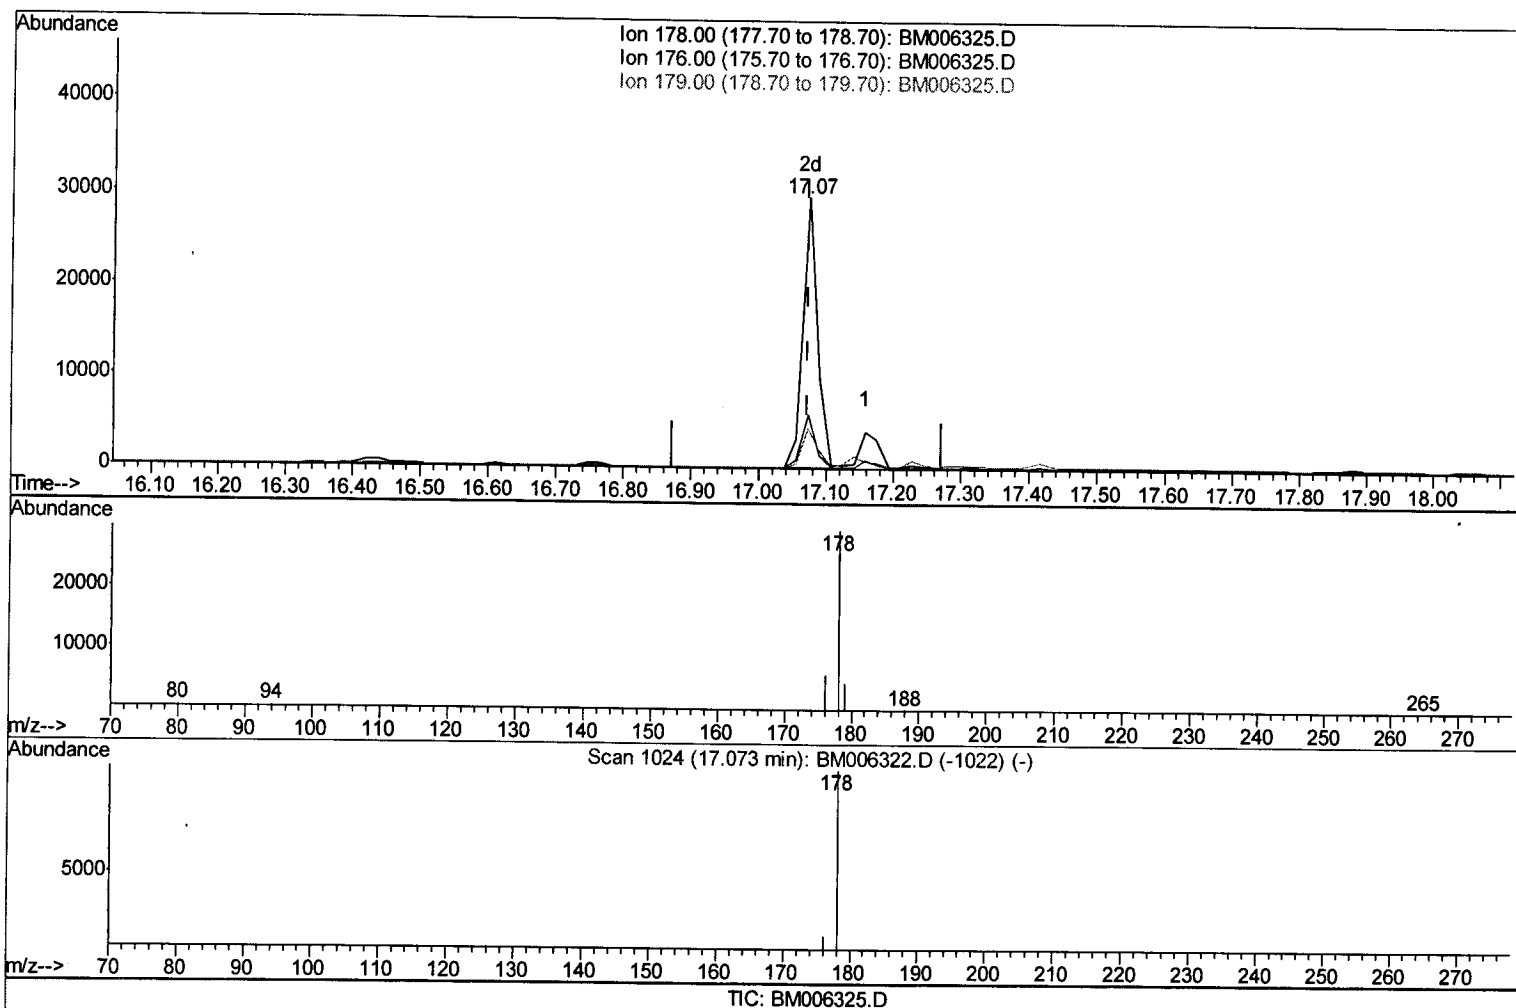

(14) Phenanthrene

17.073min (-0.000) 0.67ng/ul m U.M

response 44186

07/12/16

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	20.09#
179.00	17.70	15.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integrati

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 03:46:20 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

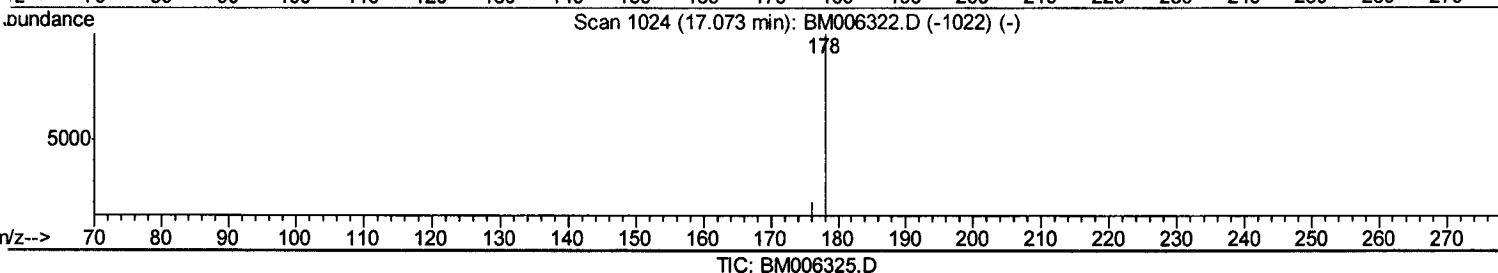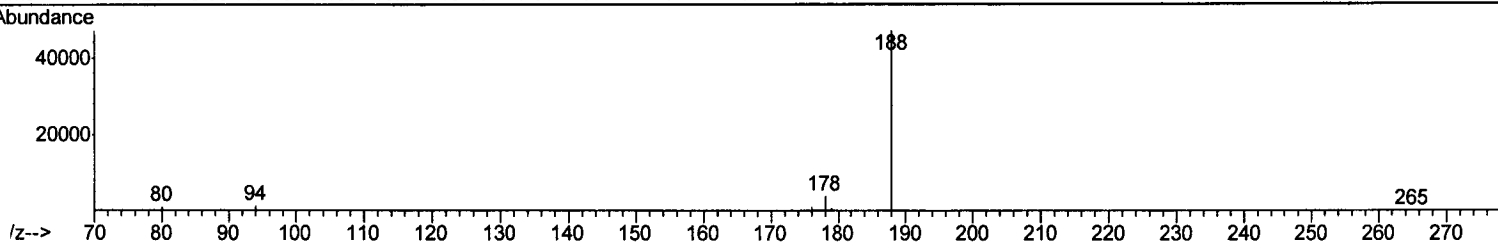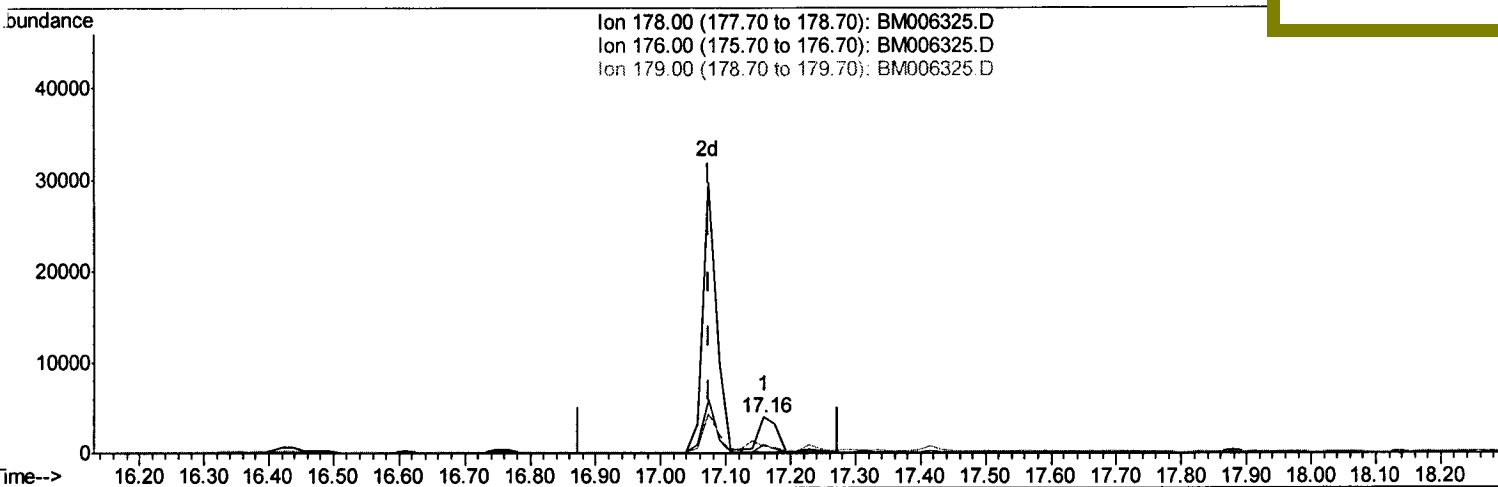

(14) Phenanthrene

17.159min (+0.086) 0.12ng/ul

response 8038

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	23.42#
179.00	17.70	20.51
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006325.D
Acq On : 07 Jul 2016 18:41
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample ID :
A4TV6MSD

Manual Integration

umangi
7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:29:44 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

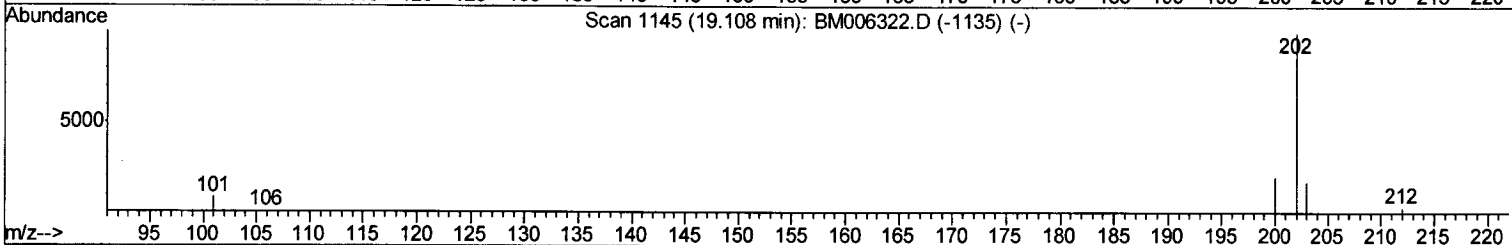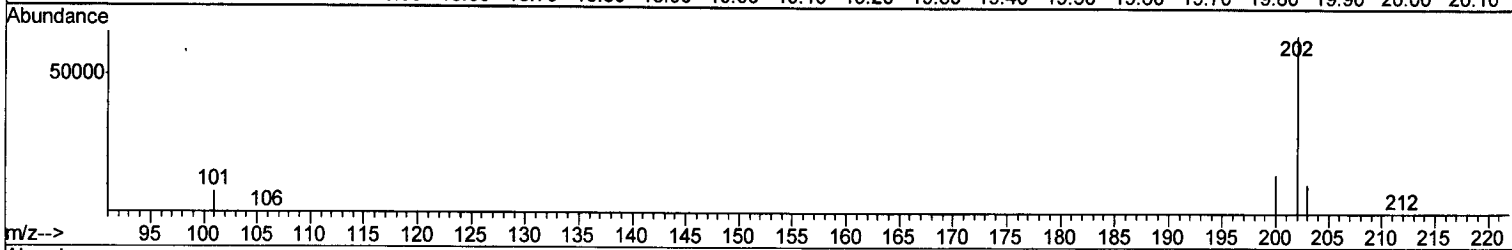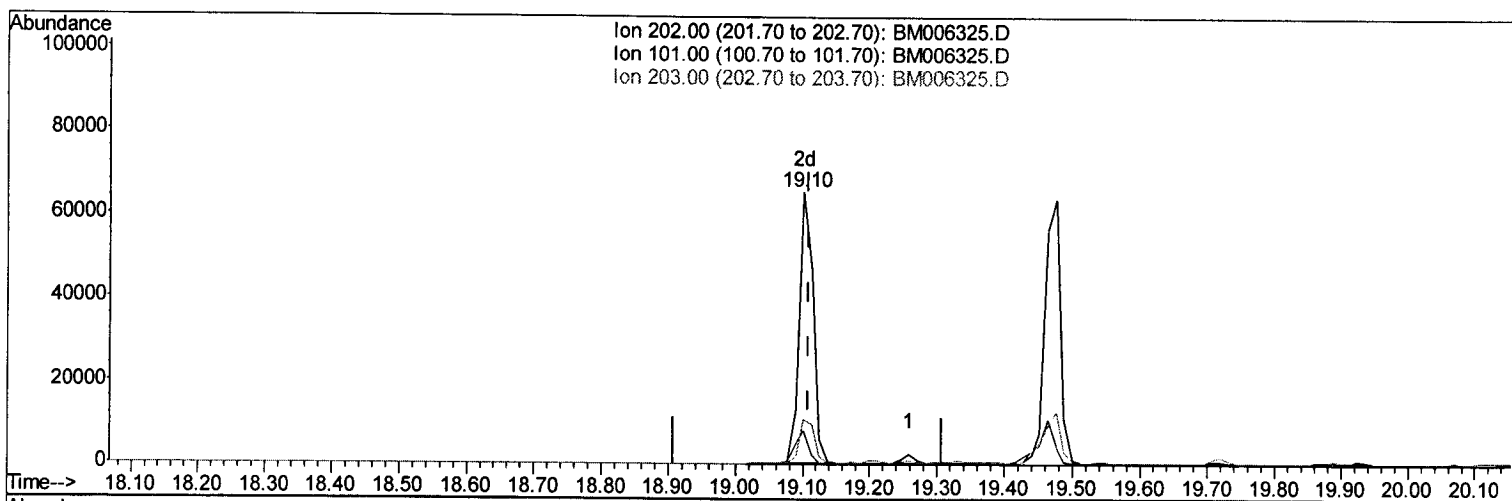

TIC: BM006325.D

(17) Fluoranthene (C)

19.101min (-0.007) 1.31ng/ul m U.M

response 95308

07/12/16

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	12.18
203.00	16.30	16.34
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006325.D
Acq On : 07 Jul 2016 18:41
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Manual Integration

umangi
7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:29:44 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

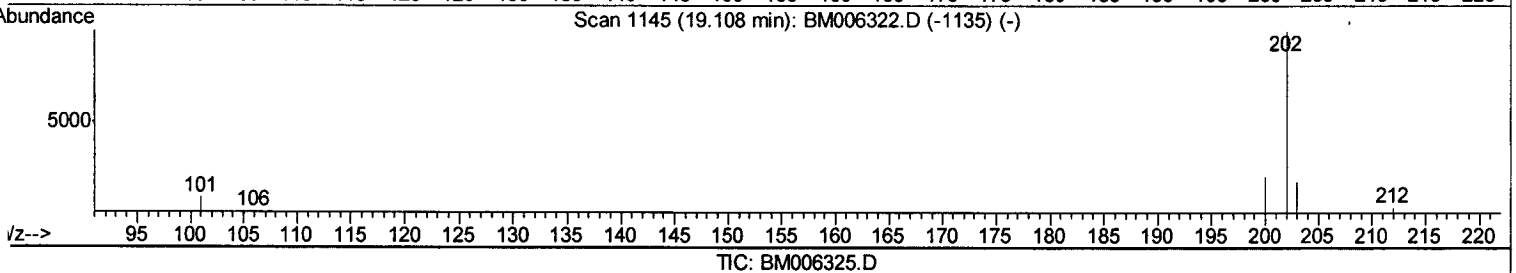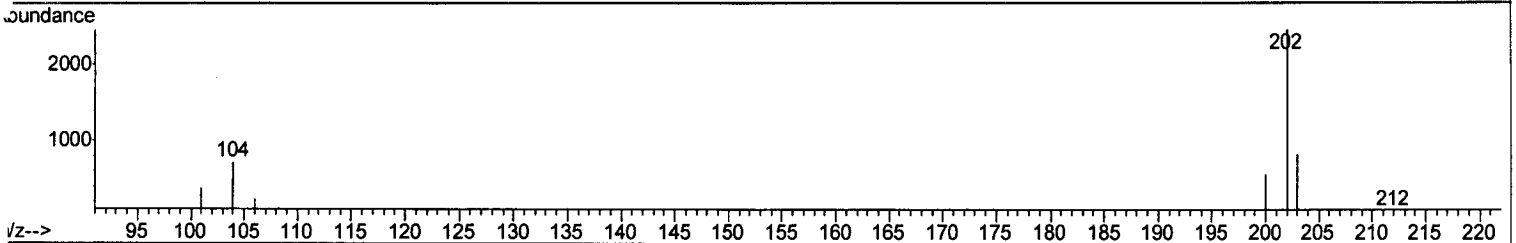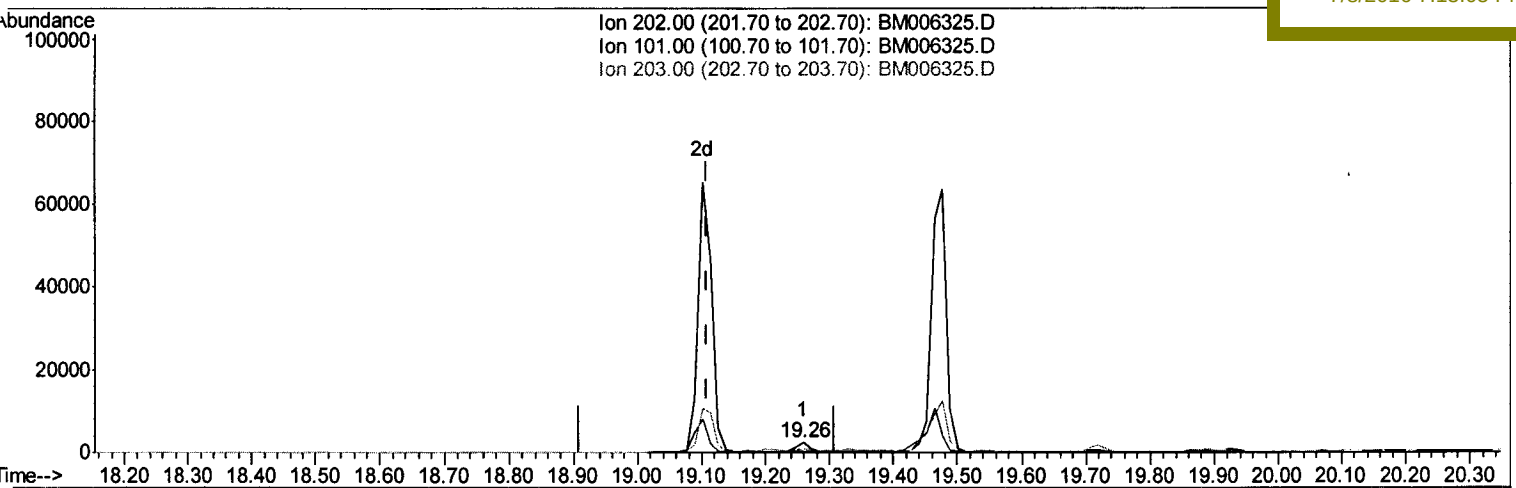

(17) Fluoranthene (C)

19.259min (+0.150) 0.04ng/ul

response 3158

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	15.05
203.00	16.30	33.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 08 04:29:44 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

umangi
 7/8/2016 7:13:05 PM

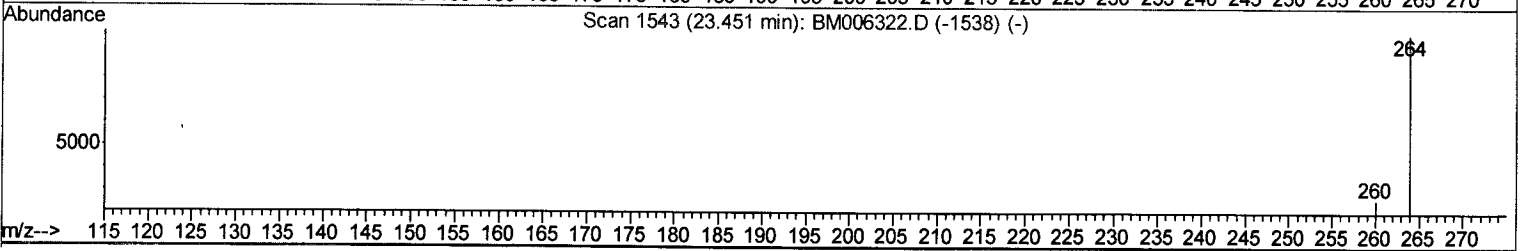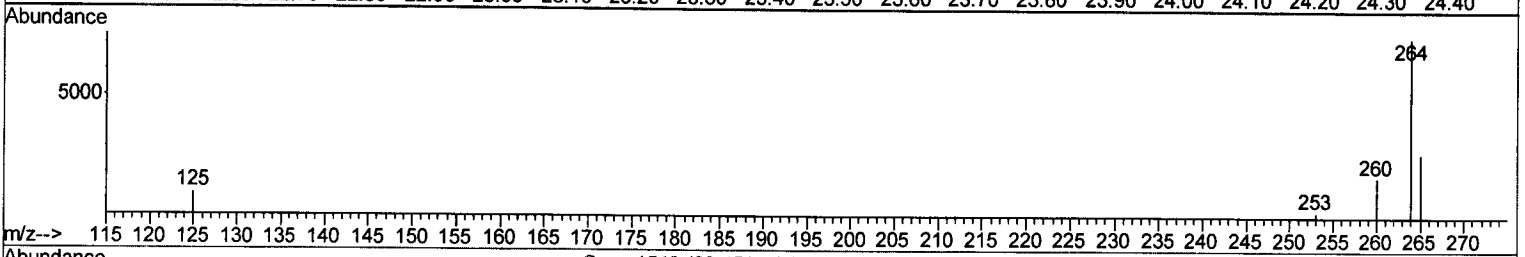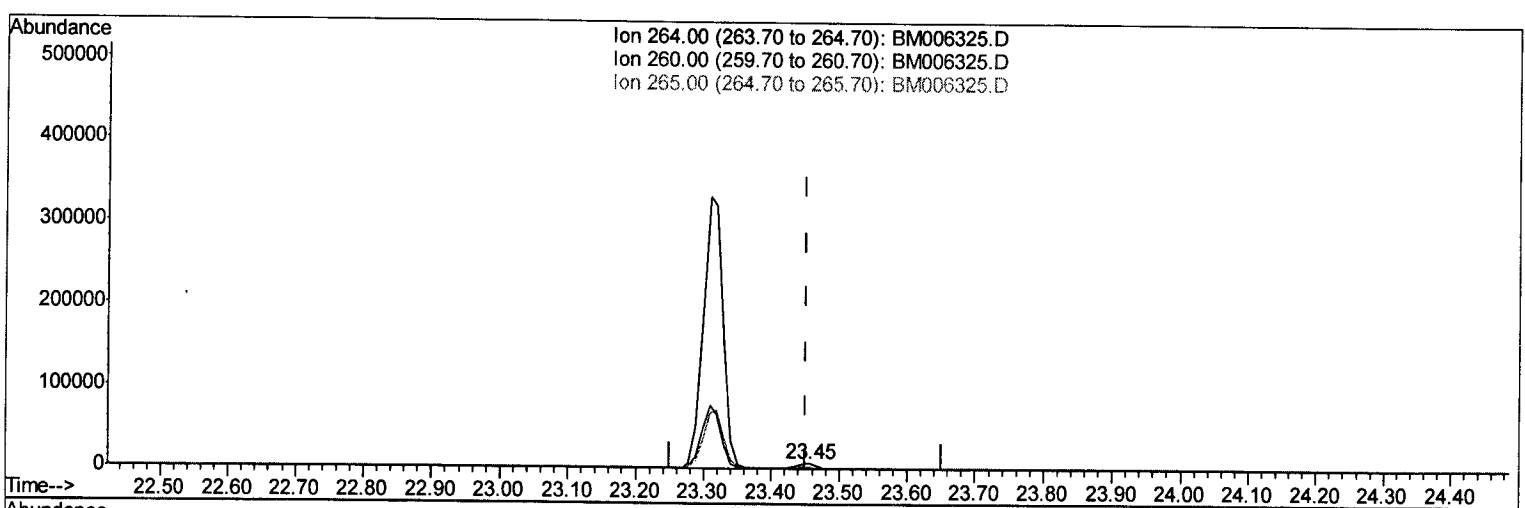

TIC: BM006325.D

(22) Perylene-d12 (I)

23.455min (+0.003) 0.40ng/ul m

response 11894

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.63
265.00	38.20	39.03
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Quant Time: Jul 08 04:29:44 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/8/2016 7:13:05 PM

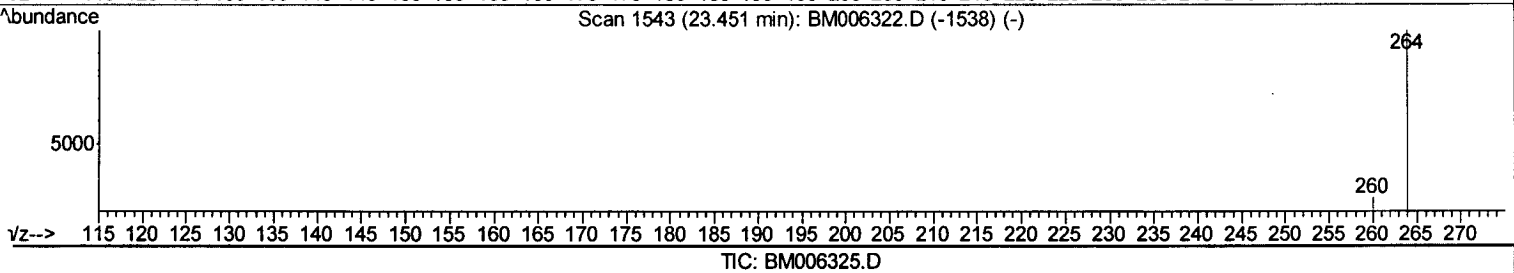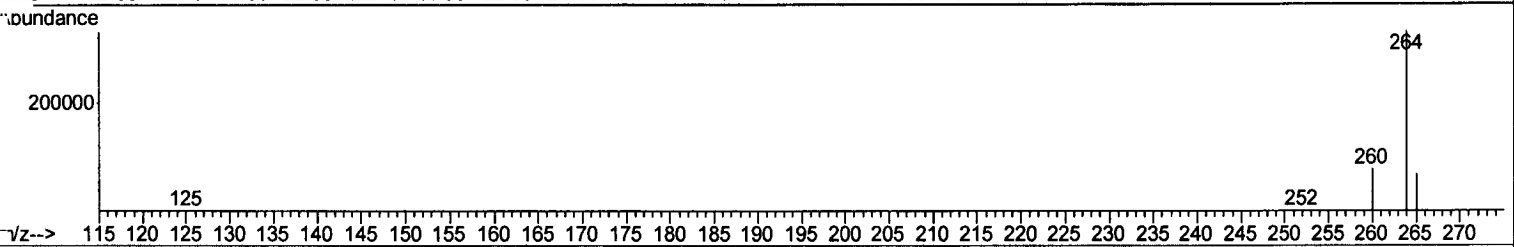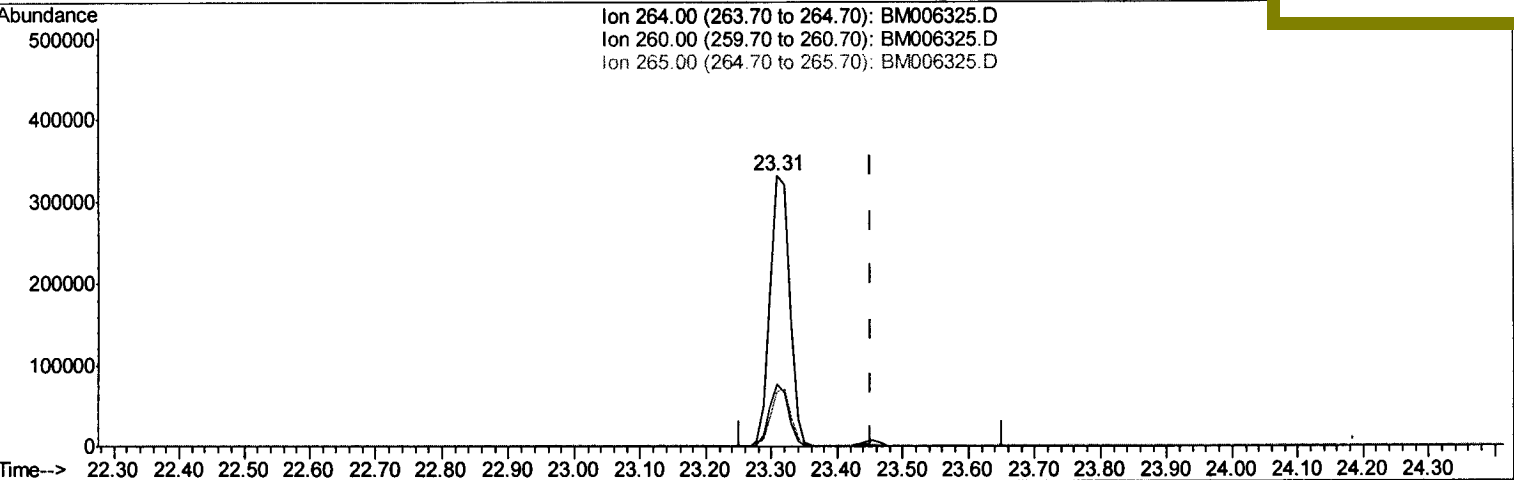

(22) Perylene-d12 (I)

23.309min (-0.143) 0.40ng/ul

response 674602

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	23.29
265.00	38.20	20.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

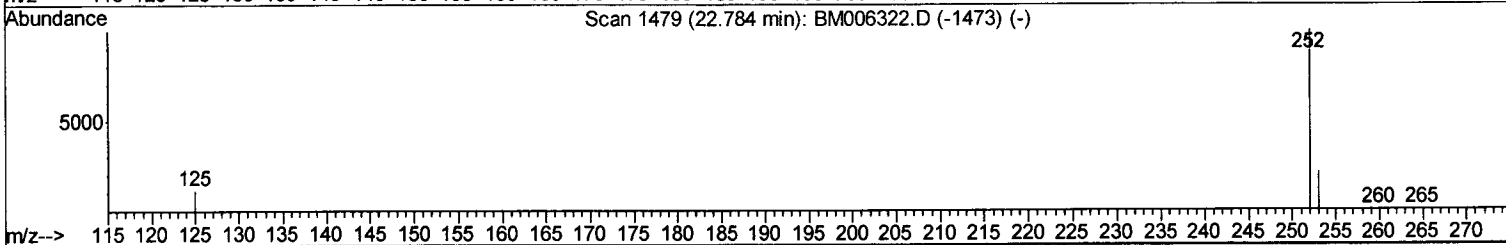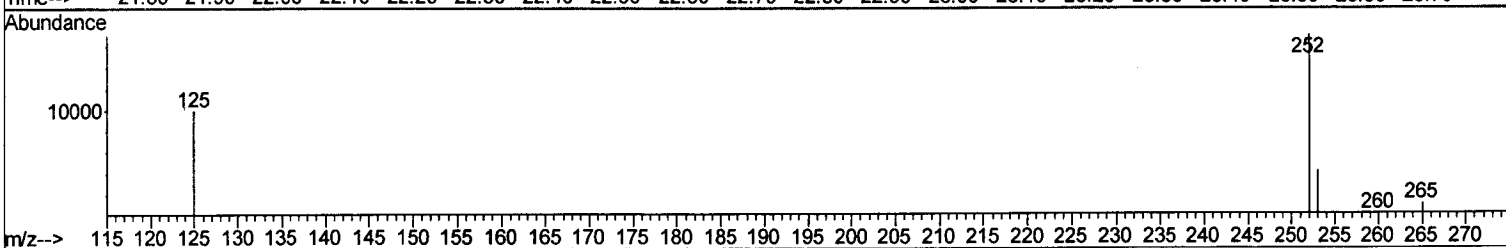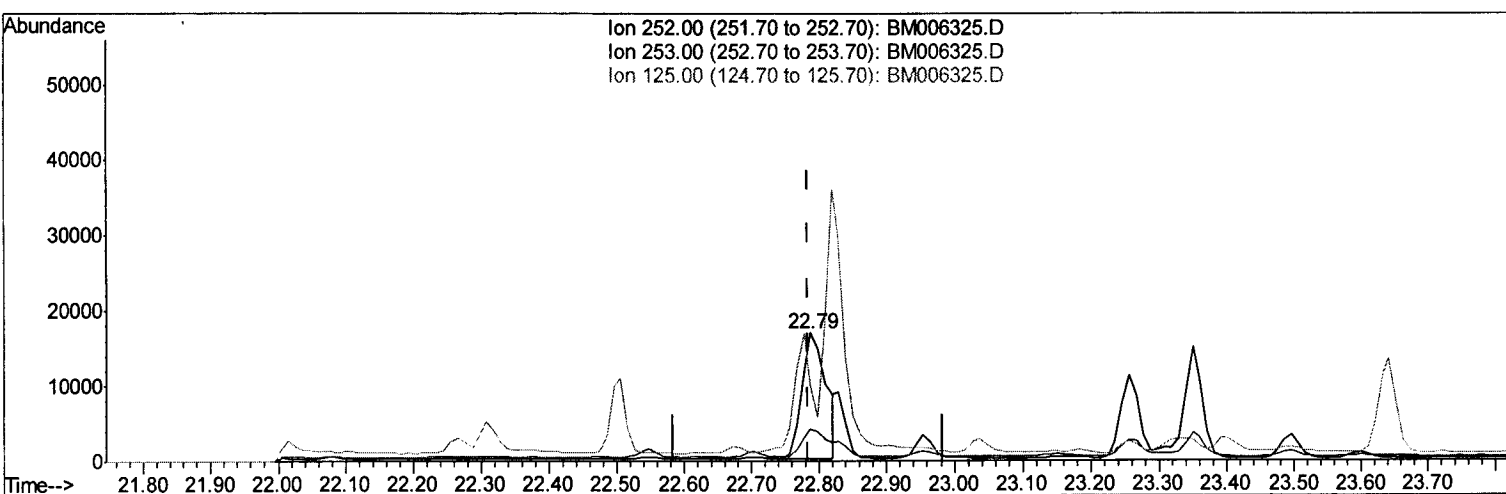

TIC: BM006325.D

(23) Benzo(b)fluoranthene

22.787min (+0.003) 0.98ng/ul m

response 41798

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	24.75
125.00	14.40	58.54#
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/8/2016 7:13:05 PM

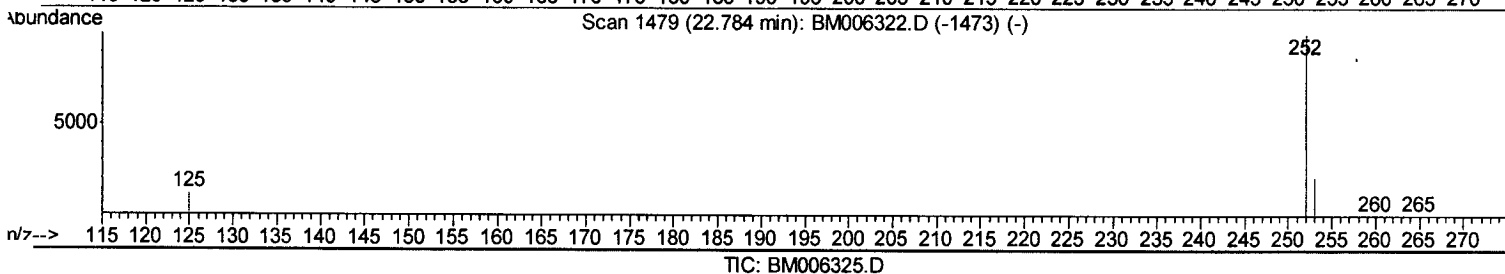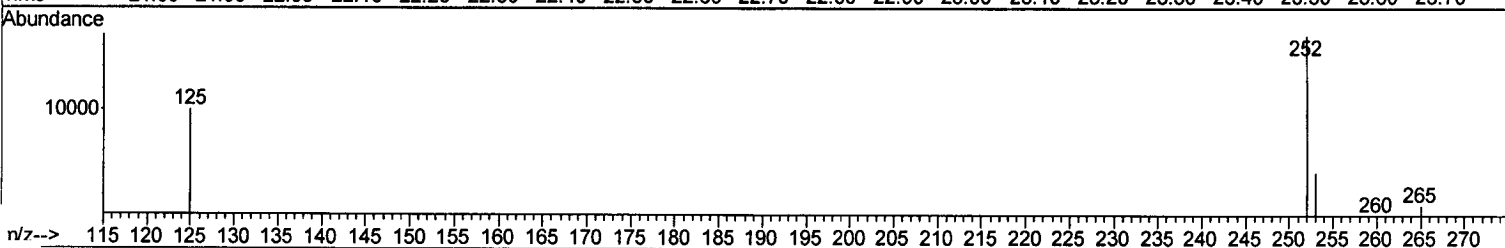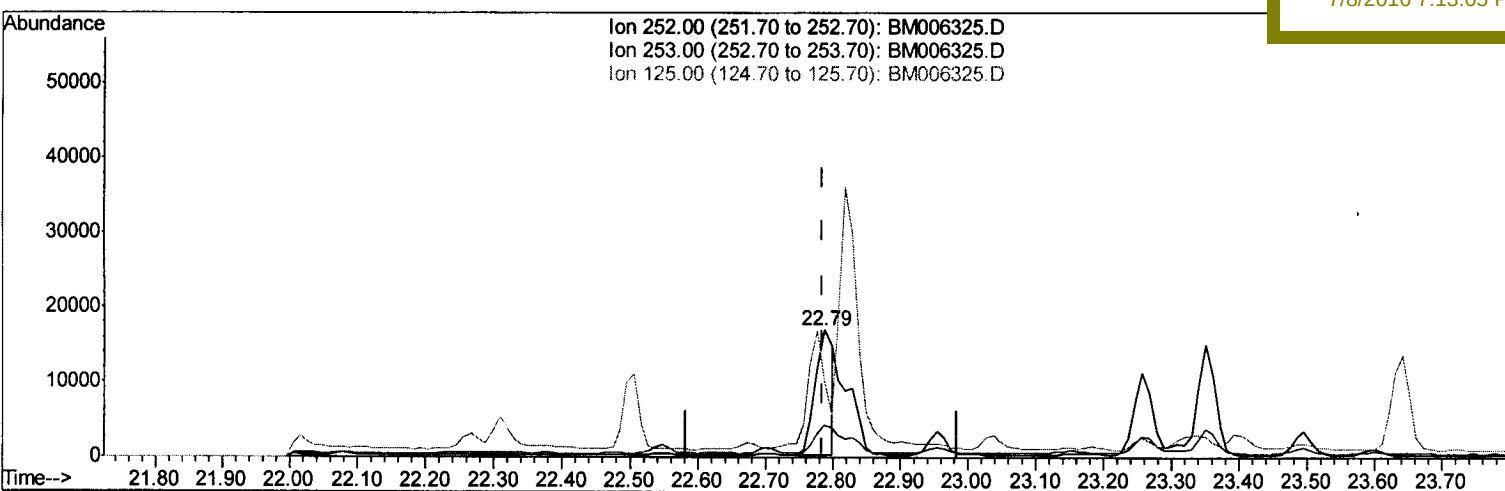

(23) Benzo(b)fluoranthene

22.787min (+0.003) 0.70ng/ul

response 29880

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	24.75
125.00	14.40	58.54#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

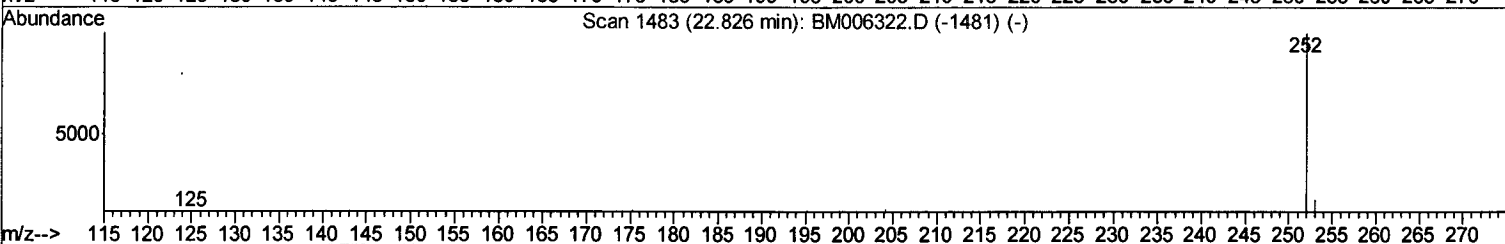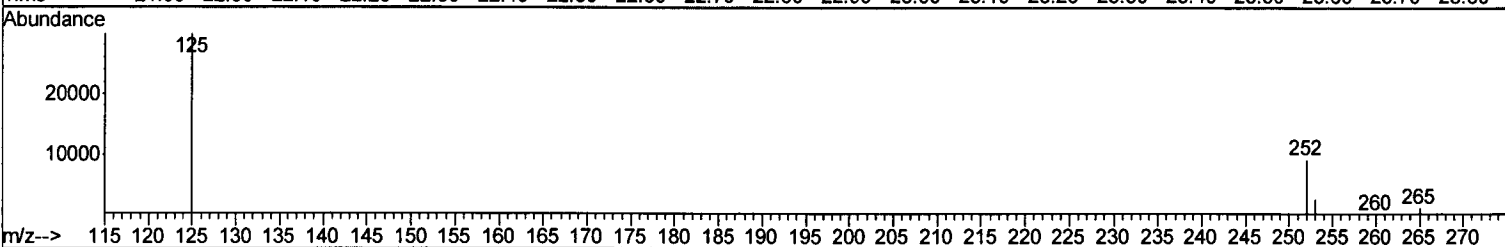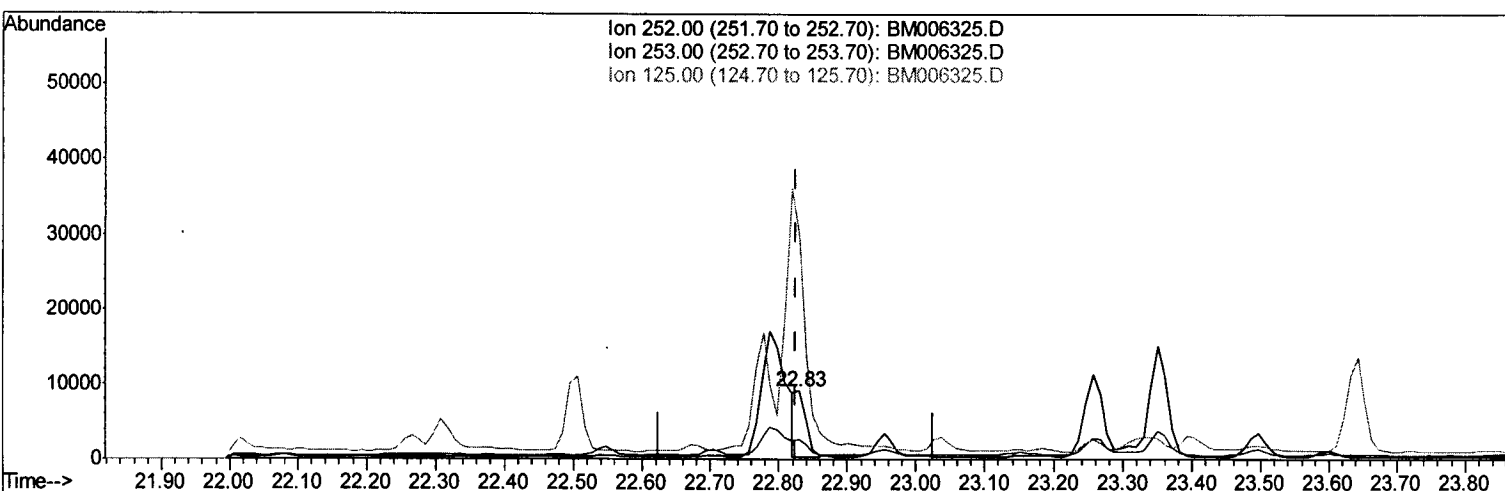

TIC: BM006325.D

(24) Benzo(k)fluoranthene

22.829min (+0.003) 0.24ng/ul m U.M

response 9374

Ion Exp% Act%

252.00 100 100

253.00 24.80 28.05

125.00 13.00 326.91#

0.00 0.00 0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/8/2016 7:13:05 PM

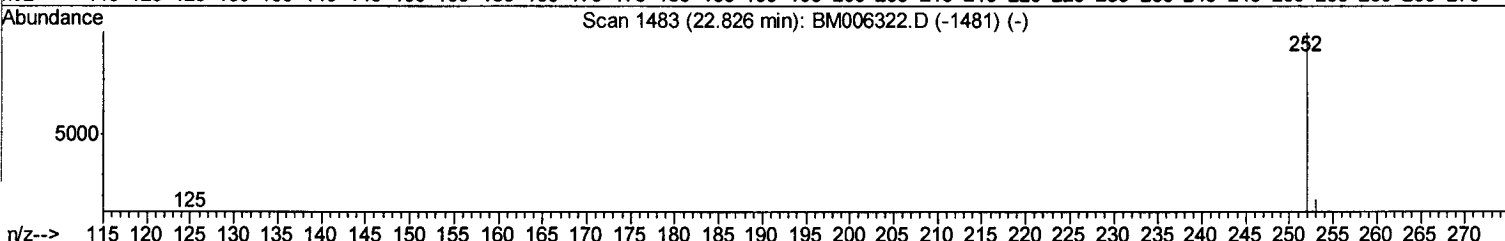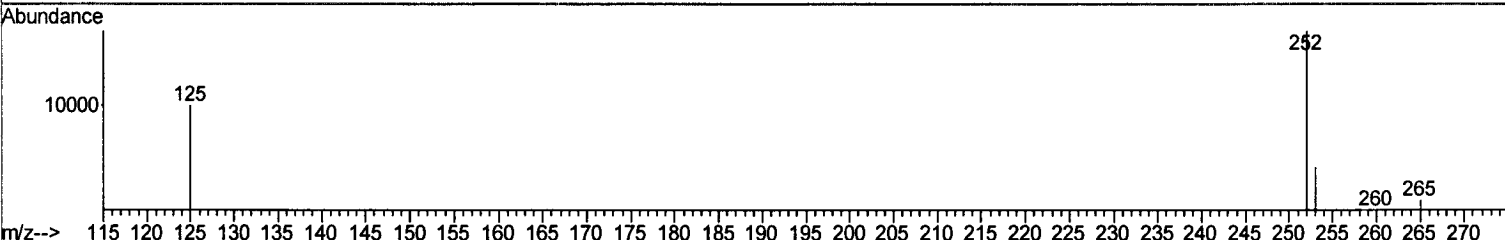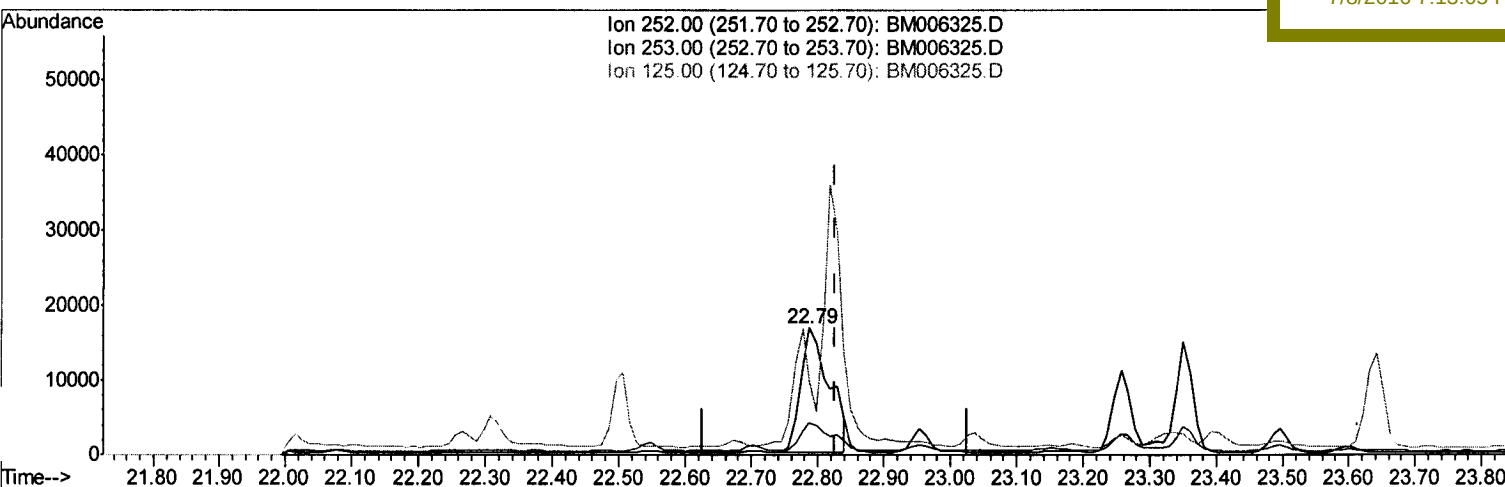

TIC: BM006325.D

(24) Benzo(k)fluoranthene

22.787min (-0.039) 1.26ng/ul

response 49844

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	24.75
125.00	13.00	58.54#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

umangi
 7/8/2016 7:13:05 PM

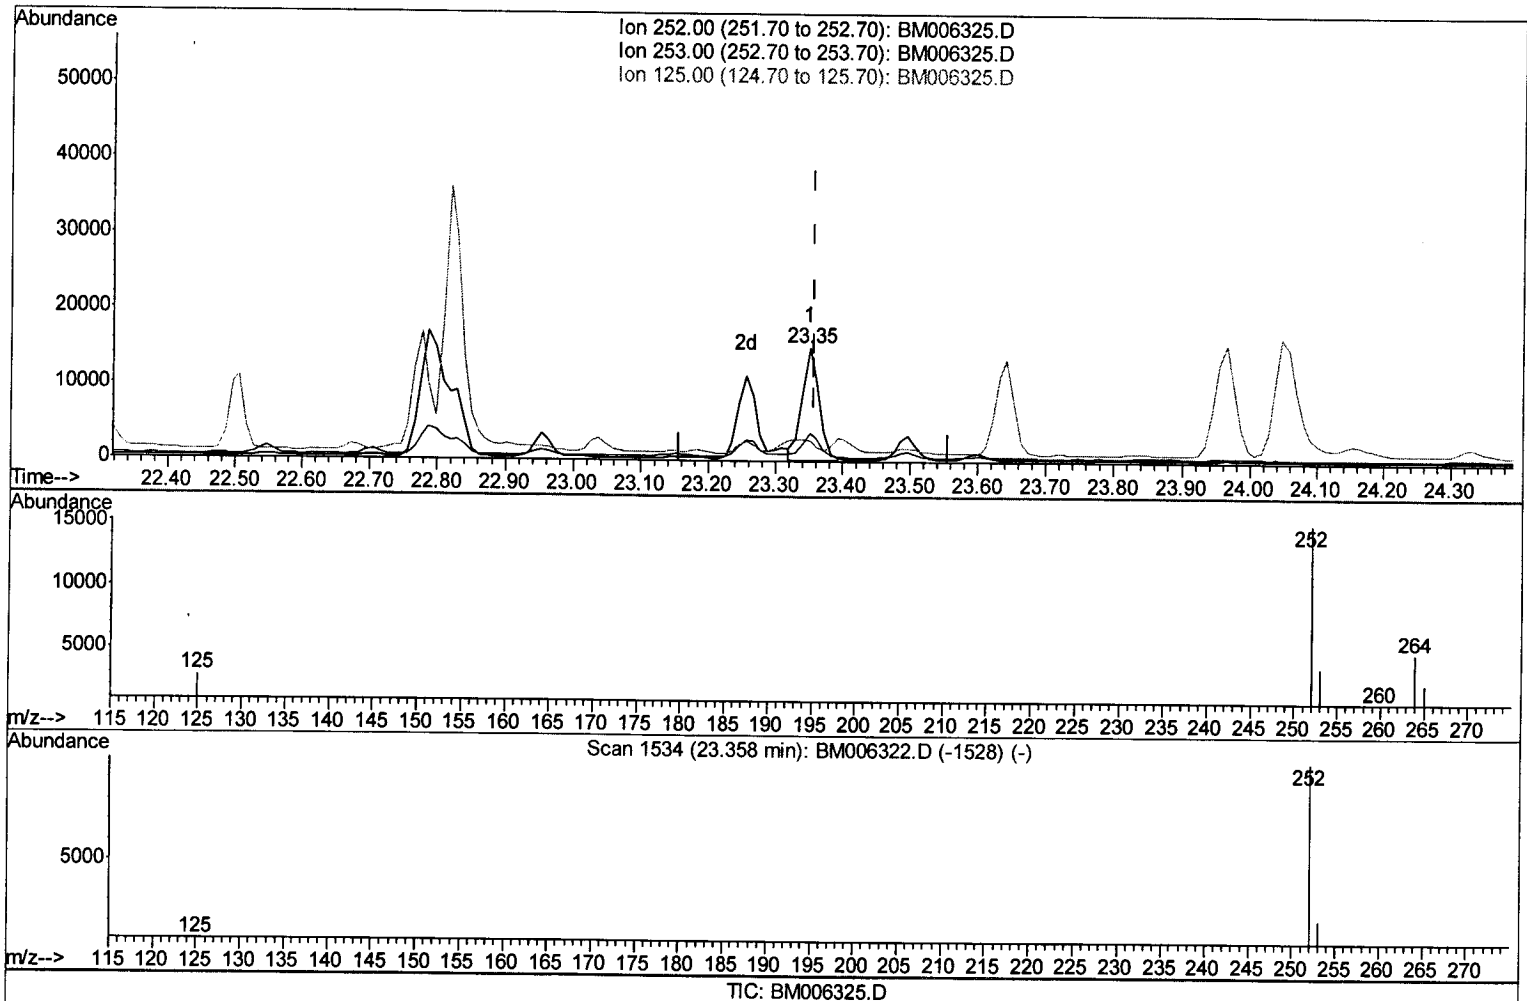

(25) Benzo(a)pyrene (C)

23.350min (-0.007) 0.66ng/ul m

response 26041

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	24.87
125.00	15.90	18.40
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)


```
Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\  
Data File : BM006325.D  
Acq On    : 07 Jul 2016   18:41  
Operator  : UM/SJ  
Sample    : H3811-08MSD  
Misc      :  
ALS Vial  : 16      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Manual Integrati

umangi
7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:32:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

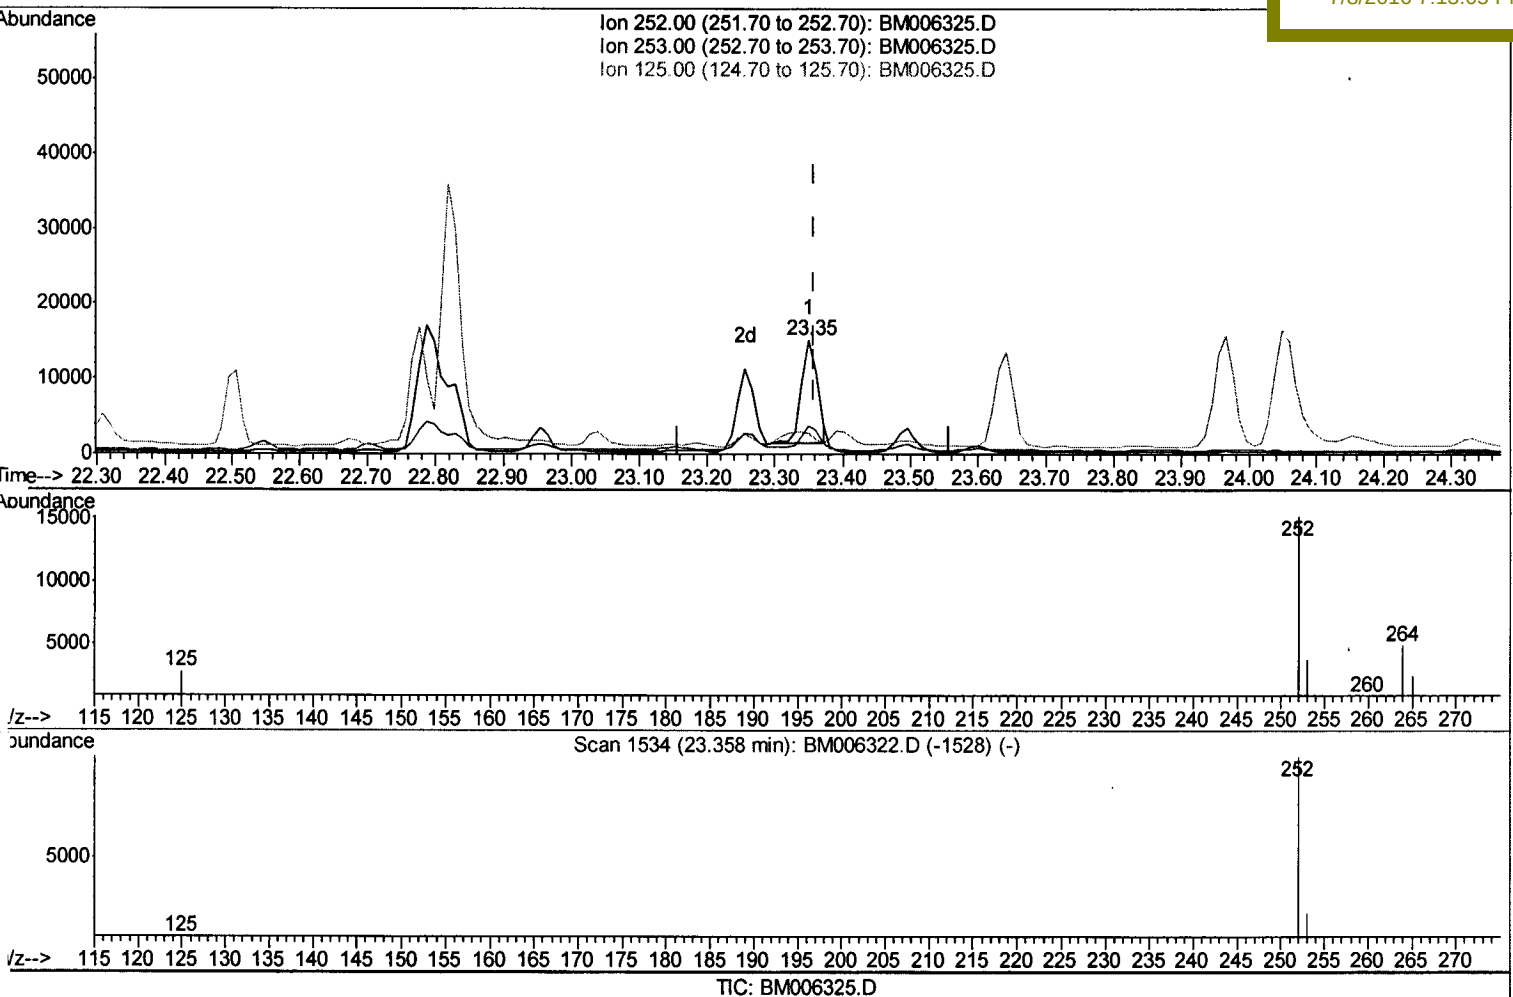

(25) Benzo(a)pyrene (C)

23.350min (-0.007) 0.55ng/ul

response 21812

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	24.87
125.00	15.90	18.40
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

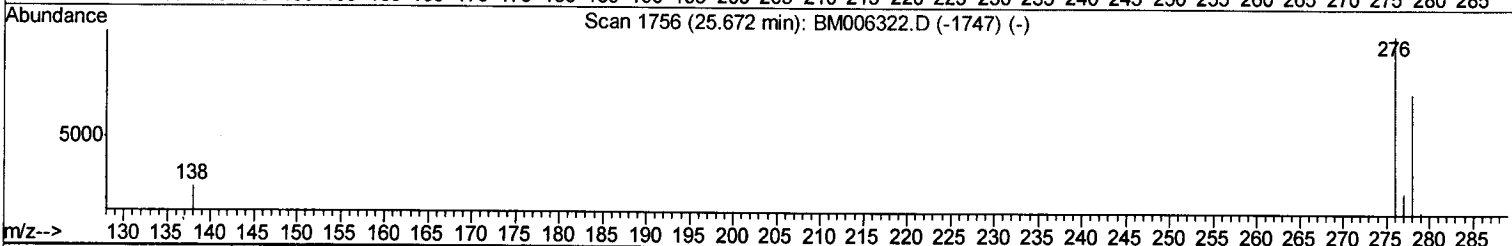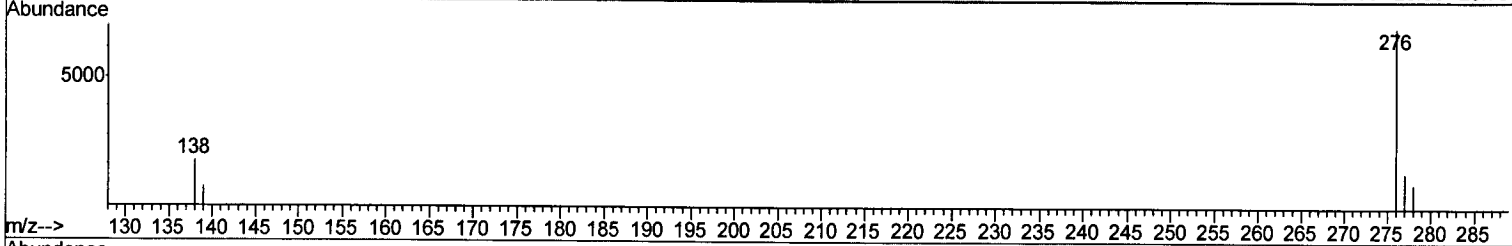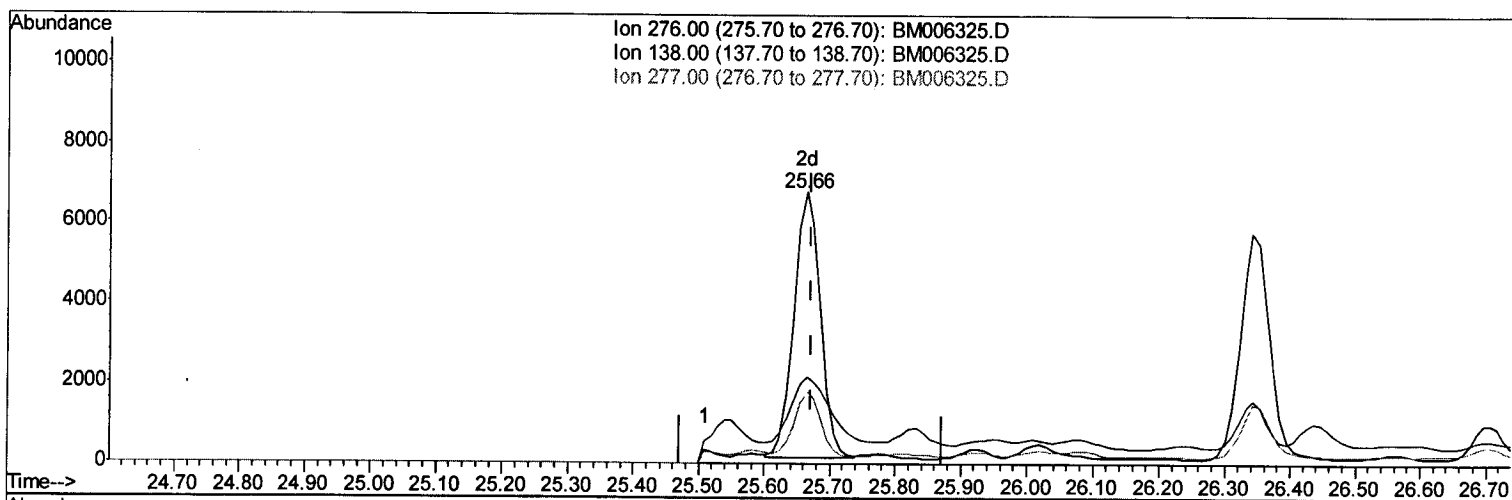

TIC: BM006325.D

(26) Indeno(1,2,3-cd)pyrene

25.665min (-0.007) 0.42ng/ul m

response 18633

Ion Exp% Act%

276.00 100 100

138.00 20.40 0.00#

277.00 24.80 4.18#

0.00 0.00 0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integrati

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

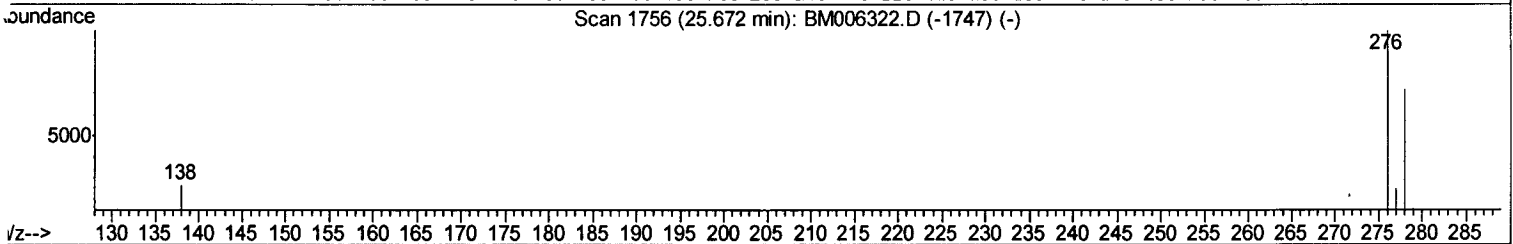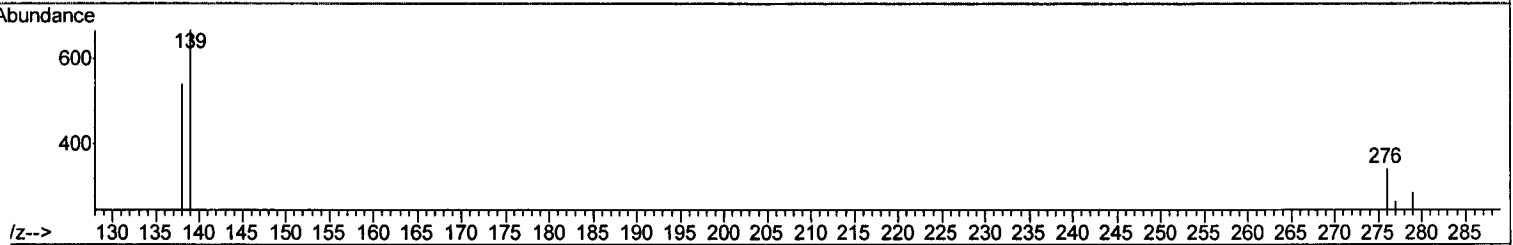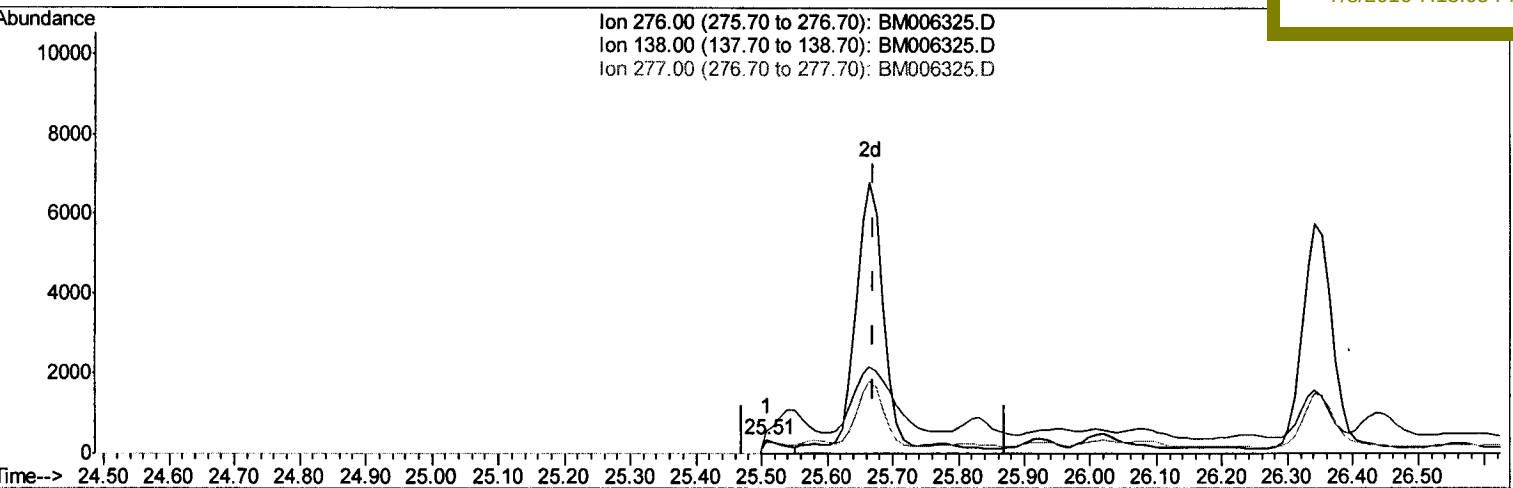

TIC: BM006325.D

(26) Indeno(1,2,3-cd)pyrene

25.508min (-0.164) 0.02ng/ul

response 740

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	0.00#
277.00	24.80	105.14#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/8/2016 7:13:05 PM

Quant Time: Jul 08 04:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

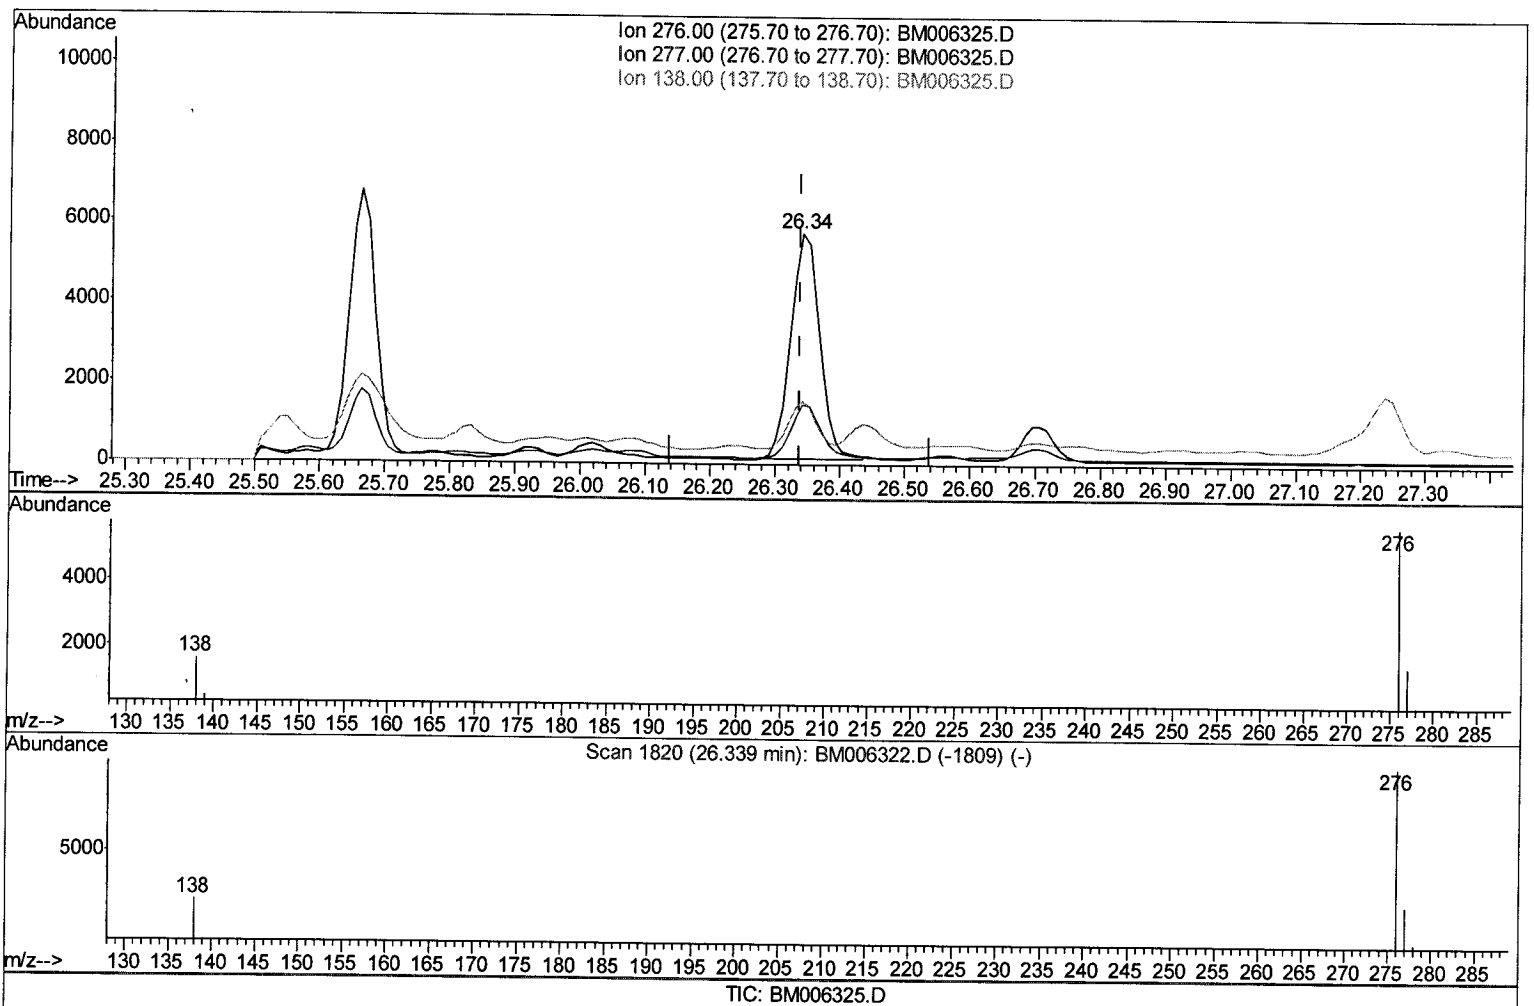

TIC: BM006325.D

(28) Benzo(g,h,i)perylene

26.342min (+0.003) 0.47ng/ul m *U.M*
07/12/16
 response 17541

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	25.73
138.00	28.10	27.33
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006325.D
Acq On : 07 Jul 2016 18:41
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Quant Time: Jul 08 04:32:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

Manual Integration

APPROVED
umangi
7/8/2016 7:13:05 PM

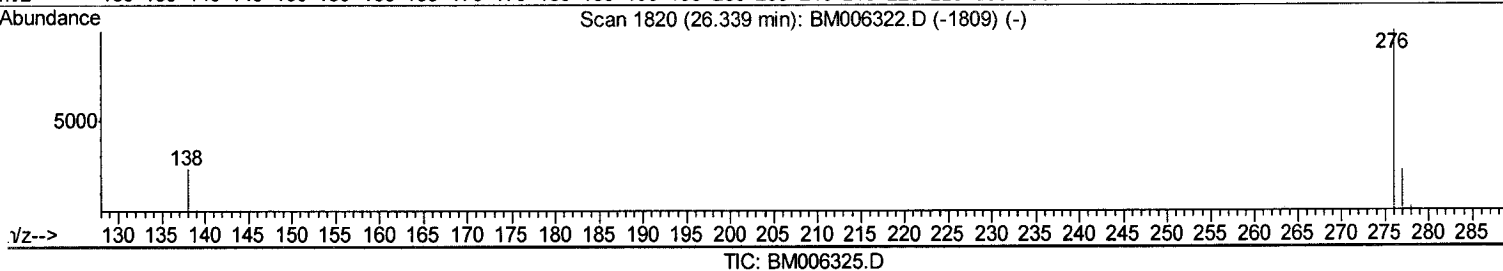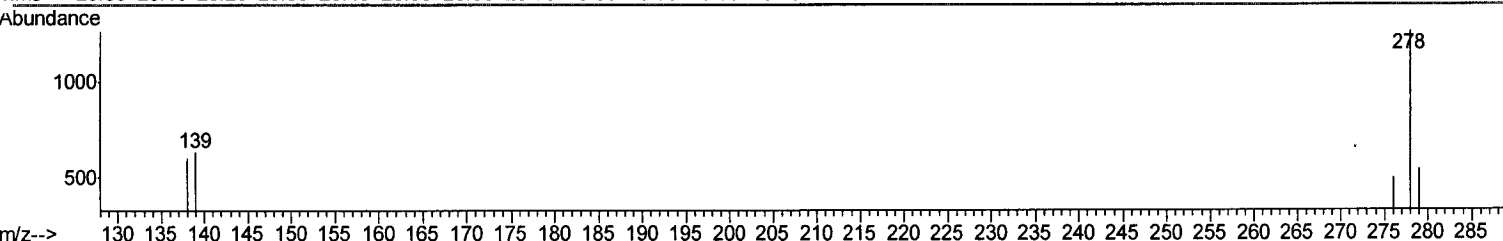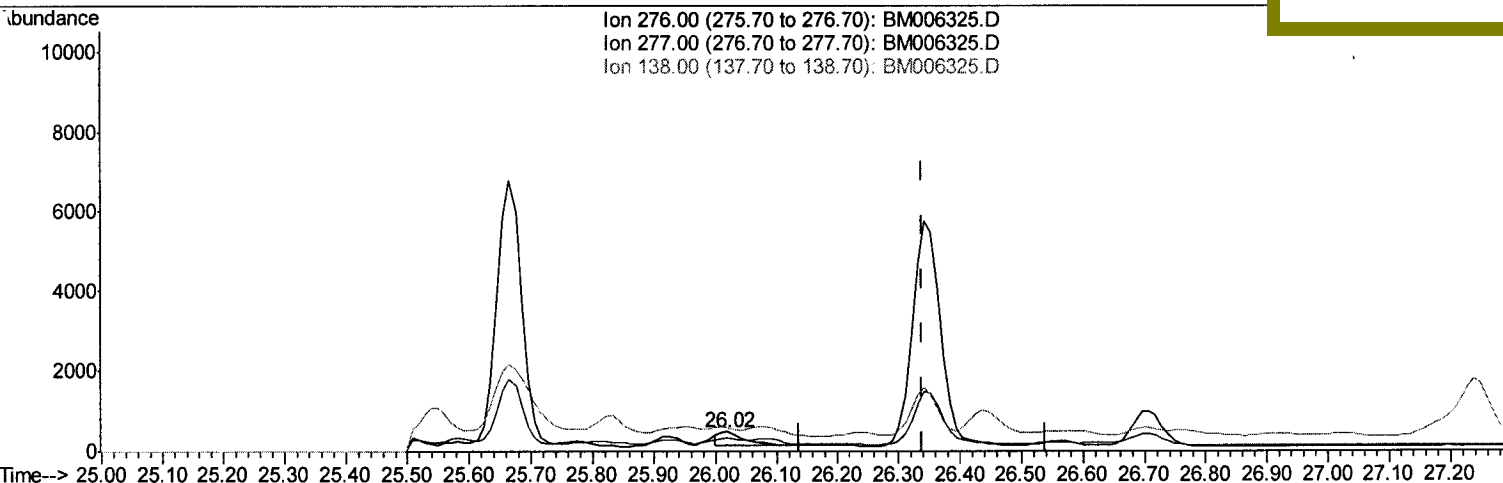

(28) Benzo(g,h,i)perylene

26.019min (-0.320) 0.03ng/ul

response 1007

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	66.40#
138.00	28.10	122.40#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006325.D
 Acq On : 07 Jul 2016 18:41
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Quant Time: Jul 08 04:35:16 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/8/2016 7:13:05 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4648	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	18543	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	10878	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.04	188	23858m	0.40	ng/ul	0.00
18) Chrysene-d12	21.24	240	18062	0.40	ng/ul	0.00
22) Perylene-d12	23.45	264	11894m	0.40	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	7243	3.69	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.02	152	7007	0.32	ng/ul	0.00
16) Fluoranthene-d10	19.08	212	16140	0.32	ng/ul	0.00

Target Compounds

					Ovalue
5) Naphthalene	10.48	128	1436	0.03	ng/ul# 80
7) 2-Methylnaphthalene	12.09	142	766	0.03	ng/ul 97
9) Acenaphthylene	14.01	152	3834	0.10	ng/ul# 94
10) Acenaphthene	14.35	153	10119	0.28	ng/ul 90
11) Fluorene	15.34	166	1587	0.04	ng/ul# 78
13) Pentachlorophenol	16.70	266	1985	0.54	ng/ul 96
14) Phenanthrene	17.07	178	44186m	0.67	ng/ul 88
15) Anthracene	17.16	178	8058	0.13	ng/ul# 92
17) Fluoranthene	19.10	202	95308m	1.31	ng/ul 91
19) Pyrene	19.48	202	101960	1.35	ng/ul# 96
20) Benzo(a)anthracene	21.22	228	32824	0.56	ng/ul# 91
21) Chrysene	21.28	228	36737	0.64	ng/ul 96
23) Benzo(b)fluoranthene	22.79	252	41798m	0.98	ng/ul
24) Benzo(k)fluoranthene	22.83	252	9374m	0.24	ng/ul
25) Benzo(a)pyrene	23.35	252	26041m	0.66	ng/ul
26) Indeno(1,2,3-cd)pyrene	25.66	276	18633m	0.42	ng/ul
28) Benzo(a,h,i)perylene	26.34	276	17541m	0.47	ng/ul

(#) = qualifier out of range (m) = manual integration (+) = signals summed