

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:52:09 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

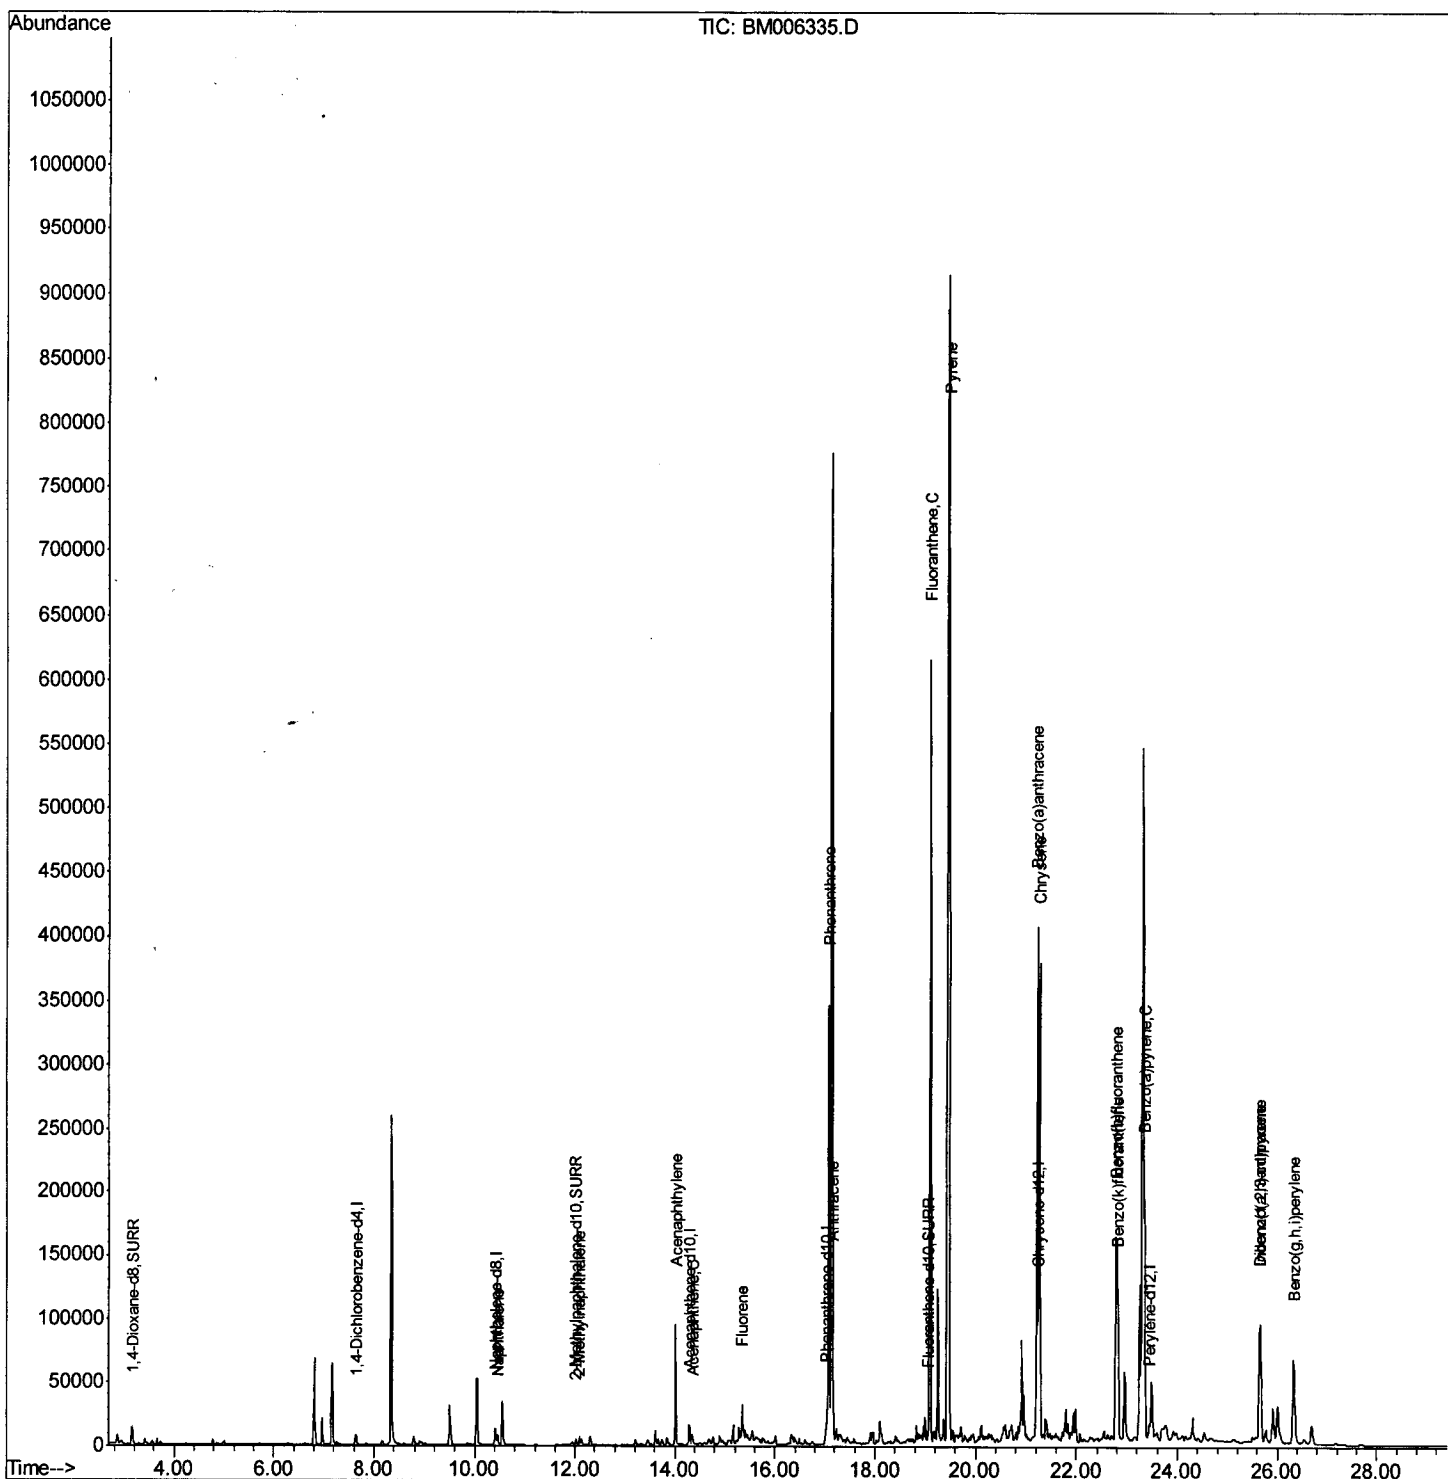

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integration

Quant Time: Jul 08 03:48:02 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/8/2016 7:14:15 PM

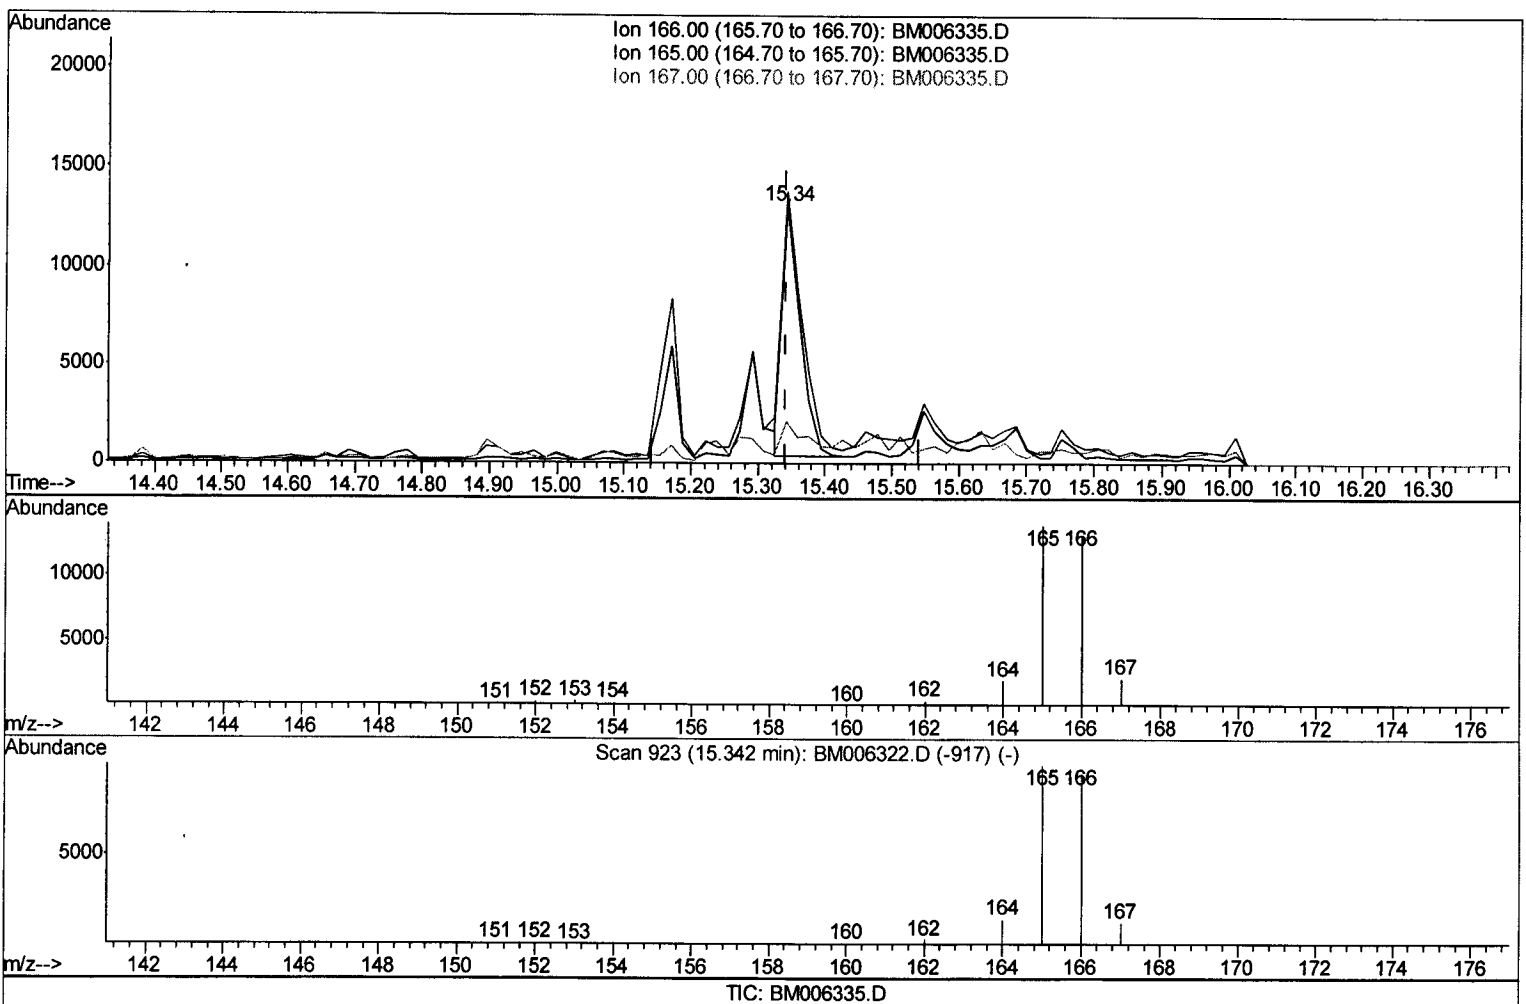

(11) Fluorene

15.342min (+0.000) 0.55ng/ul m

response 24257

Ion	Exp%	Act%
166.00	100	100
165.00	87.00	105.44#
167.00	14.90	16.15
0.00	0.00	0.00

U.M
 07/12/16


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006335.D
Acq On : 08 Jul 2016 00:43
Operator : UM/SJ
Sample : H3811-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TW3

Manual Integration

umangi
7/8/2016 7:14:15 PM

Quant Time: Jul 08 03:48:02 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

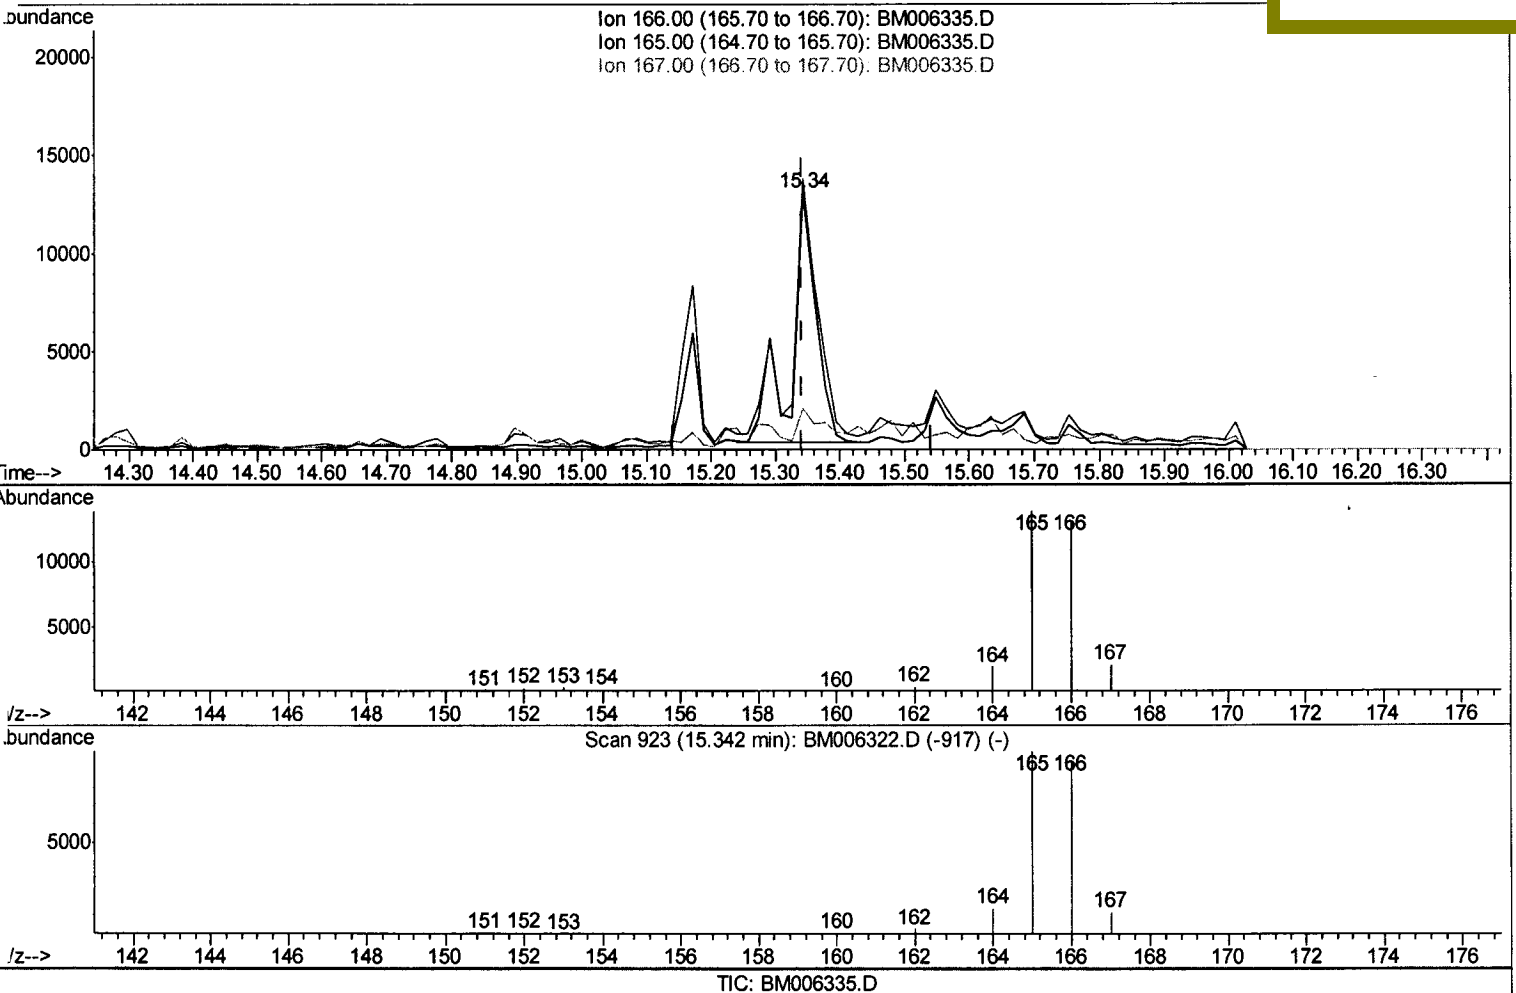

(11) Fluorene

15.342min (+0.000) 0.77ng/ul

response 33713

Ion	Exp%	Act%
166.00	100	100
165.00	87.00	105.44#
167.00	14.90	16.15
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006335.D
Acq On : 08 Jul 2016 00:43
Operator : UM/SJ
Sample : H3811-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
Client Sampled :
A4TW3

Manual Integration

APPROVED
umangi
7/8/2016 7:14:15 PM

Quant Time: Jul 08 03:48:02 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

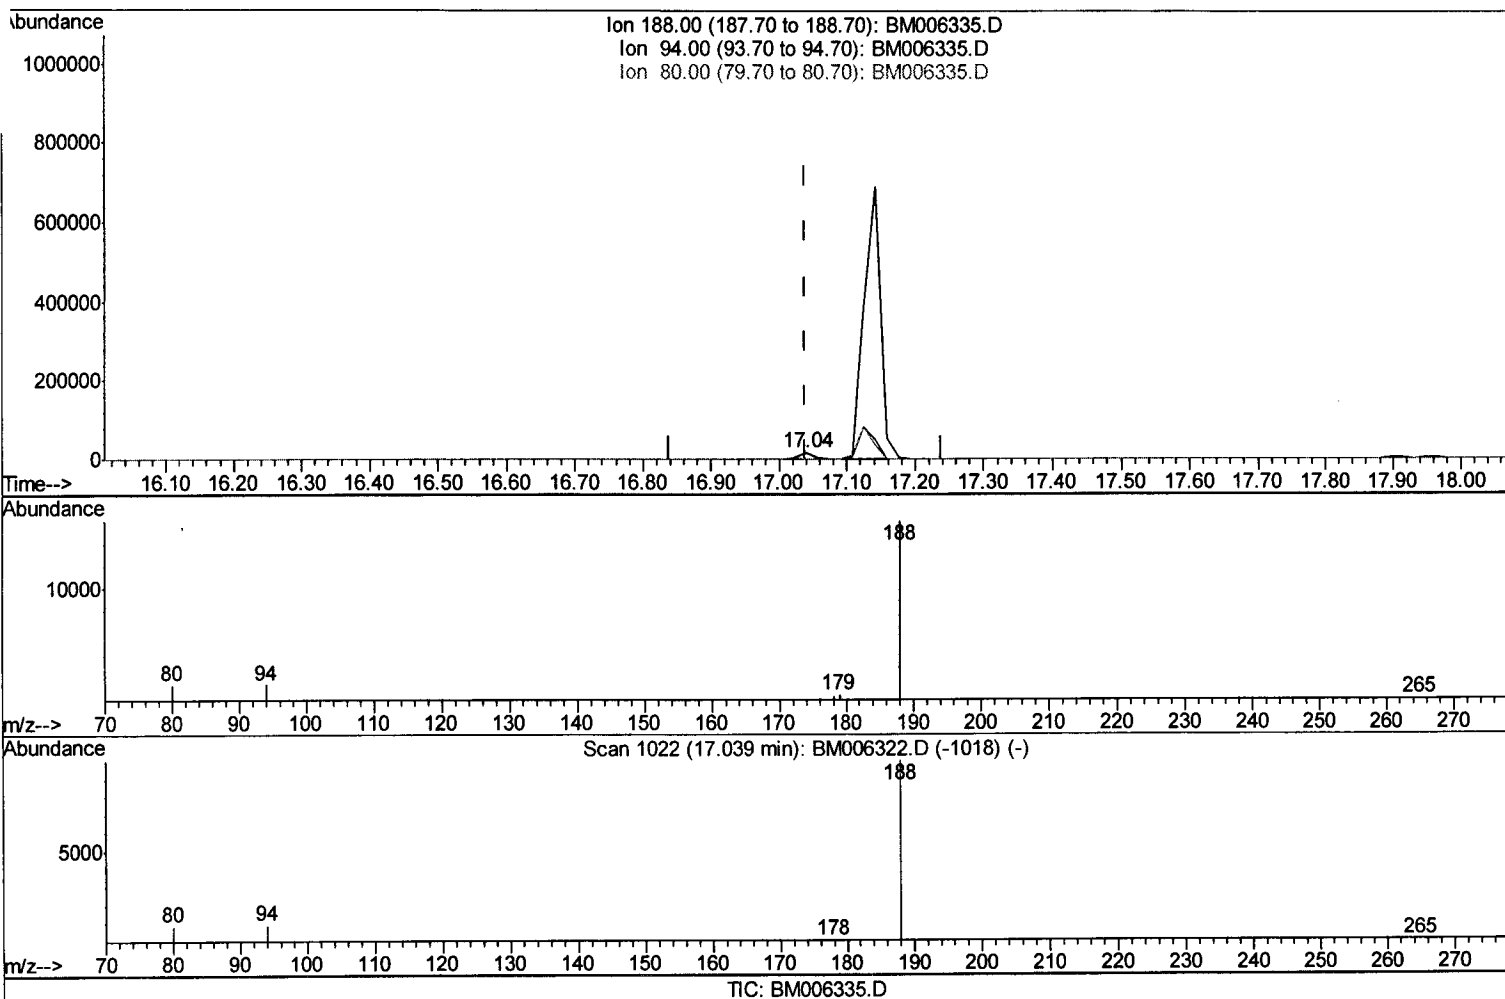

(12) Phenanthrene-d10 (I)

17.039min (+0.000) 0.40ng/ul m

response 23605

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	8.96#
80.00	11.90	8.69#
0.00	0.00	0.00

U.M
07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Quant Time: Jul 08 03:48:02 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/8/2016 7:14:15 PM

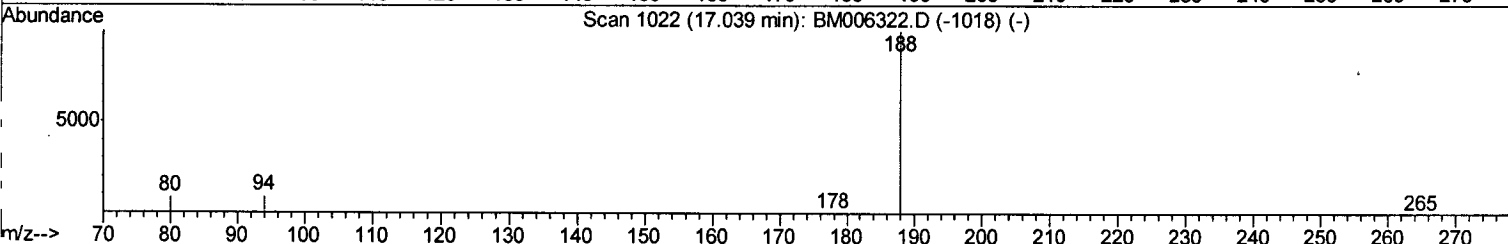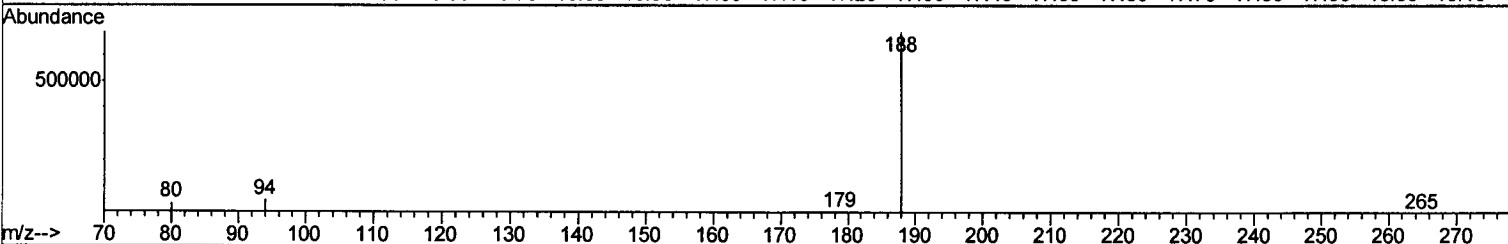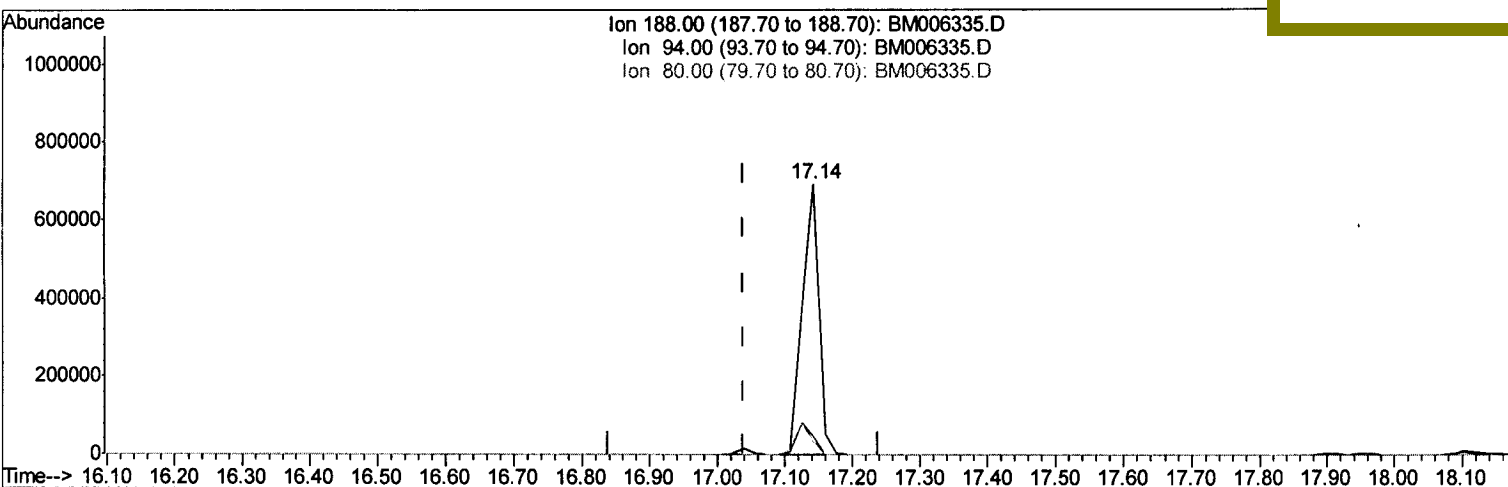

TIC: BM006335.D

(12) Phenanthrene-d10 (I)

17.142min (+0.103) 0.40ng/ul

response 1165719

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	6.73#
80.00	11.90	5.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integrati

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

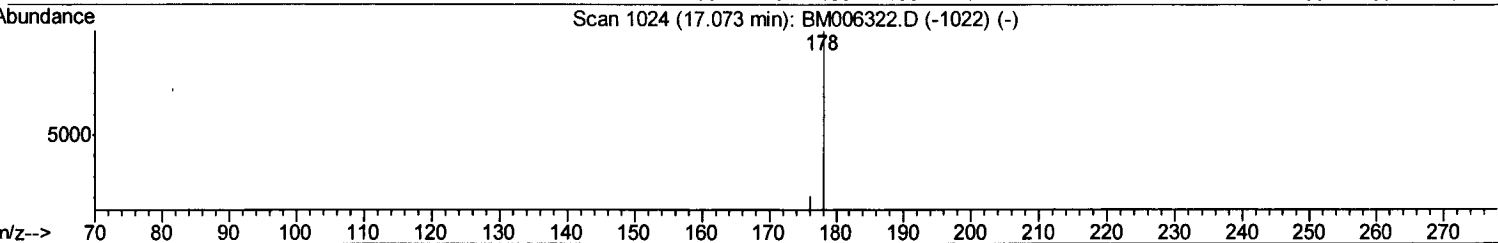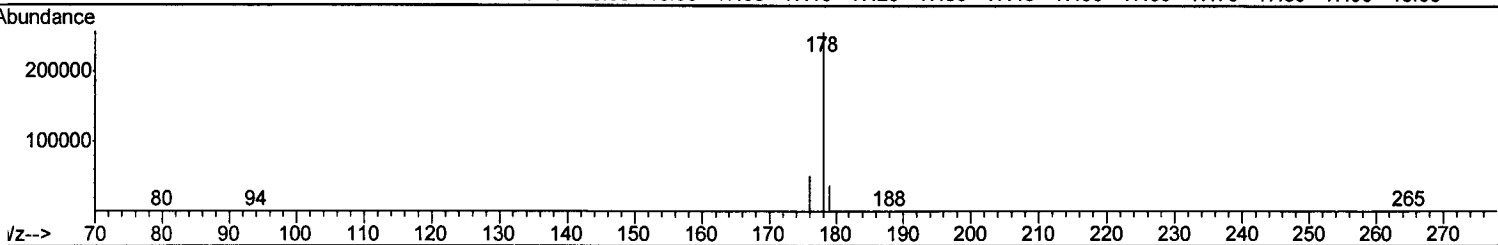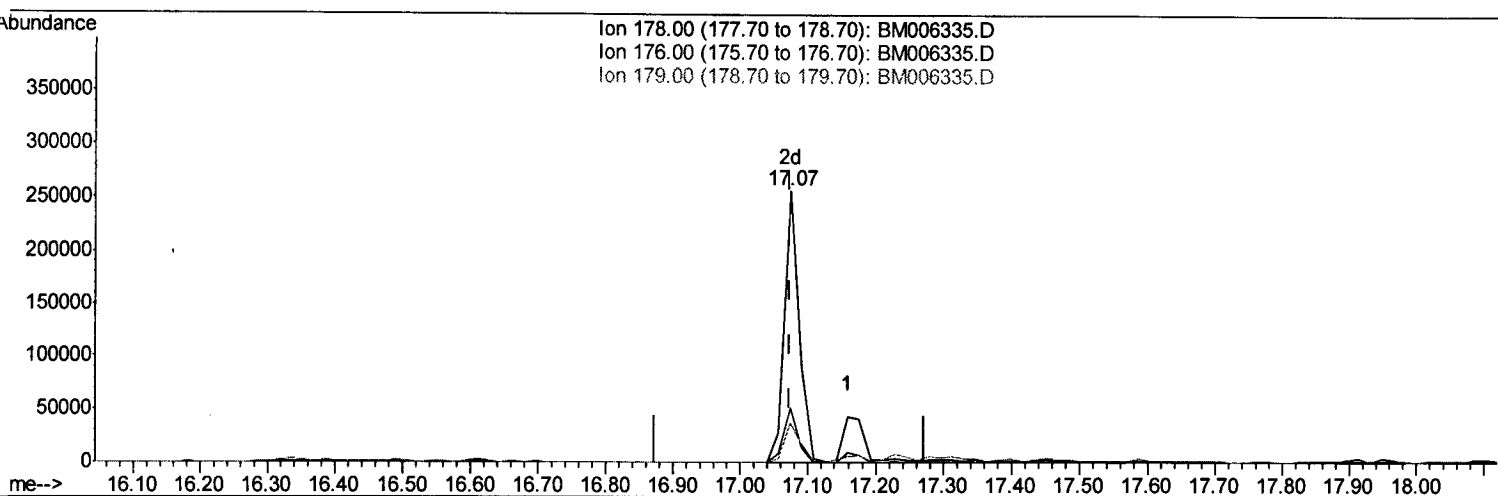

TIC: BM006335.D

(14) Phenanthrene

17.073min (+0.000) 5.96ng/ul m

response 388843

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	20.04#
179.00	17.70	14.61
0.00	0.00	0.00

V.M
07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Quant Time: Jul 08 07:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

APPROVED
 umangi
 7/8/2016 7:14:15 PM

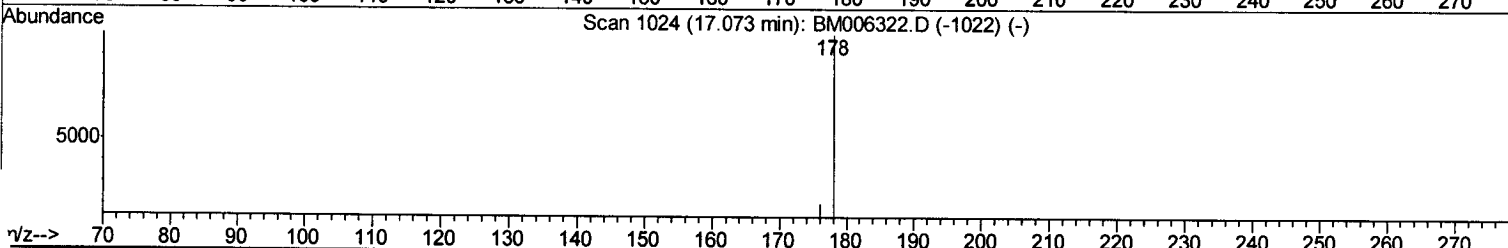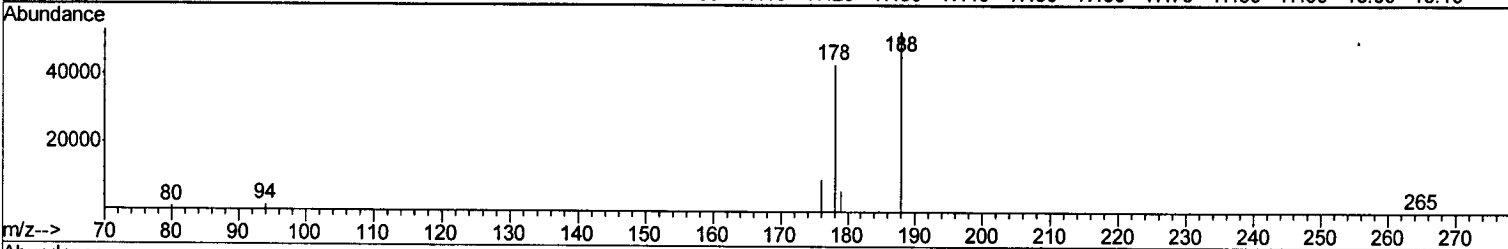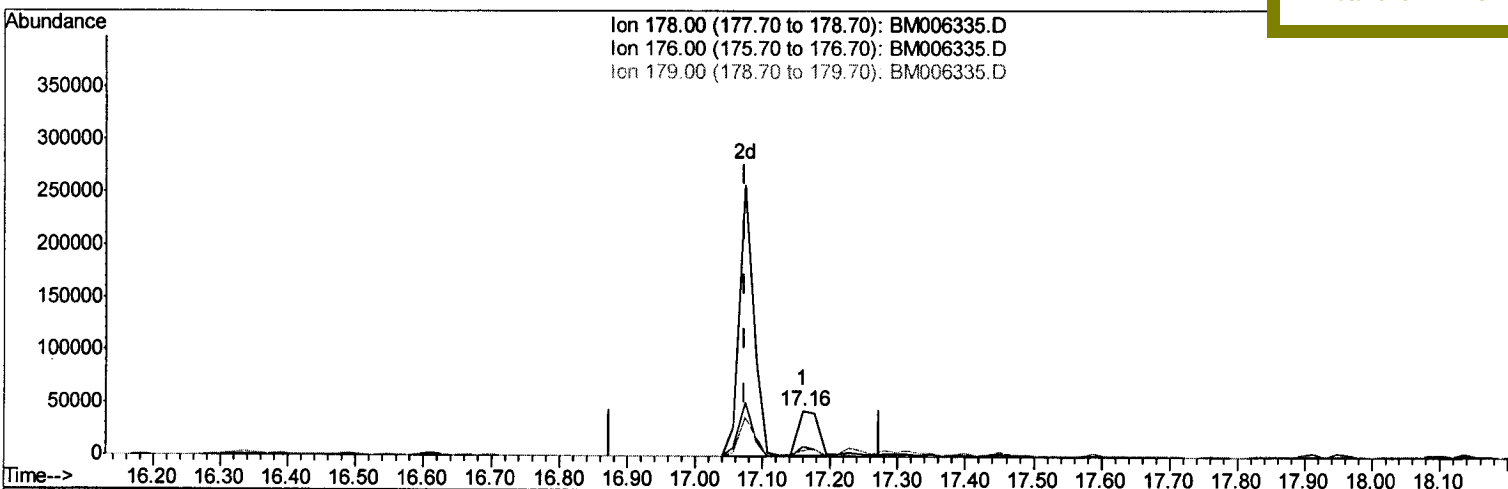

TIC: BM006335.D

(14) Phenanthrene

17.159min (+0.086) 1.36ng/ul

response 88573

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	22.12#
179.00	17.70	14.35
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

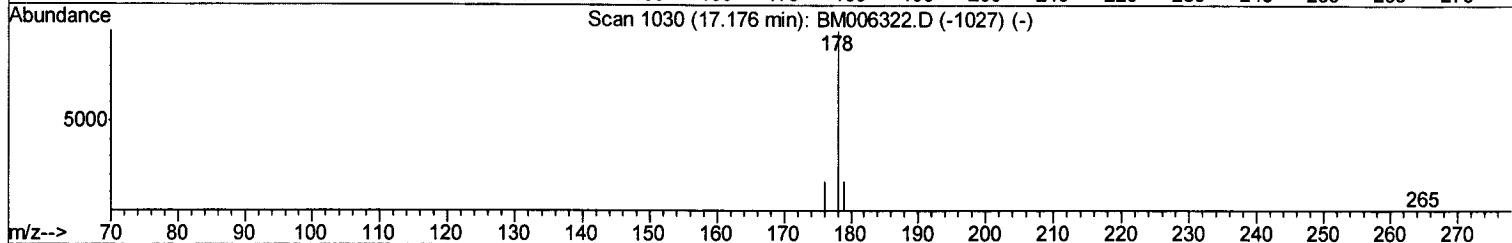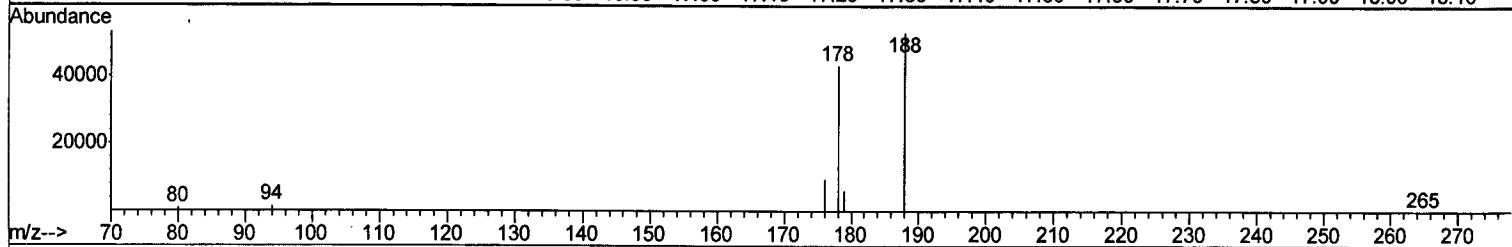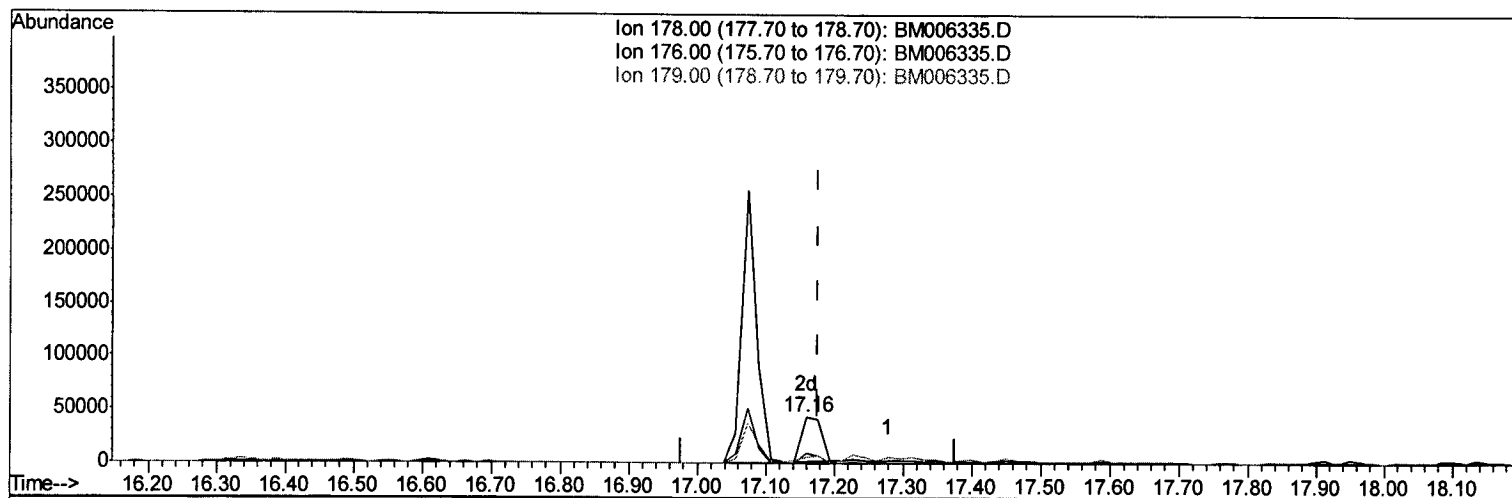

TIC: BM006335.D

(15) Anthracene

17.159min (-0.017) 1.39ng/ul m U.M
 response 84242
 07/12/16

Ion	Exp%	Act%
178.00	100	100
176.00	17.50	22.12#
179.00	16.10	14.35
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006335.D
Acq On : 08 Jul 2016 00:43
Operator : UM/SJ
Sample : H3811-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TW3

Manual Integration

umangi
7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

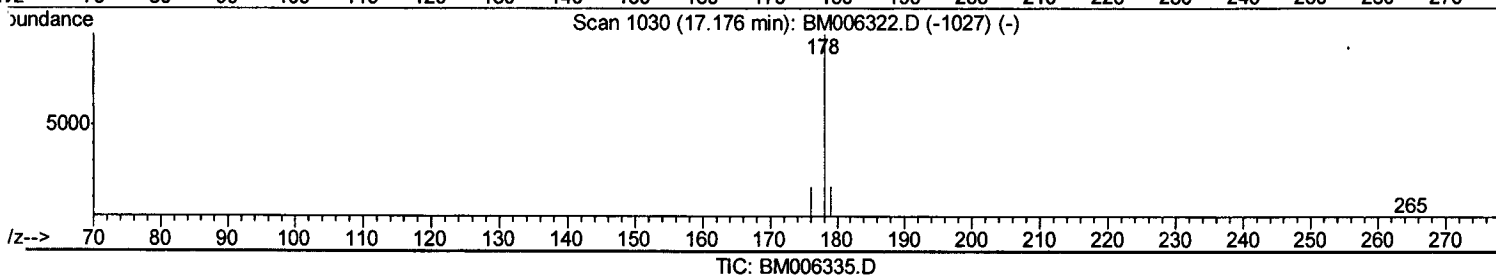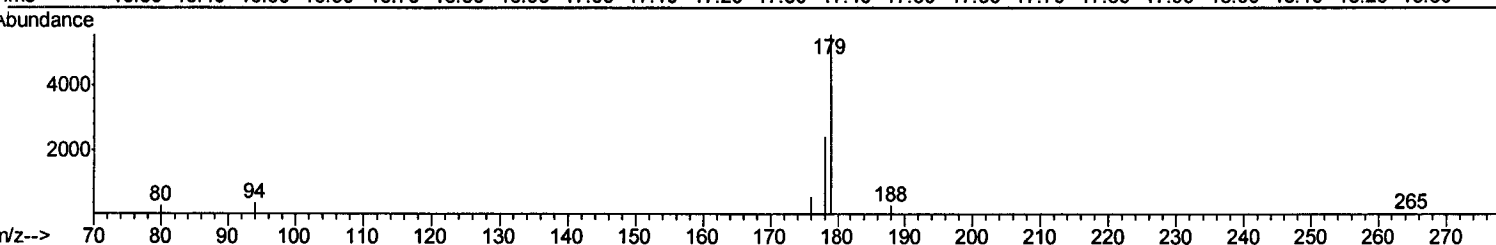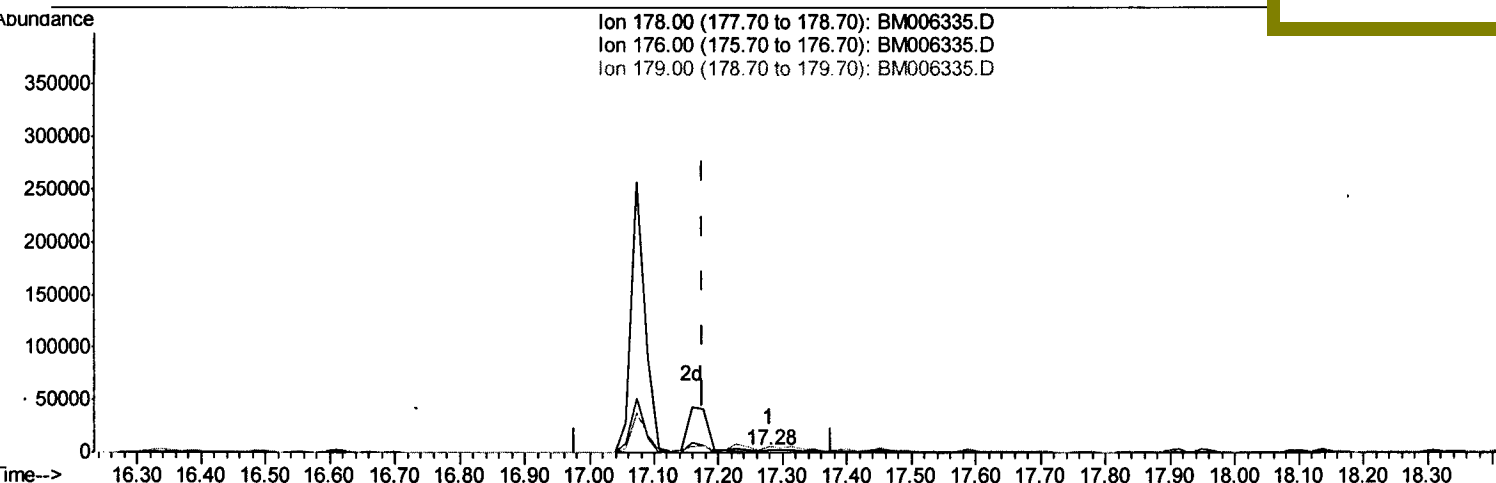

(15) Anthracene

17.279min (+0.103) 0.16ng/ul

response 9814

Ion	Exp%	Act%
178.00	100	100
176.00	17.50	24.09#
179.00	16.10	227.78#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

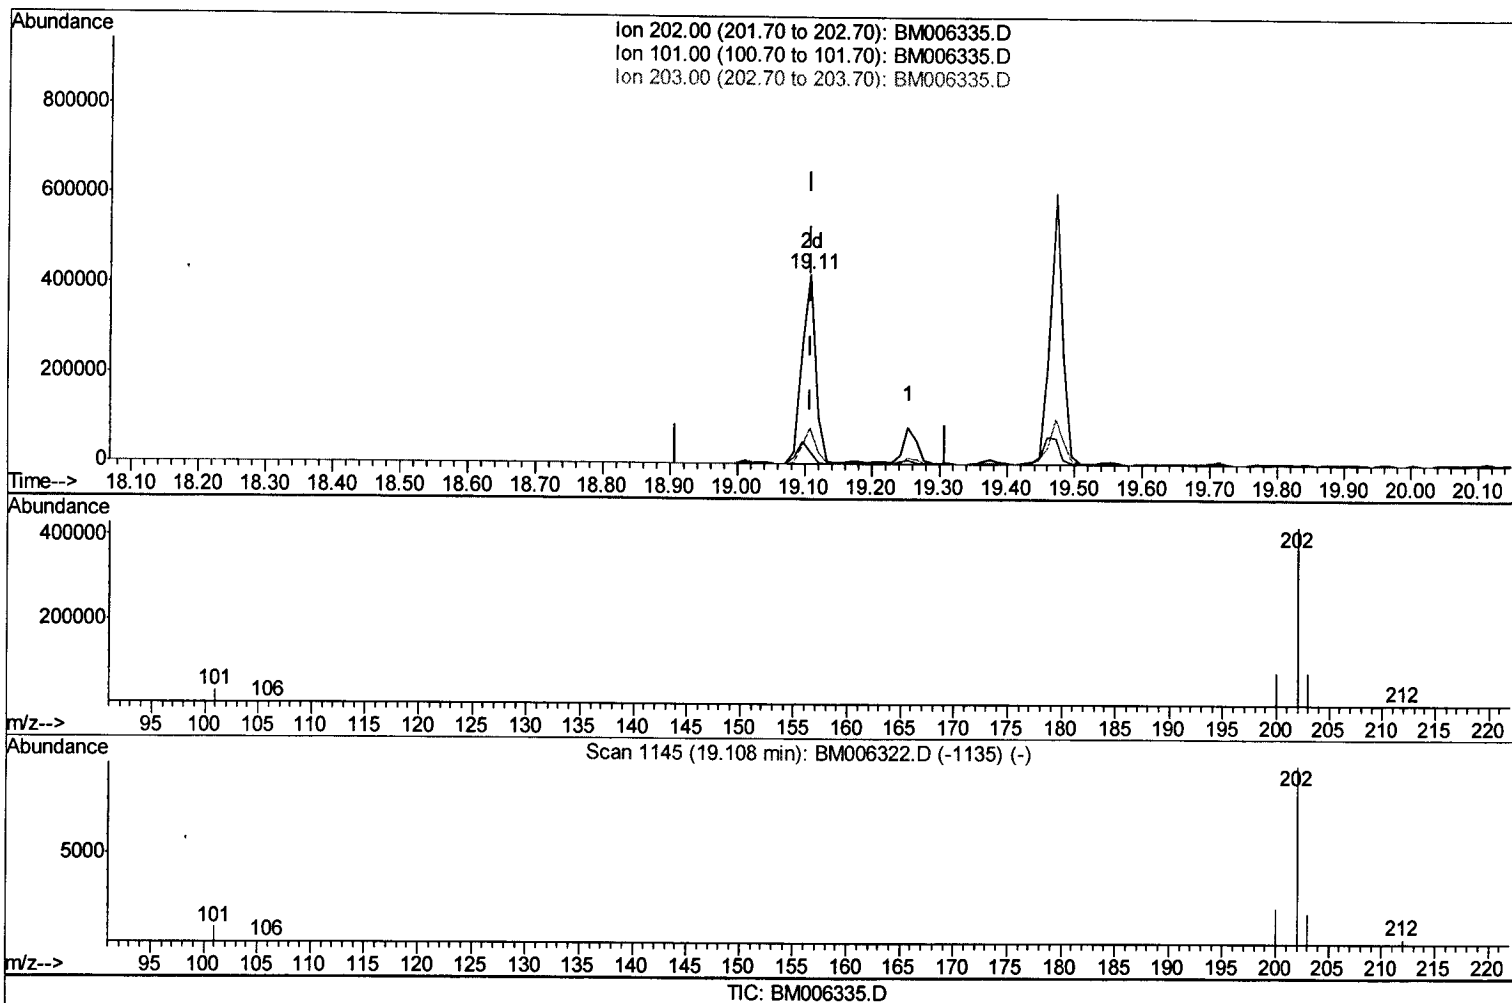

(17) Fluoranthene (C)

19.108min (+0.000) 8.38ng/ul m

response 603410

U.M
 07/12/16

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	6.66
203.00	16.30	18.62
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integrati

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

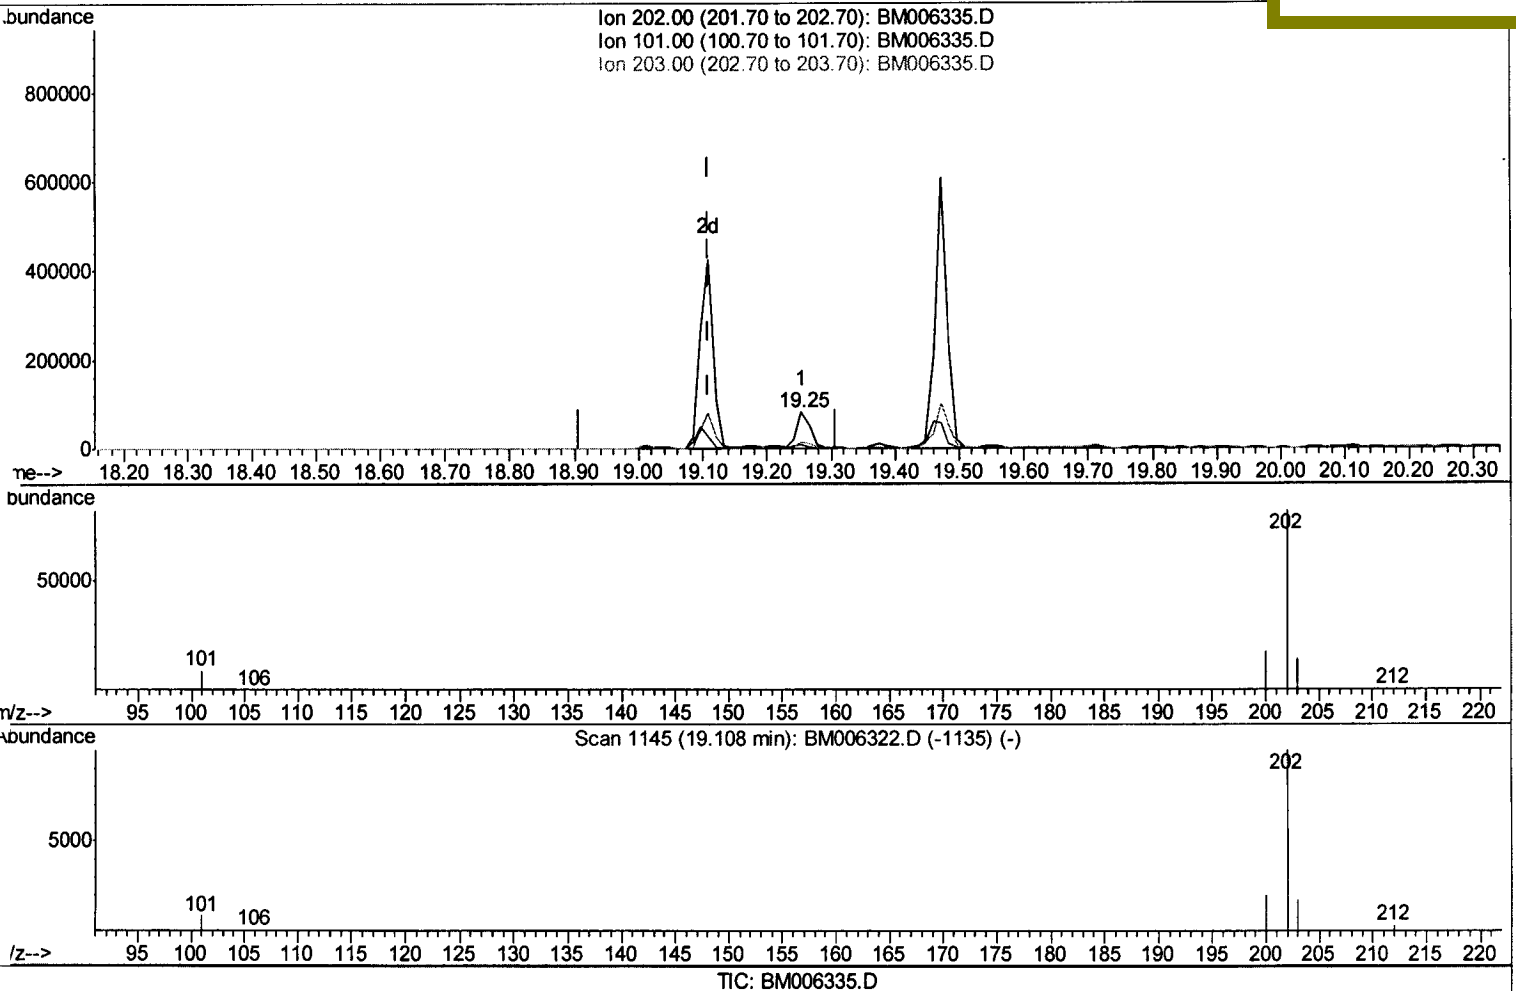

(17) Fluoranthene (C)

19.254min (+0.145) 1.74ng/ul

response 125146

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	10.89
203.00	16.30	17.40
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

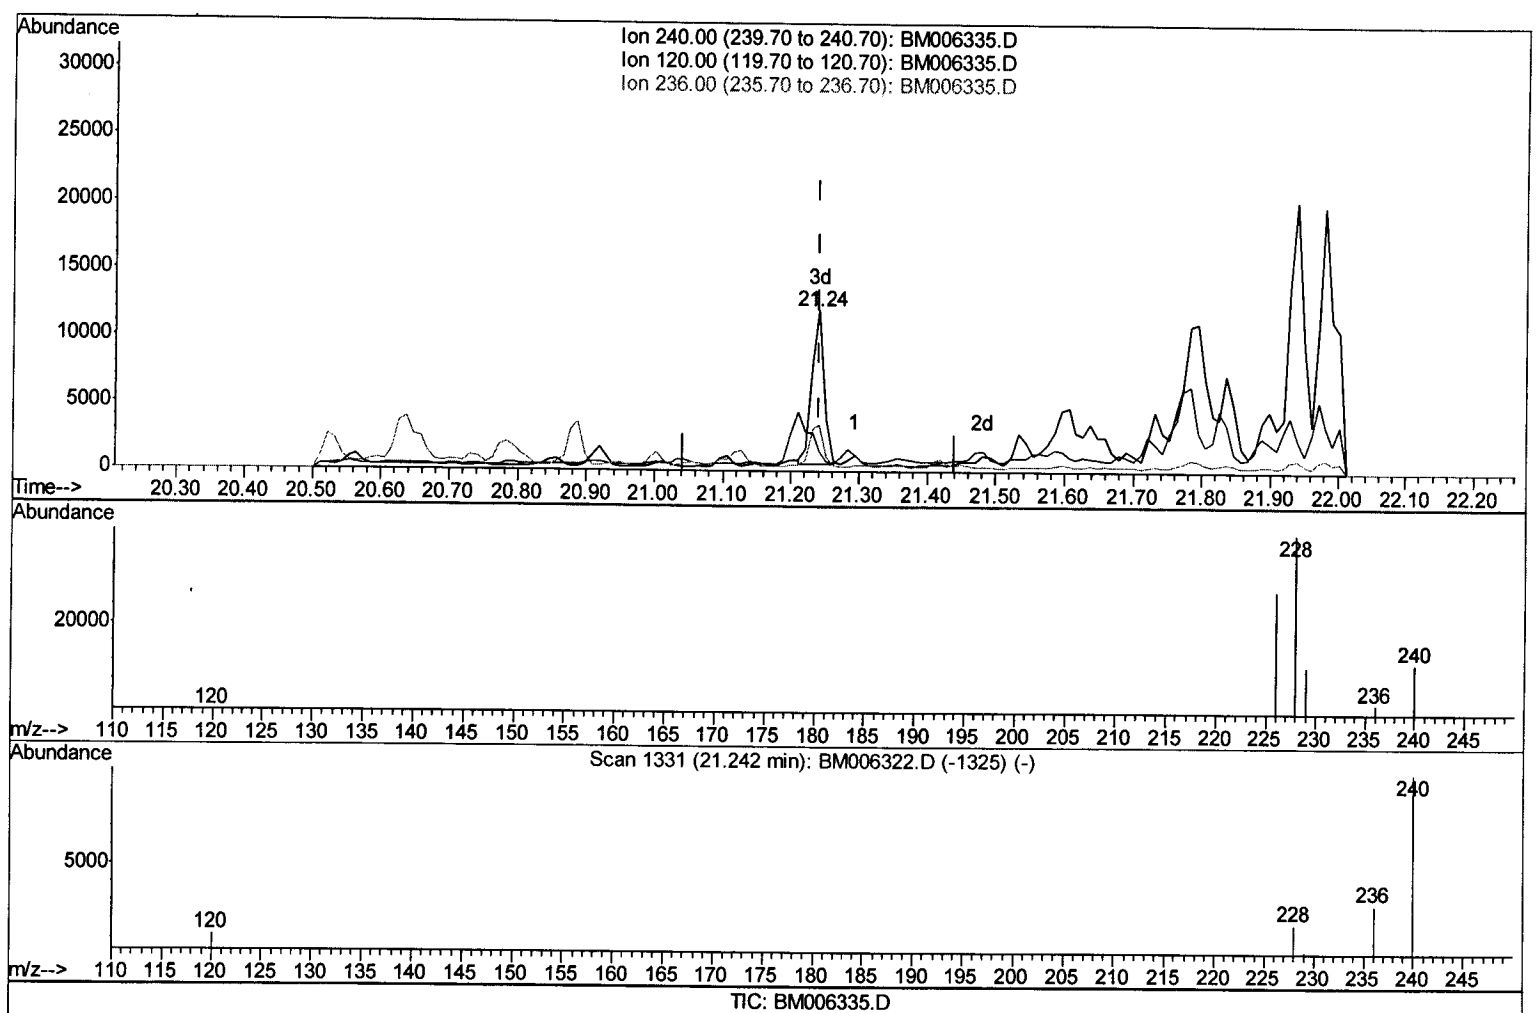

(18) Chrysene-d12 (I)

21.242min (+0.000) 0.40ng/ul m

response 14775

Ion	Exp%	Act%
240.00	100	100
120.00	17.20	12.76#
236.00	30.80	29.31
0.00	0.00	0.00

U.M
 07/12/16




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006335.D
Acq On : 08 Jul 2016 00:43
Operator : UM/SJ
Sample : H3811-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TW3

Manual Integration

umangi
7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:45:28 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

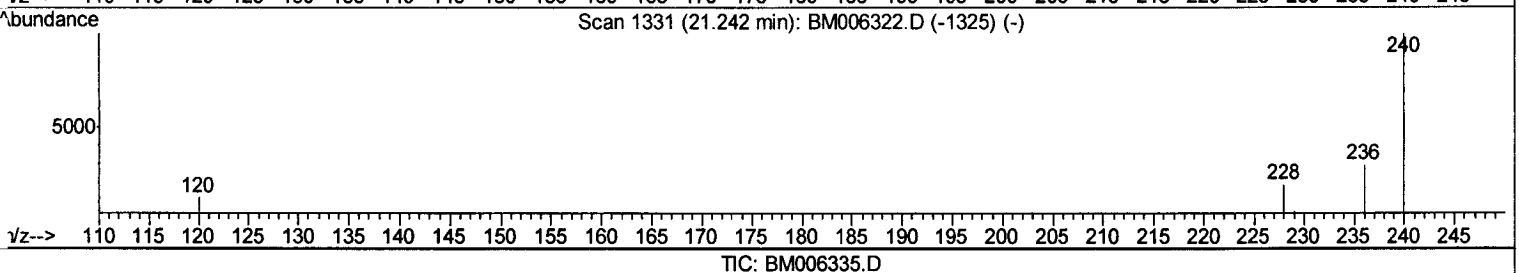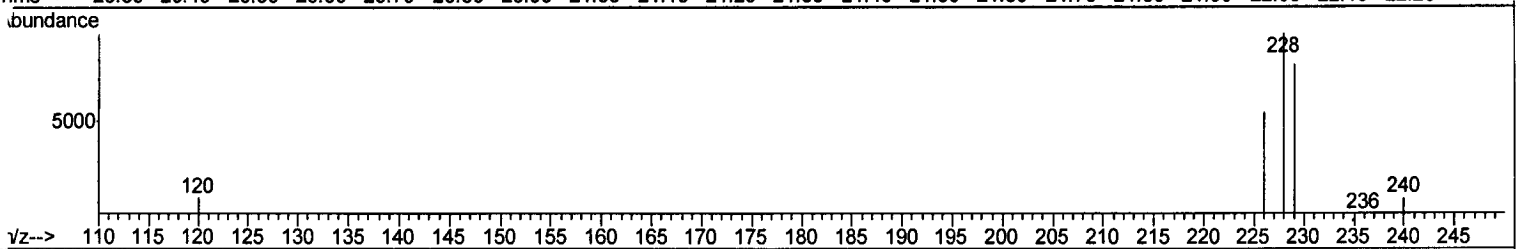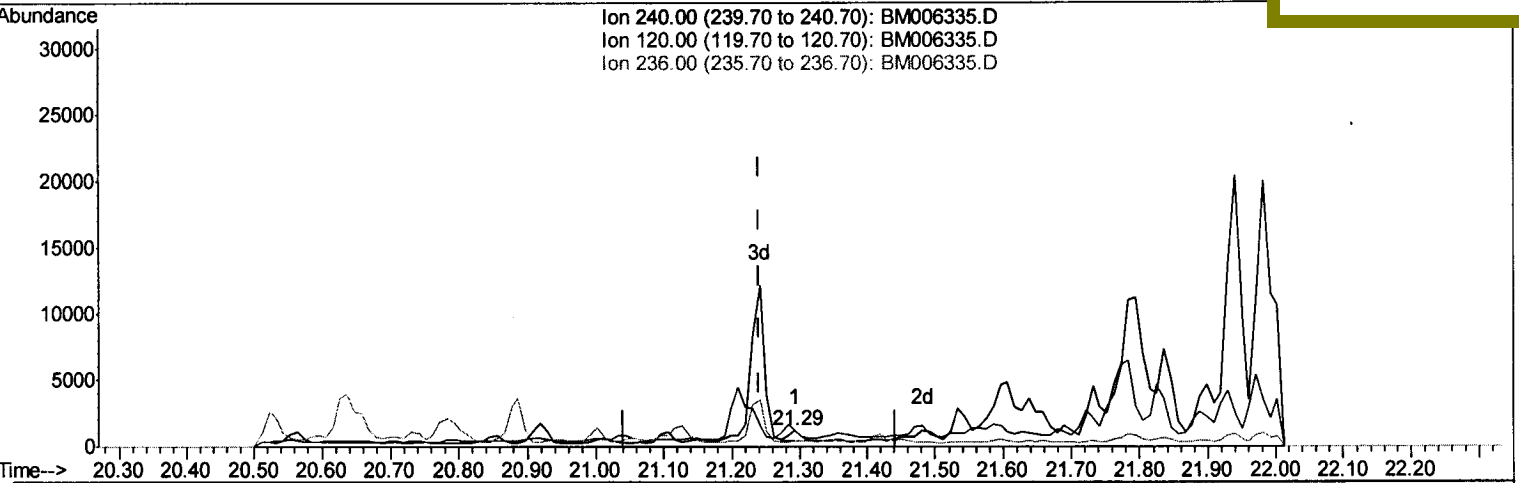

(18) Chrysene-d12 (I)

21.294min (+0.052) 0.40ng/ul

response 950

Ion	Exp%	Act%
240.00	100	100
120.00	17.20	102.39#
236.00	30.80	38.40#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

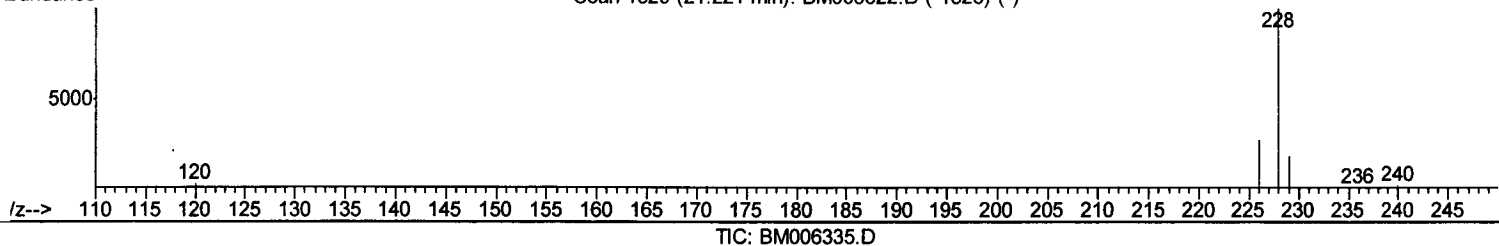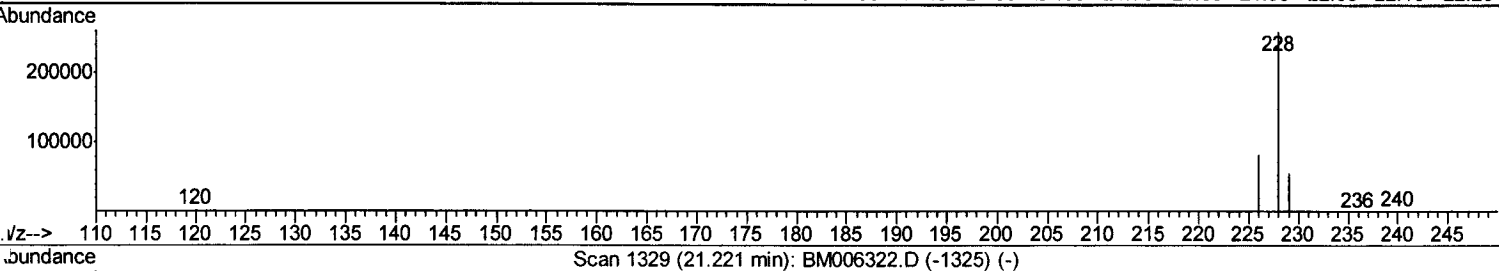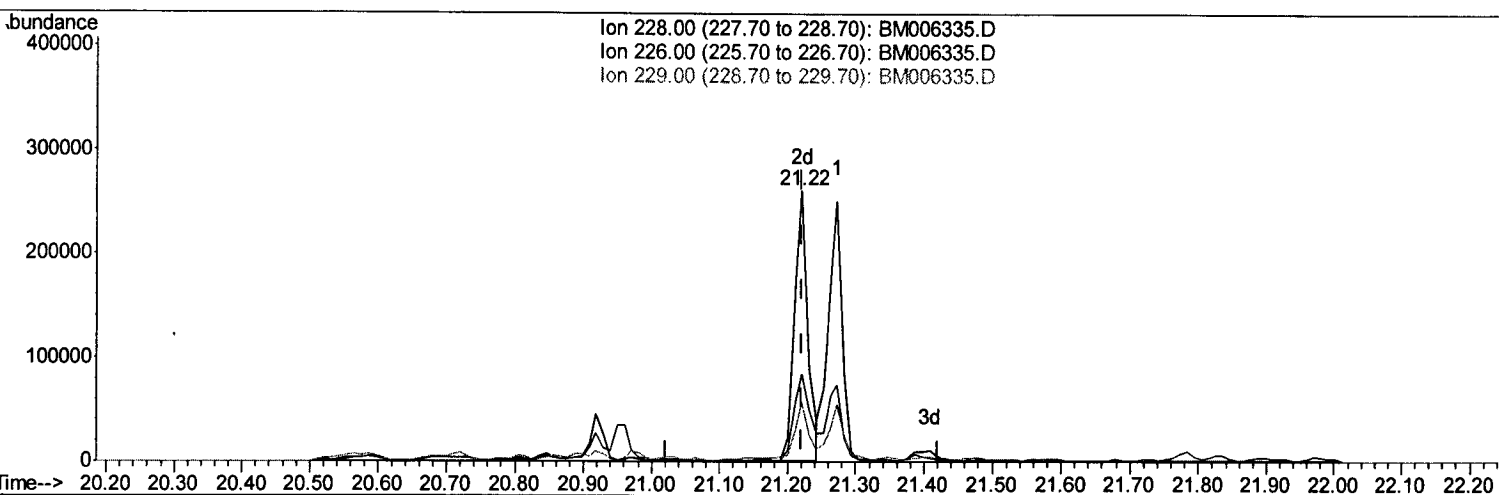

(20) Benzo(a)anthracene

21.221min (+0.000) 7.57ng/ul m

response 362076

Ion	Exp%	Act%
228.00	100	100
226.00	23.50	32.09#
229.00	21.40	21.77
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integration

APPROVED
 umangi
 7/8/2016 7:14:15 PM

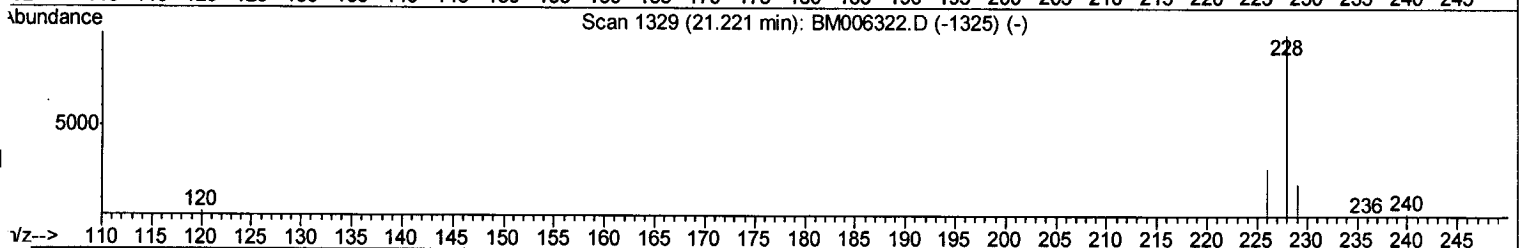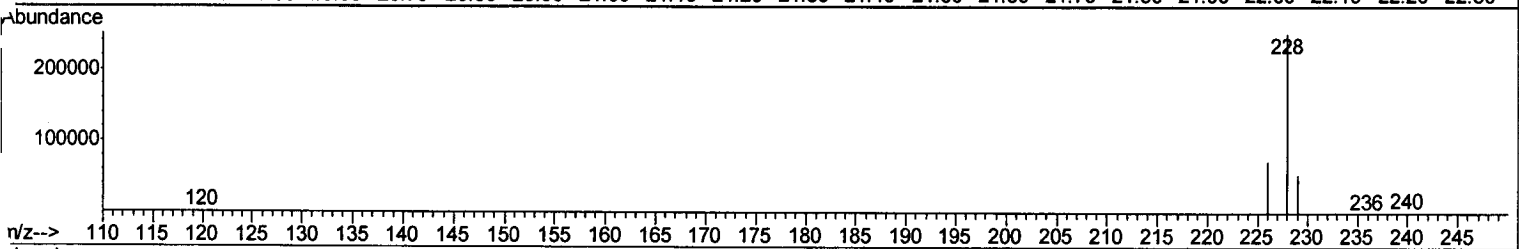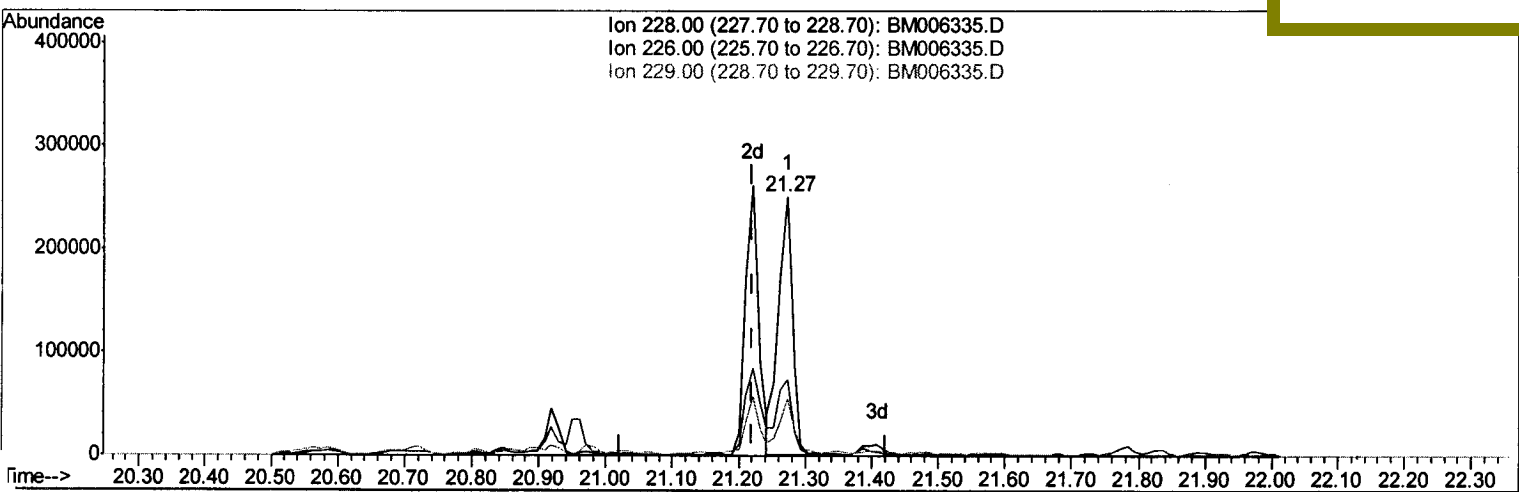

TIC: BM006335.D

(20) Benzo(a)anthracene

21.273min (+0.052) 7.59ng/ul

response 363080

Ion	Exp%	Act%
228.00	100	100
226.00	23.50	29.20#
229.00	21.40	21.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

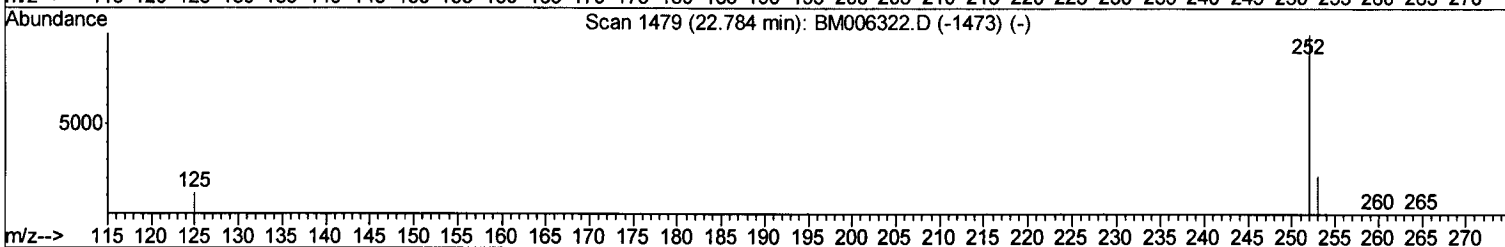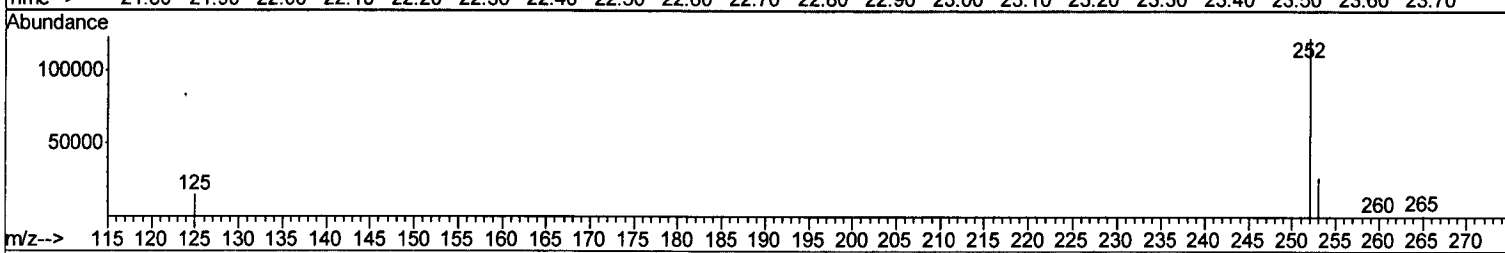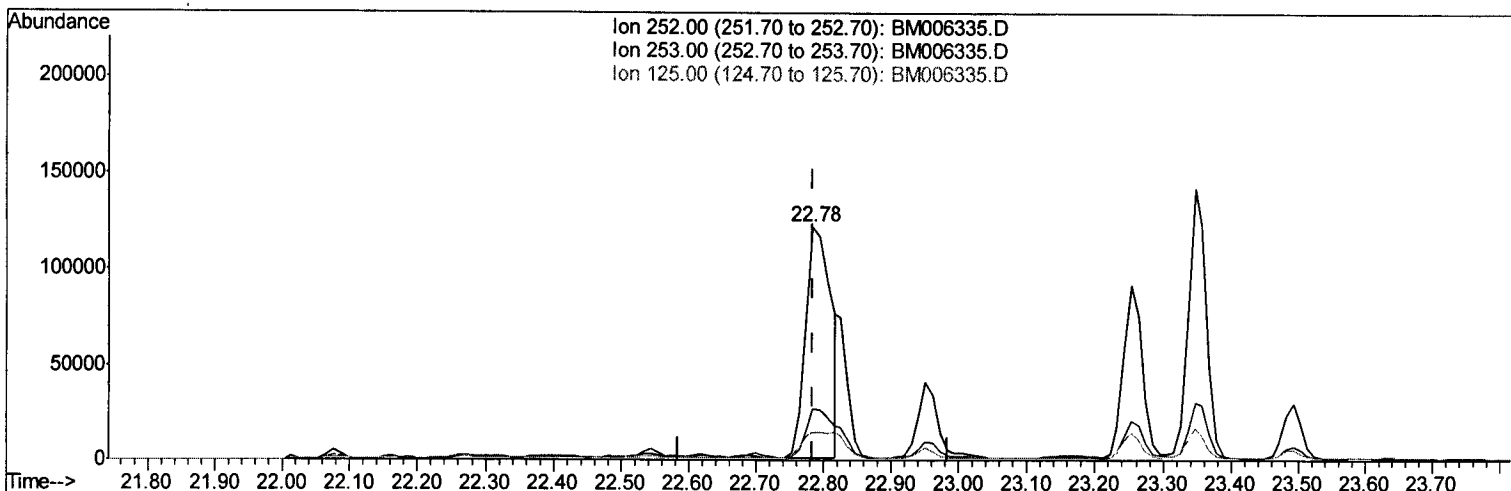

(23) Benzo(b)fluoranthene

22.784min (+0.000) 6.10ng/ul m

response 318074

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	21.99
125.00	14.40	12.41
0.00	0.00	0.00

U.M
 07/12/16




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
Data File : BM006335.D
Acq On : 08 Jul 2016 00:43
Operator : UM/SJ
Sample : H3811-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TW3

Manual Integrati

umangi
7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:47:55 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

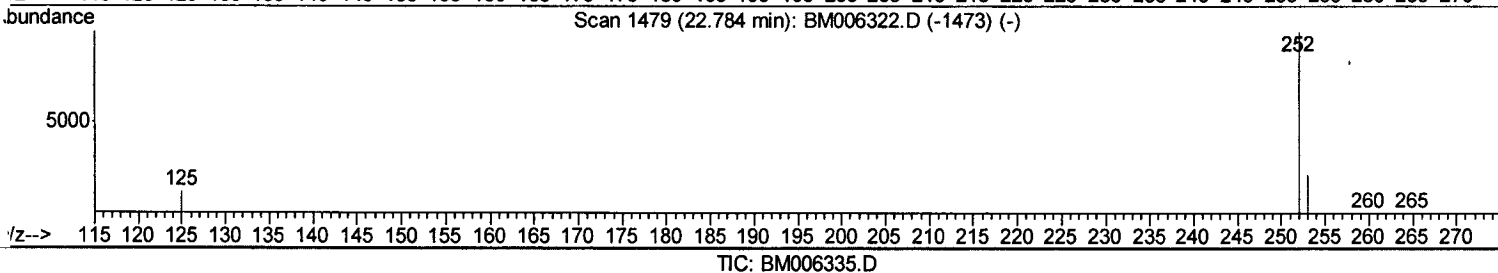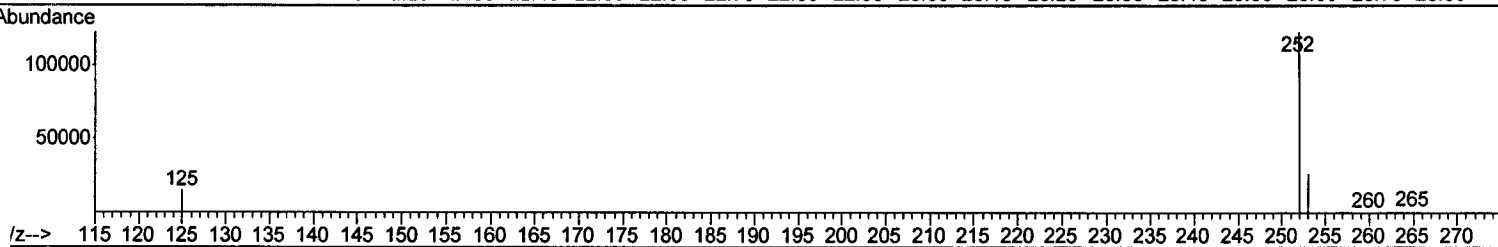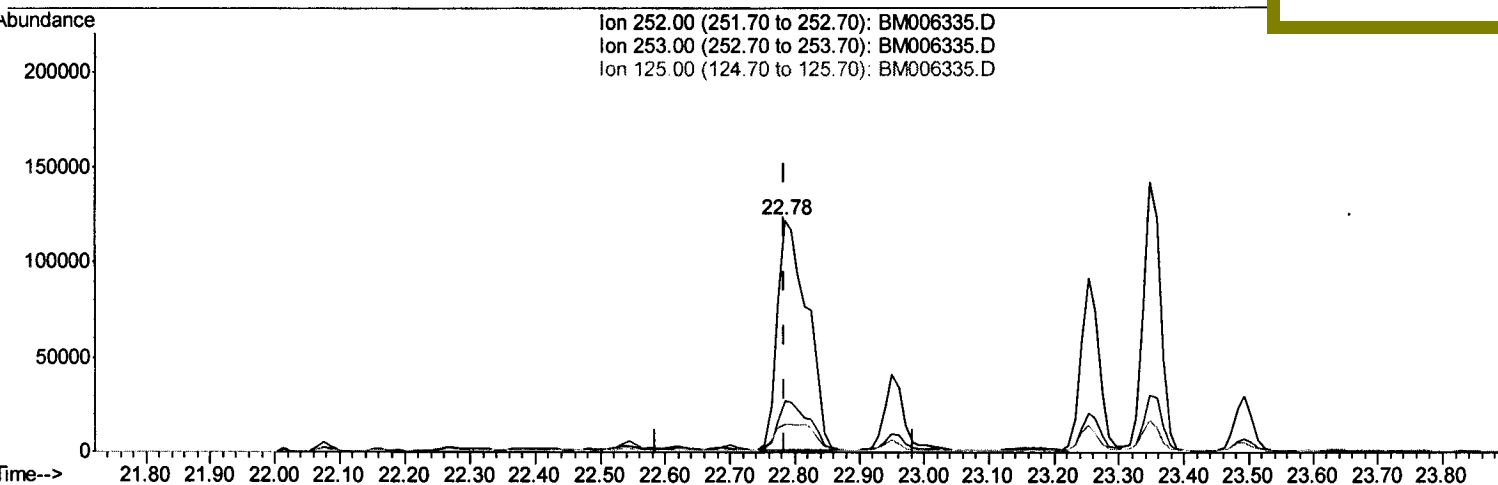

(23) Benzo(b)fluoranthene

22.784min (+0.000) 7.57ng/ul

response 394602

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	21.99
125.00	14.40	12.41
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integrati

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

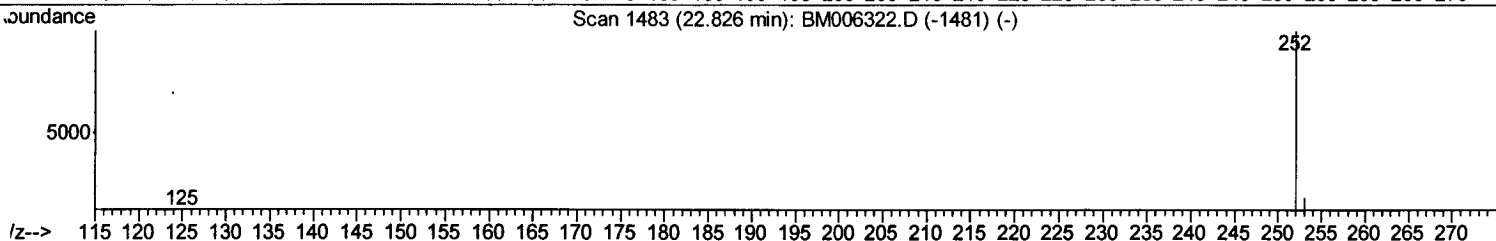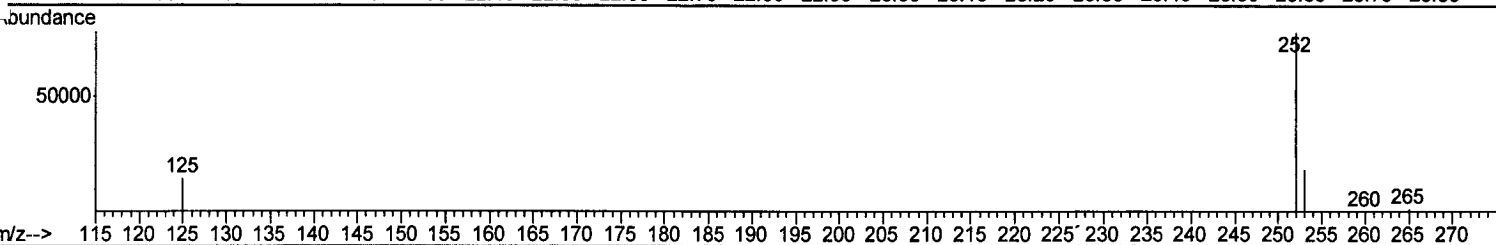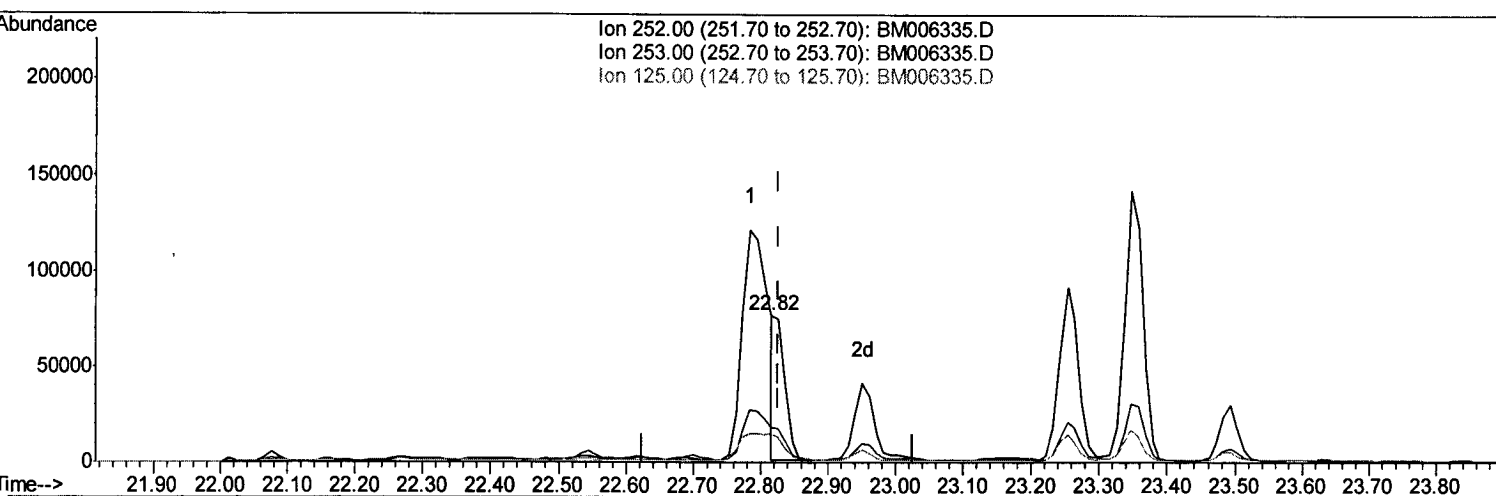

TIC: BM006335.D

(24) Benzo(k)fluoranthene

22.816min (-0.010) 1.59ng/ul m

response 77226

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.30
125.00	13.00	18.88#
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Manual Integrati

umangi
 7/8/2016 7:14:15 PM

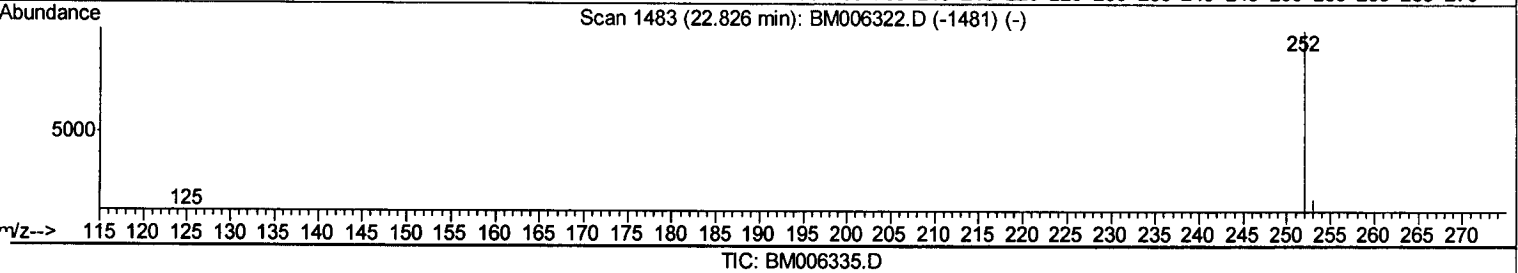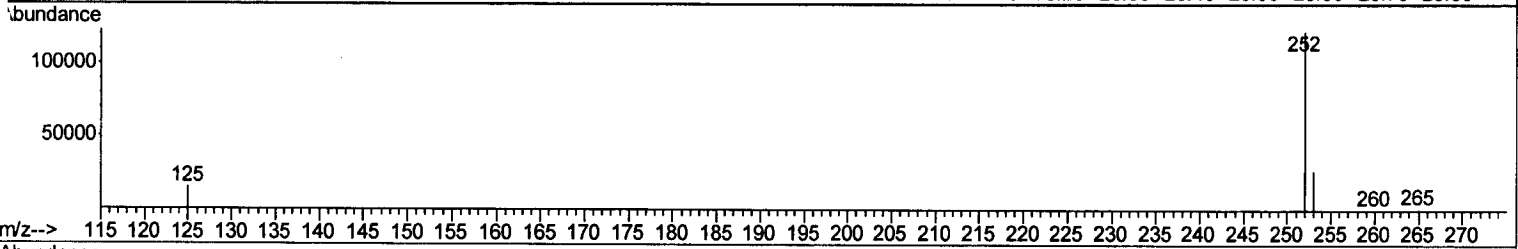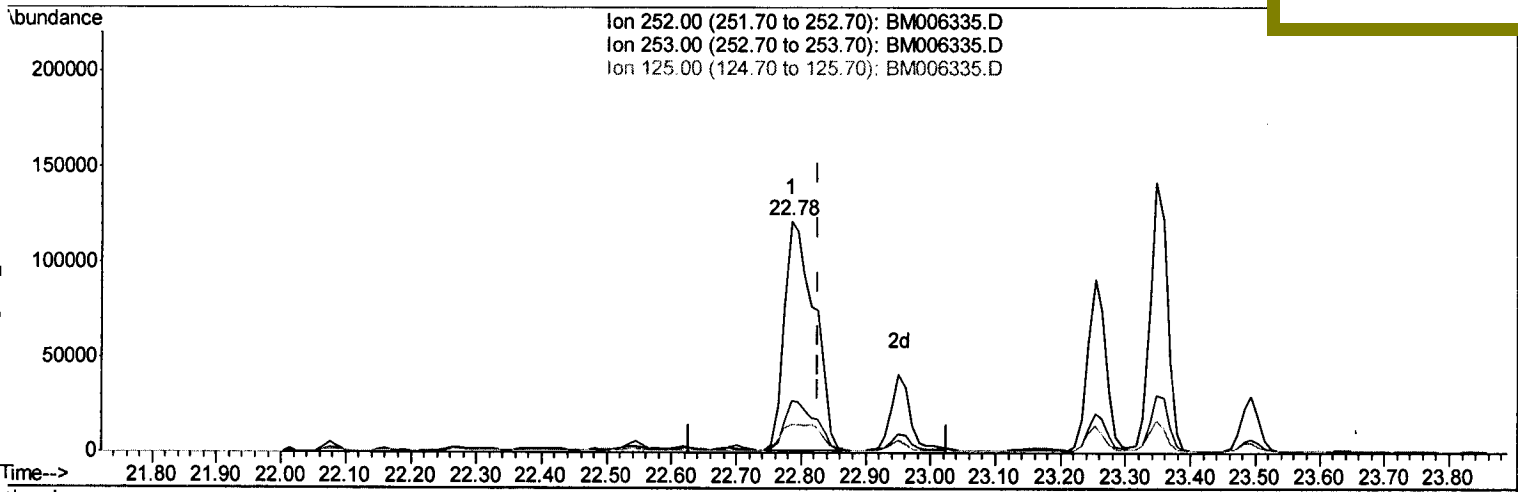

(24) Benzo(k)fluoranthene

22.784min (-0.042) 8.13ng/ul

response 394602

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	21.99
125.00	13.00	12.41
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 A4TW3

Manual Integration

APPROVED
 umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

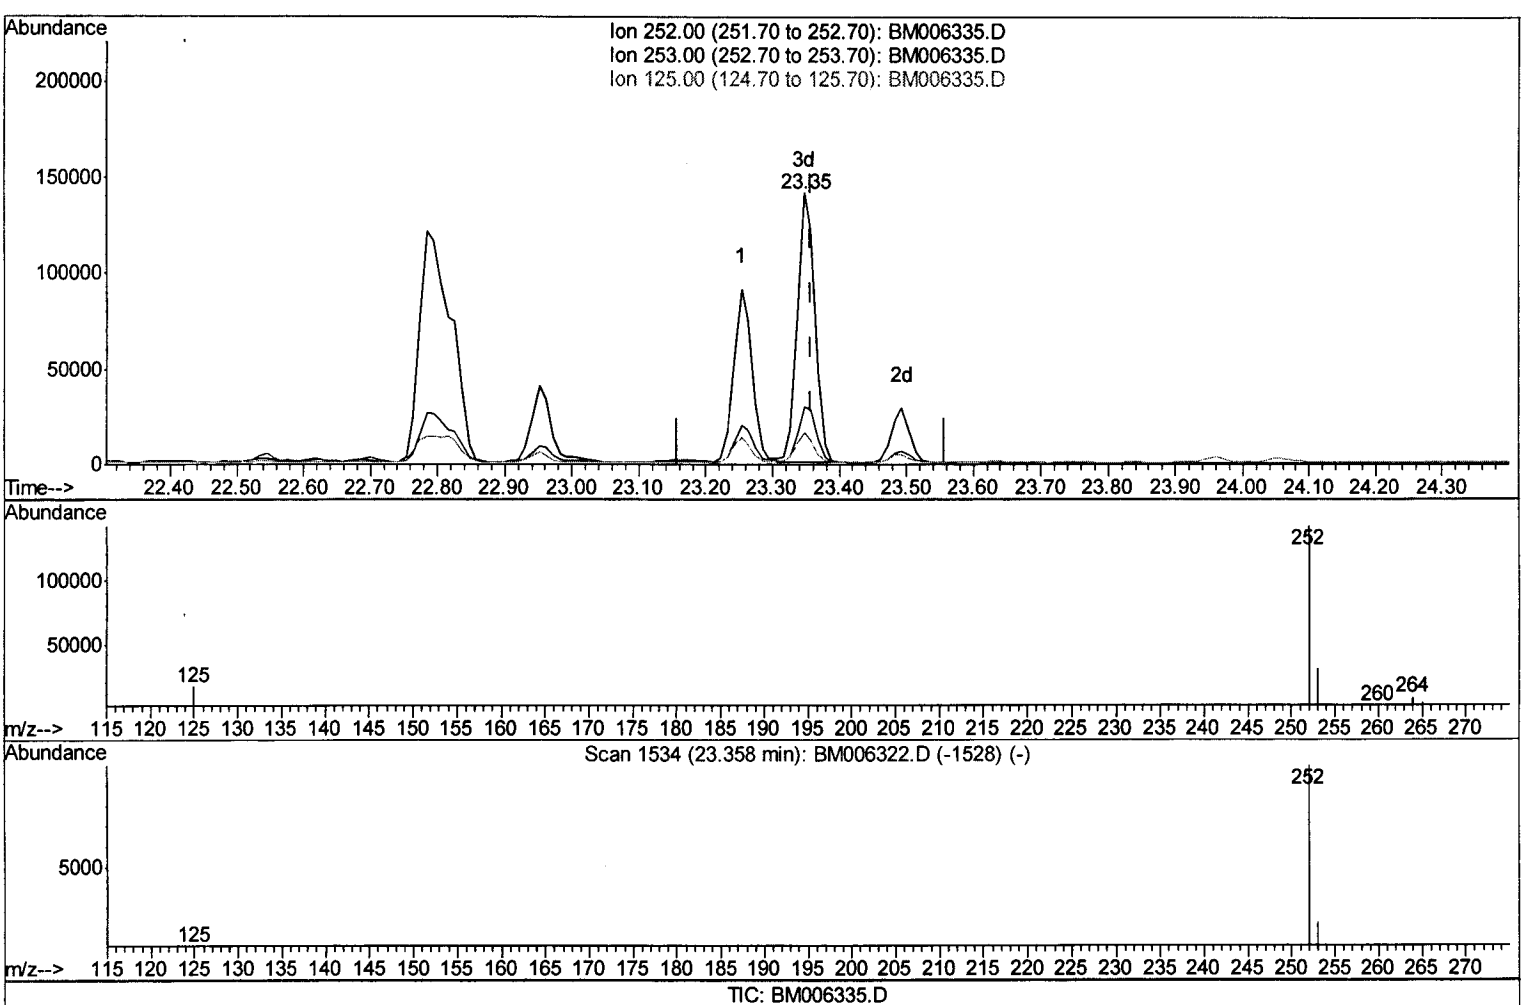

TIC: BM006335.D

(25) Benzo(a)pyrene (C)

23.347min (-0.010) 5.36ng/ul m

response 260296

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	21.37
125.00	15.90	11.71#
0.00	0.00	0.00

U.M
 07/12/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integrati

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:47:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

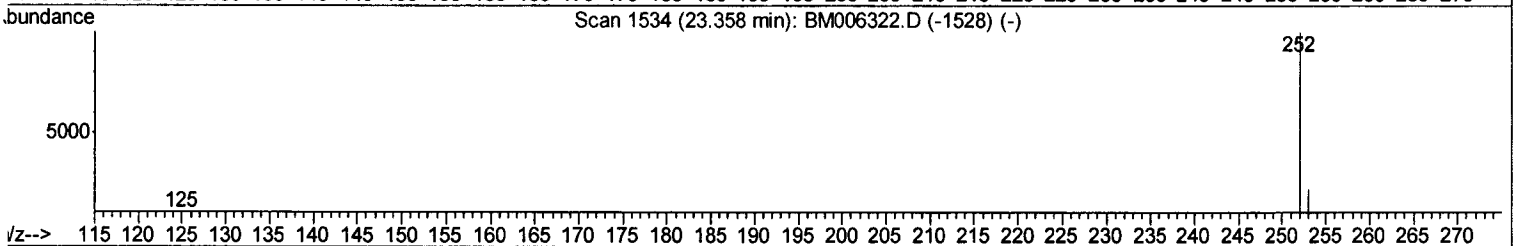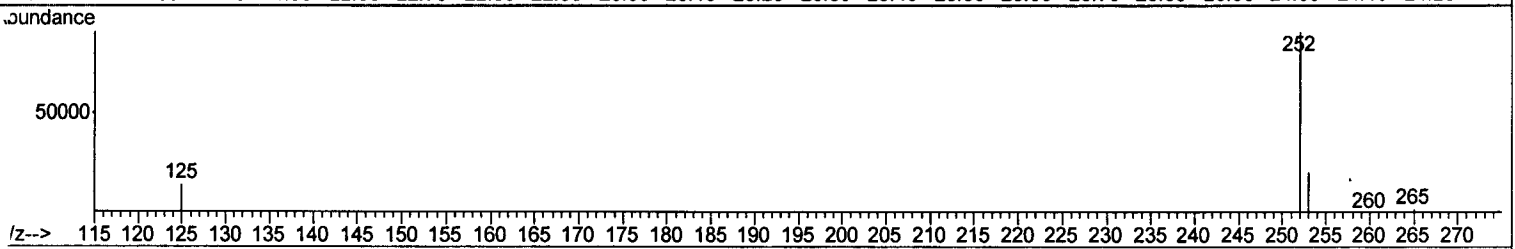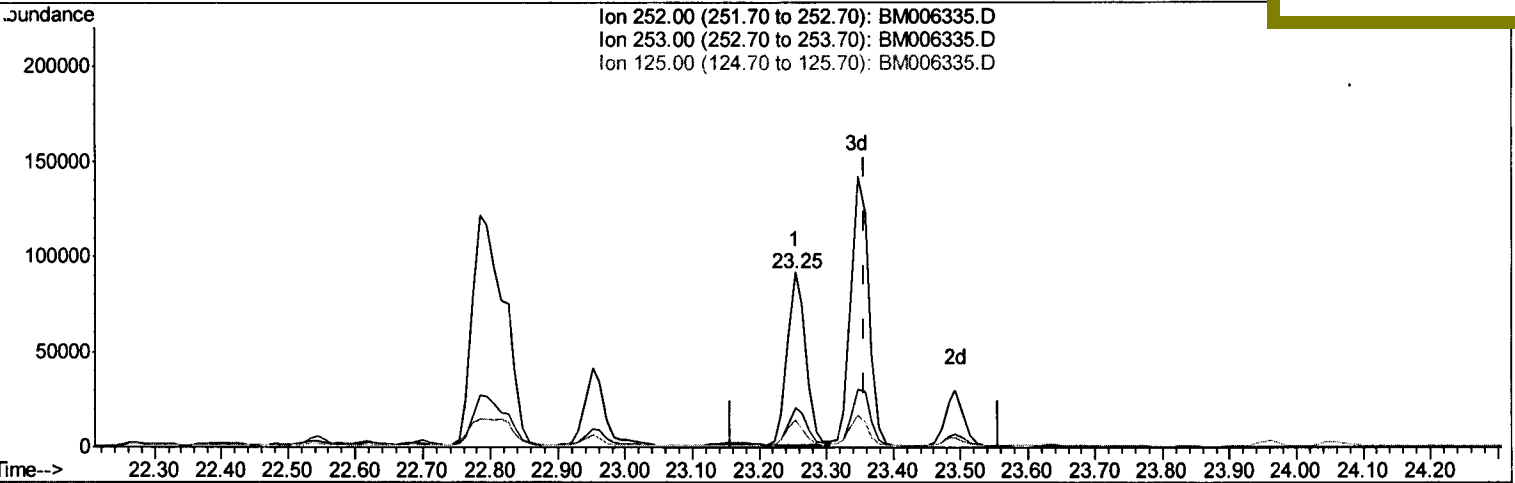

TIC: BM006335.D

(25) Benzo(a)pyrene (C)

23.253min (-0.104) 3.60ng/ul

response 174663

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	22.35
125.00	15.90	15.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM070816\
 Data File : BM006335.D
 Acq On : 08 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3811-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TW3

Manual Integration

umangi
 7/8/2016 7:14:15 PM

Quant Time: Jul 08 07:52:09 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	5028	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	20035	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	11653	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.04	188	23605m	0.40	ng/ul	0.00
18) Chrysene-d12	21.24	240	14775m	0.40	ng/ul	0.00
22) Perylene-d12	23.45	264	14565	0.40	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	9855	4.64	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.02	152	7764	0.33	ng/ul	0.00
16) Fluoranthene-d10	19.07	212	15752	0.32	ng/ul	-0.01

Target Compounds

						Ovalue
5) Naphthalene	10.46	128	11818	0.25	ng/ul	97
7) 2-Methylnaphthalene	12.09	142	6284	0.20	ng/ul	100
9) Acenaphthylene	14.01	152	60774	1.55	ng/ul	92
10) Acenaphthene	14.35	153	5893	0.15	ng/ul	89
11) Fluorene	15.34	166	24257m	0.55	ng/ul	
14) Phenanthrene	17.07	178	388843m	5.96	ng/ul	
15) Anthracene	17.16	178	84242m	1.39	ng/ul	
17) Fluoranthene	19.11	202	603410m	8.38	ng/ul	
19) Pyrene	19.47	202	799339	12.92	ng/ul	97
20) Benzo(a)anthracene	21.22	228	362076m	7.57	ng/ul	
21) Chrysene	21.27	228	363462	7.75	ng/ul	97
23) Benzo(b)fluoranthene	22.78	252	318074m	6.10	ng/ul	
24) Benzo(k)fluoranthene	22.82	252	77226m	1.59	ng/ul	
25) Benzo(a)pyrene	23.35	252	260296m	5.36	ng/ul	
26) Indeno(1,2,3-cd)pyrene	25.66	276	148219	2.75	ng/ul	97
27) Dibenzo(a,h)anthracene	25.66	278	44731	1.06	ng/ul	97
28) Benzo(a,h,i)perylene	26.34	276	136765	3.00	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed