

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070816\
 Data File : BM006327.D
 Acq On : 07 Jul 2016 19:53
 Operator : UM/SJ
 Sample : H3914-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TR9

Manual Integrations

APPROVED
 umangi
 7/8/2016 7:13:08 PM

Quant Time: Jul 08 06:57:05 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 03:28:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4361	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	17952	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	11111	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.04	188	24405m	0.40	ng/ul	0.00
18) Chrysene-d12	21.24	240	18172	0.40	ng/ul	0.00
22) Perylene-d12	23.45	264	11610m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.17	96	2601	1.41	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.02	152	7461	0.36	ng/ul	0.00
16) Fluoranthene-d10	19.07	212	22041	0.43	ng/ul	-0.01
Target Compounds						
15) Anthracene	17.18	178	8439	0.13	ng/ul	Ovalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM070816\
Data File : BM006327.D
Acq On : 07 Jul 2016 19:53
Operator : UM/SJ
Sample : H3914-08
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4TR9

Manual Integrations

umangi
7/8/2016 7:13:08 PM

Quant Time: Jul 08 06:57:05 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 03:28:13 2016
Response via : Initial Calibration

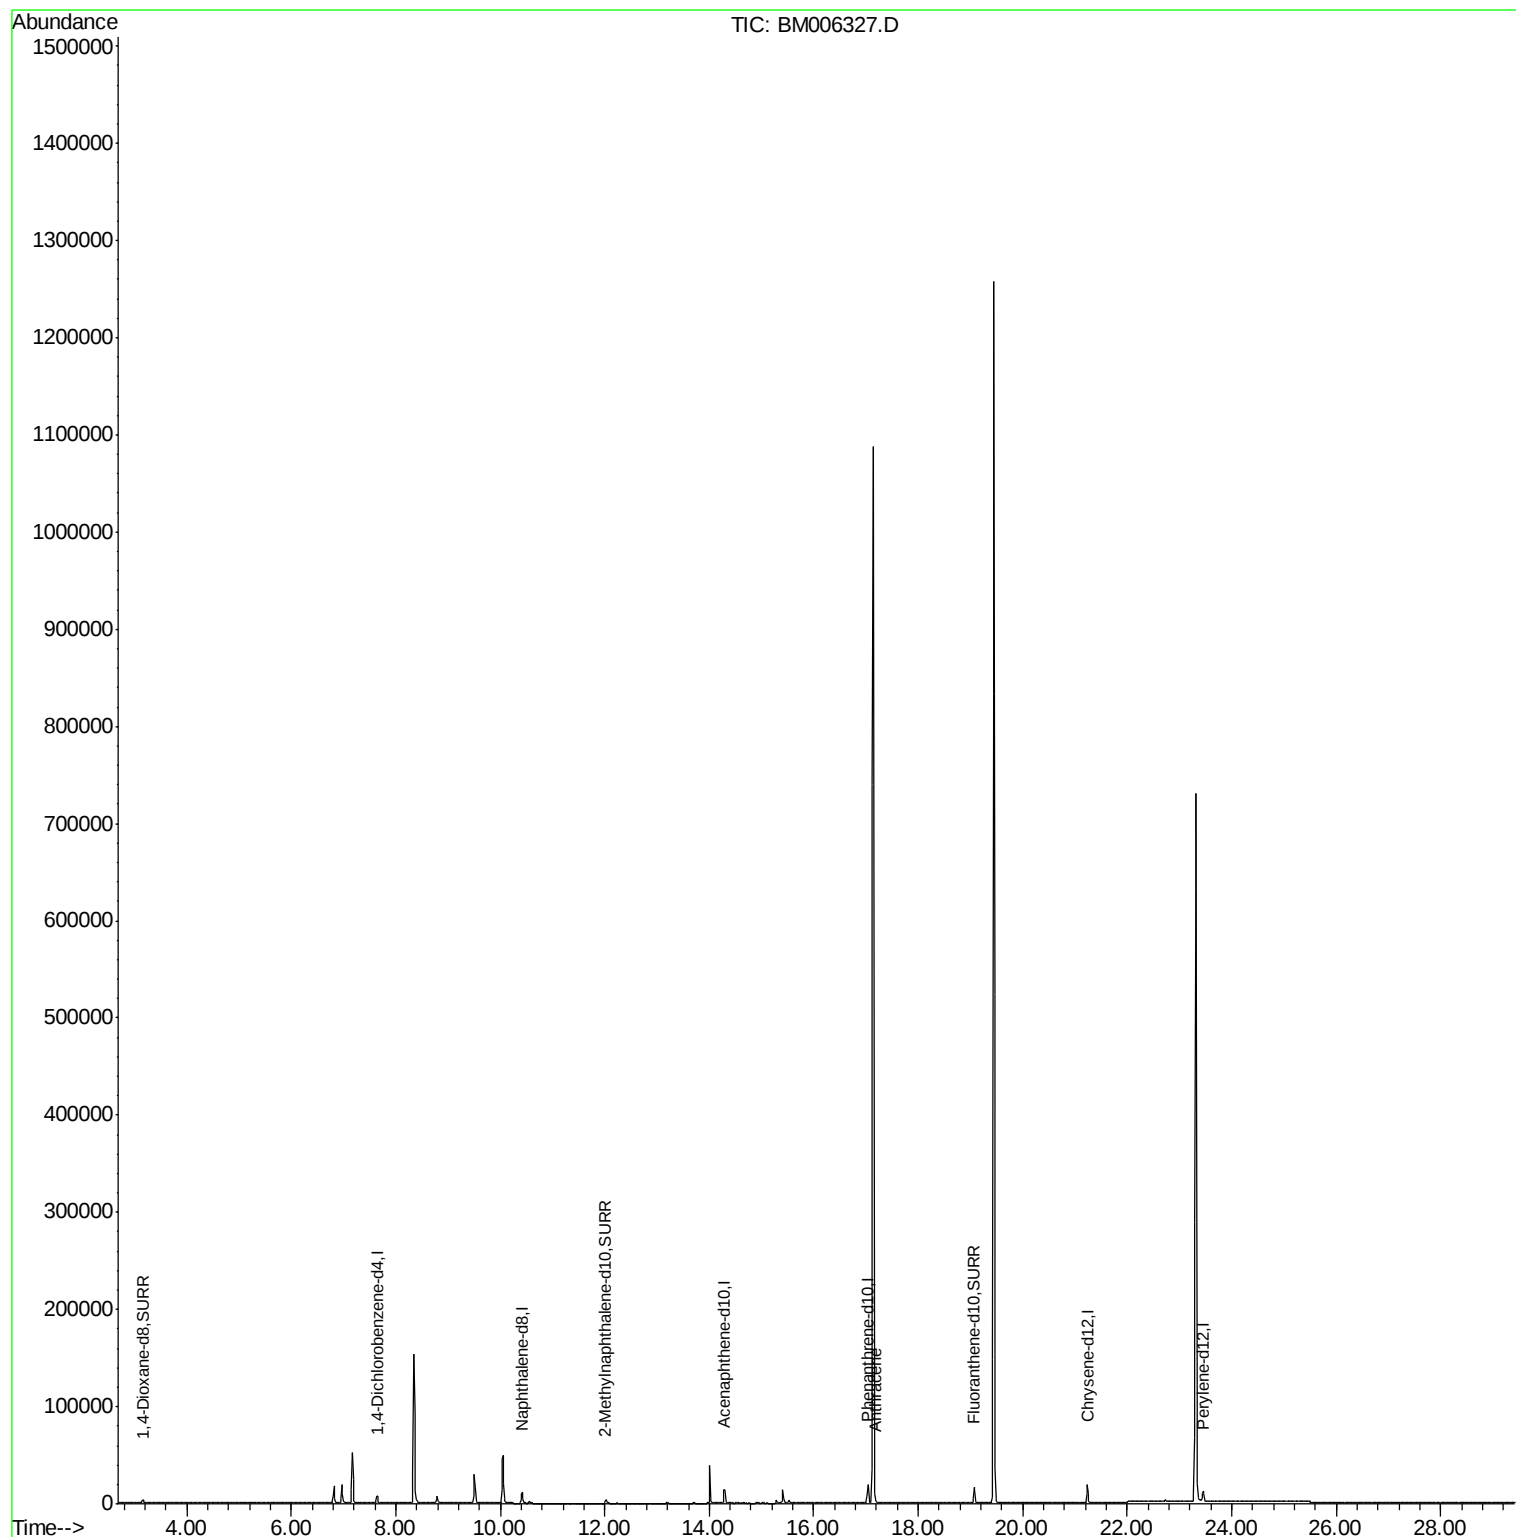

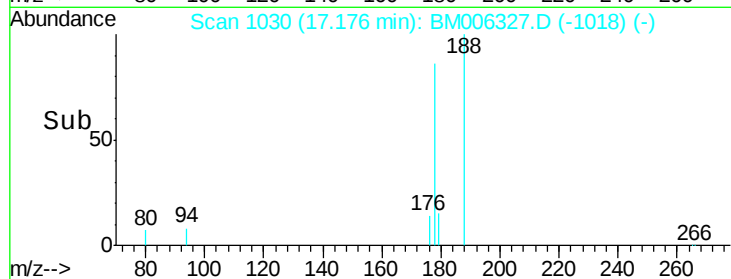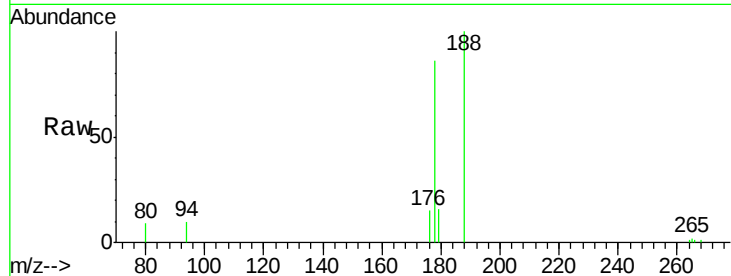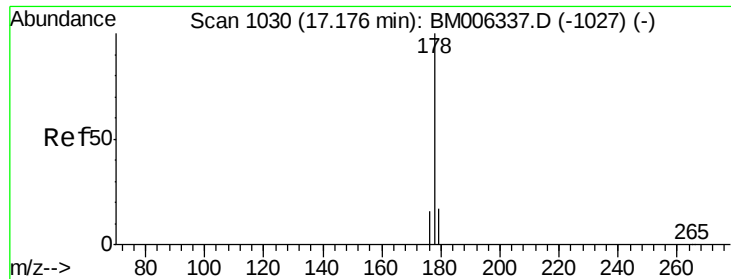

#15

Anthracene

Concen: 0.13 ng/ul

RT: 17.18 min Scan# 1030

Delta R.T. -0.00 min

Lab File: BM006327.D

Acq: 07 Jul 2016 19:53

Tot Ion: 178 Resp: 8439

Ion Ratio Lower Upper

178 100

176 17.6 14.0 21.0

179 19.2 12.9 19.3

Instrument :

BNA_M

ClientSampleId :

A4TR9

Manual Integrations

APPROVED

umangi

7/8/2016 7:13:08 PM

