

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070816\
 Data File : BM006350.D
 Acq On : 08 Jul 2016 14:51
 Operator : UM/SJ
 Sample : H3914-17
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TS8

Manual Integrations

APPROVED
 umangi
 7/8/2016 7:19:49 PM

Quant Time: Jul 08 15:27:53 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 08:04:54 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3807	0.40	ng/ul	-0.02
4) Naphthalene-d8	10.43	136	15030	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.28	164	8979	0.40	ng/ul	-0.02
12) Phenanthrene-d10	17.04	188	19489m	0.40	ng/ul	0.00
18) Chrysene-d12	21.25	240	14721	0.40	ng/ul	0.00
22) Perylene-d12	23.44	264	9977m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.17	96	2114	1.31	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.02	152	6878	0.39	ng/ul	0.00
16) Fluoranthene-d10	19.08	212	20417	0.50	ng/ul	0.00
Target Compounds						
3) 1,4-Dioxane	3.20	88	7267	3.49	ng/ul#	Ovalue 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM070816\
Data File : BM006350.D
Acq On : 08 Jul 2016 14:51
Operator : UM/SJ
Sample : H3914-17
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4TS8

Manual Integrations

umangi
7/8/2016 7:19:49 PM

Quant Time: Jul 08 15:27:53 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 08:04:54 2016
Response via : Initial Calibration

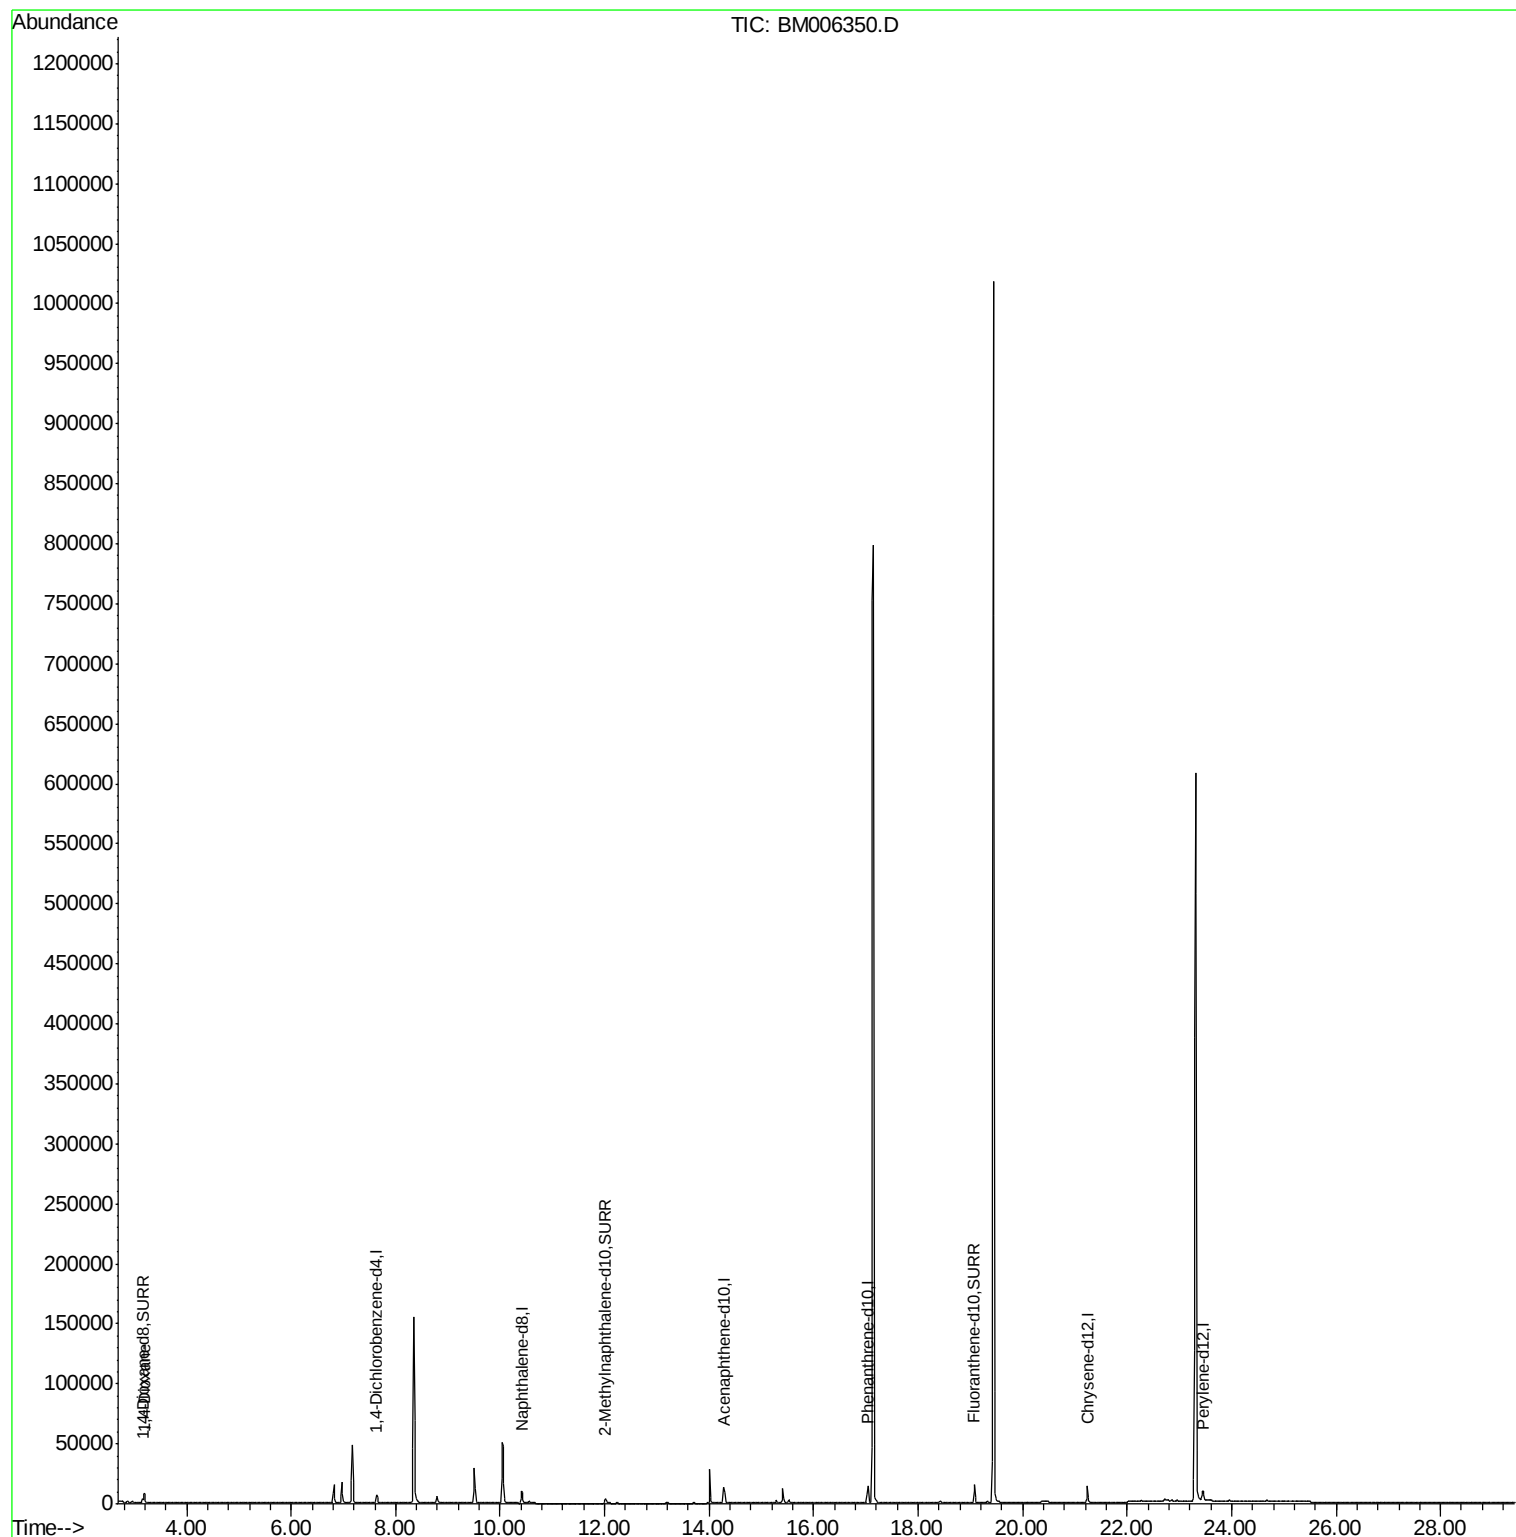

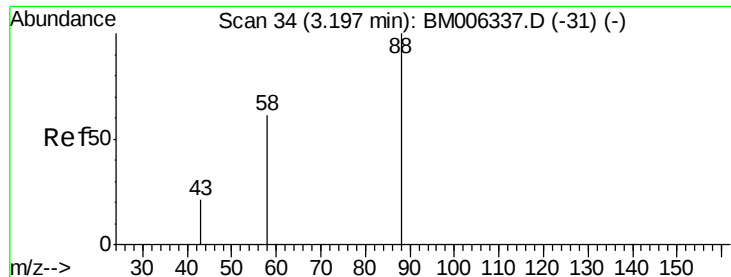

#3
 1,4-Dioxane
 Concen: 3.49 ng/ul
 RT: 3.20 min Scan# 34
 Delta R.T. 0.00 min
 Lab File: BM006350.D
 Acq: 08 Jul 2016 14:51

Instrument :
 BNA_M
 ClientSampleId :
 A4TS8

Tot Ion	Ratio	Lower	Upper
88	100		
58	81.3	8.0	12.0#
43	38.7	8.0	12.0#

Manual Integrations

umangi
 7/8/2016 7:19:49 PM

