



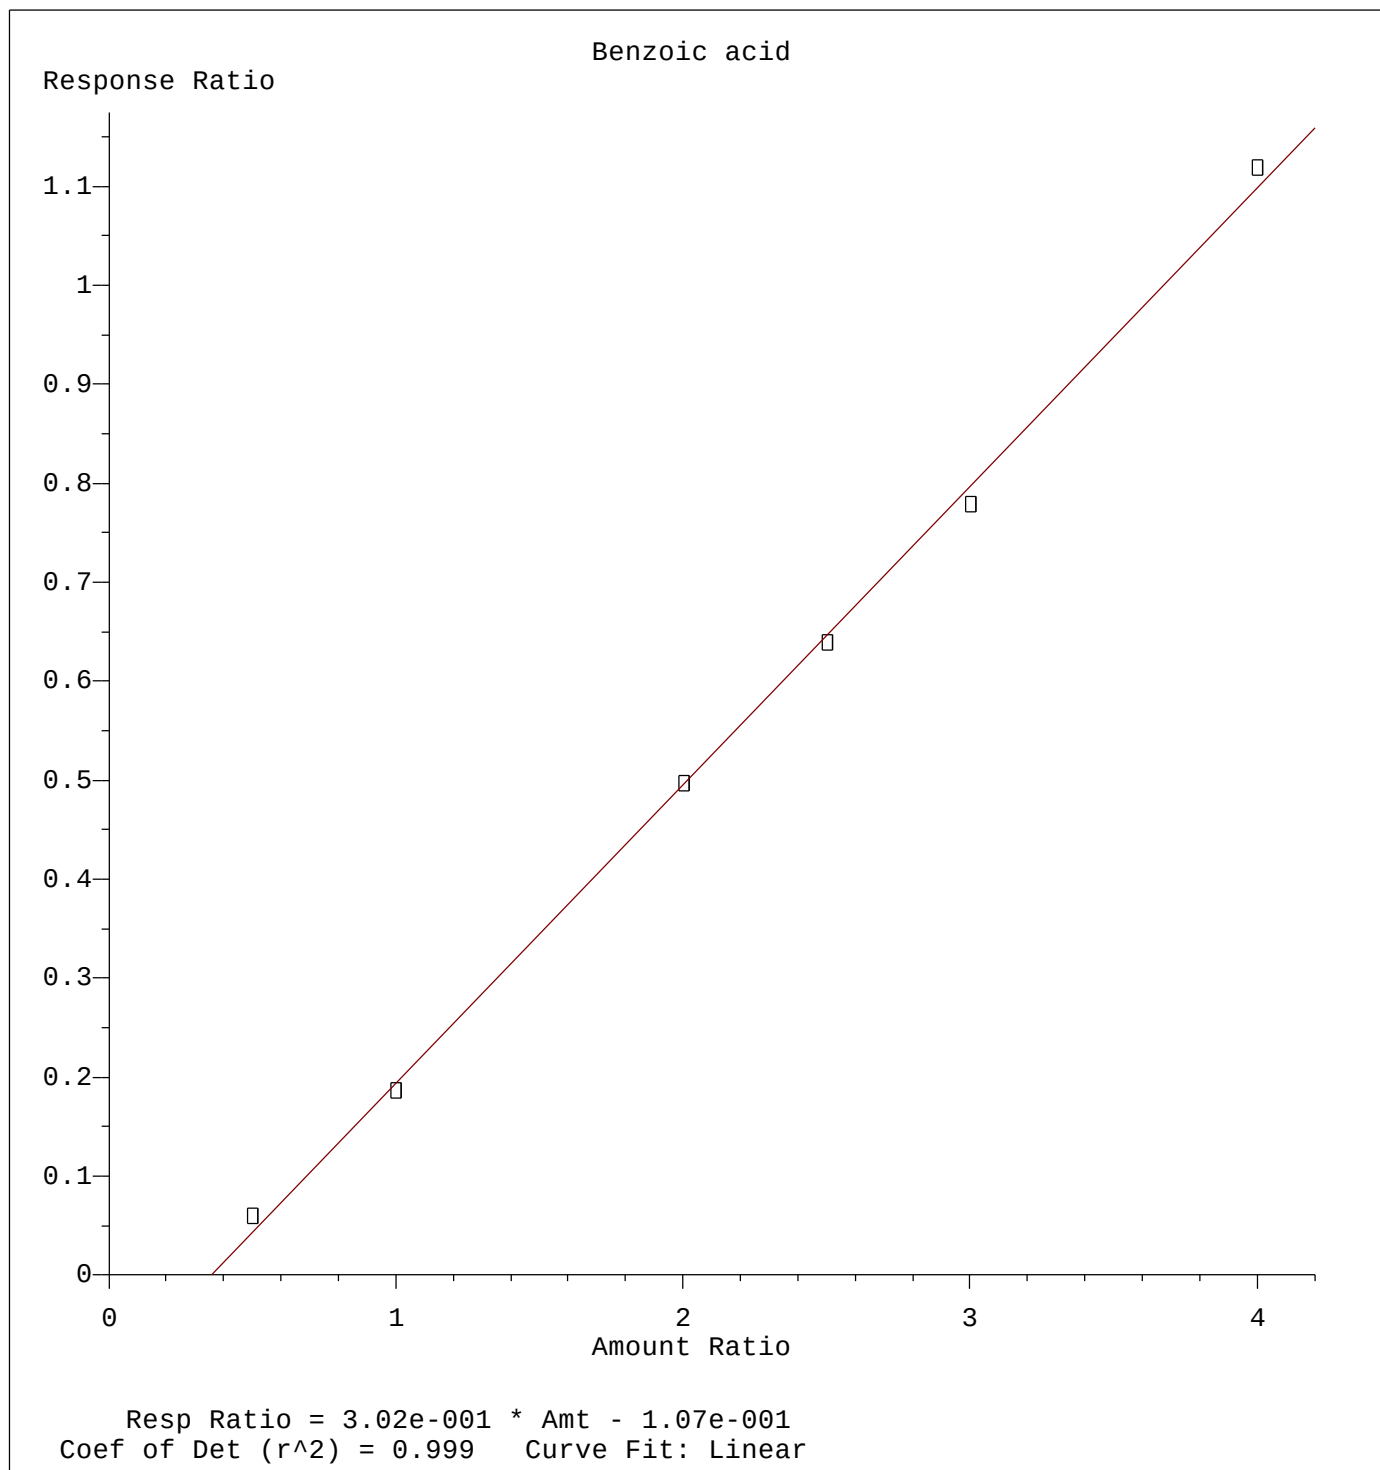

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Calibration Table Last Updated: Wed Jul 08 11:38:47 2020

Hexachlorocyclopentadiene

Response Ratio

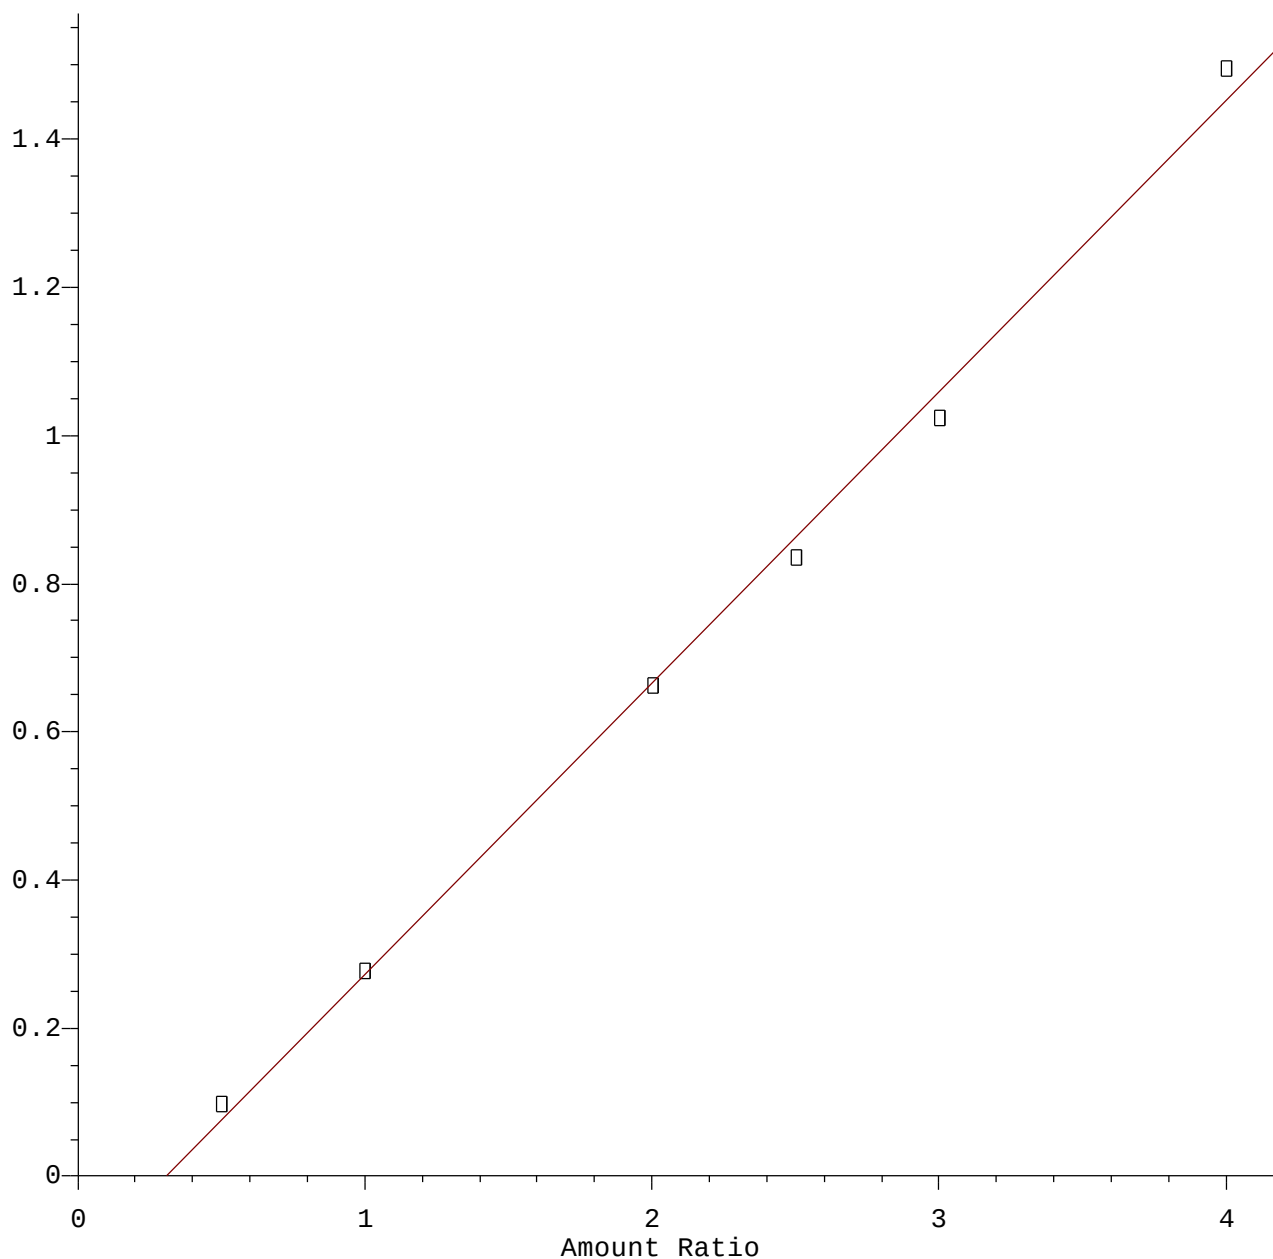


Resp Ratio = $3.93 \times 10^{-1} \times \text{Amt} - 1.20 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Calibration Table Last Updated: Wed Jul 08 11:38:47 2020


2,4-Dinitrophenol

Response Ratio

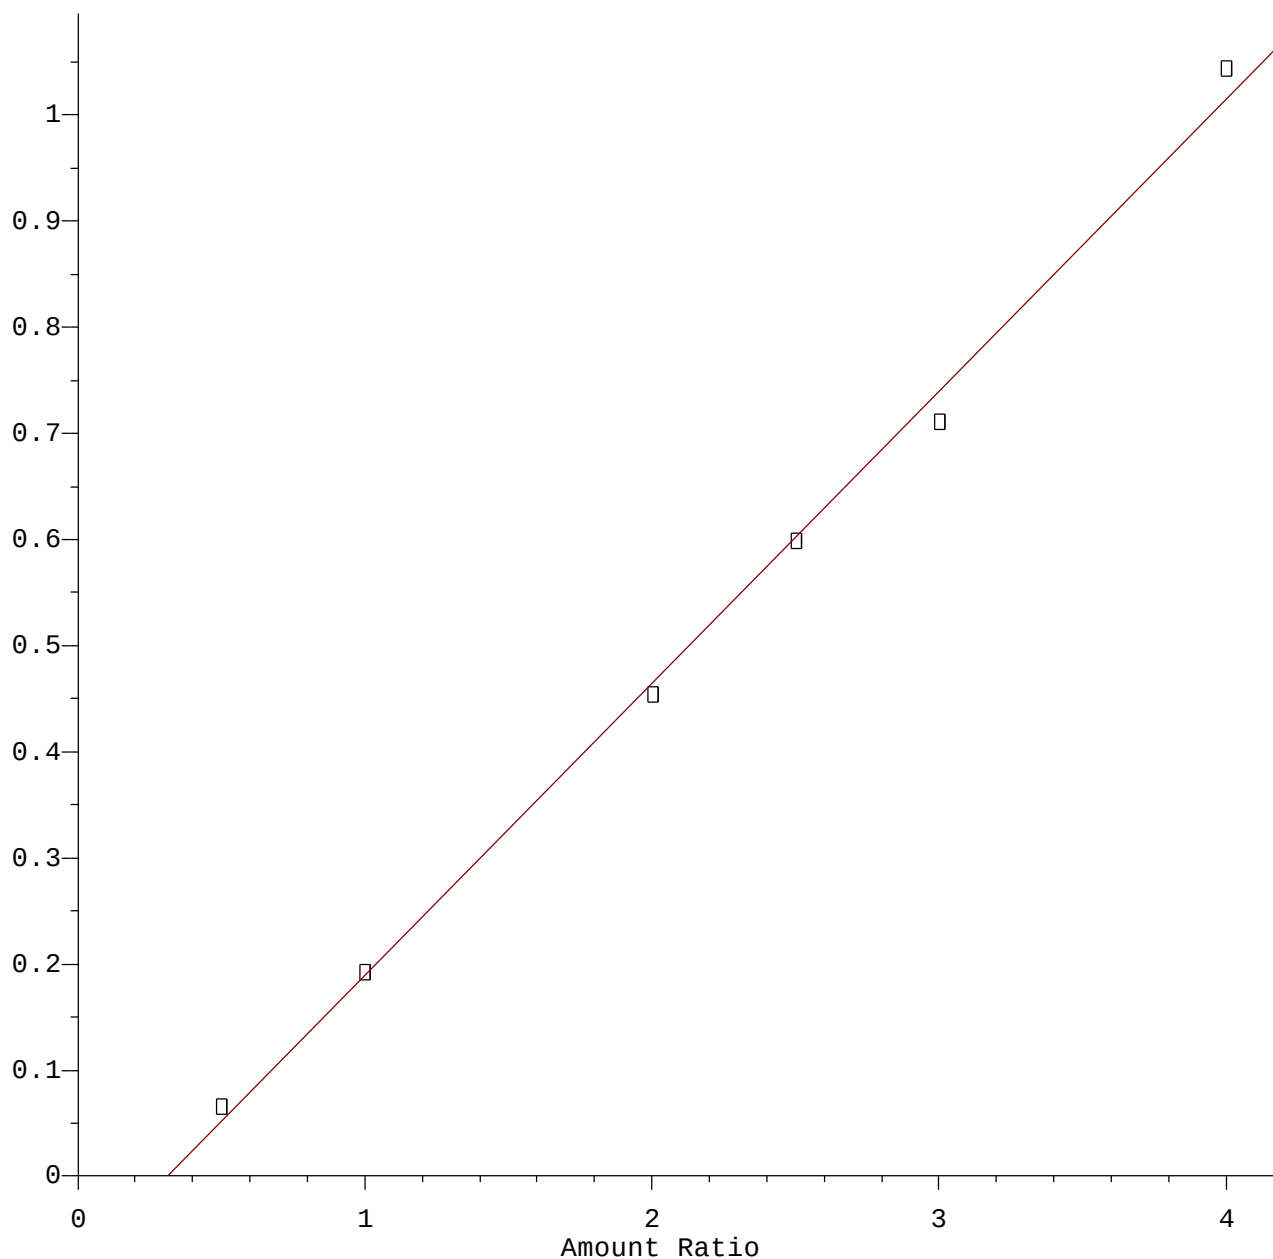

Resp Ratio = $2.75 \times 10^{-1} \times \text{Amt} - 8.63 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Calibration Table Last Updated: Wed Jul 08 11:38:47 2020

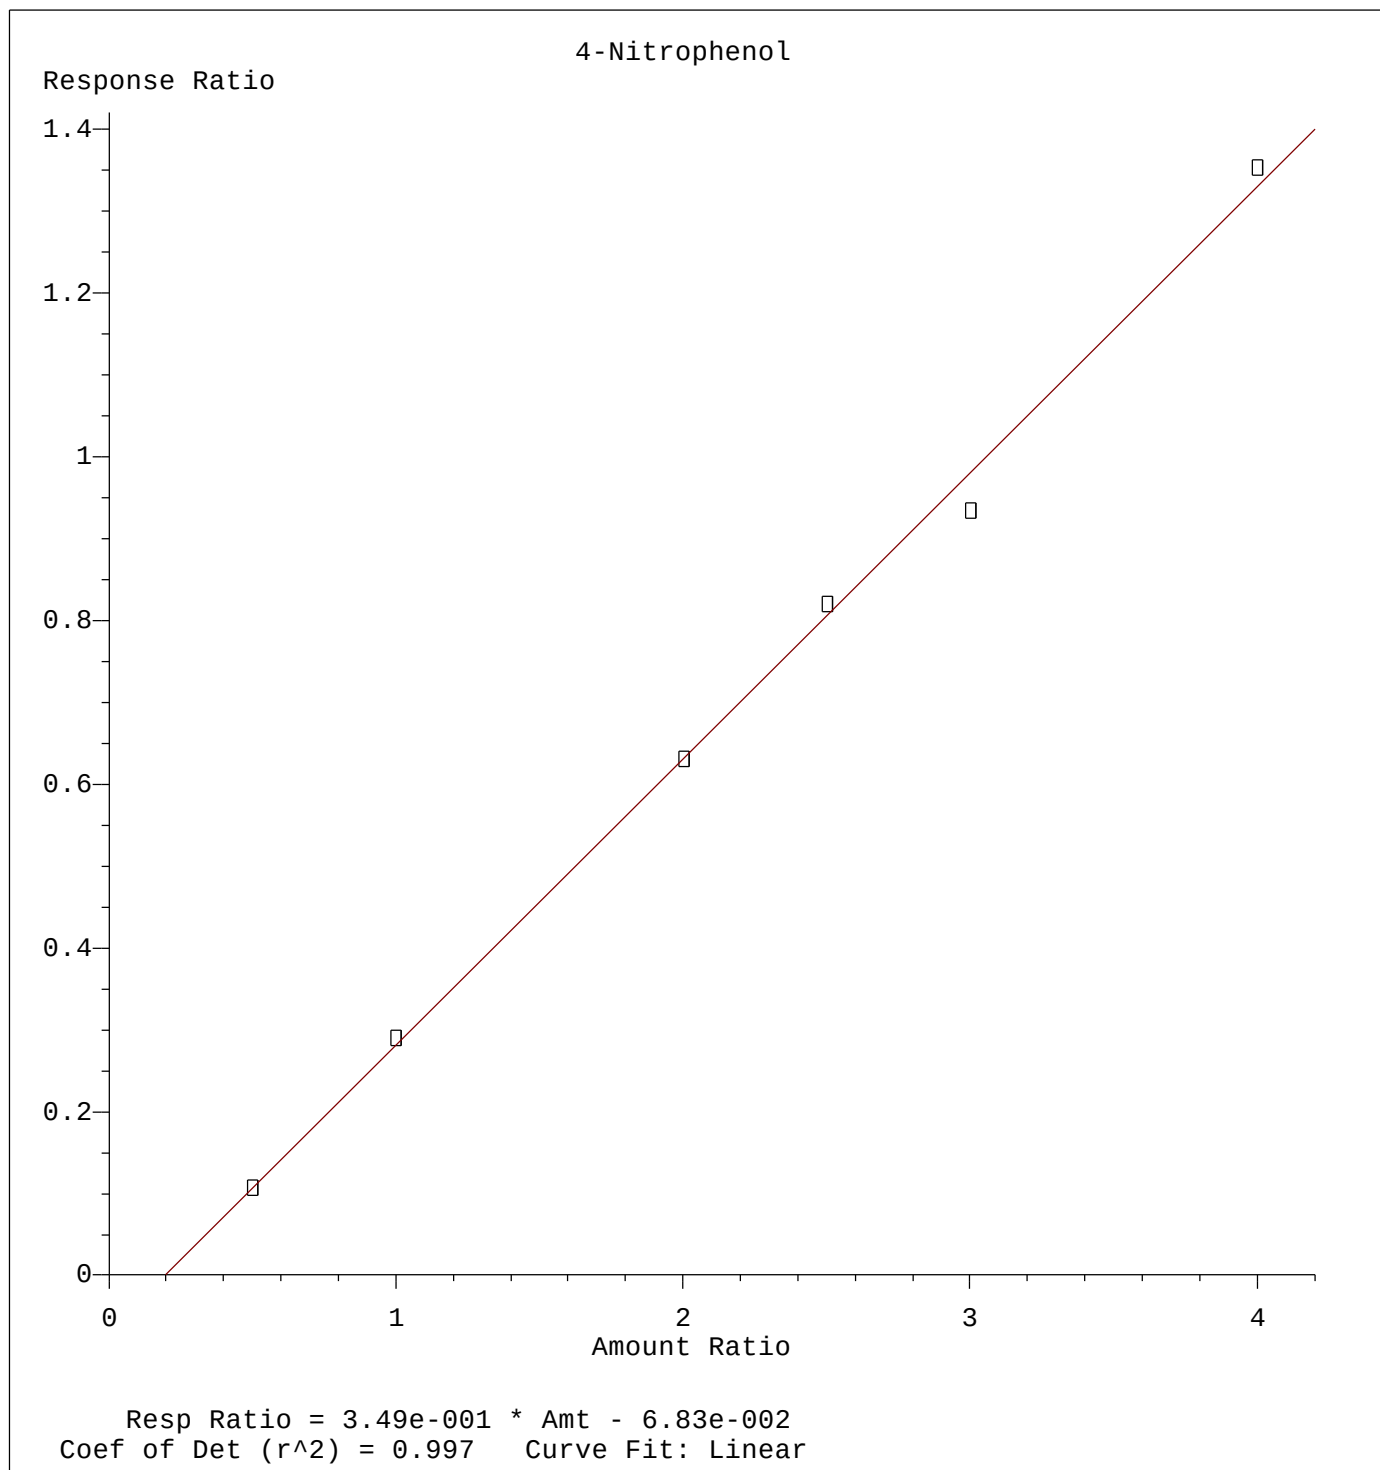

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Calibration Table Last Updated: Wed Jul 08 11:38:47 2020

4-Nitroaniline

Response Ratio

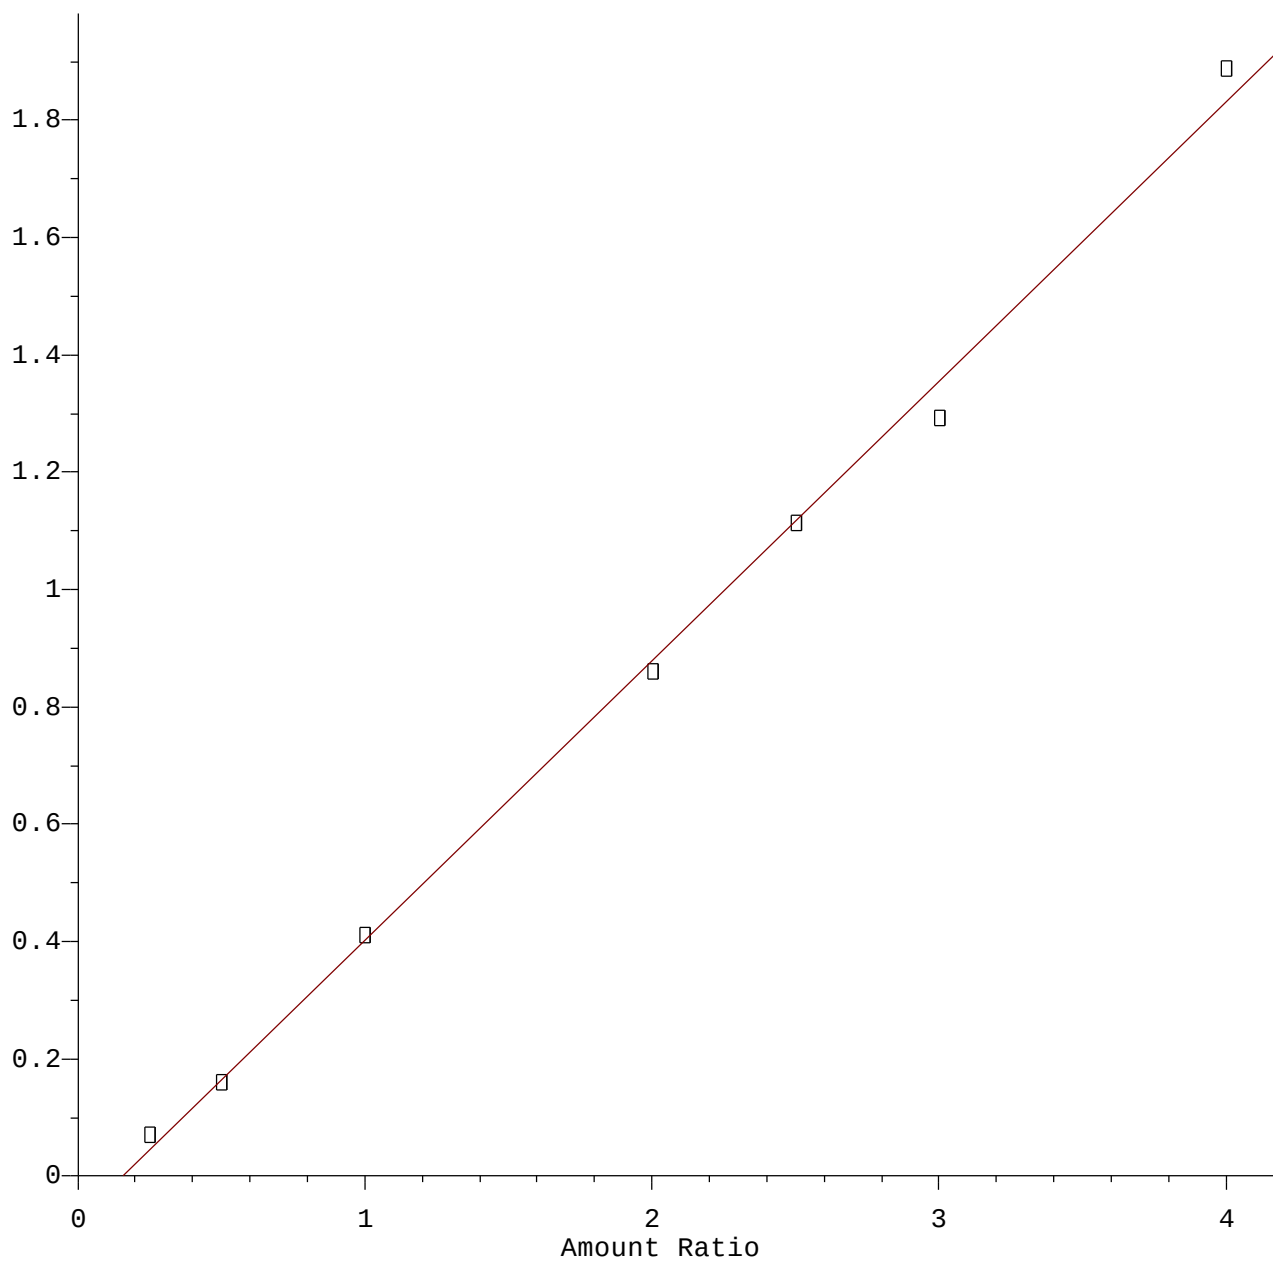


Resp Ratio = $4.76 \times 10^{-1} \times \text{Amt} - 7.48 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Calibration Table Last Updated: Wed Jul 08 11:38:47 2020

4,6-Dinitro-2-methylphenol

Response Ratio

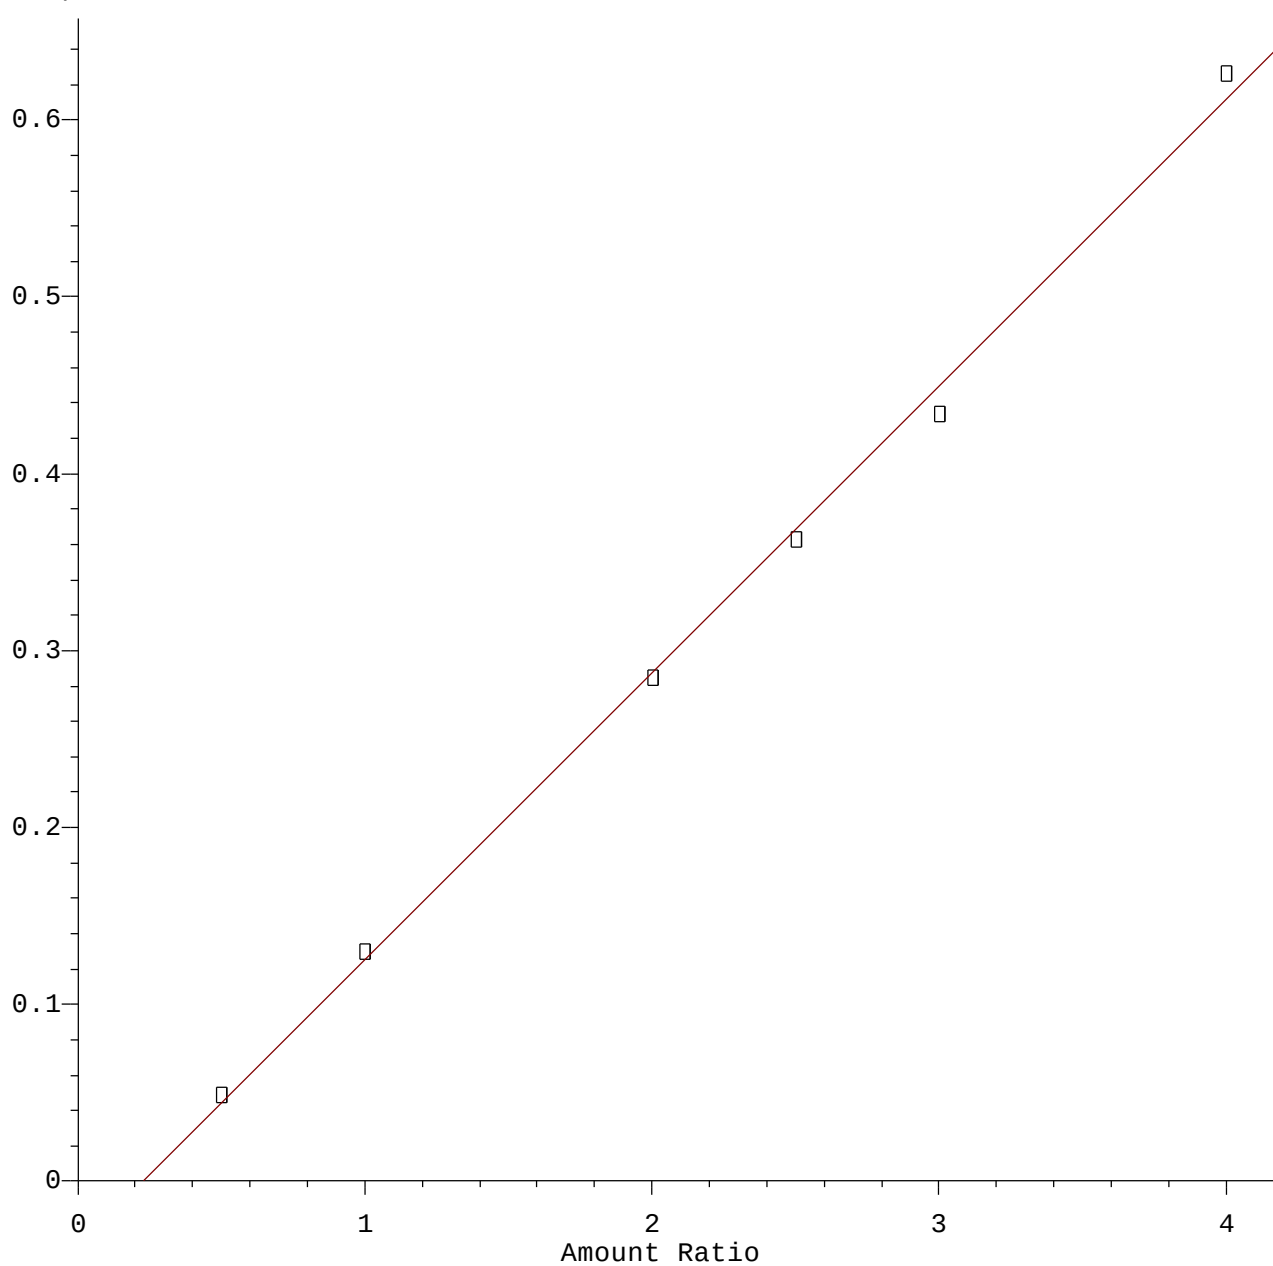

Resp Ratio = $1.62 \times 10^{-1} \times \text{Amt} - 3.67 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Calibration Table Last Updated: Wed Jul 08 11:38:47 2020