
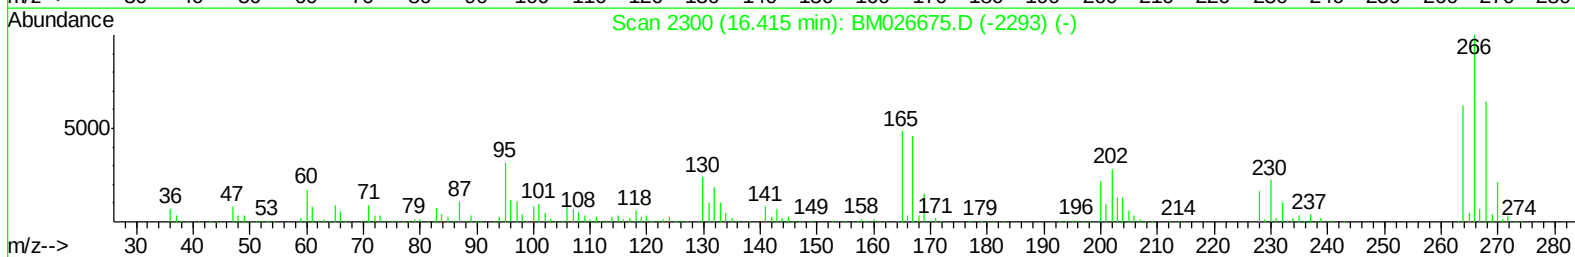
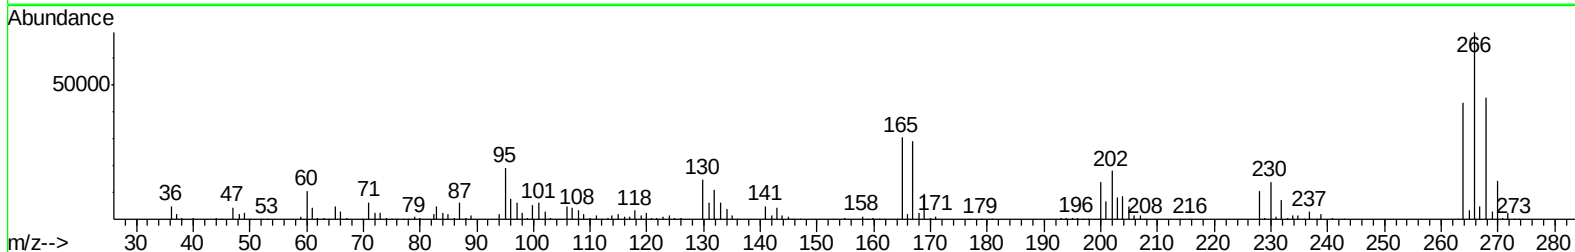


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070820\
Data File : BM026670.D
Acq On : 07 Jul 2020 08:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 06:44:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 16:22:38 2020
Response via : Initial Calibration

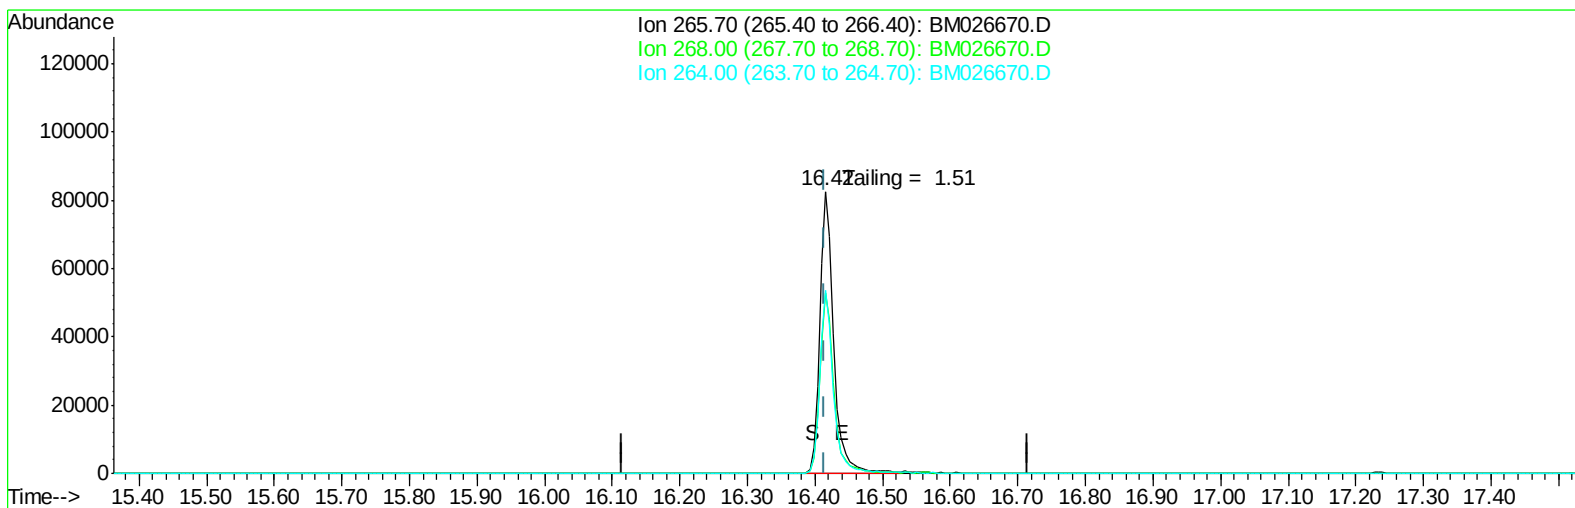

TIC: BM026670.D

(70) Pentachlorophenol (C)

16.415min (0.000) 39278.44ng

response 119931

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	64.24
264.00	62.60	65.16
0.00	0.00	0.00

