


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070820\
 Data File : BM026670.D
 Acq On : 07 Jul 2020 08:09
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 08 11:38:47 2020

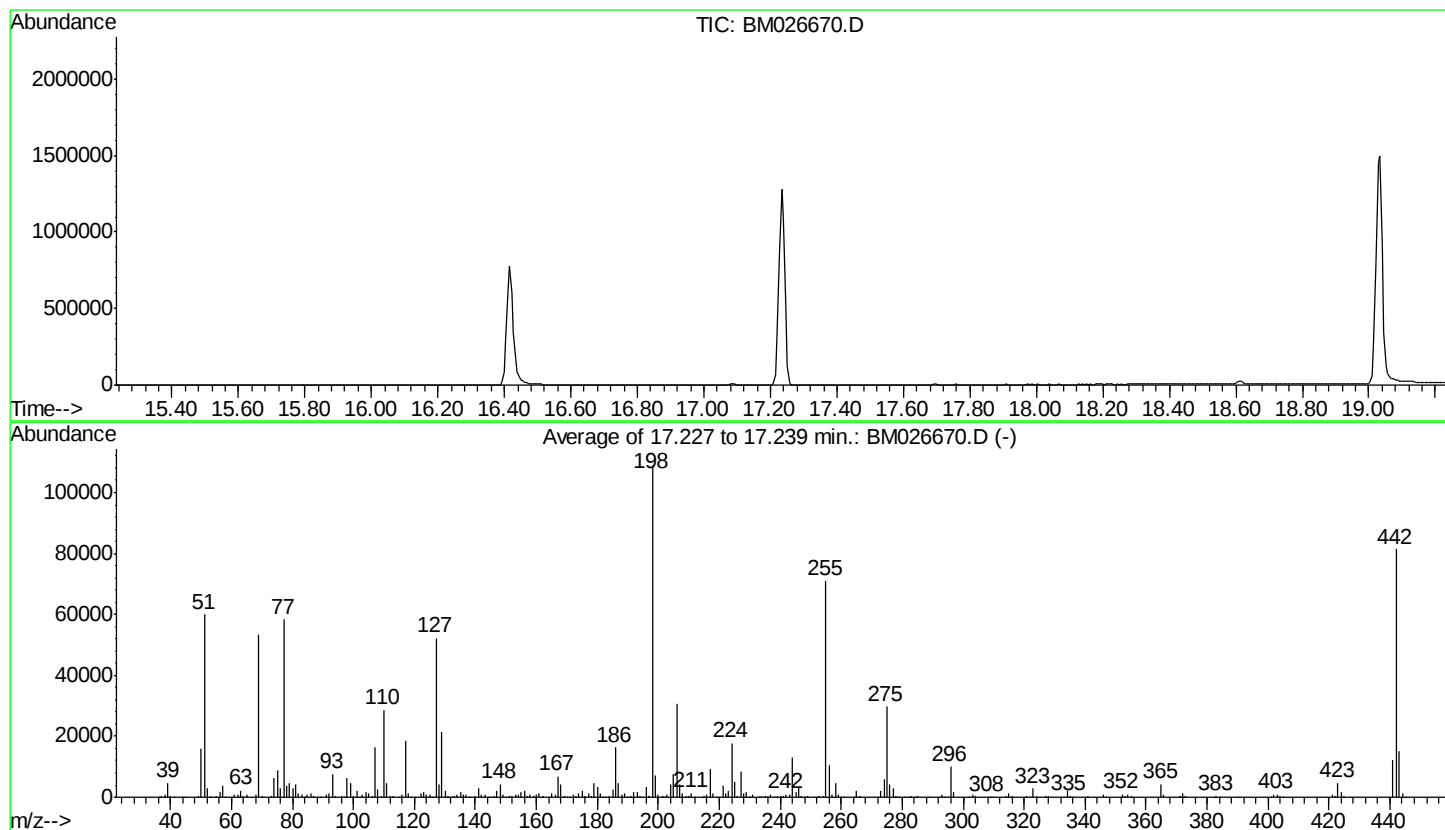

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.1	59992	PASS
68	69	0.00	2	1.8	969	PASS
69	198	0.00	100	49.1	53424	PASS
70	69	0.00	2	0.6	307	PASS
127	198	10	80	47.9	52106	PASS
197	198	0.00	2	0.3	346	PASS
198	198	100	100	100.0	108829	PASS
199	198	5	9	6.6	7184	PASS
275	198	10	60	27.4	29821	PASS
365	198	1	100	4.1	4417	PASS
441	198	0.01	100	11.2	12238	PASS
442	198	50	100	74.8	81368	PASS
443	442	15	24	18.8	15318	PASS