


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070820\
 Data File : BM026680.D
 Acq On : 07 Jul 2020 16:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 08 11:38:47 2020

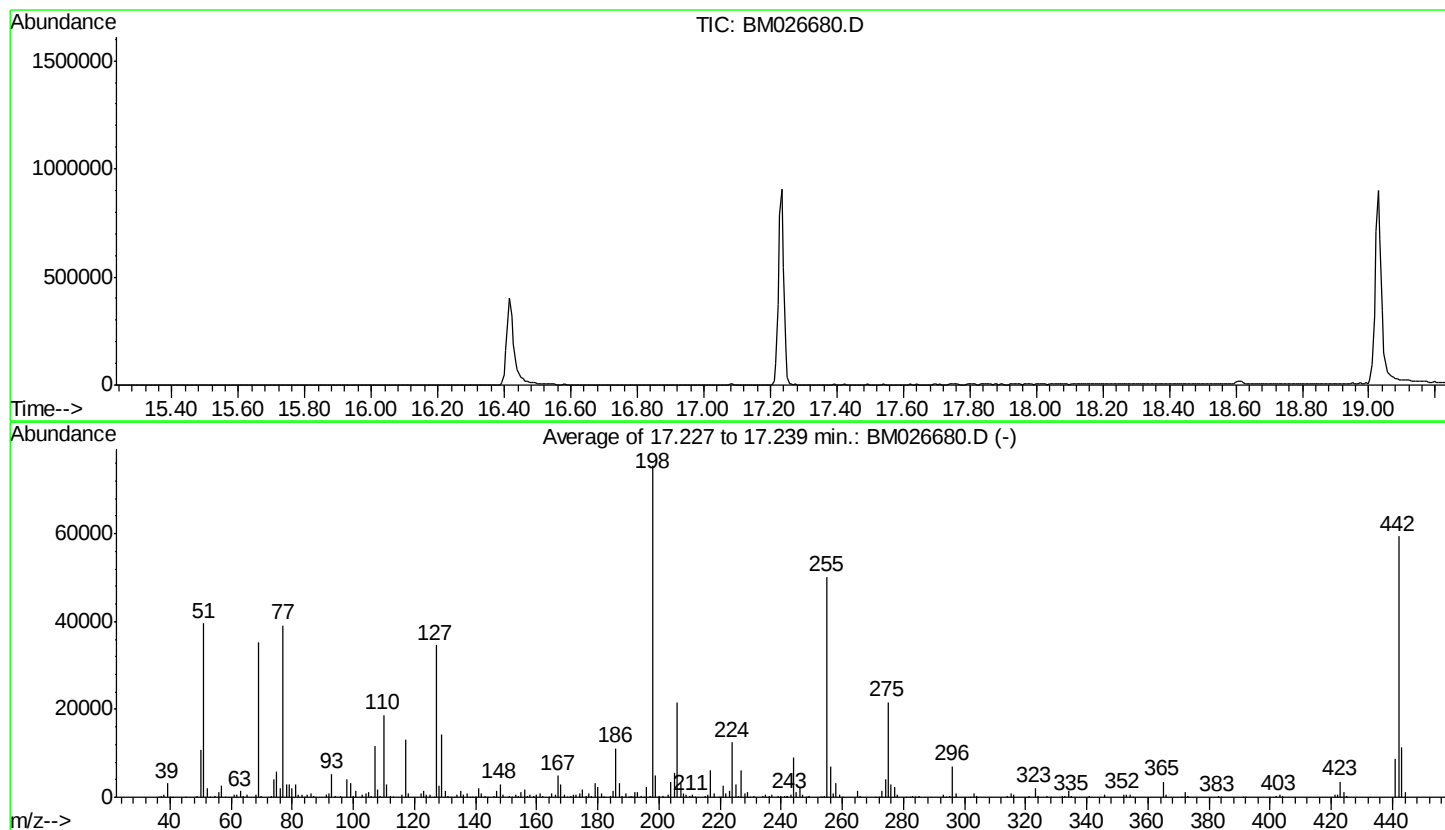

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	39605	PASS
68	69	0.00	2	1.8	649	PASS
69	198	0.00	100	46.6	35213	PASS
70	69	0.00	2	0.5	168	PASS
127	198	10	80	45.9	34632	PASS
197	198	0.00	2	0.5	379	PASS
198	198	100	100	100.0	75493	PASS
199	198	5	9	6.4	4837	PASS
275	198	10	60	28.8	21706	PASS
365	198	1	100	4.7	3533	PASS
441	198	0.01	100	11.8	8887	PASS
442	198	50	100	78.7	59413	PASS
443	442	15	24	19.3	11450	PASS