


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
Data File : BM030916.D
Acq On : 09 Jul 2021 11:39
Operator : CG/JU
Sample : PB137515BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK515

Manual Integrations
APPROVED

mohammad
7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:13:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 10:44:22 2021
Response via : Initial Calibration

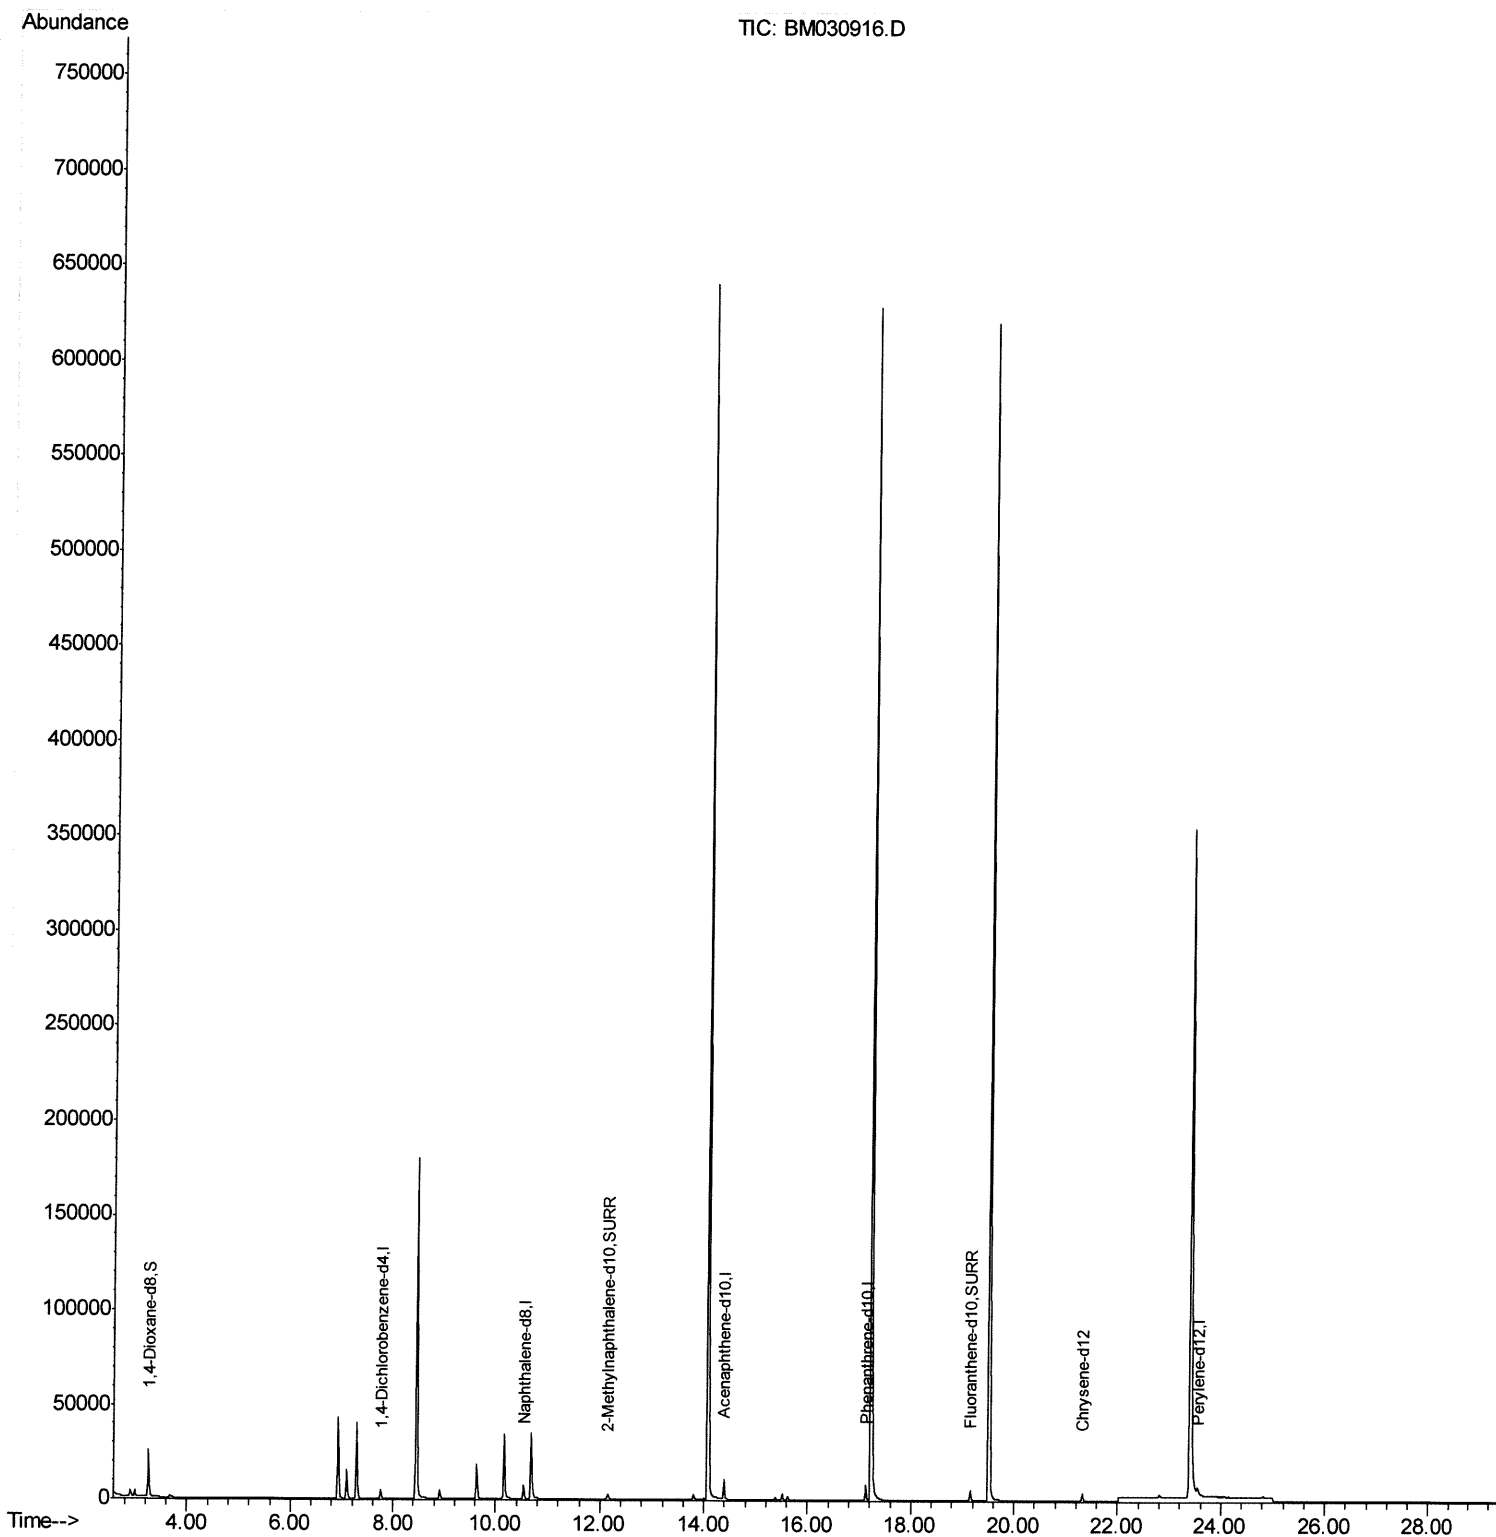


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
Data File : BM030916.D
Acq On : 09 Jul 2021 11:39
Operator : CG/JU
Sample : PB137515BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK515

Manual Integrations
APPROVED

mohammad
7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:11:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 10:44:22 2021
Response via : Initial Calibration

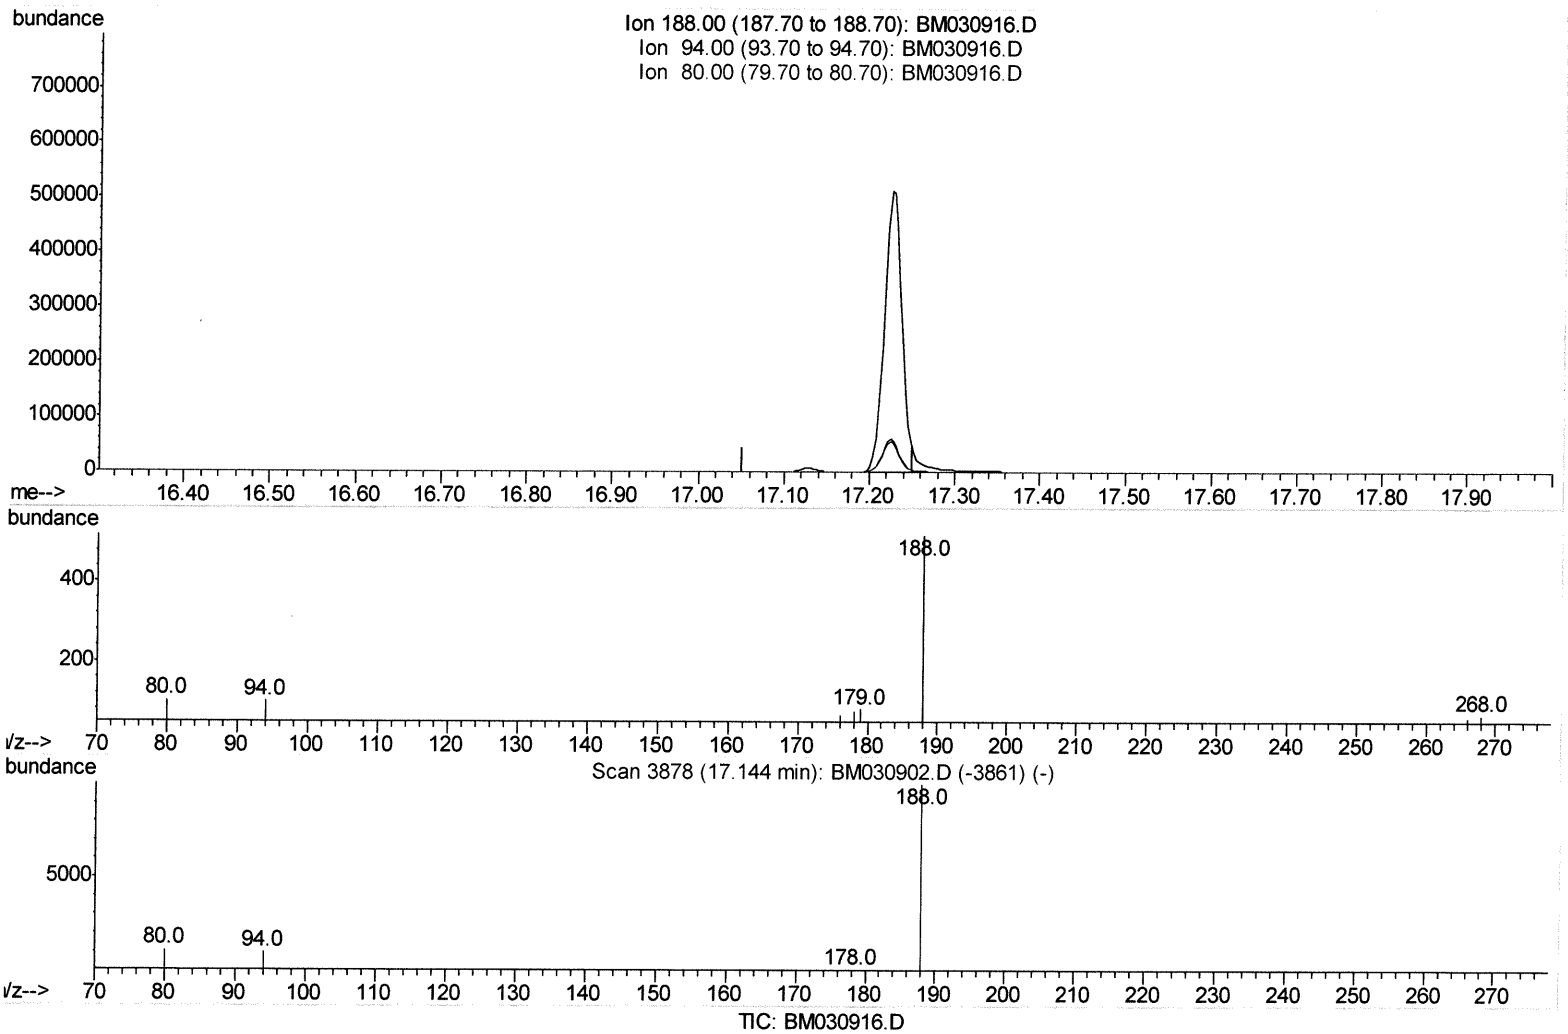

(13) Phenanthrene-d10 (I)

17.152min (-17.152) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.30	0.00#
80.00	11.60	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
 Data File : BM030916.D
 Acq On : 09 Jul 2021 11:39
 Operator : CG/JU
 Sample : PB137515BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK515

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:11:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 10:44:22 2021
 Response via : Initial Calibration

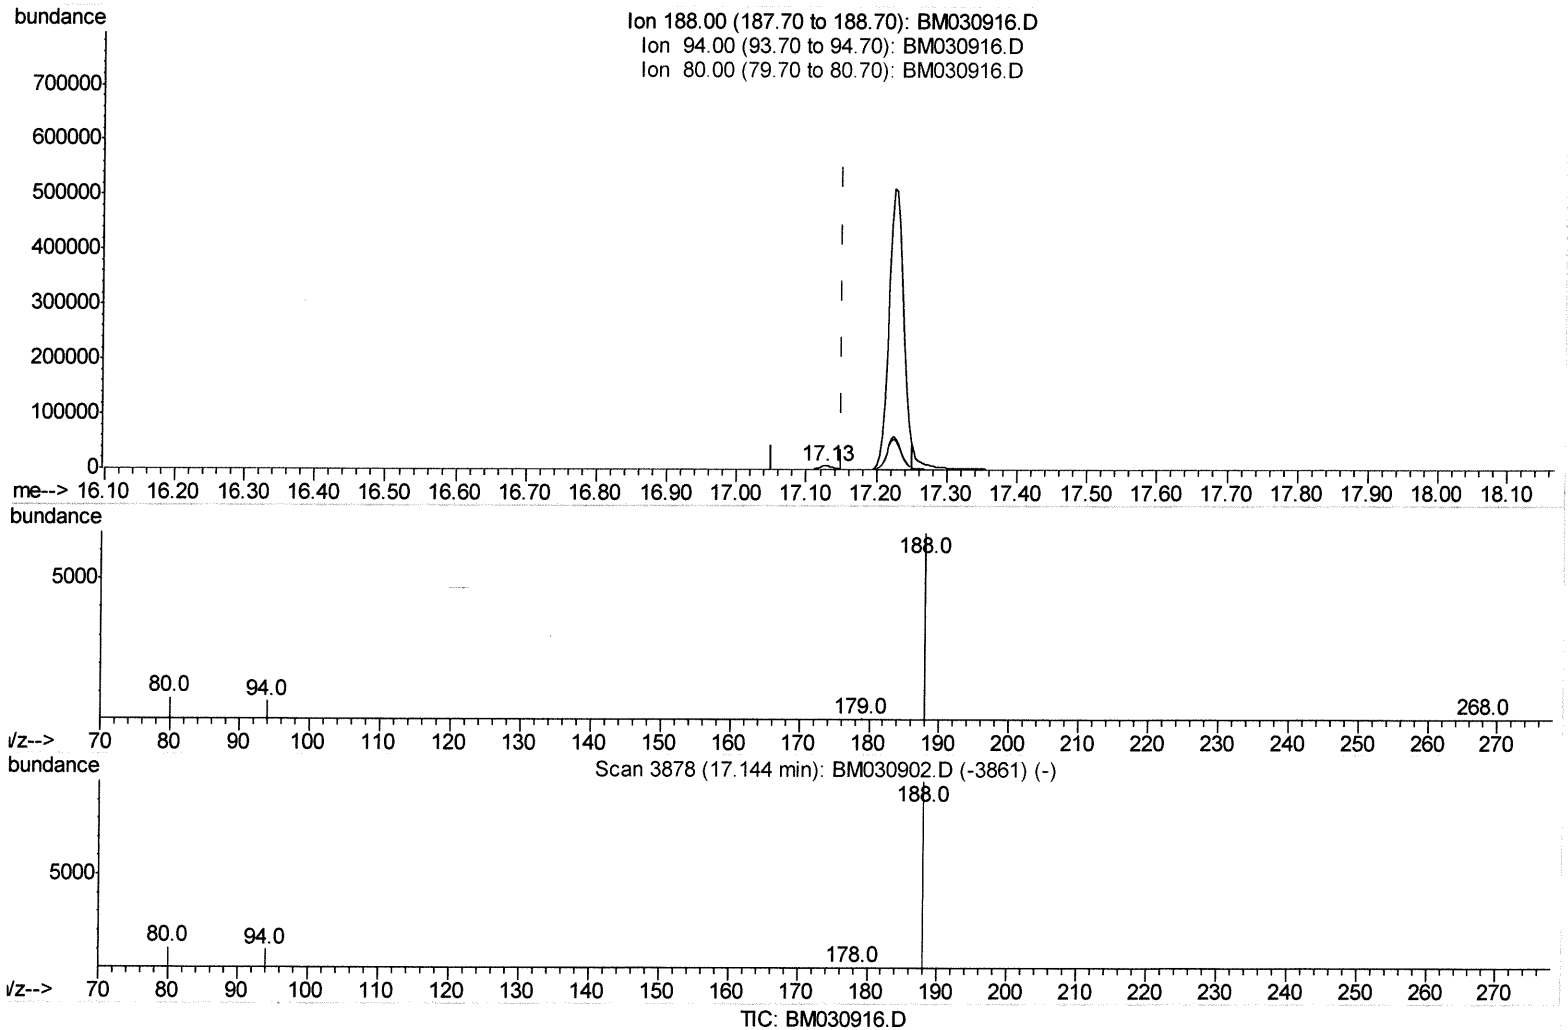

(13) Phenanthrene-d10 (I)

17.127min (-0.024) 0.40ng/ul m 07/12/21 JU

response 9616

Ion	Exp%	Act%
188.00	100	100
94.00	10.30	10.15
80.00	11.60	11.72
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
 Data File : BM030916.D
 Acq On : 09 Jul 2021 11:39
 Operator : CG/JU
 Sample : PB137515BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK515

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:12:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 10:44:22 2021
 Response via : Initial Calibration

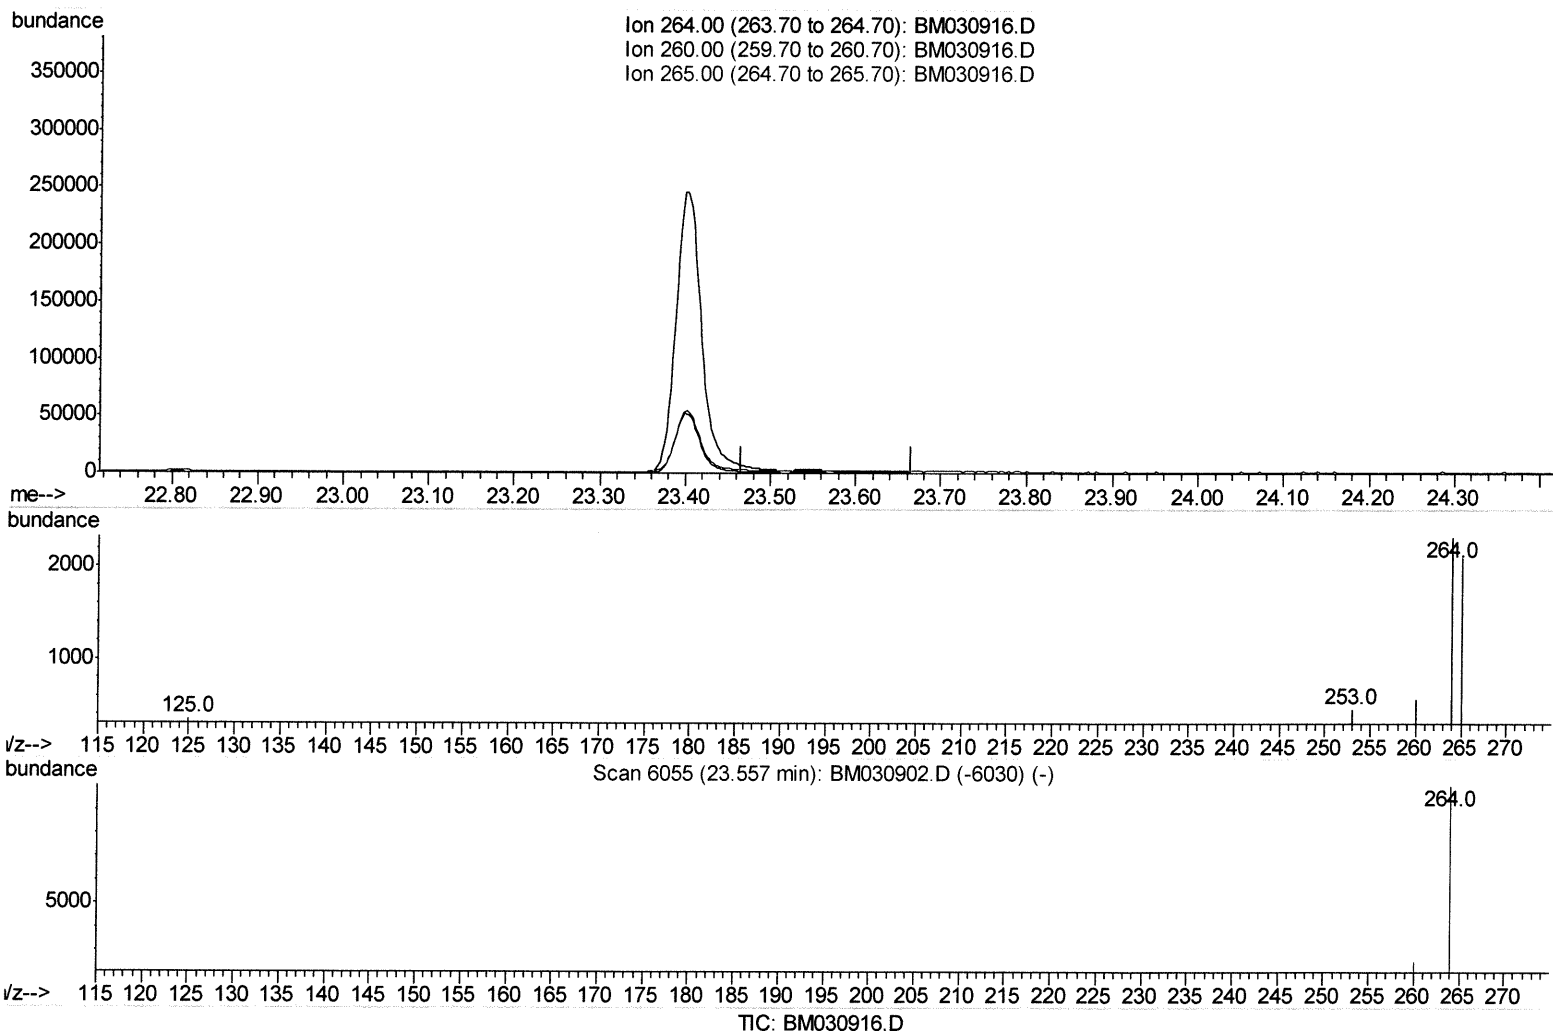

(23) Perylene-d12 (I)

23.566min (-23.566) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	26.10	0.00#
265.00	65.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
 Data File : BM030916.D
 Acq On : 09 Jul 2021 11:39
 Operator : CG/JU
 Sample : PB137515BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK515

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:12:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 10:44:22 2021
 Response via : Initial Calibration

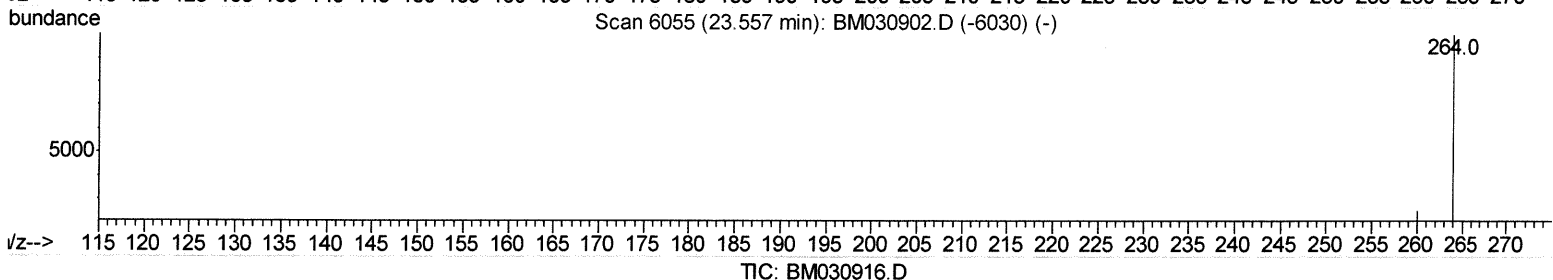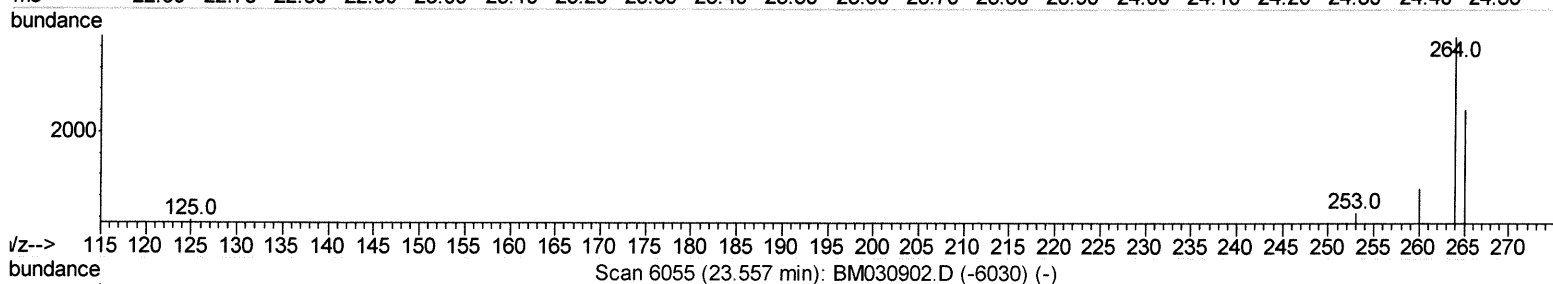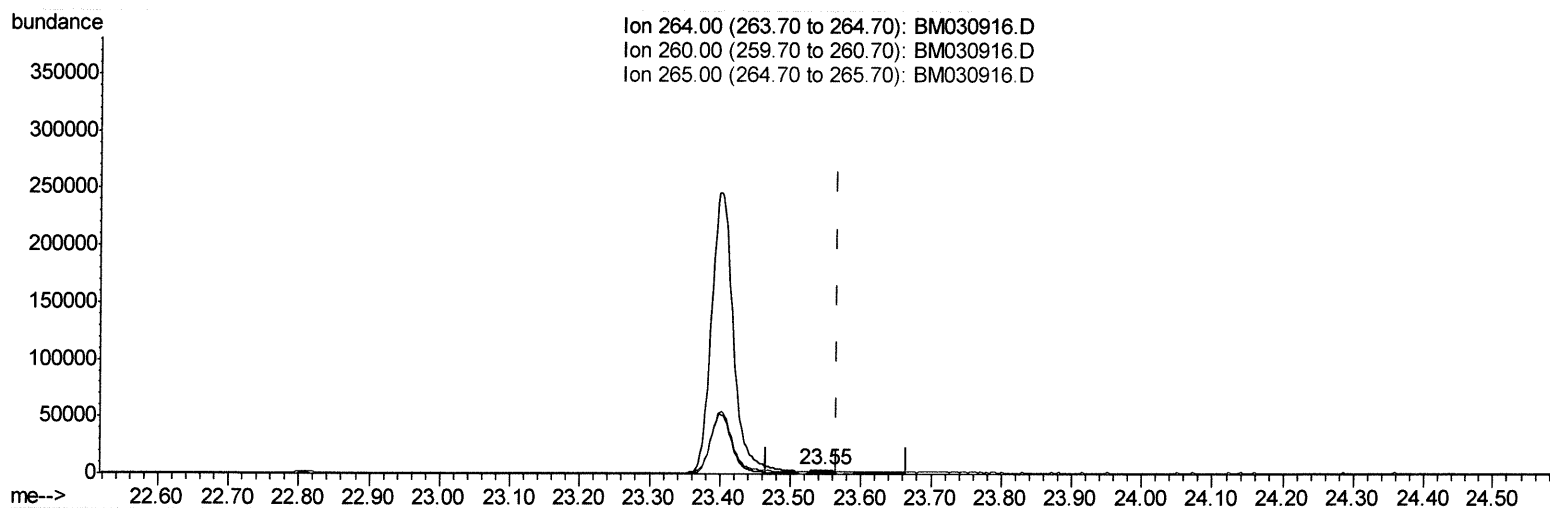

(23) Perylene-d12 (I)

23.547min (-0.019) 0.40ng/ul m 07/12/21 JU

response 3272




Ion	Exp%	Act%
264.00	100	100
260.00	26.10	24.91
265.00	65.90	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
 Data File : BM030916.D
 Acq On : 09 Jul 2021 11:39
 Operator : CG/JU
 Sample : PB137515BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK515

Manual Integrations
 APPROVED
 mohammad
 7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:12:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 10:44:22 2021
 Response via : Initial Calibration

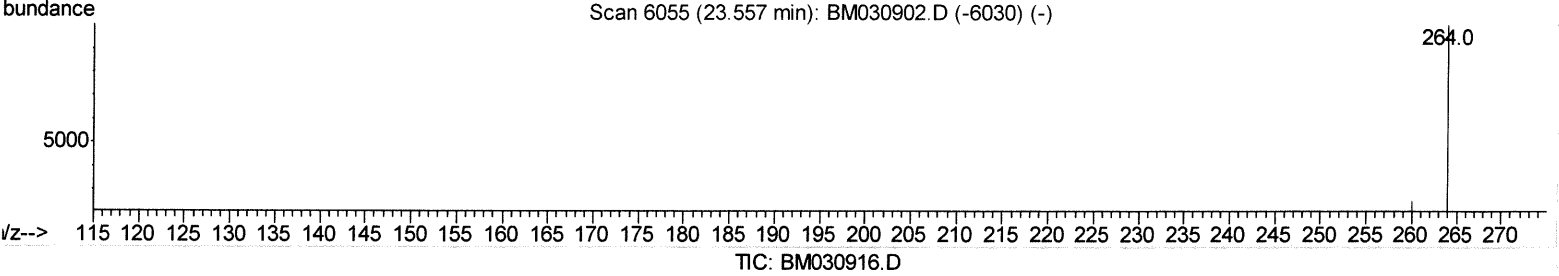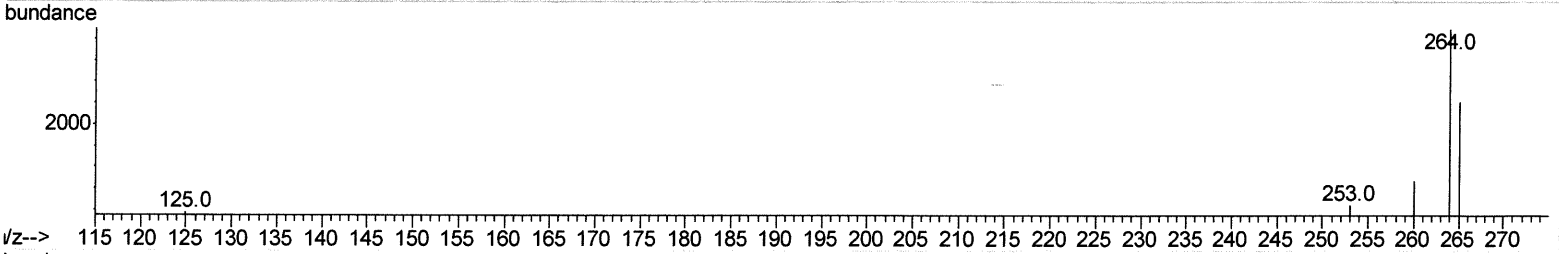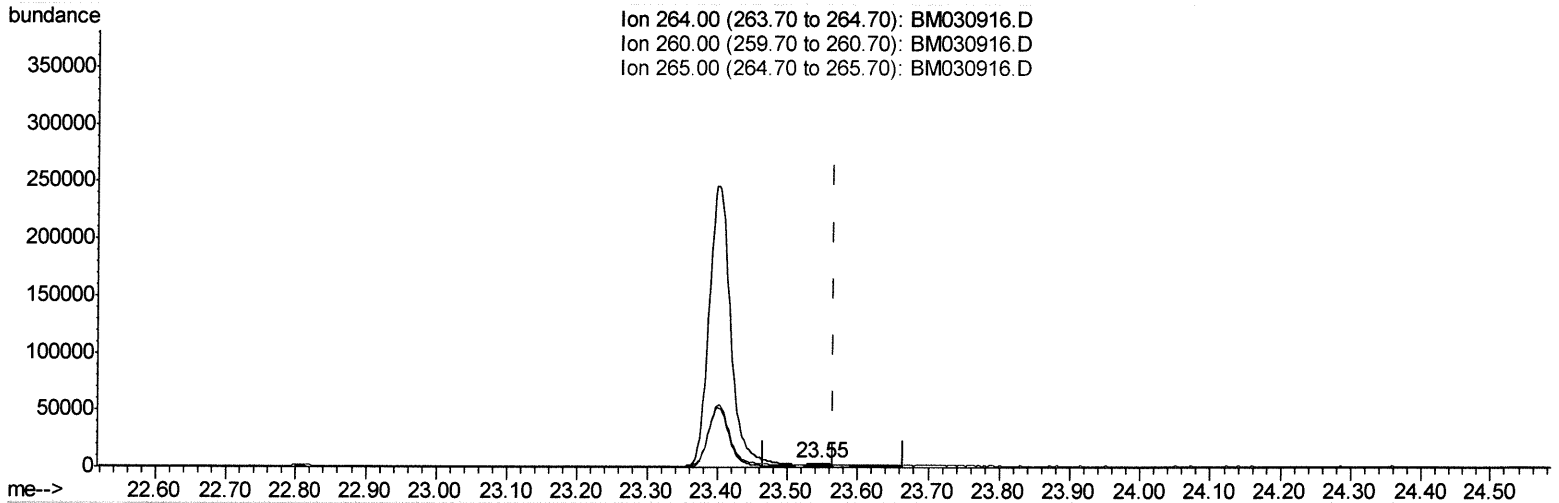

(23) Perylene-d12 (I)
 23.547min (-0.019) 0.40ng/ul m 07/12/21 JU

response 3272

Ion	Exp%	Act%
264.00	100	100
260.00	26.10	24.91
265.00	65.90	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070821\
 Data File : BM030916.D
 Acq On : 09 Jul 2021 11:39
 Operator : CG/JU
 Sample : PB137515BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK515

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:02:54 PM

Quant Time: Jul 09 12:13:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 10:44:22 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	2374	0.40	ng/ul	0.00
4) Naphthalene-d8	10.54	136	9761	0.40	ng/ul	-0.02
9) Acenaphthene-d10	14.39	164	5882	0.40	ng/ul	-0.02
13) Phenanthrene-d10	17.13	188	9616m>	0.40	ng/ul>	-0.02 07/12/21JU
17) Chrysene-d12	21.32	240	5178	0.40	ng/ul	0.00
23) Perylene-d12	23.55	264	3272m>	0.40	ng/ul>	-0.02 07/12/21JU
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	15585	6.02	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.15	152	4990	0.33	ng/ul	0.00
18) Fluoranthene-d10	19.15	212	6865	0.46	ng/ul	-0.02

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed