

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070824\
 Data File : BM046472.D
 Acq On : 09 Jul 2024 13:47
 Operator : MA/JU
 Sample : P3059-16
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GP3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/09/2024
 Supervised By :mohammad ahmed 07/10/2024

Quant Time: Jul 09 14:37:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 09 08:09:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	6102	0.400	ng/ul	0.00
4) Naphthalene-d8	10.288	136	16283	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	10323	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	21286m	0.400	ng/ul	0.00
17) Chrysene-d12	21.128	240	13781	0.400	ng/ul	0.00
23) Perylene-d12	23.276	264	12525m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	17729	2.813	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	8632	0.358	ng/ul	0.00
18) Fluoranthene-d10	18.960	212	18571	0.385	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.160	88	377	0.053	ng/ul#	34

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070824\
Data File : BM046472.D
Acq On : 09 Jul 2024 13:47
Operator : MA/JU
Sample : P3059-16
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E1GP3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/09/2024
Supervised By :mohammad ahmed 07/10/2024


Quant Time: Jul 09 14:37:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 08:09:14 2024
Response via : Initial Calibration

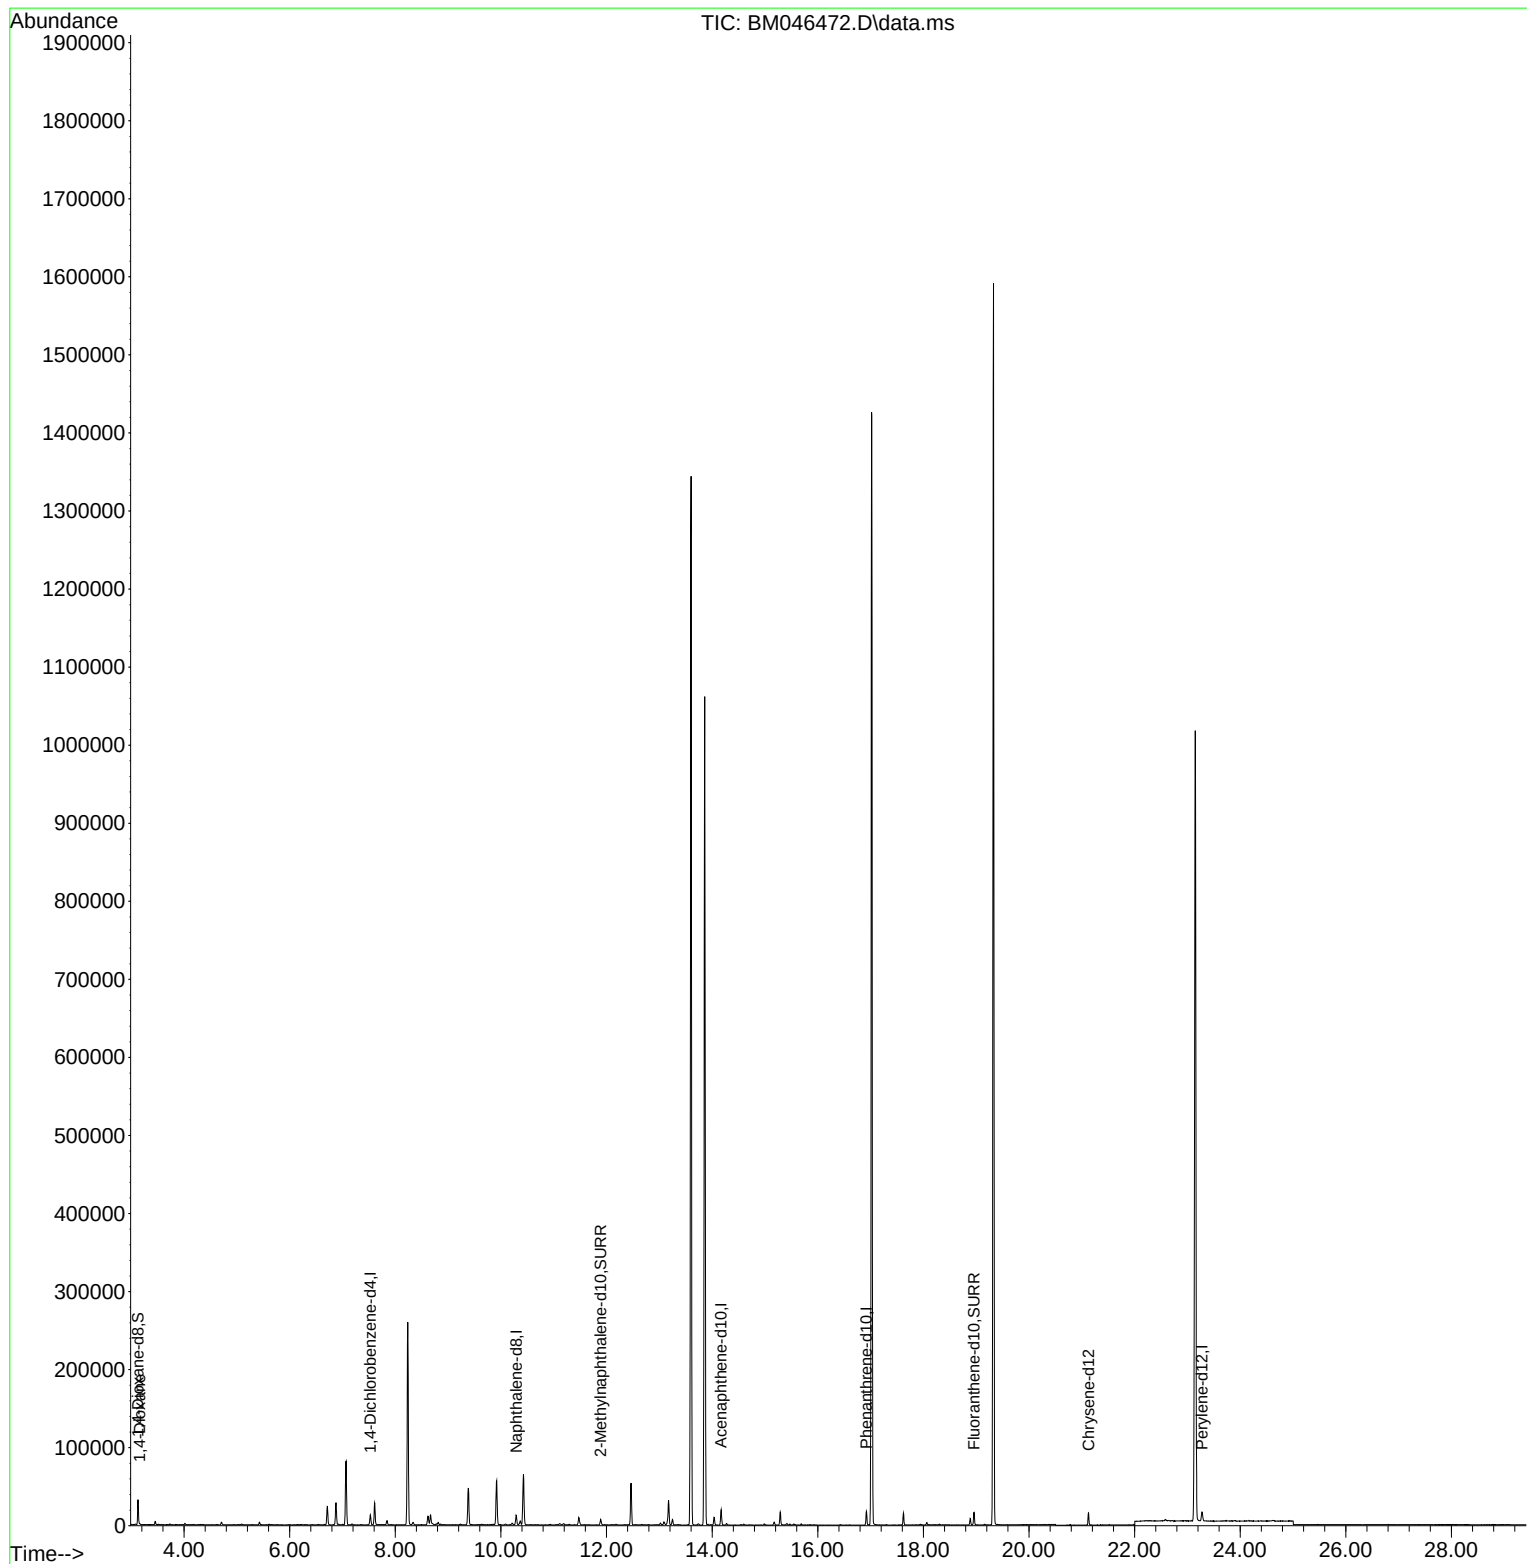

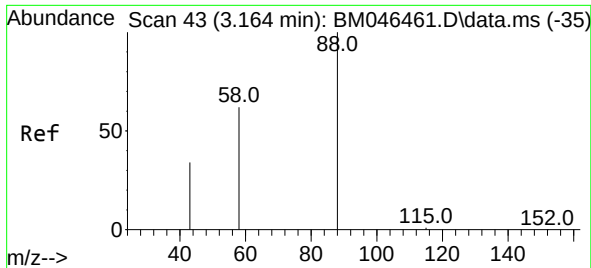

#2
1,4-Dioxane
Concen: 0.053 ng/ul
RT: 3.160 min Scan# 41
Delta R.T. -0.004 min
Lab File: BM046472.D
Acq: 09 Jul 2024 13:47

Instrument :
BNA_M
ClientSampleId :
E1GP3

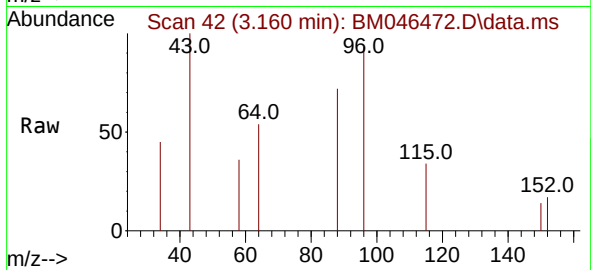

Tgt Ion: 88 Resp: 37
Ion Ratio Lower Upper
88 100
43 138.7 41.9 62.9
58 50.5 56.5 84.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/09/2024
Supervised By :mohammad ahmed 07/10/2024

