

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070824\
 Data File : BM046473.D
 Acq On : 09 Jul 2024 14:24
 Operator : MA/JU
 Sample : P3059-17
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GP4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/09/2024
 Supervised By :mohammad ahmed 07/10/2024

Quant Time: Jul 09 15:12:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 09 08:09:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	6405	0.400	ng/ul	0.00
4) Naphthalene-d8	10.287	136	17909	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.169	164	11548	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	24262m	0.400	ng/ul	0.00
17) Chrysene-d12	21.125	240	14685	0.400	ng/ul	0.00
23) Perylene-d12	23.276	264	12701m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	15924	2.407	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	9064	0.342	ng/ul	0.00
18) Fluoranthene-d10	18.960	212	19250	0.374	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.159	88	335	0.045	ng/ul#	23

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070824\
Data File : BM046473.D
Acq On : 09 Jul 2024 14:24
Operator : MA/JU
Sample : P3059-17
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E1GP4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/09/2024
Supervised By :mohammad ahmed 07/10/2024


Quant Time: Jul 09 15:12:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 08:09:14 2024
Response via : Initial Calibration

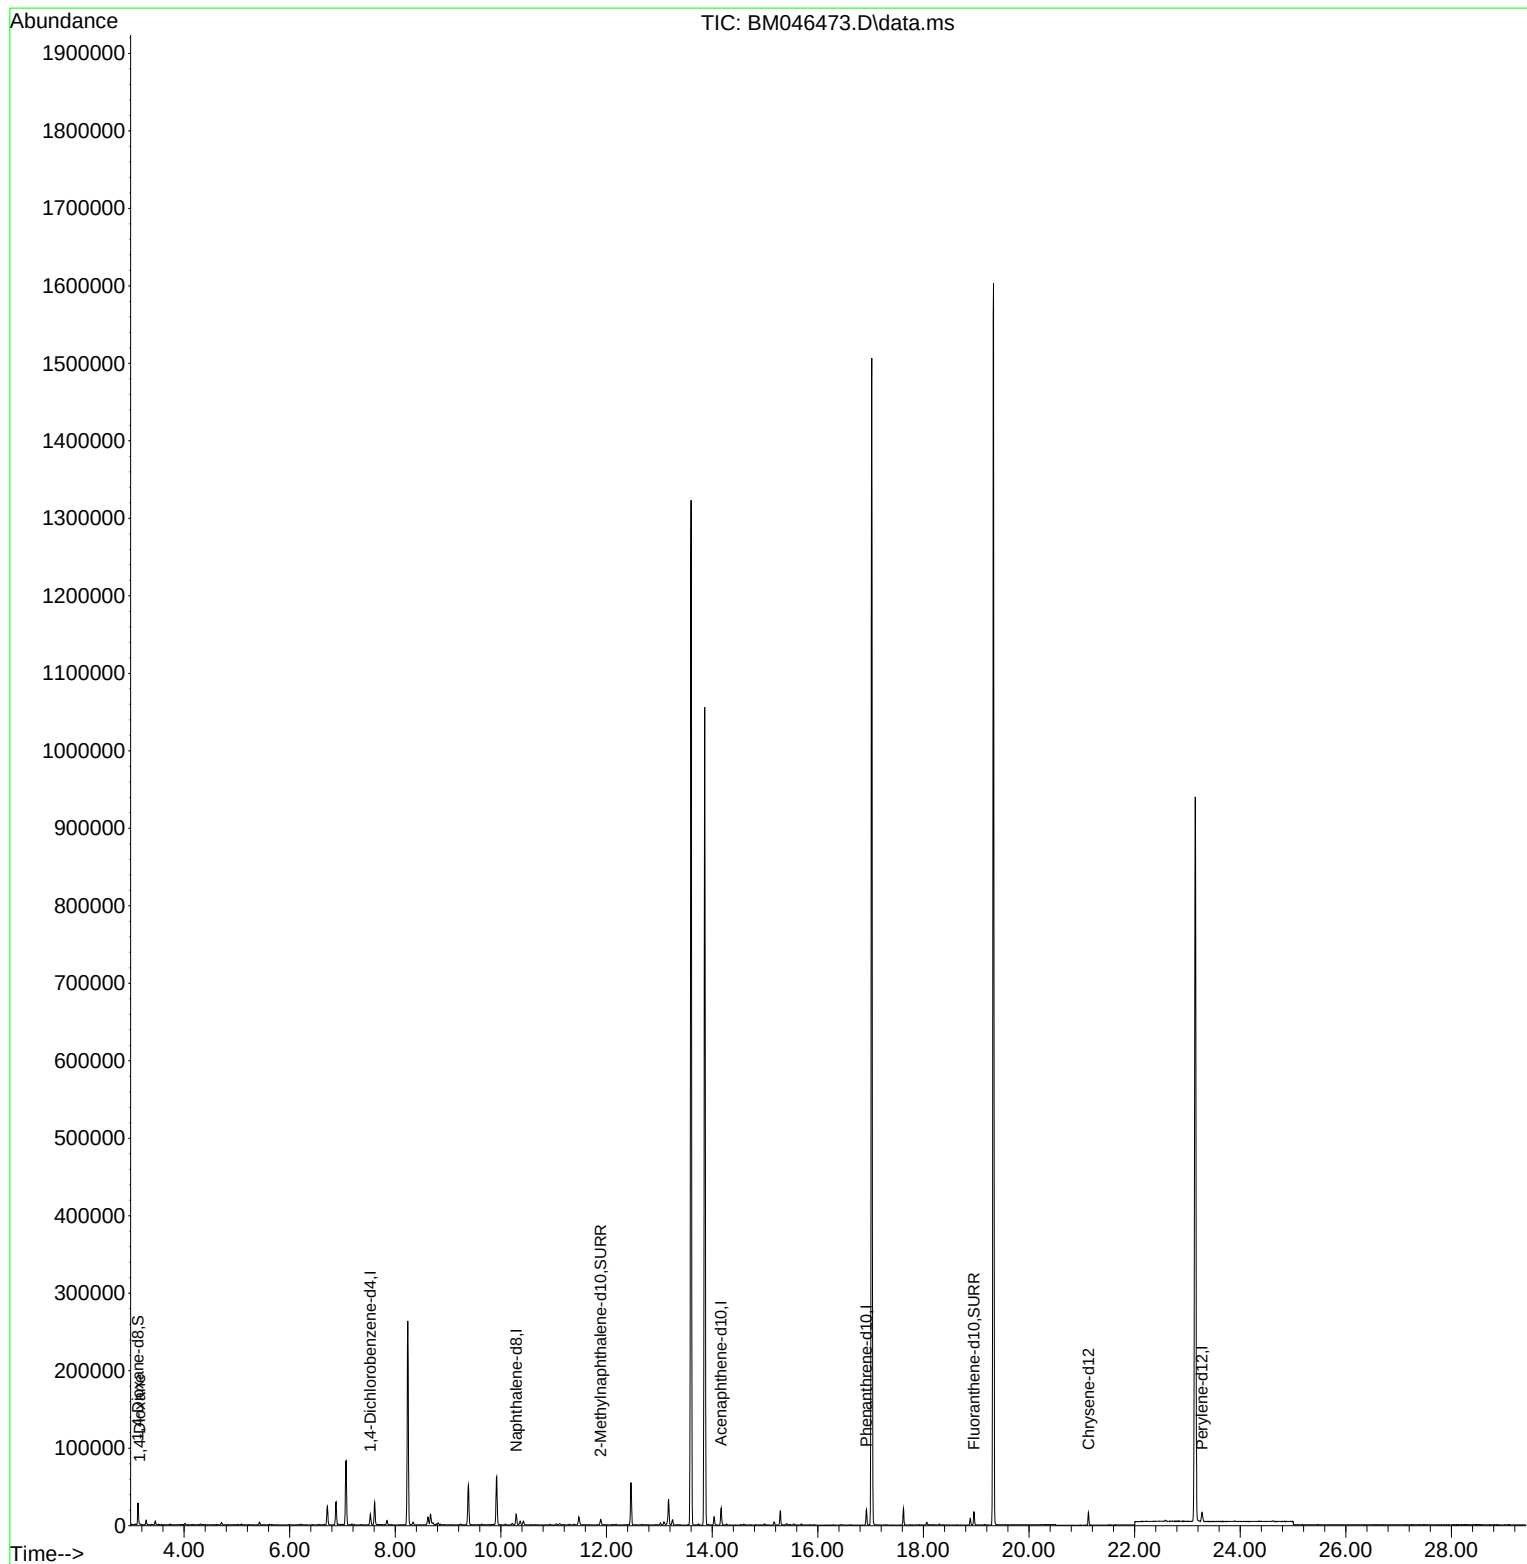

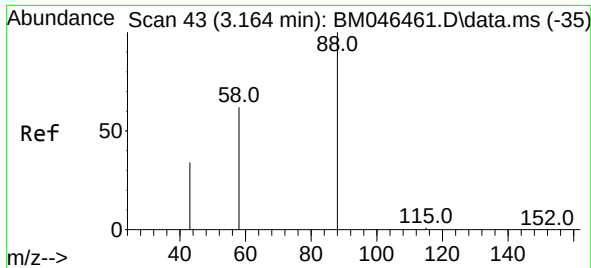

#2
 1,4-Dioxane
 Concen: 0.045 ng/ul
 RT: 3.159 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BM046473.D
 Acq: 09 Jul 2024 14:24

Instrument :
 BNA_M
 ClientSampleId :
 E1GP4

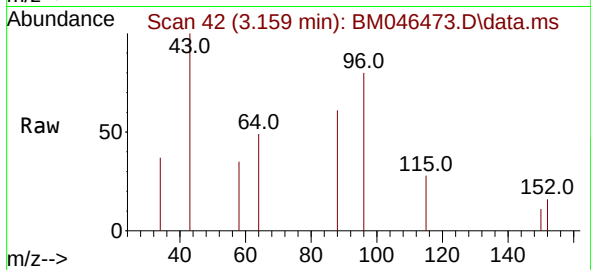

Tgt Ion: 88 Resp: 335

Ion	Ratio	Lower	Upper
88	100		
43	164.9	41.9	62.9
58	58.0	56.5	84.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/09/2024
 Supervised By :mohammad ahmed 07/10/2024

