

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070824\
 Data File : BM046484.D
 Acq On : 09 Jul 2024 21:49
 Operator : MA/JU
 Sample : P3084-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GE3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/10/2024
 Supervised By :mohammad ahmed 07/10/2024

Quant Time: Jul 10 00:47:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 09 08:09:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	4314	0.400	ng/ul	0.00
4) Naphthalene-d8	10.287	136	11860	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.168	164	8251	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.917	188	18533m	0.400	ng/ul	0.00
17) Chrysene-d12	21.123	240	14004	0.400	ng/ul	# 0.00
23) Perylene-d12	23.271	264	13817m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	16366	3.673	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.887	152	7727	0.441	ng/ul	0.00
18) Fluoranthene-d10	18.955	212	18891	0.385	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.336	128	11714	0.372	ng/ul	100
7) 2-Methylnaphthalene	11.964	142	3725	0.175	ng/ul	98
8) 1-Methylnaphthalene	12.184	142	2666	0.122	ng/ul	99
15) Phenanthrene	16.959	178	1772	0.032	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070824\
Data File : BM046484.D
Acq On : 09 Jul 2024 21:49
Operator : MA/JU
Sample : P3084-04
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E1GE3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/10/2024
Supervised By :mohammad ahmed 07/10/2024


Quant Time: Jul 10 00:47:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 08:09:14 2024
Response via : Initial Calibration

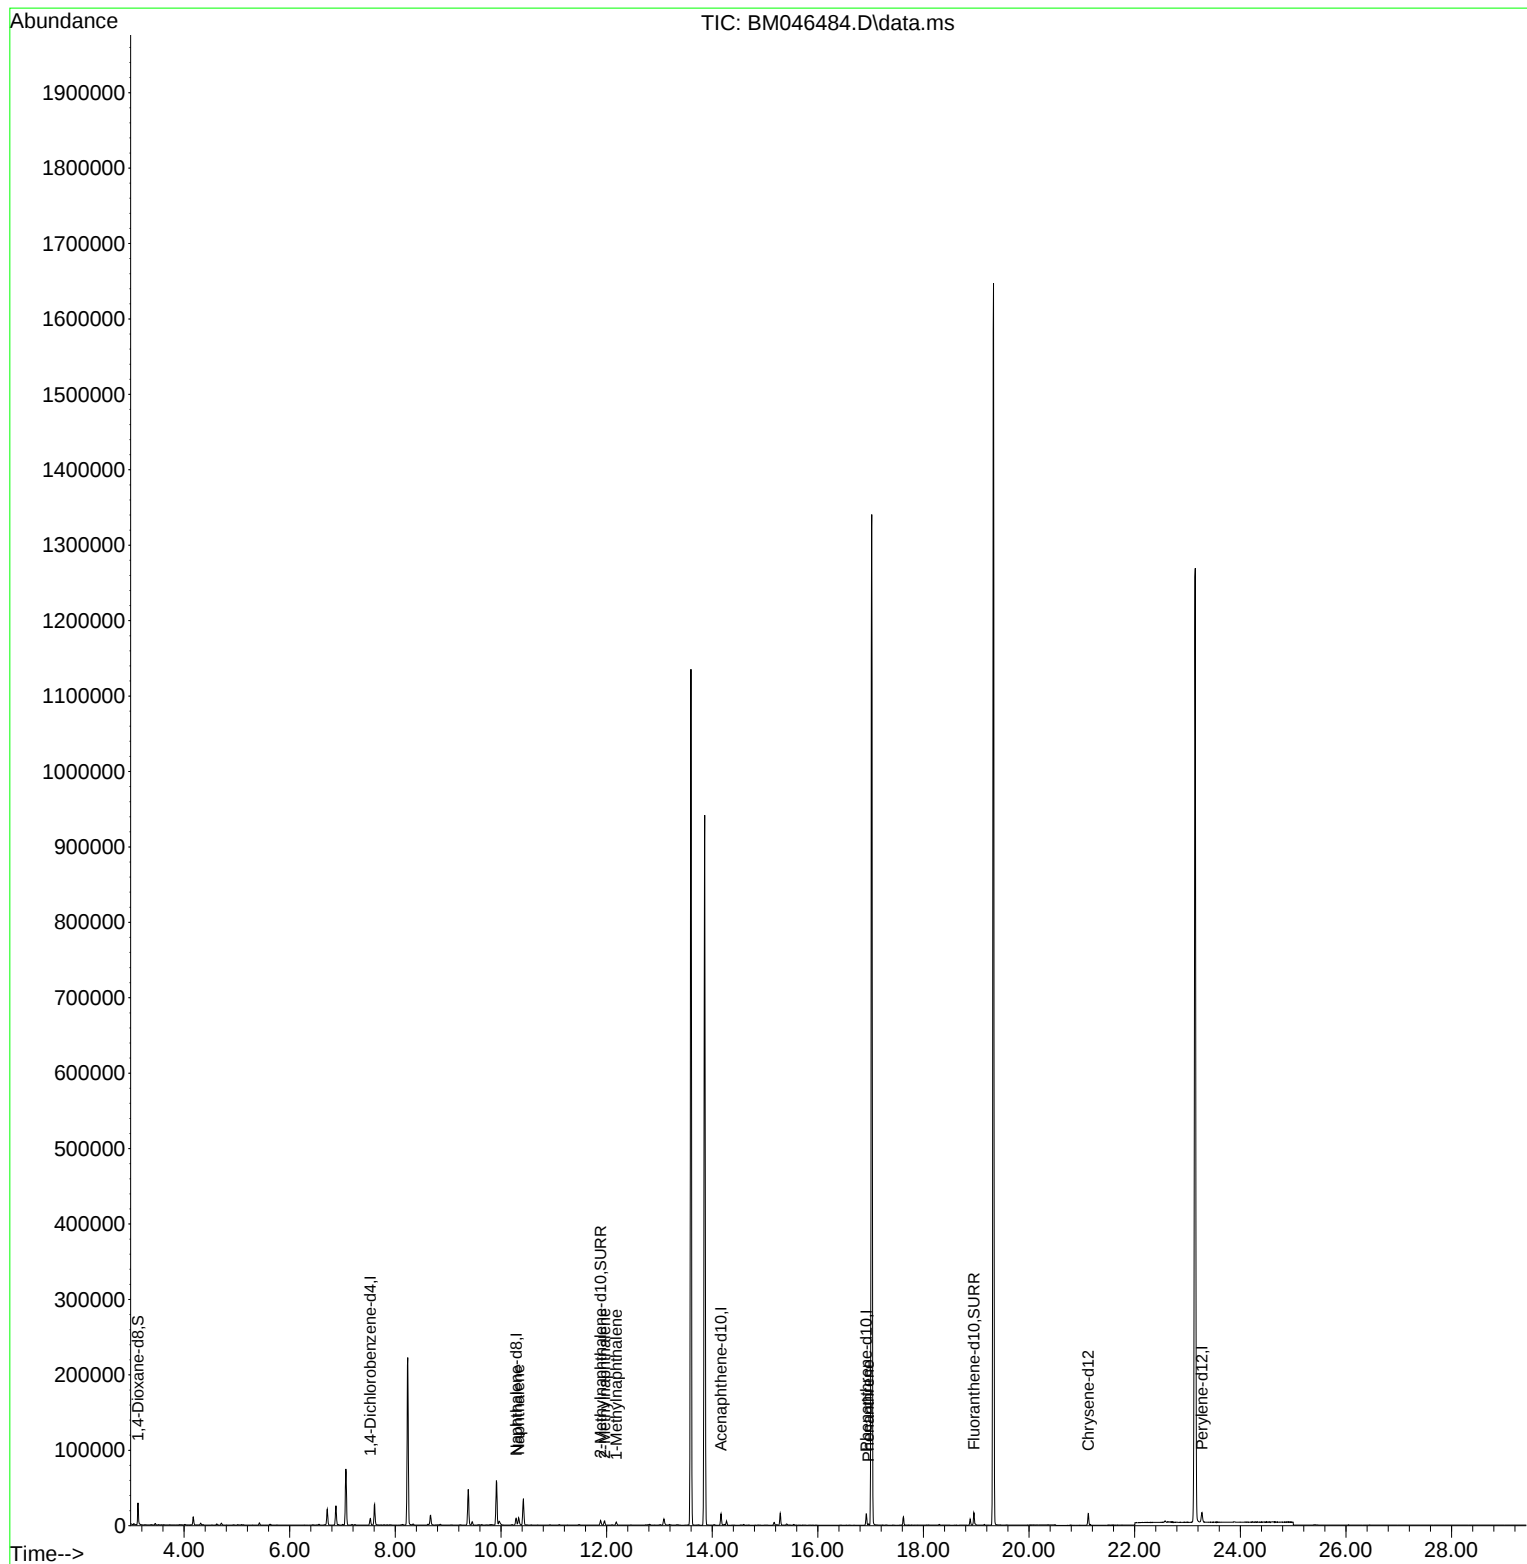

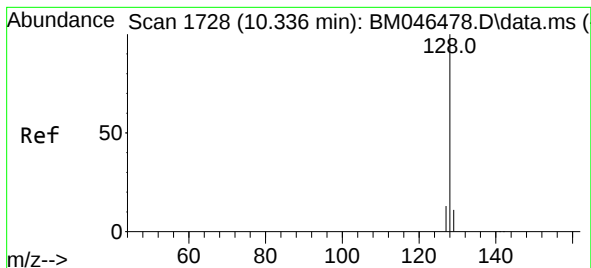

#5
Naphthalene
Concen: 0.372 ng/ul
RT: 10.336 min Scan# 1728
Delta R.T. -0.005 min
Lab File: BM046484.D
Acq: 09 Jul 2024 21:49




Instrument :
BNA_M
ClientSampleId :
E1GE3

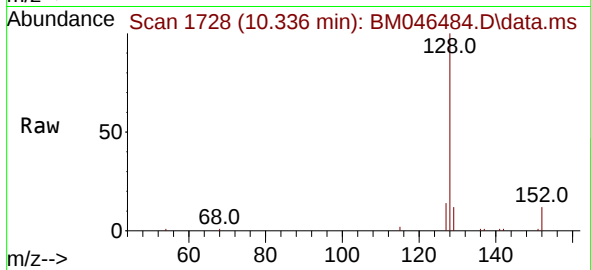

Tgt Ion:128 Resp: 11714
Ion Ratio Lower Upper
128 100
129 11.6 9.4 14.0
127 13.6 10.8 16.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/10/2024
Supervised By :mohammad ahmed 07/10/2024

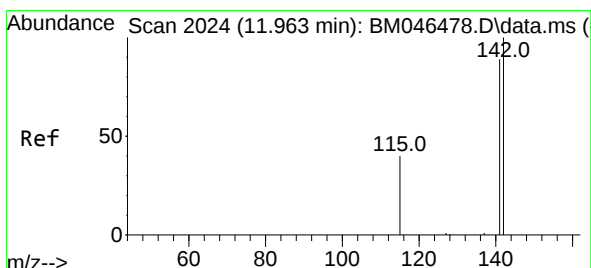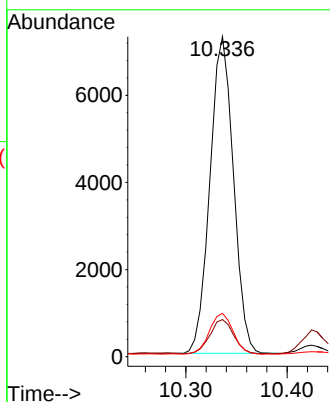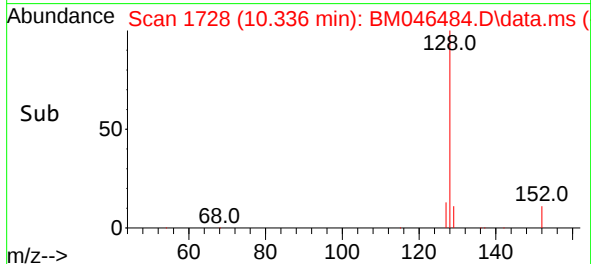

#7
2-Methylnaphthalene
Concen: 0.175 ng/ul
RT: 11.964 min Scan# 2024
Delta R.T. 0.000 min
Lab File: BM046484.D
Acq: 09 Jul 2024 21:49

Tgt Ion:142 Resp: 3725
Ion Ratio Lower Upper
142 100
141 89.2 69.8 104.6

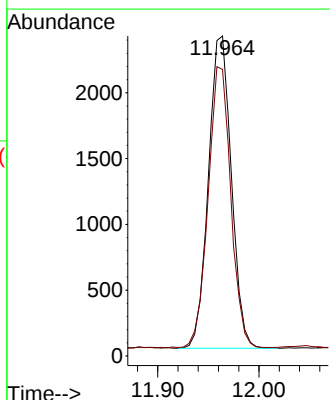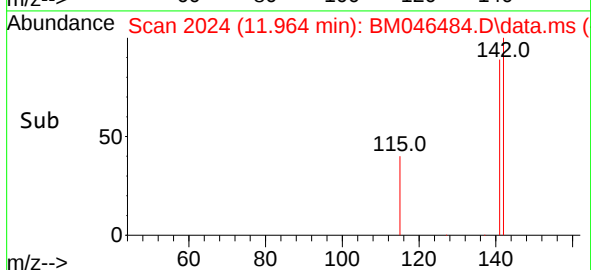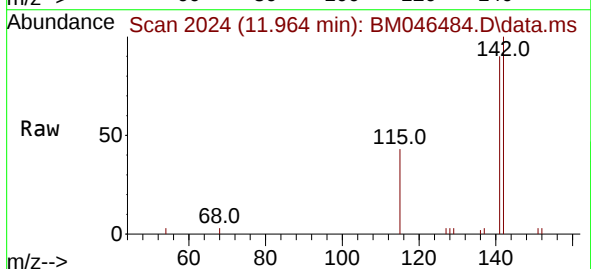

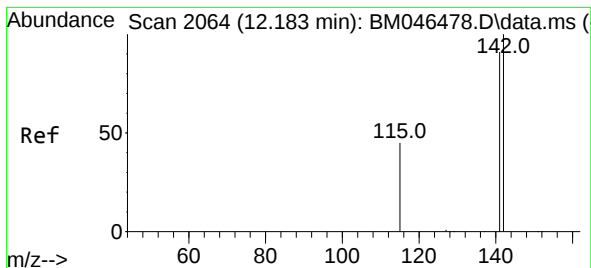

#8

1-Methylnaphthalene

Concen: 0.122 ng/ul

RT: 12.184 min Scan# 2064

Delta R.T. -0.005 min

Lab File: BM046484.D

Acq: 09 Jul 2024 21:49

Instrument :

BNA_M

ClientSampleId :

E1GE3

Tgt Ion:142 Resp: 2660

Ion Ratio Lower Upper

142 100





141 91.2 72.4 108.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/10/2024

Supervised By :mohammad ahmed 07/10/2024

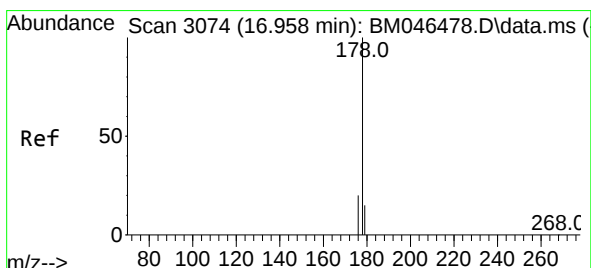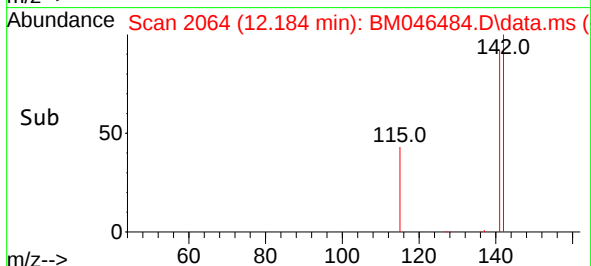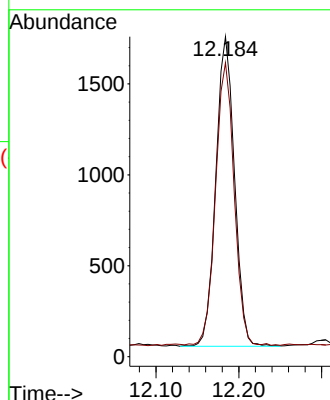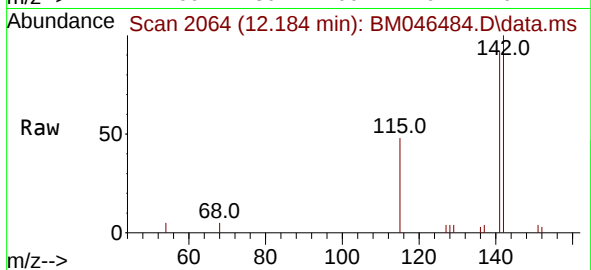

#15

Phenanthrene

Concen: 0.032 ng/ul

RT: 16.959 min Scan# 3074

Delta R.T. -0.004 min

Lab File: BM046484.D

Acq: 09 Jul 2024 21:49

Tgt Ion:178 Resp: 1772

Ion Ratio Lower Upper

178 100

179 19.6 12.7 19.1#

176 23.2 16.0 24.0

