

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070915\
 Data File : BM001888.D
 Acq On : 09 Jul 2015 18:38
 Operator : TP/UM
 Sample : G2860-04DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G93H9DL

Quant Time: Jul 10 05:16:37 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 10 05:15:13 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	34613	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	152888	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	97674	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	227490	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	265053	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	270923	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	1404	1.93	ng/uL	0.00
5) Phenol-d5	6.83	99	30113	11.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	17635	11.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	25050	11.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	20061	9.40	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	11771	11.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	13669	11.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	25298	10.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	19714	7.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	72110	9.96	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	81487	8.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	9491	7.10	ng/ul	0.00
57) Fluorene-d10	15.32	176	56836	8.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	5159	3.71	ng/ul	0.00
70) Anthracene-d10	17.17	188	91116	8.60	ng/ul	0.00
78) Pyrene-d10	19.47	212	86728	7.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	85631	7.17	ng/ul	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	2.88	88	5746	6.93	ng/uL#	1
6) Phenol	6.86	94	3912	1.43	ng/ul#	90
14) Acetophenone	8.49	105	20029	5.91	ng/ul	99
28) Naphthalene	10.50	128	34389	4.45	ng/ul	99
34) 2-Methylnaphthalene	12.12	142	8338	1.49	ng/ul	88
44) Dimethylphthalate	13.77	163	21472	2.71	ng/ul	99
47) Acenaphthylene	14.04	152	37678	3.89	ng/ul	97
49) Acenaphthene	14.38	153	25043	3.87	ng/ul	94
53) Dibenzofuran	14.72	168	25997	2.81	ng/ul	98
58) Fluorene	15.37	166	30848	4.00	ng/ul	99
69) Phenanthrene	17.11	178	619523	50.22	ng/ul	99
71) Anthracene	17.20	178	126690	10.00	ng/ul	99
74) Carbazole	17.47	167	39851	3.59	ng/ul	97
76) Fluoranthene	19.13	202	1056738	71.63	ng/ul	99
79) Pyrene	19.50	202	1049887	71.40	ng/ul	99
82) Benzo(a)anthracene	21.24	228	500382	32.31	ng/ul	97
84) Chrysene	21.30	228	483275	32.92	ng/ul	97
87) Benzo(b)fluoranthene	22.83	252	648796	41.14	ng/ul	99
88) Benzo(k)fluoranthene	22.83	252	247634	16.25	ng/ul	98
90) Benzo(a)pyrene	23.40	252	445852	29.06	ng/ul	99
91) Indeno(1,2,3-cd)pyrene	25.74	276	309415	17.01	ng/ul#	95
92) Dibenzo(a,h)anthracene	25.74	278	75502	4.92	ng/ul#	87
93) Benzo(g,h,i)perylene	26.43	276	145348	9.50	ng/ul	99

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070915\
Data File : BM001888.D
Acq On : 09 Jul 2015 18:38
Operator : TP/UM
Sample : G2860-04DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G93H9DL

Quant Time: Jul 10 05:16:37 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 10 05:15:13 2015
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070915\
Data File : BM001888.D
Acq On : 09 Jul 2015 18:38
Operator : TP/UM
Sample : G2860-04DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G93H9DL

Quant Time: Jul 10 05:16:37 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 10 05:15:13 2015
Response via : Initial Calibration

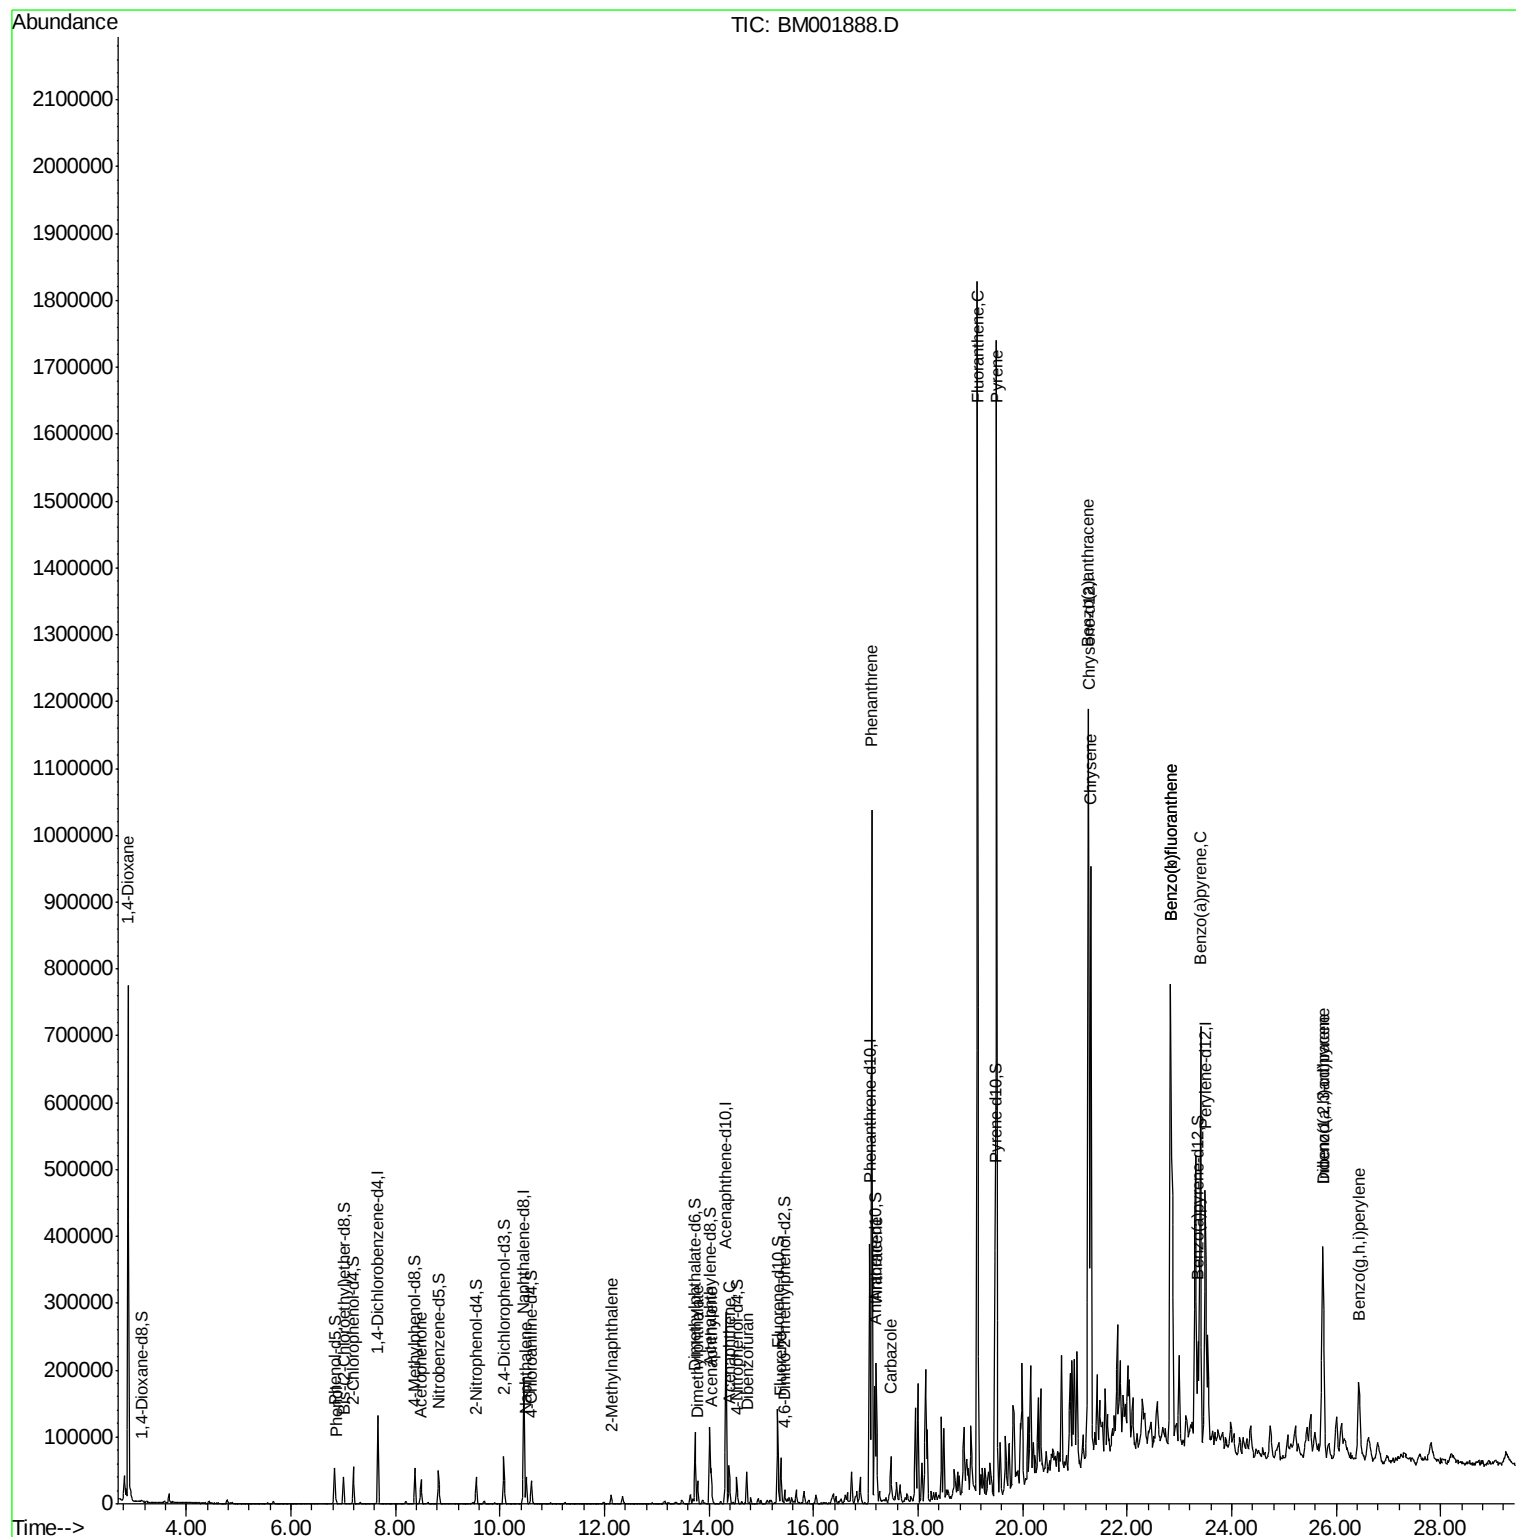



#2

1,4-Dioxane

Concen: 6.93 ng/uL

RT: 2.88 min Scan# 33

Delta R.T. -0.29 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38

Instrument :

BNA_M

ClientSampleId :

G93H9DL


Tgt Ion: 88 Resp: 5746

Ion Ratio Lower Upper

88 100

43 2361.2 24.2 36.4#




58 29.3 56.2 84.2#

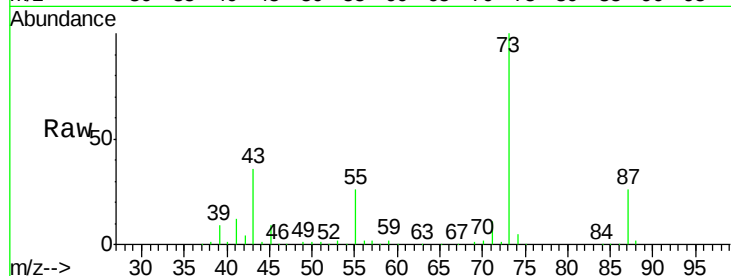

Abundance Ion 88.00 (87.70 to 88.70): BM001888.D (-1) (-)

Ion 43.00 (42.70 to 43.70): BM001888.D (-1) (-)

Ion 58.00 (57.70 to 58.70): BM001888.D (-1) (-)

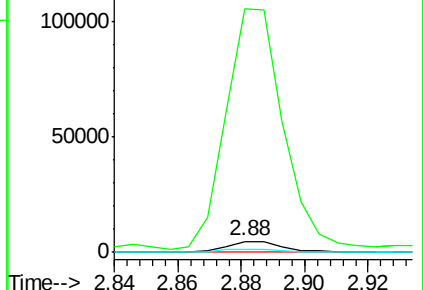

#6

Phenol

Concen: 1.43 ng/uL

RT: 6.86 min Scan# 710

Delta R.T. 0.01 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38


Tgt Ion: 94 Resp: 3912

Ion Ratio Lower Upper

94 100

65 30.7 26.1 39.1



66 34.8 35.9 53.9#




Abundance Ion 94.00 (93.70 to 94.70): BM001888.D (-675) (-)

Ion 65.00 (64.70 to 65.70): BM001888.D (-675) (-)

Ion 66.00 (65.70 to 66.70): BM001888.D (-675) (-)



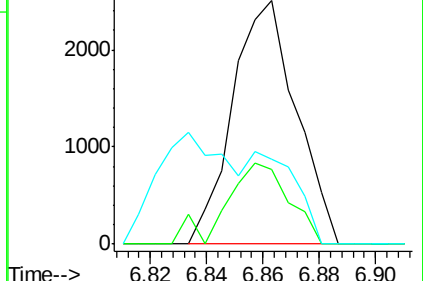





#14
Acetophenone
Concen: 5.91 ng/ul
RT: 8.49 min Scan# 986
Delta R.T. 0.00 min
Lab File: BM001888.D
Acq: 09 Jul 2015 18:38




Instrument :
BNA_M
ClientSampleId :
G93H9DL


Tgt Ion:105 Resp: 20029
Ion Ratio Lower Upper
105 100
77 80.5 64.2 96.4
51 25.7 22.0 33.0

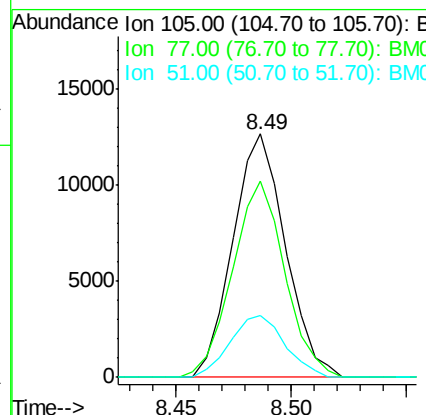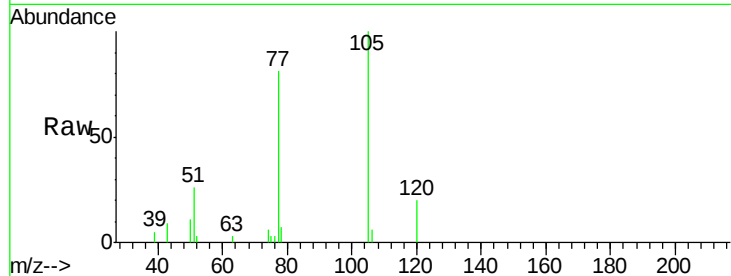

#28
Naphthalene
Concen: 4.45 ng/ul
RT: 10.50 min Scan# 1329
Delta R.T. 0.00 min
Lab File: BM001888.D
Acq: 09 Jul 2015 18:38

Tgt Ion:128 Resp: 34389
Ion Ratio Lower Upper
128 100
129 10.5 8.7 13.1
127 12.7 10.0 15.0



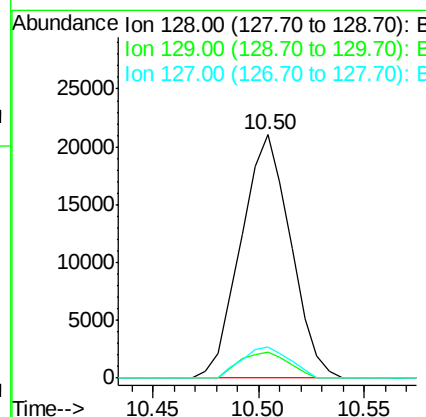
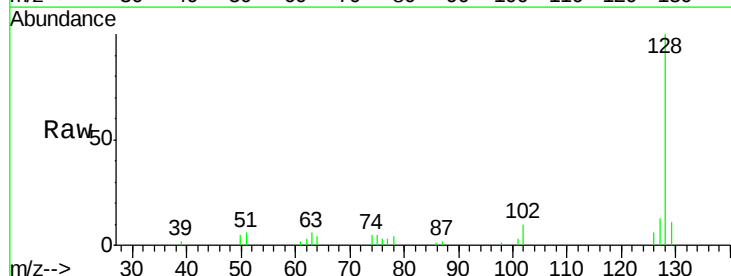




#34
 2-Methylnaphthalene
 Concen: 1.49 ng/ul
 RT: 12.12 min Scan# 1604
 Delta R.T. 0.00 min
 Lab File: BM001888.D
 Acq: 09 Jul 2015 18:38




Instrument :
 BNA_M
 ClientSampleId :
 G93H9DL


Tgt Ion:142 Resp: 8338
 Ion Ratio Lower Upper
 142 100
 141 78.6 71.6 107.4

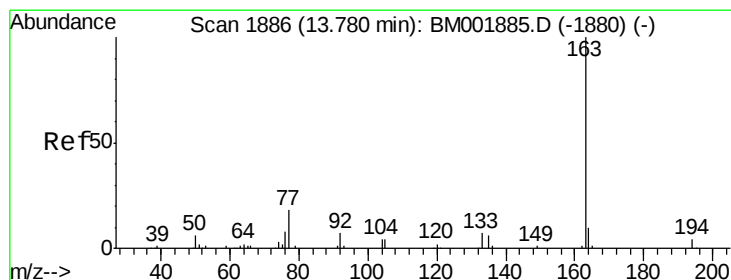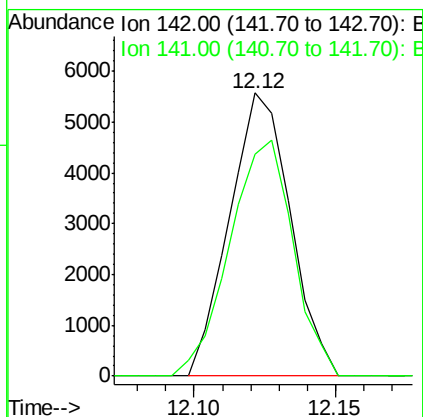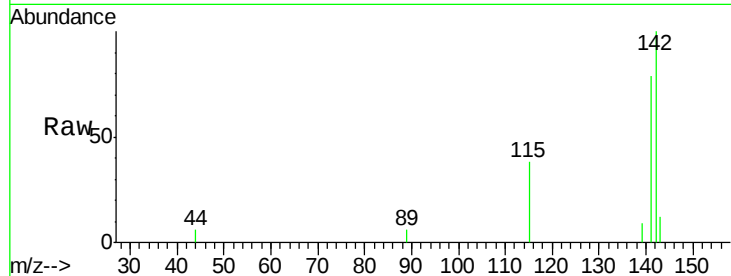

#44
 Dimethylphthalate
 Concen: 2.71 ng/ul
 RT: 13.77 min Scan# 1885
 Delta R.T. -0.01 min
 Lab File: BM001888.D
 Acq: 09 Jul 2015 18:38

Tgt Ion:163 Resp: 21472
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.6 5.4
 164 9.7 8.0 12.0

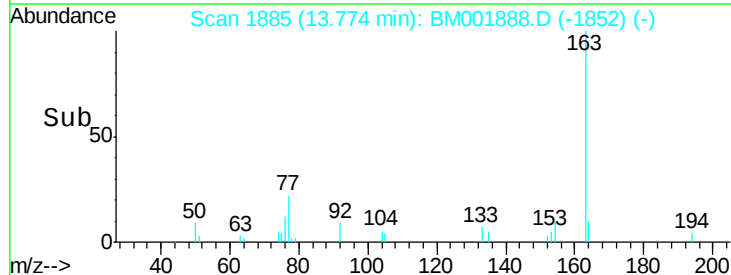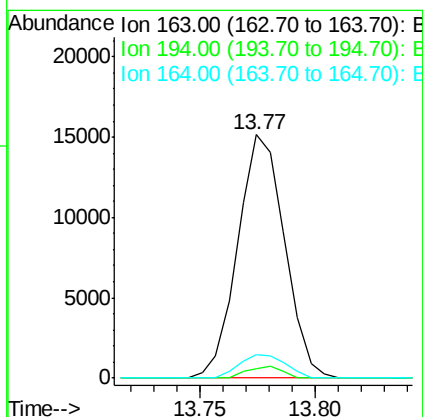



#47

Acenaphthylene

Concen: 3.89 ng/ul

RT: 14.04 min Scan# 1930

Delta R.T. 0.00 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38

Instrument :

BNA_M

ClientSampleId :

G93H9DL





Tgt Ion:152 Resp: 37678

Ion Ratio Lower Upper

152 100

151 18.7 15.9 23.9

153 13.8 10.0 15.0

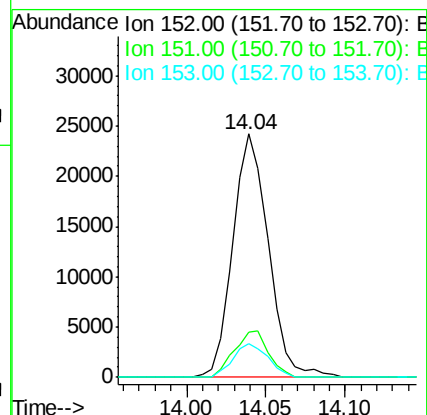

#49

Acenaphthene

Concen: 3.87 ng/ul

RT: 14.38 min Scan# 1988

Delta R.T. -0.01 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38




Tgt Ion:153 Resp: 25043


Ion Ratio Lower Upper

153 100

152 41.9 36.6 55.0

154 85.6 72.6 108.8


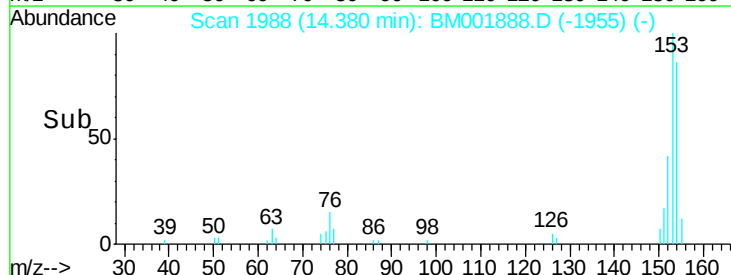
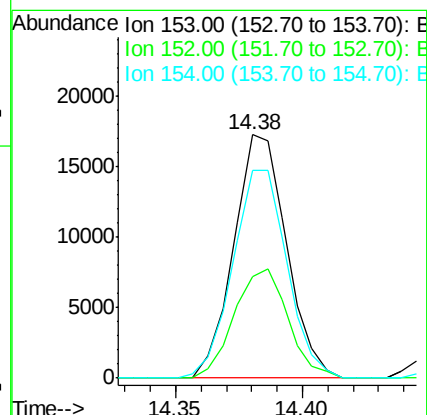





#53
Dibenzenofuran
Concen: 2.81 ng/ul
RT: 14.72 min Scan# 2046
Delta R.T. 0.00 min
Lab File: BM001888.D
Acq: 09 Jul 2015 18:38




Instrument :
BNA_M
ClientSampleId :
G93H9DL


Tgt Ion:168 Resp: 25997
Ion Ratio Lower Upper
168 100
139 36.3 30.1 45.1

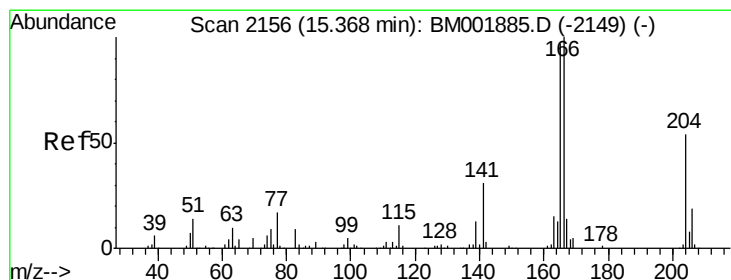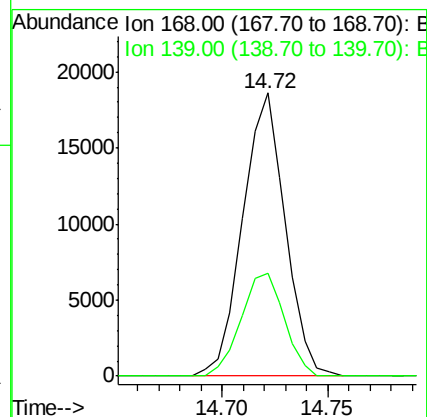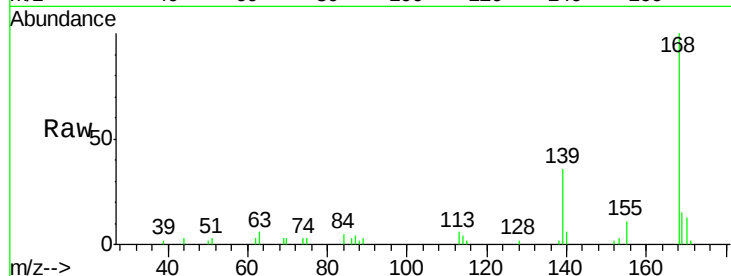

#58
Fluorene
Concen: 4.00 ng/ul
RT: 15.37 min Scan# 2156
Delta R.T. 0.00 min
Lab File: BM001888.D
Acq: 09 Jul 2015 18:38

Tgt Ion:166 Resp: 30848
Ion Ratio Lower Upper
166 100
165 96.8 77.4 116.2
167 15.9 11.3 16.9

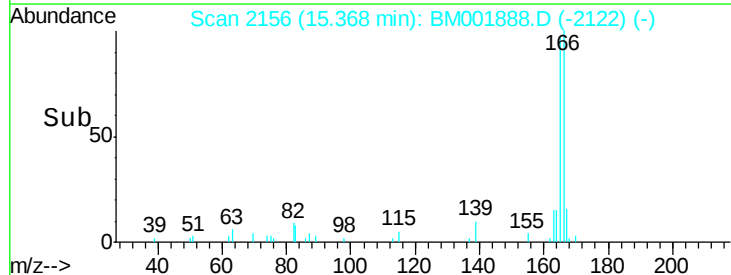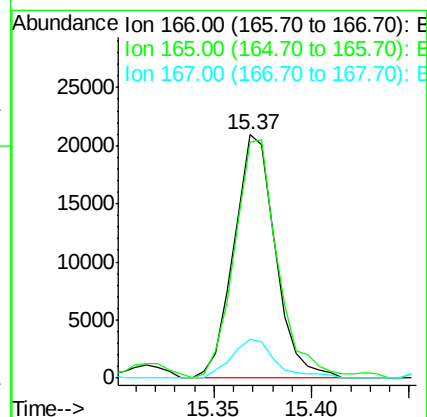



#69

Phenanthrene

Concen: 50.22 ng/u1

RT: 17.11 min Scan# 2452

Delta R.T. 0.00 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38

Instrument :

BNA_M

ClientSampleId :

G93H9DL


Tgt Ion:178 Resp: 619523

Ion Ratio Lower Upper

178 100

179 15.4 11.9 17.9




176 18.4 15.2 22.8



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

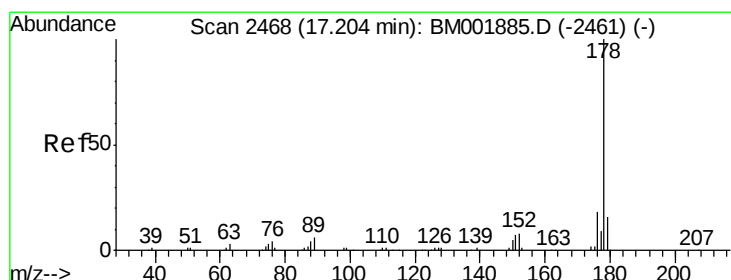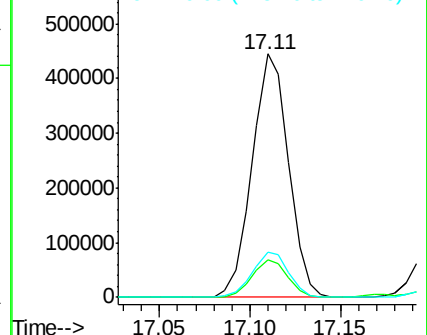

#71

Anthracene

Concen: 10.00 ng/u1

RT: 17.20 min Scan# 2467

Delta R.T. -0.01 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38


Tgt Ion:178 Resp: 126690

Ion Ratio Lower Upper

178 100

179 15.7 11.8 17.8



176 18.0 14.4 21.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



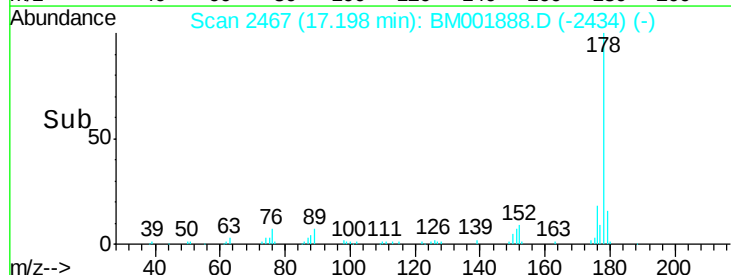
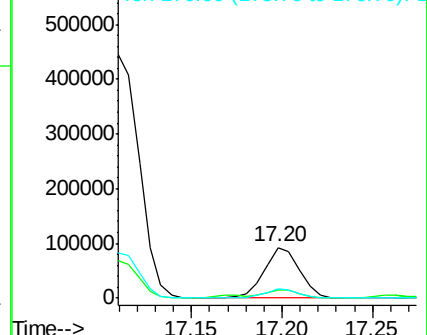




#74
 Carbazole
 Concen: 3.59 ng/ul
 RT: 17.47 min Scan# 2514
 Delta R.T. 0.00 min
 Lab File: BM001888.D
 Acq: 09 Jul 2015 18:38




Instrument :
 BNA_M
 ClientSampleId :
 G93H9DL


Tgt Ion:167 Resp: 39851
 Ion Ratio Lower Upper
 167 100
 166 20.4 17.4 26.2
 139 11.1 10.1 15.1

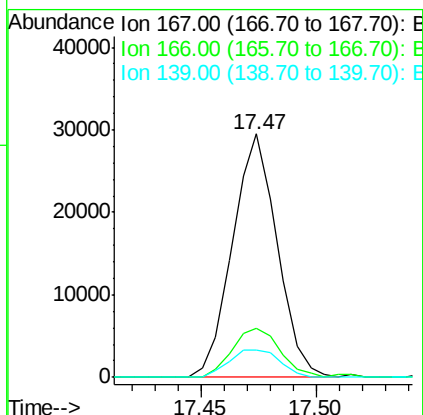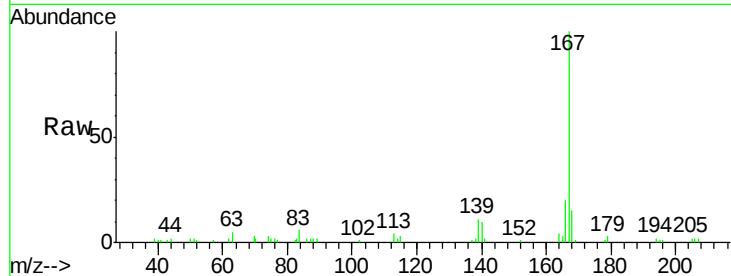

#76
 Fluoranthene
 Concen: 71.63 ng/ul
 RT: 19.13 min Scan# 2796
 Delta R.T. 0.00 min
 Lab File: BM001888.D
 Acq: 09 Jul 2015 18:38

Tgt Ion:202 Resp: 1056738
 Ion Ratio Lower Upper
 202 100
 101 8.0 6.1 9.1
 100 6.0 4.8 7.2



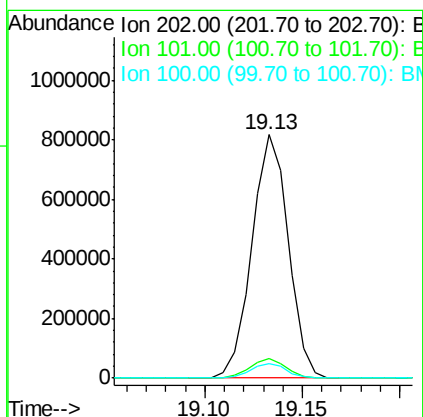





#79
 Pyrene
 Concen: 71.40 ng/ul
 RT: 19.50 min Scan# 2858
 Delta R.T. 0.00 min
 Lab File: BM001888.D
 Acq: 09 Jul 2015 18:38




Instrument :
 BNA_M
 ClientSampleId :
 G93H9DL


Tgt Ion:202 Resp: 1049887
 Ion Ratio Lower Upper
 202 100
 101 9.1 6.9 10.3
 100 7.9 6.2 9.2

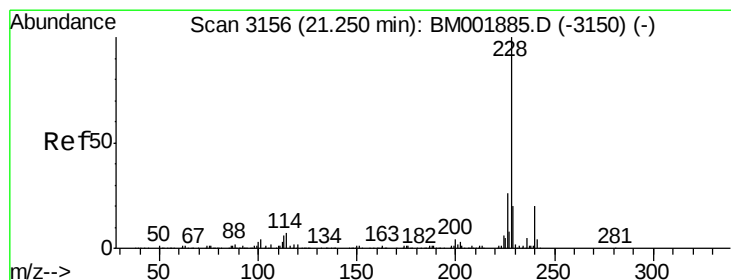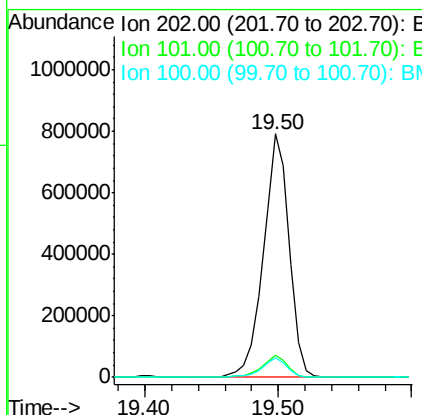

#82
 Benzo(a)anthracene
 Concen: 32.31 ng/ul
 RT: 21.24 min Scan# 3155
 Delta R.T. -0.01 min
 Lab File: BM001888.D
 Acq: 09 Jul 2015 18:38

Tgt Ion:228 Resp: 500382
 Ion Ratio Lower Upper
 228 100
 229 20.4 15.4 23.0
 226 27.3 20.6 30.8

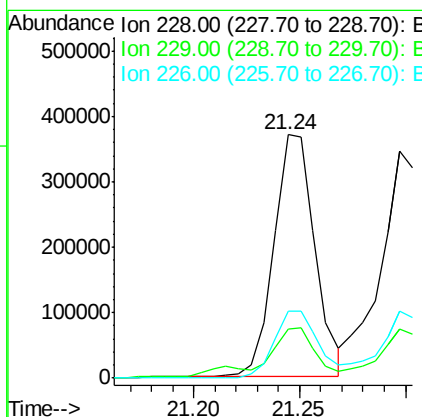



#84

Chrysene

Concen: 32.92 ng/ul

RT: 21.30 min Scan# 3164

Delta R.T. -0.01 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38

Instrument :

BNA_M

ClientSampleId :

G93H9DL


Tgt Ion:228 Resp: 483275

Ion Ratio Lower Upper

228 100

226 29.4 23.0 34.4




229 21.4 15.4 23.2

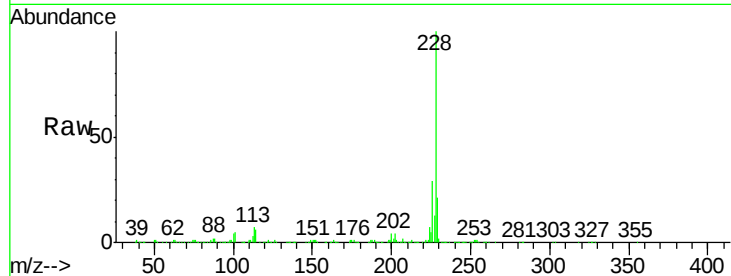

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

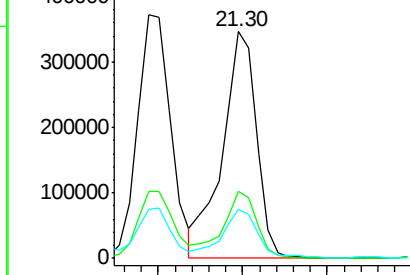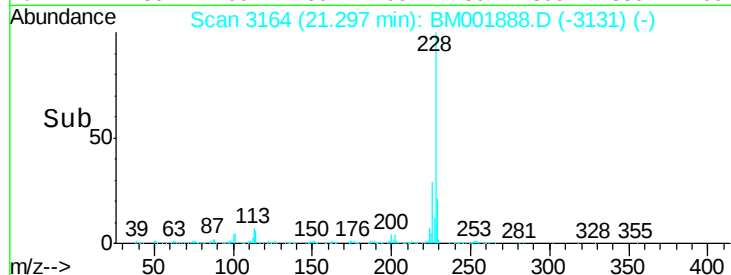

#87

Benzo(b)fluoranthene

Concen: 41.14 ng/ul

RT: 22.83 min Scan# 3424

Delta R.T. 0.01 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38


Tgt Ion:252 Resp: 648796

Ion Ratio Lower Upper

252 100

253 22.2 17.8 26.6



125 7.6 5.3 7.9




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



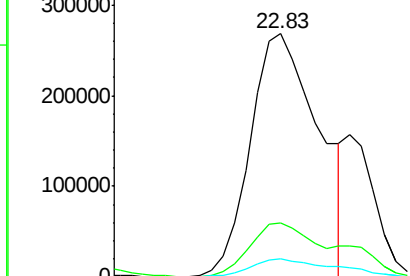





#88
Benzo(k)fluoranthene
Concen: 16.25 ng/ul
RT: 22.83 min Scan# 3424
Delta R.T. -0.04 min
Lab File: BM001888.D
Acq: 09 Jul 2015 18:38




Instrument :
BNA_M
ClientSampleId :
G93H9DL


Tgt Ion:252 Resp: 247634
Ion Ratio Lower Upper
252 100
253 22.2 17.1 25.7
125 7.6 5.3 7.9

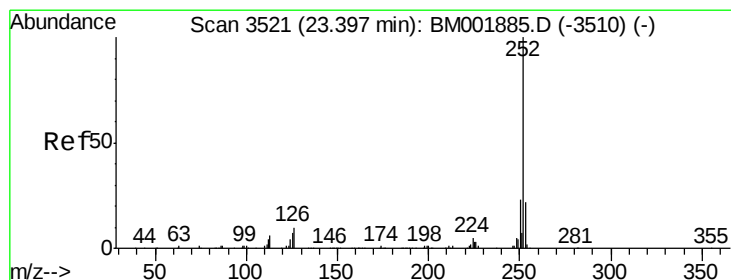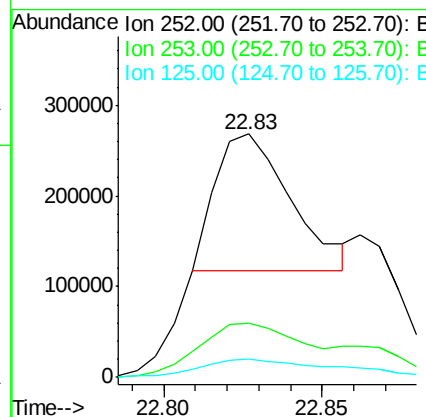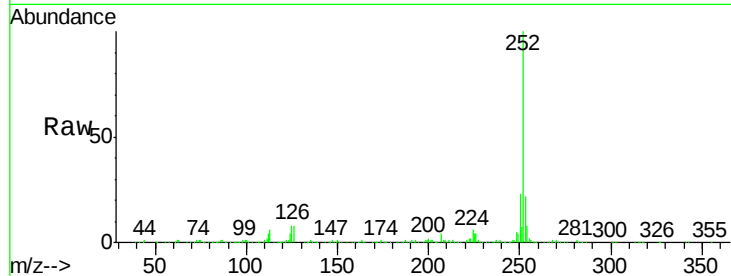

#90
Benzo(a)pyrene
Concen: 29.06 ng/ul
RT: 23.40 min Scan# 3521
Delta R.T. 0.00 min
Lab File: BM001888.D
Acq: 09 Jul 2015 18:38

Tgt Ion:252 Resp: 445852
Ion Ratio Lower Upper
252 100
253 22.4 17.4 26.0
125 7.9 6.0 9.0

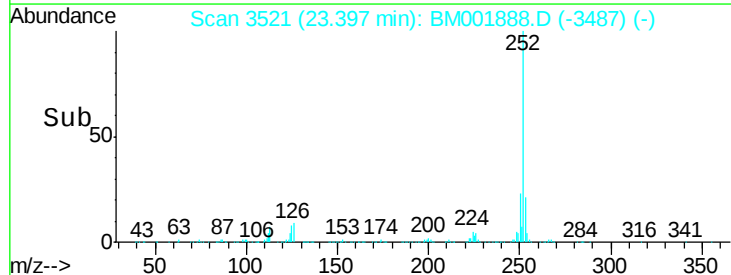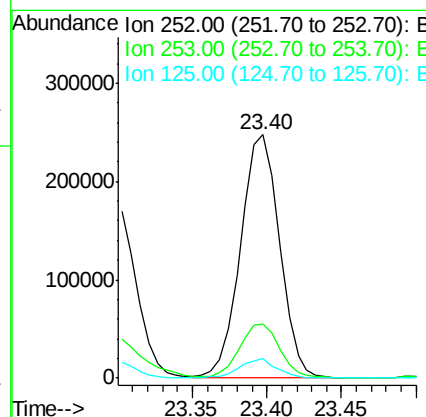

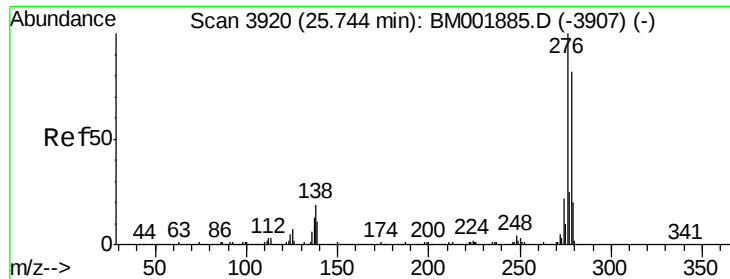

#91

Indeno(1,2,3-cd)pyrene

Concen: 17.01 ng/ul

RT: 25.74 min Scan# 3920

Delta R.T. 0.00 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38

Instrument :

BNA_M

ClientSampleId :

G93H9DL


Tgt Ion:276 Resp: 309415

Ion Ratio Lower Upper

276 100

138 14.2 14.7 22.1#




277 23.4 19.7 29.5

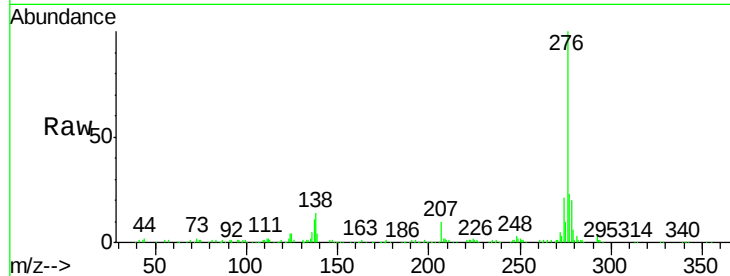

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

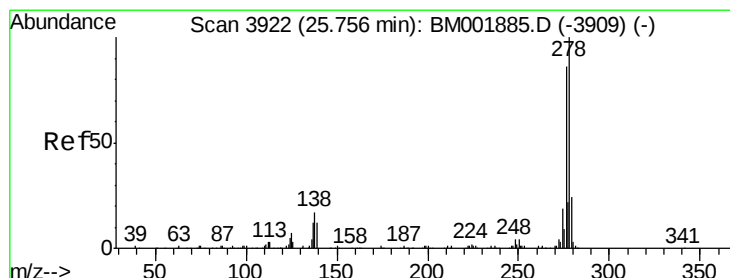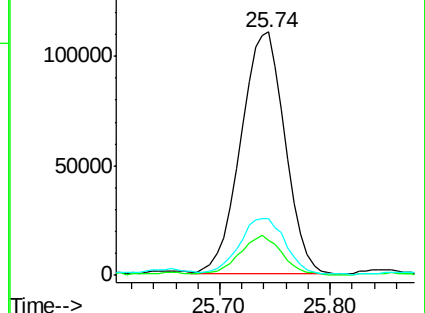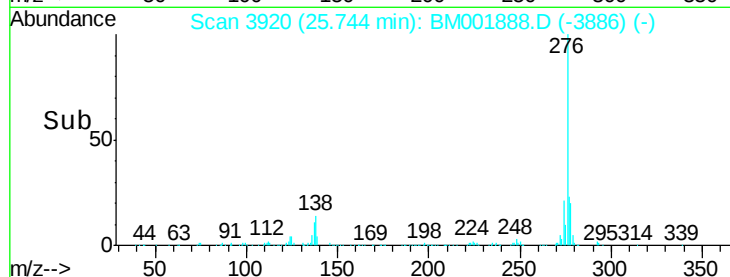

#92

Dibenzo(a,h)anthracene

Concen: 4.92 ng/ul

RT: 25.74 min Scan# 3919

Delta R.T. -0.02 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38


Tgt Ion:278 Resp: 75502

Ion Ratio Lower Upper

278 100

139 0.0 9.2 13.8#



279 26.3 19.1 28.7

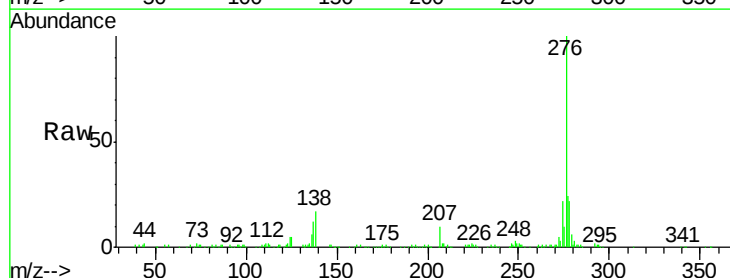


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

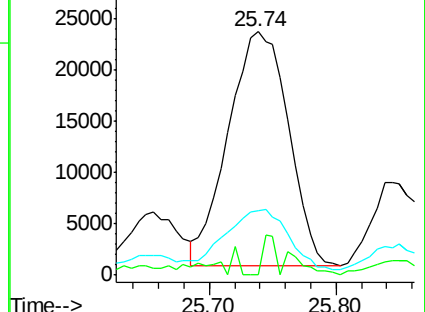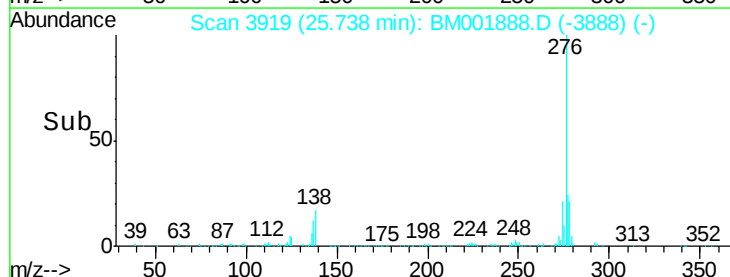



#93

Benzo(g,h,i)perylene

Concen: 9.50 ng/ul

RT: 26.43 min Scan# 4037

Delta R.T. 0.00 min

Lab File: BM001888.D

Acq: 09 Jul 2015 18:38

Instrument :

BNA_M

ClientSampleId :

G93H9DL

Tgt Ion: 276 Resp: 145348

Ion Ratio Lower Upper

276 100

138 16.7 12.6 19.0

277 23.8 18.7 28.1

