


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070915\
Data File : BM001884.D
Acq On : 09 Jul 2015 10:02
Operator : TP/UM
Sample : DFTPP70
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP70

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041515.M
Title : SVOA CALIBRATION
Last Update : Wed Apr 15 18:00:48 2015

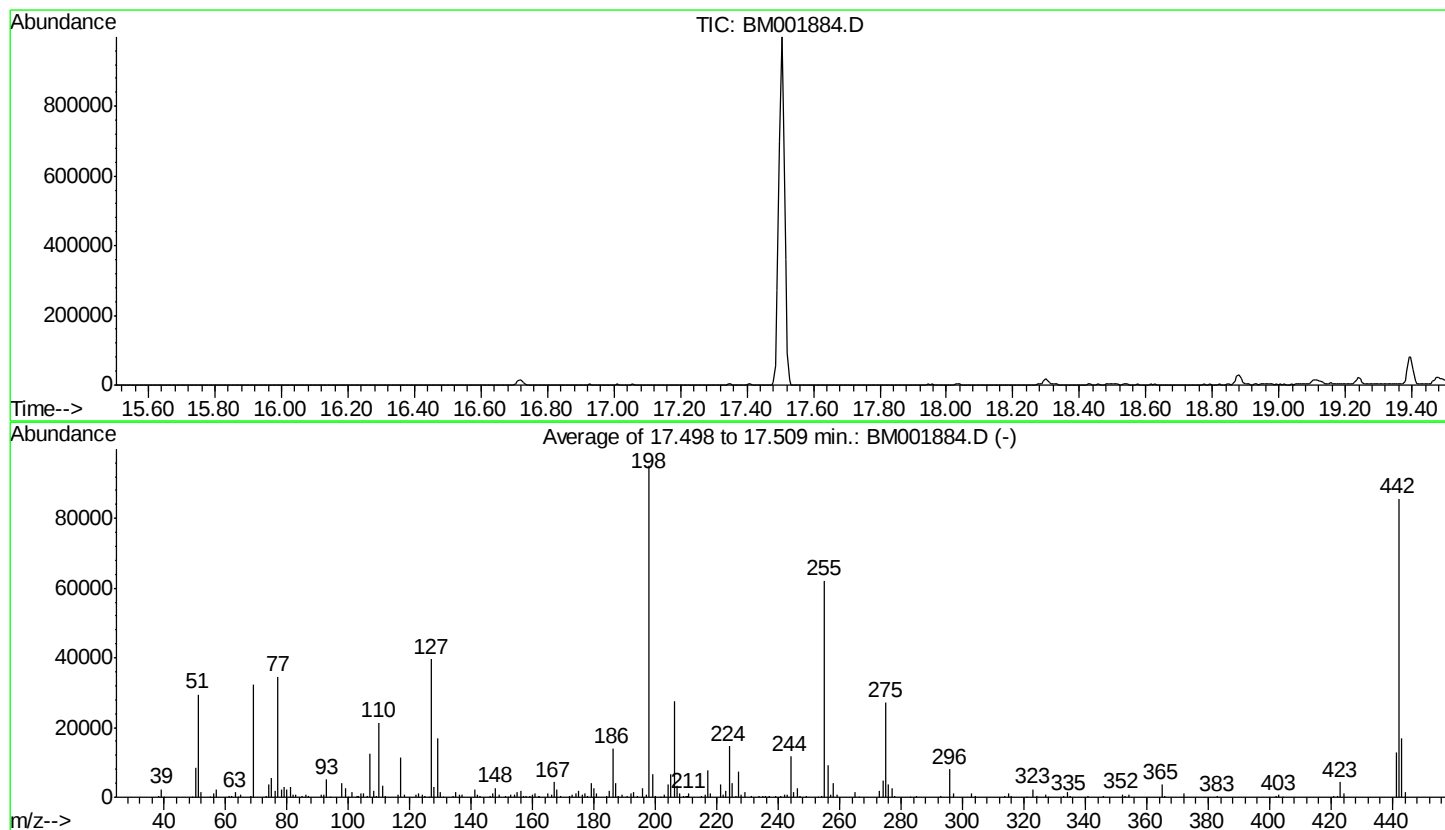

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	29560	PASS
68	69	0.00	2	1.3	431	PASS
69	198	0.00	100	33.9	32269	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.6	39584	PASS
197	198	0.00	2	0.7	691	PASS
198	198	100	100	100.0	95152	PASS
199	198	5	9	6.9	6555	PASS
275	198	10	60	28.5	27104	PASS
365	198	1	100	3.7	3542	PASS
441	443	0.01	100	76.1	12738	PASS
442	198	50	100	89.9	85586	PASS
443	442	15	24	19.6	16749	PASS

m/z	Abundance
38.00	408.0
39.10	2142.0
40.00	357.0
43.90	673.0
50.10	8382.0
51.10	29512.0
52.00	1564.0
55.90	950.0
57.00	1726.0
61.00	411.0
62.00	307.0
63.00	1400.0
64.10	311.0
65.00	562.0
69.00	31208.0
73.10	532.0
74.10	3463.0
75.00	5262.0
76.00	1759.0
77.10	33312.0
78.10	2416.0
79.00	2560.0
79.90	1985.0
81.00	2843.0
81.90	622.0
83.00	548.0
85.00	495.0
86.00	827.0
91.00	775.0
92.00	775.0
93.00	4598.0
98.00	3648.0
98.90	2884.0
101.00	1353.0
102.90	616.0
104.00	916.0
105.00	1084.0
105.90	324.0
107.00	11621.0
108.00	1771.0
109.00	348.0
110.00	20752.0
110.90	2711.0
112.10	320.0
116.00	914.0
117.00	10319.0
118.00	730.0
122.00	674.0
123.00	1184.0
124.00	541.0
125.00	447.0
127.00	35888.0
128.00	2904.0
129.00	15656.0
130.00	1234.0
134.00	572.0
135.00	1145.0
136.00	572.0
137.00	772.0
140.90	2177.0
141.90	502.0
142.90	344.0
146.00	554.0
146.90	1224.0
148.00	2369.0
149.00	495.0
151.10	337.0
153.00	740.0
154.00	483.0
154.90	1297.0
156.10	1759.0
157.10	343.0
158.00	389.0
160.00	448.0
161.00	862.0
162.00	321.0
164.90	836.0
166.00	622.0
167.00	3918.0
168.00	2114.0
169.00	448.0
171.80	504.0
173.00	521.0
173.90	1194.0
175.00	1865.0
176.00	528.0
176.90	1025.0
177.90	333.0
179.00	3571.0
180.00	2169.0
180.90	936.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

183.90	315.0
185.00	1636.0
186.00	11670.0
187.10	3520.0
189.00	682.0
190.90	461.0
192.00	950.0
193.00	1368.0
194.00	342.0
195.90	2449.0
197.10	626.0
198.00	82920.0
198.90	5372.0
200.00	559.0
202.90	755.0
204.00	2836.0
205.00	5336.0
206.10	23864.0
207.00	3462.0
208.00	849.0
209.90	410.0
210.90	835.0
214.90	412.0
216.00	583.0
217.00	6244.0
217.90	855.0
221.00	3397.0
223.00	1276.0
224.00	11459.0
225.00	3525.0
226.00	397.0
227.00	5984.0
227.90	791.0
228.90	1193.0
231.00	305.0
233.80	322.0
235.00	317.0
237.00	361.0
241.00	345.0
242.00	827.0
243.10	670.0
244.00	9267.0
245.10	1229.0
246.00	2115.0
247.00	399.0
254.10	375.0
255.00	49832.0
256.00	7365.0
256.90	552.0
258.10	2911.0
259.00	516.0
265.00	1377.0
266.00	339.0
272.90	1215.0
274.00	3909.0
275.00	21184.0
276.00	3189.0
277.00	2236.0
278.00	322.0
285.00	383.0
293.00	359.0
296.00	6148.0
297.00	837.0
302.90	722.0
313.90	338.0
314.90	722.0
316.00	450.0
323.00	1664.0
326.90	430.0
334.00	1179.0
346.00	543.0
352.00	522.0
353.00	513.0
354.00	692.0
365.00	2382.0
366.00	386.0
372.00	966.0
402.00	301.0
403.10	423.0
420.90	448.0
423.00	3079.0
424.00	620.0
441.10	7569.0
442.10	55504.0
443.10	10712.0
444.10	818.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

m/z	Abundance
38.00	453.0
39.00	2786.0
40.00	394.0
44.00	556.0
49.10	414.0
50.10	10551.0
51.10	35216.0
52.00	1770.0
55.00	356.0
56.00	1184.0
57.00	2657.0
61.00	439.0
61.90	507.0
63.10	1723.0
65.00	826.0
68.10	856.0
69.00	38240.0
73.00	492.0
74.10	4119.0
75.00	6287.0
76.10	2141.0
77.10	41904.0
78.00	2846.0
79.00	3555.0
80.00	2549.0
81.00	3314.0
82.00	718.0
83.00	789.0
85.00	642.0
86.00	1043.0
86.90	584.0
91.00	759.0
91.90	1083.0
93.00	5853.0
94.10	503.0
98.00	4615.0
99.00	2877.0
100.00	356.0
101.00	1761.0
103.10	644.0
104.00	1479.0
105.00	1412.0
106.00	396.0
107.00	15297.0
108.10	2051.0
109.10	558.0
110.00	25744.0
111.00	4150.0
111.90	337.0
116.10	1061.0
117.00	13674.0
118.10	865.0
122.00	1122.0
123.00	1308.0
123.90	718.0
125.10	637.0
127.00	49168.0
128.00	3617.0
129.00	20392.0
130.00	1639.0
130.90	353.0
134.00	586.0
135.00	1698.0
136.00	754.0
137.00	888.0
141.00	2918.0
142.00	1044.0
143.00	798.0
146.10	643.0
147.00	1393.0
148.00	3145.0
149.00	526.0
151.00	422.0
151.80	340.0
153.00	1117.0
153.90	809.0
155.00	1621.0
156.00	2502.0
157.00	558.0
158.00	543.0
159.00	530.0
159.90	917.0
160.90	1270.0
162.10	341.0
165.00	1097.0
166.00	949.0
167.00	5745.0
168.00	2820.0
168.90	478.0
171.90	512.0
172.90	720.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

174.00	1172.0
175.10	2193.0
176.00	818.0
177.00	1164.0
177.90	422.0
179.00	4492.0
180.00	3259.0
181.00	1391.0
184.00	329.0
185.00	2257.0
186.00	17000.0
187.00	4849.0
188.00	424.0
188.90	1214.0
190.90	504.0
192.00	1264.0
193.00	1524.0
196.00	3075.0
196.90	701.0
198.00	112280.0
199.00	7835.0
199.90	552.0
201.60	354.0
202.90	984.0
204.00	4481.0
205.00	7778.0
206.00	32320.0
207.00	4706.0
207.90	1311.0
209.00	515.0
210.30	630.0
210.90	1309.0
214.90	511.0
216.10	666.0
217.00	9155.0
217.90	1108.0
221.00	4404.0
221.90	1356.0
223.00	2107.0
224.00	17768.0
225.00	5031.0
226.00	527.0
227.00	8996.0
228.00	1180.0
228.90	1483.0
231.00	743.0
233.90	752.0
234.90	553.0
236.00	341.0
237.00	667.0
238.90	363.0
241.00	459.0
242.00	1205.0
243.00	998.0
244.10	14147.0
245.00	1989.0
246.00	3262.0
246.90	575.0
249.00	440.0
252.90	356.0
254.10	661.0
255.00	74192.0
256.00	10530.0
257.00	983.0
258.00	5041.0
259.00	781.0
265.00	1999.0
273.00	2200.0
274.00	6228.0
275.00	32912.0
276.00	4775.0
277.00	2971.0
277.80	519.0
283.00	328.0
285.00	564.0
293.00	705.0
296.00	9502.0
297.00	1526.0
303.00	1177.0
304.00	349.0
314.00	499.0
315.00	1198.0
316.00	664.0
323.10	3100.0
324.00	545.0
327.00	774.0
333.00	413.0
334.00	1716.0
335.00	493.0
341.00	362.0
346.00	623.0
351.90	900.0
353.00	421.0
354.00	938.0
365.00	4360.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

366.00	611.0
372.10	1362.0
383.00	510.0
402.00	570.0
403.00	981.0
404.10	342.0
421.00	537.0
422.00	578.0
423.10	5276.0
424.10	1197.0
441.10	14664.0
442.10	99352.0
443.10	19816.0
444.00	1771.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

m/z	Abundance
39.10	1770.0
40.00	406.0
44.00	545.0
50.10	6067.0
51.10	23952.0
52.00	1194.0
55.90	706.0
57.00	1889.0
60.90	340.0
62.00	381.0
63.00	1052.0
65.00	386.0
68.20	439.0
69.00	27360.0
72.90	340.0
74.00	3243.0
75.00	4649.0
76.10	1623.0
77.00	28480.0
78.10	1885.0
79.00	2289.0
80.00	1747.0
81.00	2592.0
82.00	675.0
83.00	540.0
85.00	538.0
85.90	663.0
86.90	324.0
91.00	647.0
92.00	643.0
93.00	4558.0
98.00	3600.0
99.00	2150.0
101.00	1192.0
103.00	523.0
104.00	895.0
105.00	928.0
107.00	10424.0
108.00	1607.0
108.90	319.0
110.00	17640.0
111.00	2721.0
115.90	456.0
117.00	9899.0
118.00	642.0
121.90	694.0
123.00	1283.0
123.90	467.0
125.10	373.0
126.20	399.0
127.00	33696.0
128.00	2756.0
129.00	14449.0
130.10	1454.0
134.00	514.0
135.00	1401.0
136.00	607.0
136.90	560.0
141.00	1736.0
142.00	628.0
143.00	543.0
146.00	407.0
147.00	1078.0
148.00	2477.0
148.90	674.0
150.90	323.0
152.90	638.0
154.00	560.0
155.00	1258.0
156.00	1610.0
156.90	374.0
157.20	383.0
158.00	365.0
159.00	425.0
160.00	573.0
161.00	1013.0
161.80	315.0
165.00	972.0
166.00	654.0
166.90	4357.0
167.90	2006.0
169.10	521.0
171.90	598.0
172.90	510.0
174.00	1067.0
175.00	1623.0
176.00	358.0
177.00	835.0
178.90	3712.0
179.90	2234.0
181.00	1176.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

185.00	1517.0
186.00	13030.0
187.00	3651.0
188.00	313.0
189.00	840.0
191.00	447.0
192.10	1190.0
193.00	1335.0
194.00	322.0
195.90	2520.0
197.10	748.0
198.00	90256.0
198.90	6458.0
199.90	526.0
203.00	1028.0
204.00	3467.0
205.00	6542.0
206.00	26464.0
207.10	3474.0
208.00	1244.0
209.00	307.0
209.90	401.0
211.00	903.0
215.00	366.0
215.90	672.0
217.00	7380.0
218.00	1021.0
221.10	3444.0
221.90	988.0
222.90	1761.0
224.00	14661.0
225.00	3519.0
226.00	443.0
227.00	7213.0
227.90	783.0
228.90	1377.0
231.00	531.0
233.90	373.0
235.00	553.0
235.90	587.0
236.90	371.0
239.00	329.0
240.90	371.0
242.00	650.0
243.00	904.0
244.10	11673.0
245.00	1641.0
246.00	2637.0
246.90	413.0
248.90	526.0
254.00	475.0
255.00	62336.0
256.00	9378.0
257.00	729.0
258.00	4500.0
258.90	543.0
265.00	1517.0
273.00	1960.0
274.00	4713.0
275.00	27216.0
276.00	3610.0
277.00	2629.0
278.00	422.0
285.00	368.0
293.00	481.0
296.00	8481.0
297.00	1278.0
303.00	1139.0
304.00	303.0
313.80	360.0
315.00	942.0
316.00	559.0
320.90	302.0
323.00	2408.0
323.90	484.0
326.90	536.0
328.00	308.0
332.90	313.0
334.00	1716.0
334.80	408.0
335.10	384.0
341.00	356.0
345.90	407.0
352.10	877.0
353.00	482.0
354.00	928.0
365.00	3886.0
366.00	581.0
372.00	1390.0
382.90	373.0
402.10	536.0
402.90	801.0
421.00	690.0
421.90	704.0
423.10	4642.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

424.00	1307.0
441.10	15982.0
442.10	101904.0
443.10	19720.0
444.10	2062.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70

Scan 2513 (17.468 min): BM001884.D
DFTPP70

m/z	Abundance
39.90	308.0
44.00	646.0
167.10	410.0
207.10	436.0

Instrument :
BNA_M
ClientSampleId :
DFTPP70