

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006355.D
 Acq On : 08 Jul 2016 18:06
 Operator : UM/SJ
 Sample : PB91878BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 09 01:14:13 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 09 01:11:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	171306	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	794587	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	460887	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	967872	20.00	ng/ul	0.00
75) Chrysene-d12	21.23	240	867373	20.00	ng/ul	0.00
83) Perylene-d12	23.44	264	839345	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	14044	3.51	ng/uL	0.00
5) Phenol-d5	6.82	99	589504	36.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	367221	38.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	454170	36.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	485488	37.40	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	238380	37.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	266125	37.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	466127	35.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	677230	50.11	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	1459796	37.95	ng/ul	0.00
46) Acenaphthylene-d8	13.98	160	1783320	37.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	207869	28.52	ng/ul	0.00
57) Fluorene-d10	15.29	176	1213084	36.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	157774	27.82	ng/ul	0.00
70) Anthracene-d10	17.14	188	1774473	38.43	ng/ul	0.00
76) Pyrene-d10	19.44	212	1740556	42.08	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.30	264	1576298	40.42	ng/ul	0.00


Target Compounds					Ovalue
15) N-Nitroso-di-n-propylamine	8.35	70	13248	1.17 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006355.D
Acq On : 08 Jul 2016 18:06
Operator : UM/SJ
Sample : PB91878BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 09 01:14:13 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 09 01:11:24 2016
Response via : Initial Calibration

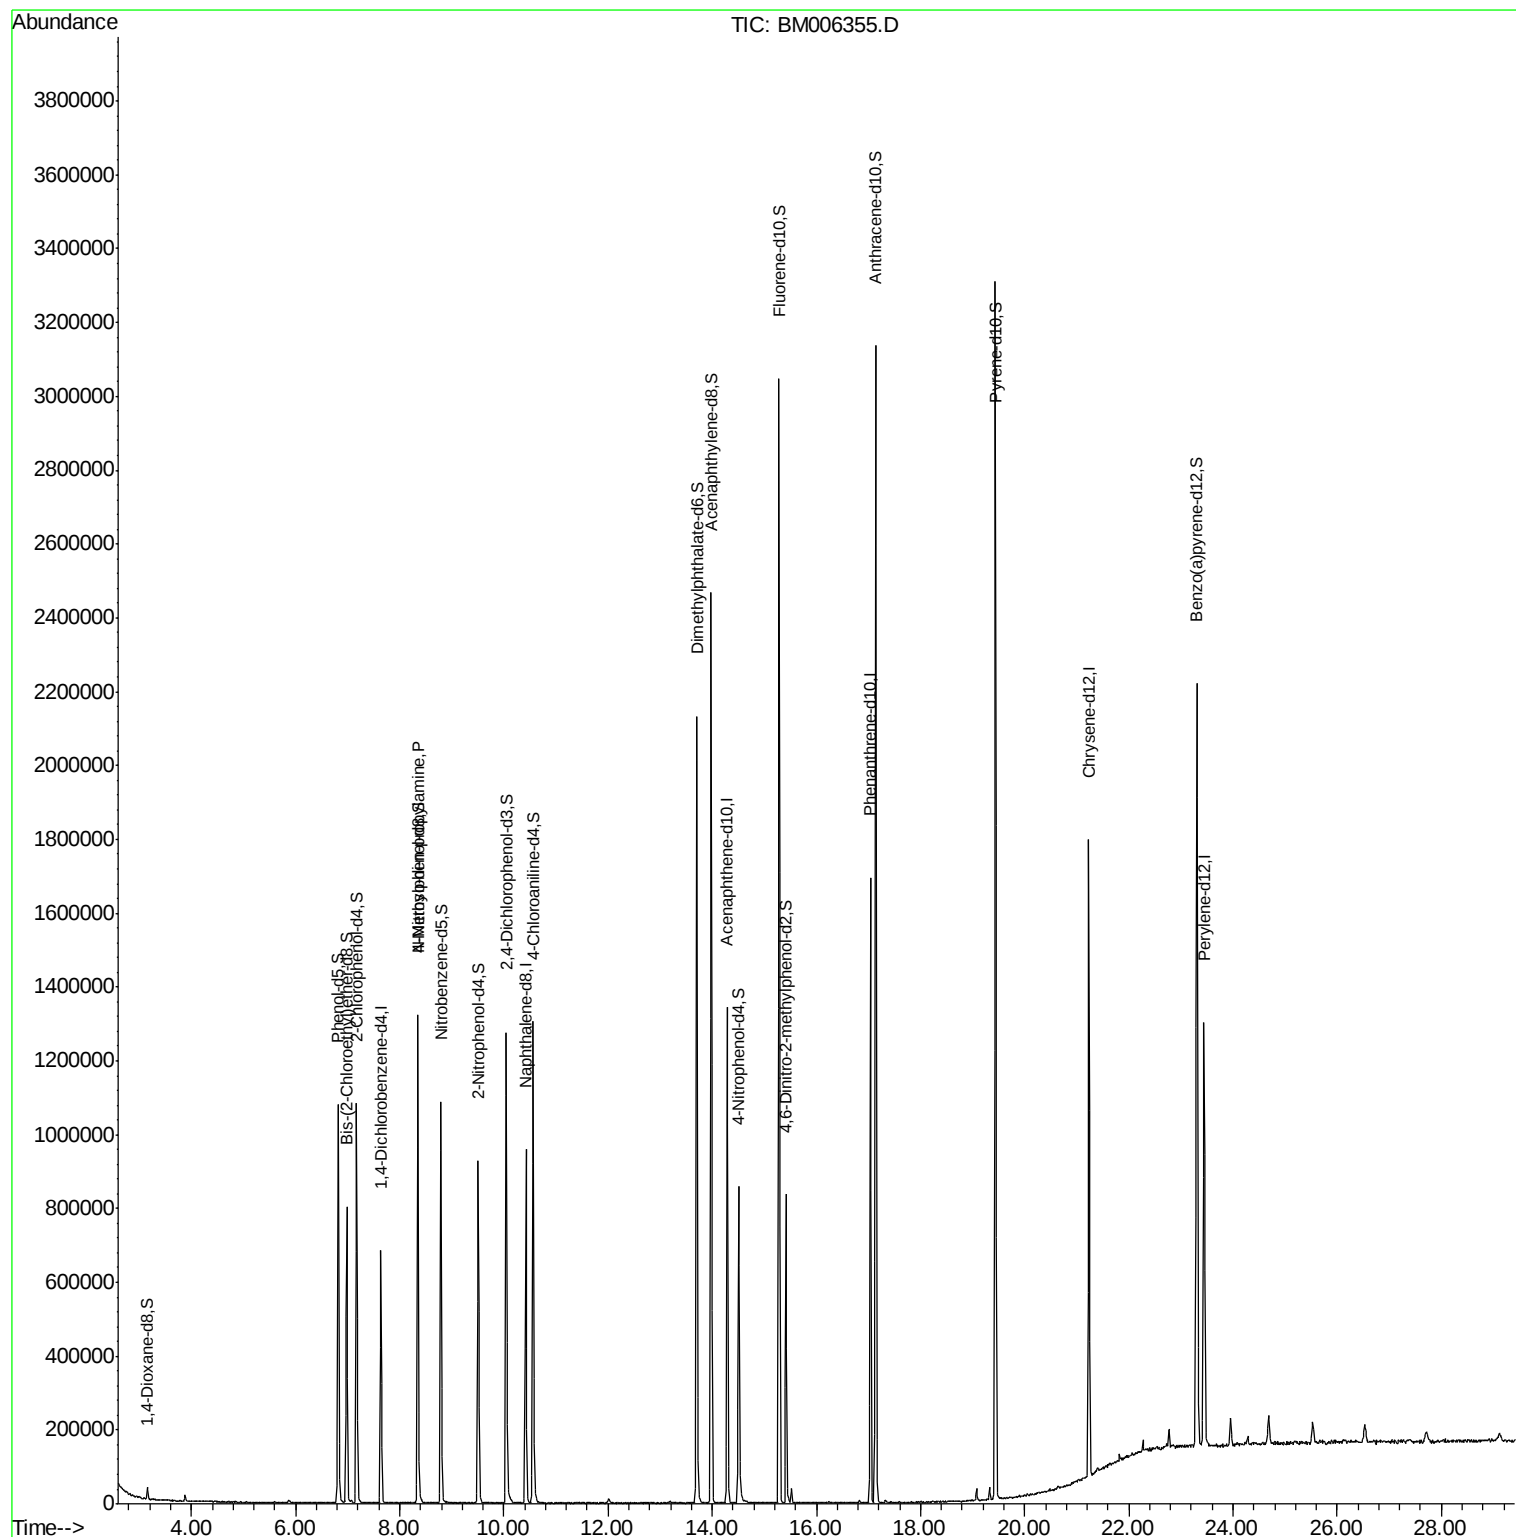

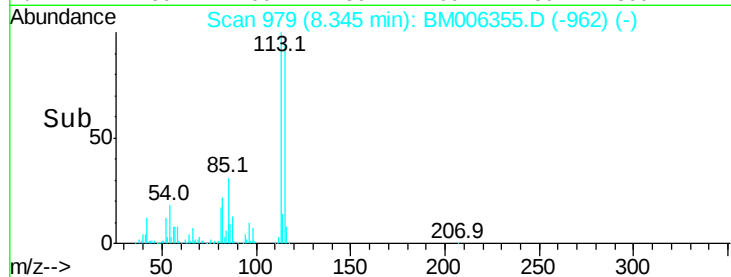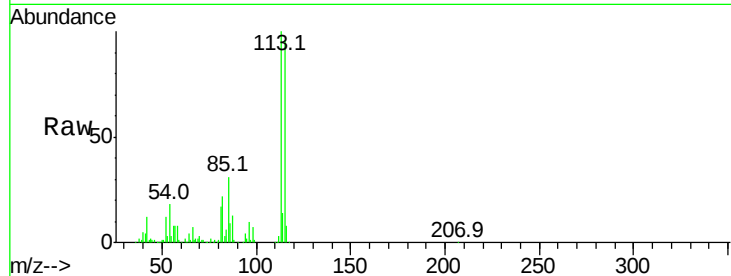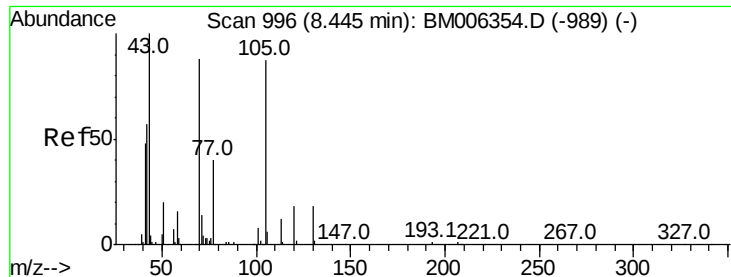

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.17 ng/ul
 RT: 8.35 min Scan# 979
 Delta R.T. -0.10 min
 Lab File: BM006355.D
 Acq: 08 Jul 2016 18:06

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 13248
 Ion Ratio Lower Upper
 70 100
 42 417.4 50.6 75.8#
 101 0.0 7.9 11.9#
 130 0.0 15.8 23.6#

