

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006359.D
 Acq On : 08 Jul 2016 20:30
 Operator : UM/SJ
 Sample : H3861-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 09 01:14:40 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 09 01:11:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	169396	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	772851	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	467446	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1048217	20.00	ng/ul	0.00
75) Chrysene-d12	21.23	240	903472	20.00	ng/ul	0.00
83) Perylene-d12	23.44	264	835127	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	7923	2.00	ng/uL	0.00
5) Phenol-d5	6.82	99	401894	25.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	235724	25.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	302977	24.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	333415	25.97	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	149641	24.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	176784	25.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	320361	25.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	466287	35.47	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	1126251	28.87	ng/ul	0.00
46) Acenaphthylene-d8	13.98	160	1321153	27.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	131905	17.84	ng/ul	0.00
57) Fluorene-d10	15.29	176	956244	28.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	95500	15.55	ng/ul	0.00
70) Anthracene-d10	17.14	188	1478078	29.55	ng/ul	0.00
76) Pyrene-d10	19.44	212	1521786	35.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.30	264	1228289	31.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.75	163	673486	17.17	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006359.D
Acq On : 08 Jul 2016 20:30
Operator : UM/SJ
Sample : H3861-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 09 01:14:40 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 09 01:11:24 2016
Response via : Initial Calibration

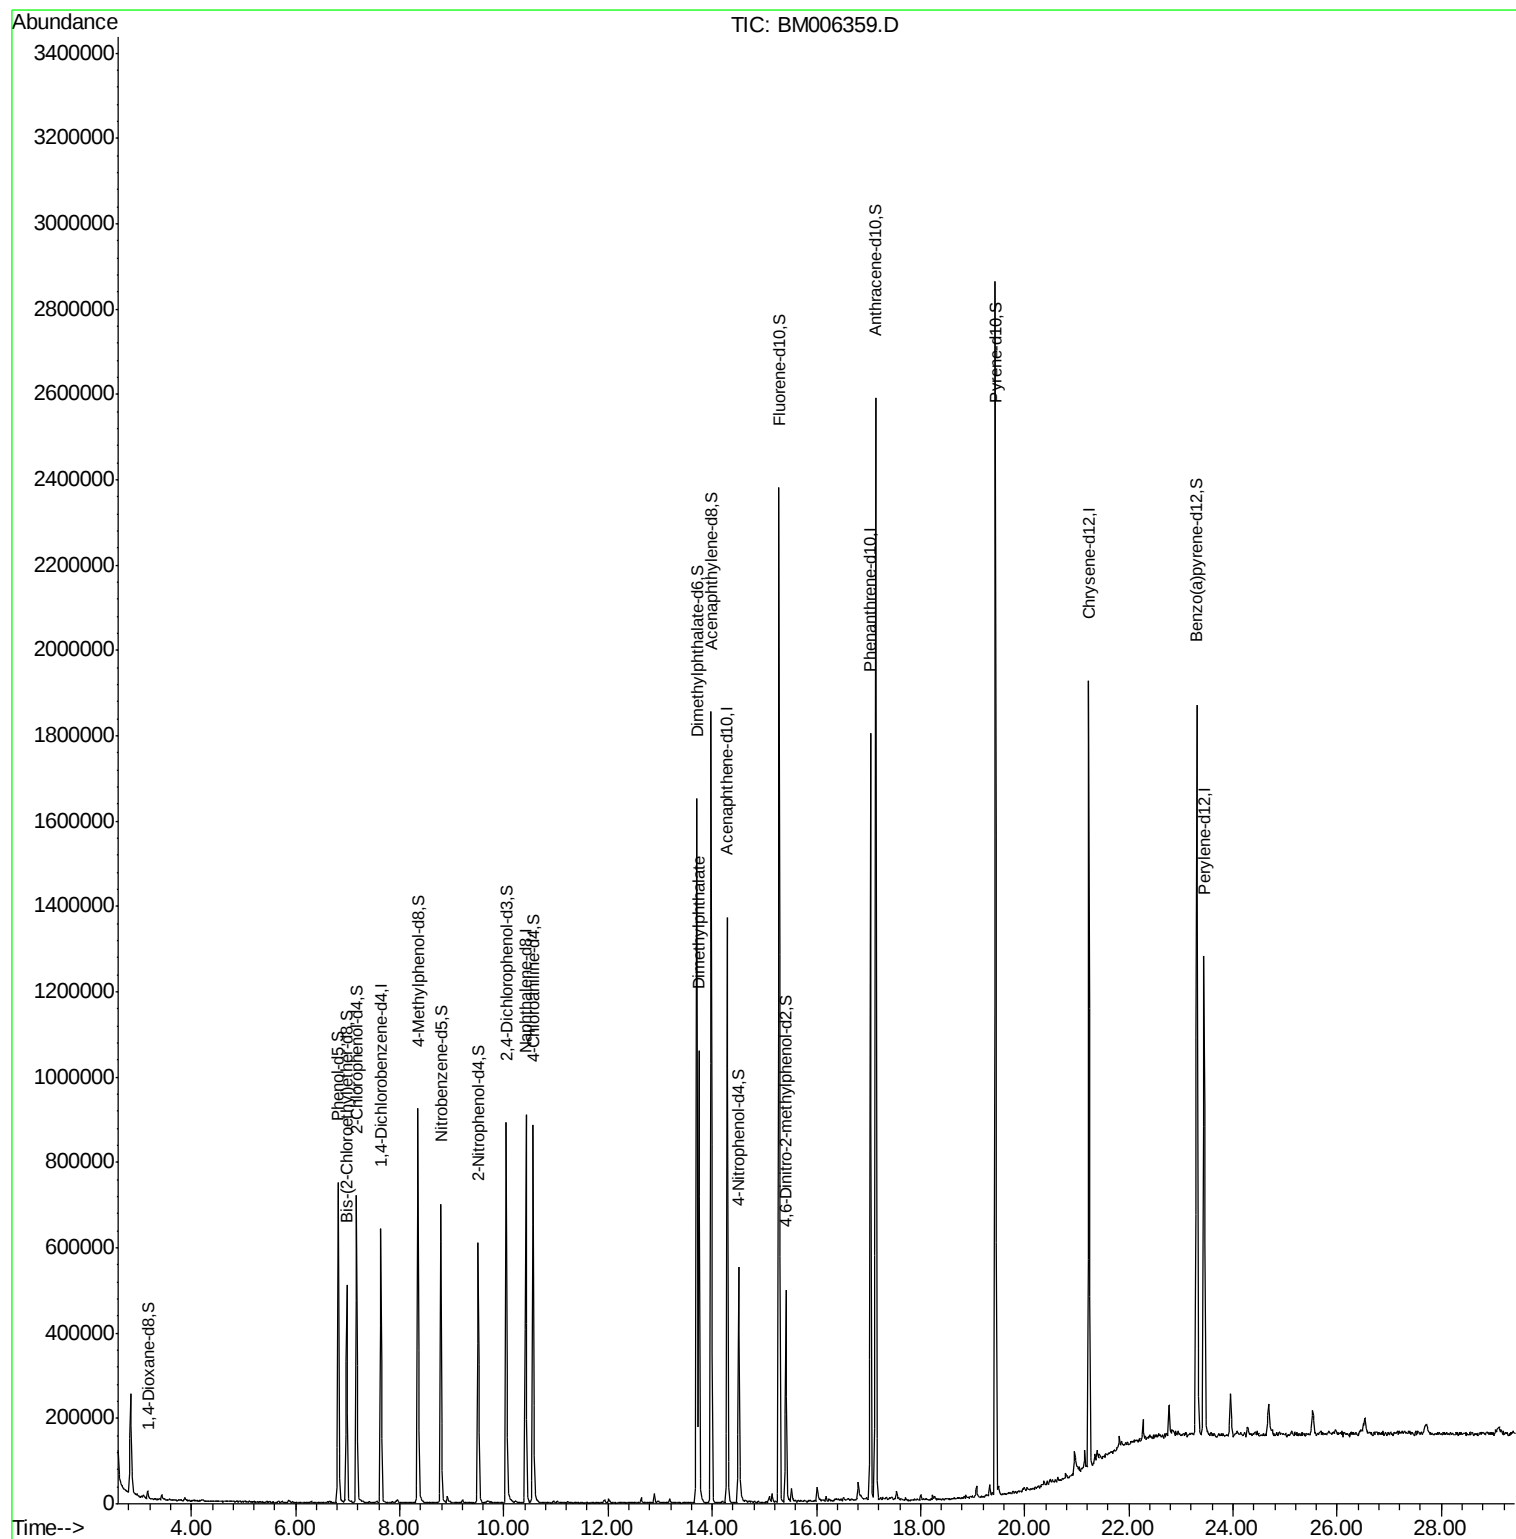

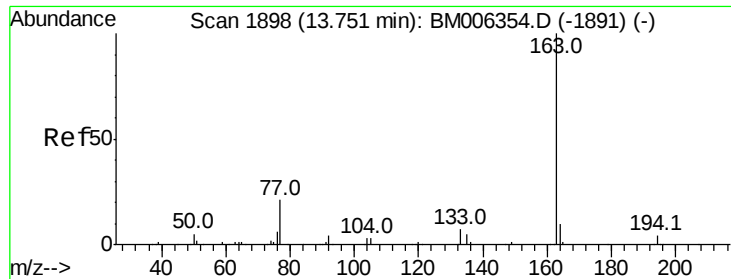

#44

Dimethylphthalate

Concen: 17.17 ng/ul

RT: 13.75 min Scan# 1898

Delta R.T. -0.00 min

Lab File: BM006359.D

Acq: 08 Jul 2016 20:30

Instrument :

BNA_M

ClientSampleId :



Tot Ion:163 Resp: 673486

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 10.3 7.8 11.8

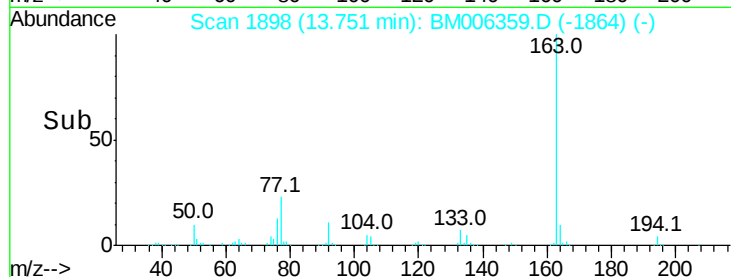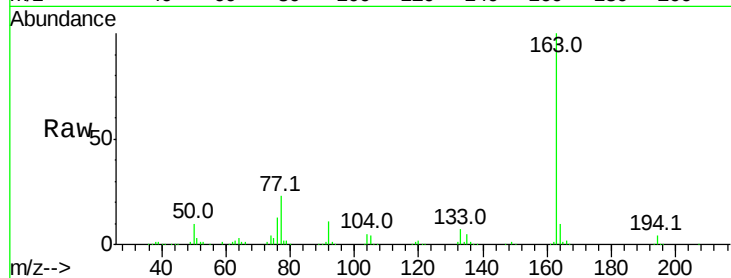

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

