

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006380.D
 Acq On : 09 Jul 2016 16:03
 Operator : UM/SJ
 Sample : H3914-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 11 04:32:44 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 11 04:31:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	154898	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	655417	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	385546	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	835807	20.00	ng/ul	0.00
75) Chrysene-d12	21.23	240	889481	20.00	ng/ul	0.00
83) Perylene-d12	23.44	264	924401	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	2203	0.61	ng/uL	0.00
5) Phenol-d5	6.81	99	99024	6.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	214598	25.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	234470	21.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	169974	14.48	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	135869	26.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	158445	26.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	261641	24.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	19421	1.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	935029	29.06	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1108039	27.81	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	45565	7.47	ng/ul	0.00
57) Fluorene-d10	15.28	176	800114	28.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	139117	28.41	ng/ul	0.00
70) Anthracene-d10	17.13	188	1304123	32.70	ng/ul	0.00
76) Pyrene-d10	19.43	212	1399636	33.00	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.30	264	1463370	34.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.74	163	66310	2.05	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006380.D
Acq On : 09 Jul 2016 16:03
Operator : UM/SJ
Sample : H3914-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 11 04:32:44 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 11 04:31:23 2016
Response via : Initial Calibration

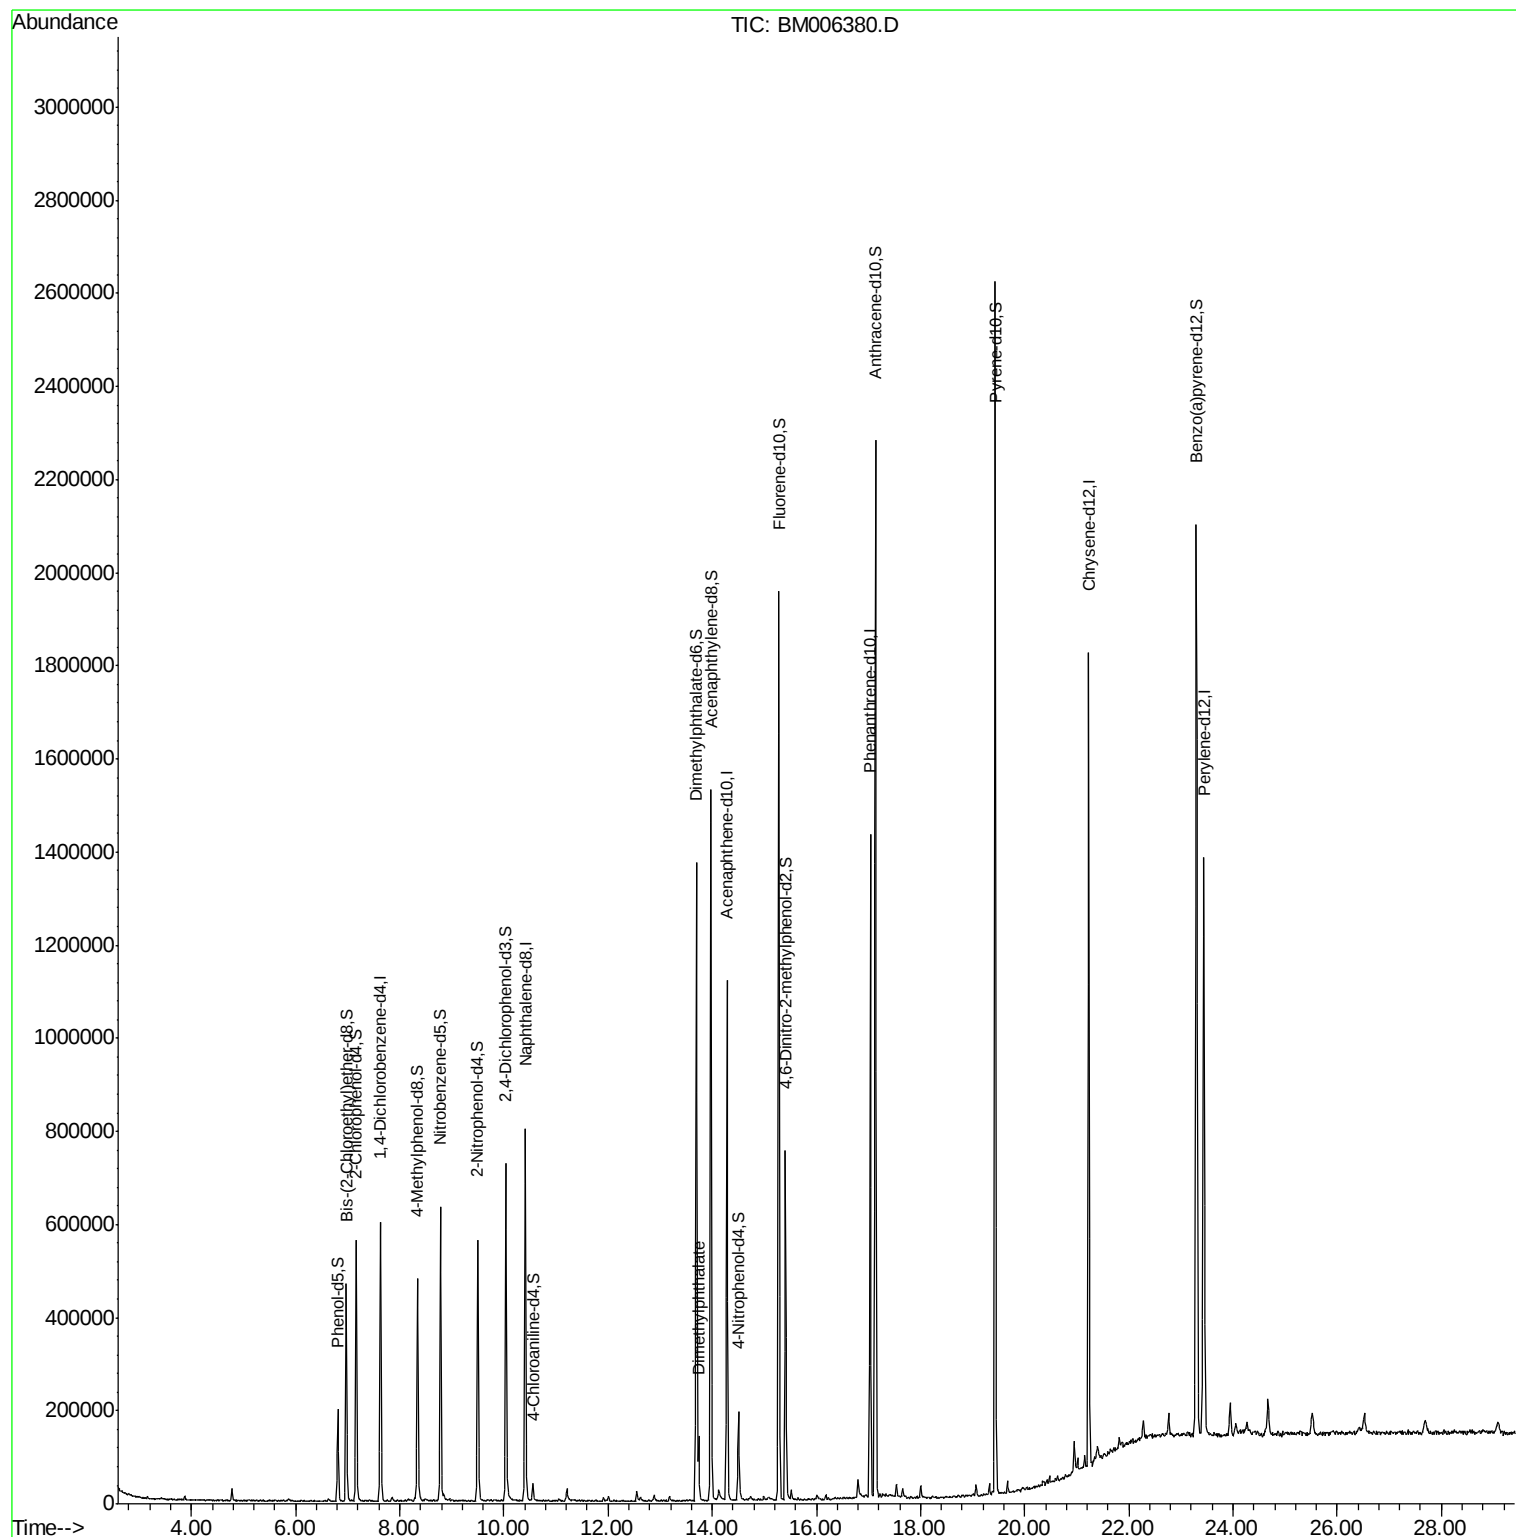

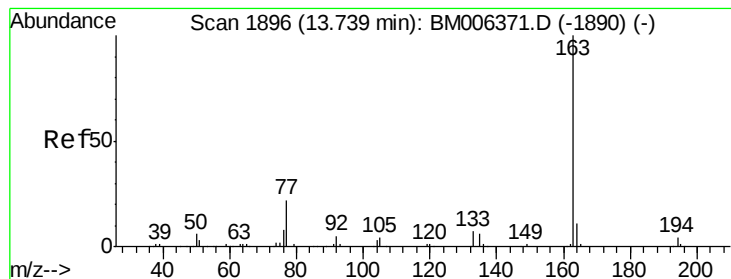

#44

Dimethylphthalate

Concen: 2.05 ng/ul

RT: 13.74 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BM006380.D

Acq: 09 Jul 2016 16:03

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 66310

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.8 7.8 11.8

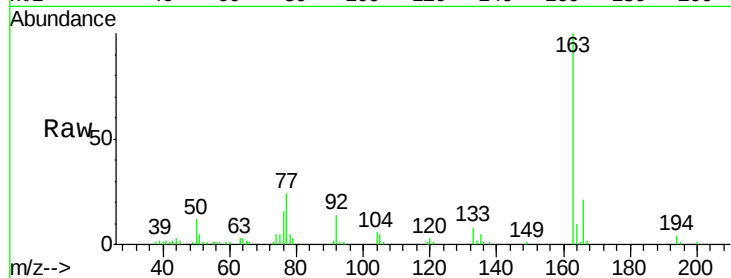

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

