

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006364.D
 Acq On : 08 Jul 2016 23:31
 Operator : UM/SJ
 Sample : H3861-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ09

Quant Time: Jul 11 04:18:57 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 11 03:50:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	189291	20.00	ng/ul	0.01
18) Naphthalene-d8	10.42	136	873910	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	528224	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1240236	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1172847	20.00	ng/ul	0.00
83) Perylene-d12	23.44	264	995846	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	11347	2.56	ng/uL	0.00
5) Phenol-d5	6.82	99	549667	31.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	335900	32.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	423868	31.24	ng/ul	0.01
13) 4-Methylphenol-d8	8.35	113	464989	32.42	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	218776	31.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	248125	31.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	453385	31.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	640935	43.12	ng/ul	0.01
43) Dimethylphthalate-d6	13.70	166	1538635	34.90	ng/ul	0.01
46) Acenaphthylene-d8	13.98	160	1862318	34.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	245948	29.44	ng/ul	0.00
57) Fluorene-d10	15.29	176	1339370	35.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	171932	23.66	ng/ul	0.00
70) Anthracene-d10	17.14	188	2069471	34.97	ng/ul	0.00
76) Pyrene-d10	19.44	212	2251550	40.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.31	264	1721288	37.20	ng/ul	0.01


Target Compounds					Ovalue
44) Dimethylphthalate	13.75	163	416546	9.40	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006364.D
Acq On : 08 Jul 2016 23:31
Operator : UM/SJ
Sample : H3861-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ09

Quant Time: Jul 11 04:18:57 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 11 03:50:07 2016
Response via : Initial Calibration

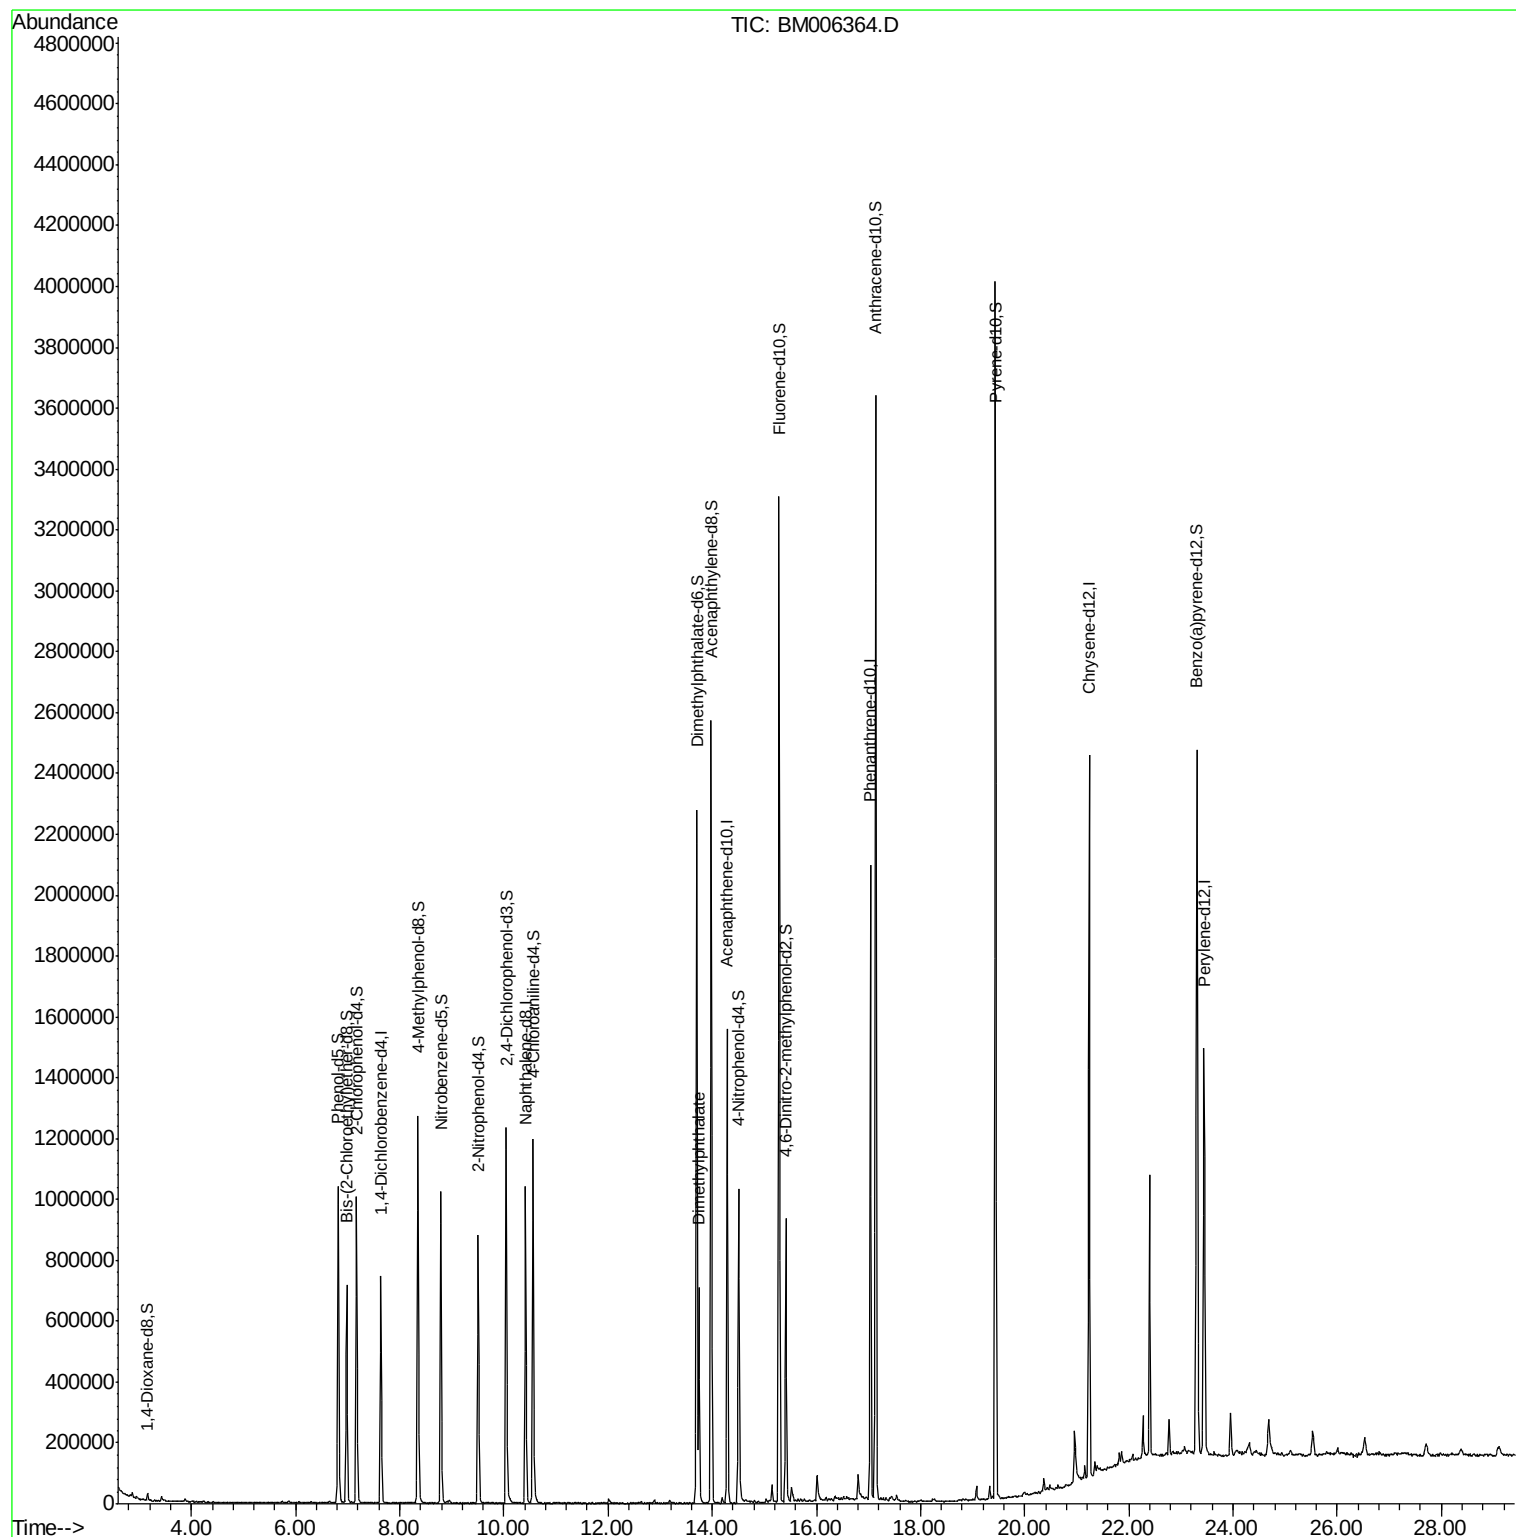


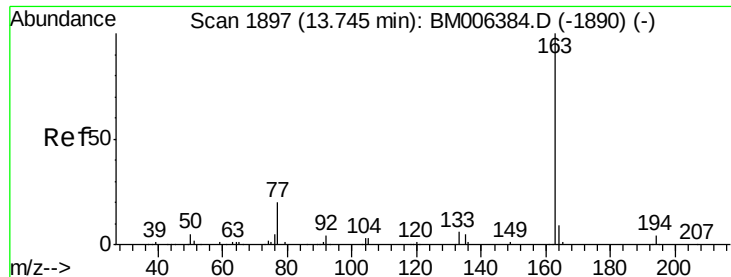

#44
 Dimethylphthalate
 Concen: 9.40 ng/ul
 RT: 13.75 min Scan# 1897
 Delta R.T. 0.01 min
 Lab File: BM006364.D
 Acq: 08 Jul 2016 23:31

Instrument :
 BNA_M
 ClientSampleId :
 BDJ09

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	10.4	7.8	11.8

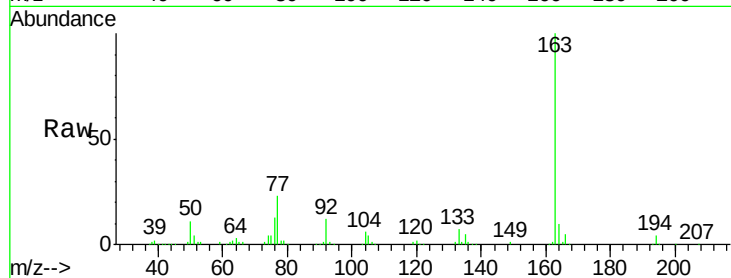

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

