

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006373.D
 Acq On : 09 Jul 2016 11:51
 Operator : UM/SJ
 Sample : H3861-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ15

Quant Time: Jul 11 04:31:51 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 11 04:31:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	138913	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	549323	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	315827	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	715285	20.00	ng/ul	0.00
75) Chrysene-d12	21.23	240	828633	20.00	ng/ul	0.00
83) Perylene-d12	23.44	264	884072	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	6376	1.96	ng/uL	0.00
5) Phenol-d5	6.81	99	289549	22.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	181806	23.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	228128	22.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	229292	21.78	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	109550	25.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	124090	25.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	214486	23.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	292137	31.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	685263	26.00	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	841982	25.80	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	113289	22.68	ng/ul	0.00
57) Fluorene-d10	15.28	176	591850	26.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	84839	20.24	ng/ul	0.00
70) Anthracene-d10	17.13	188	925644	27.12	ng/ul	0.00
76) Pyrene-d10	19.43	212	1046517	26.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.30	264	1140925	27.78	ng/ul	0.00


Target Compounds						Ovalue
44) Dimethylphthalate	13.74	163	204029	7.70	ng/ul	99
73) Di-n-butylphthalate	18.00	149	196521	4.14	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006373.D
Acq On : 09 Jul 2016 11:51
Operator : UM/SJ
Sample : H3861-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ15

Quant Time: Jul 11 04:31:51 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 11 04:31:23 2016
Response via : Initial Calibration

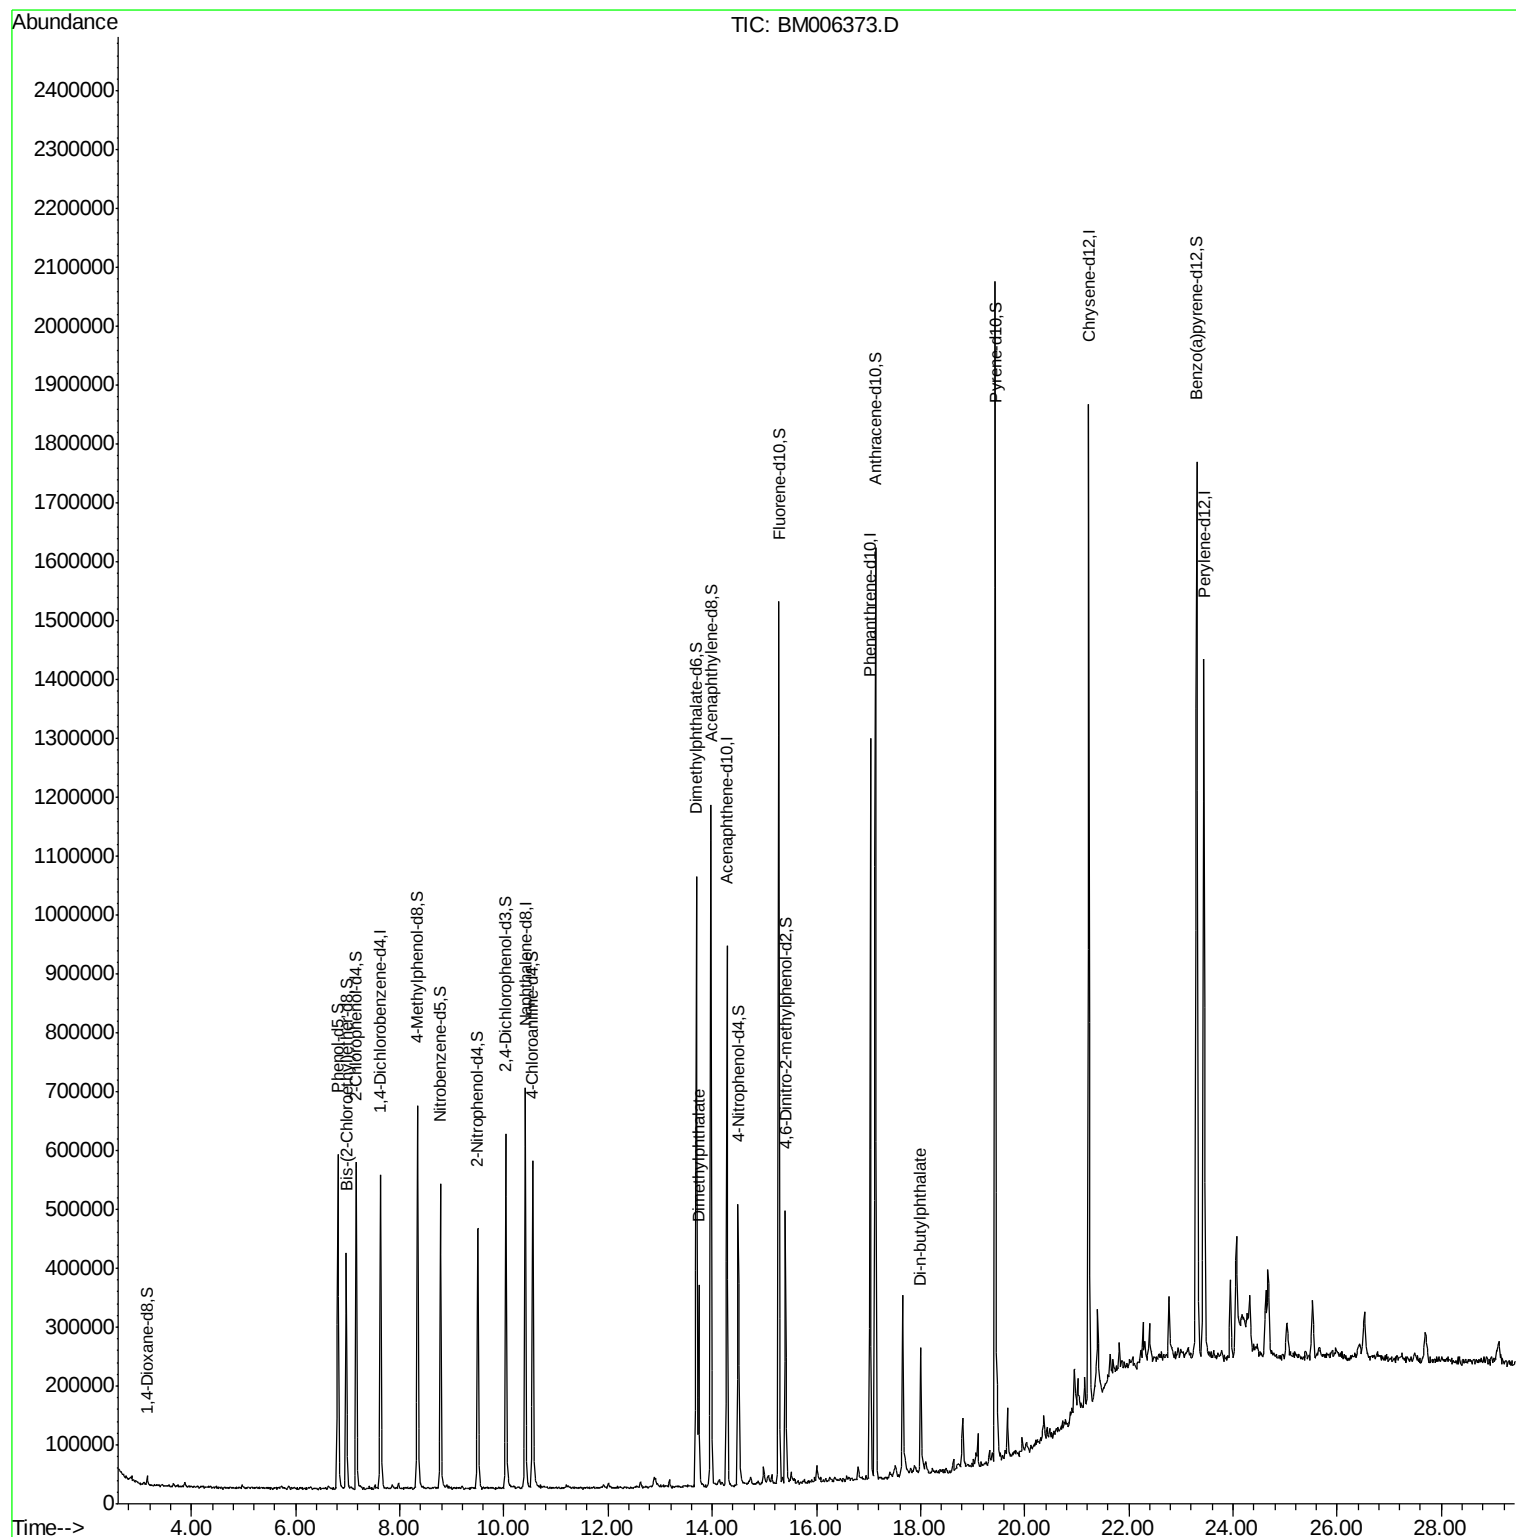


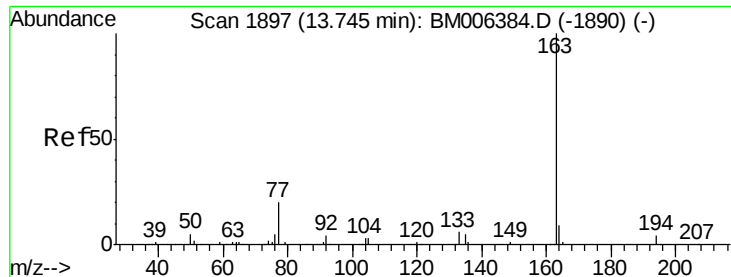




#44
Dimethylphthalate
Concen: 7.70 ng/ul
RT: 13.74 min Scan# 1896
Delta R.T. -0.00 min
Lab File: BM006373.D
Acq: 09 Jul 2016 11:51

Instrument :
BNA_M
ClientSampleId :
BDJ15

Tot Ion:163 Resp: 204029
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.0
164 9.6 7.8 11.8

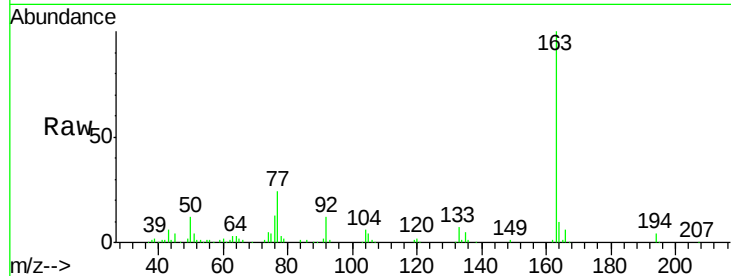


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

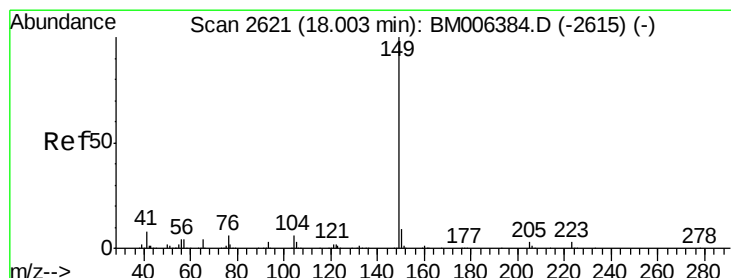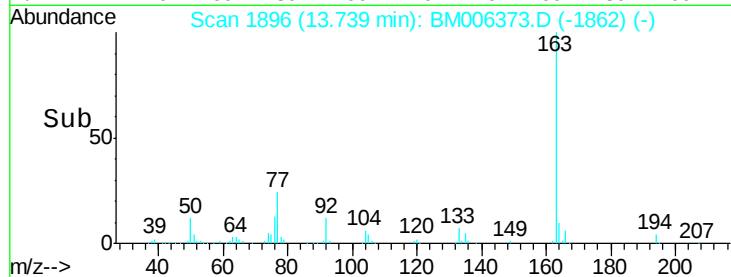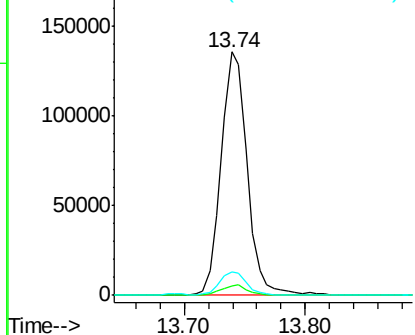

#73
Di-n-butylphthalate
Concen: 4.14 ng/ul
RT: 18.00 min Scan# 2621
Delta R.T. -0.00 min
Lab File: BM006373.D
Acq: 09 Jul 2016 11:51

Tgt Ion:149 Resp: 196521
Ion Ratio Lower Upper
149 100
150 9.9 7.1 10.7
104 5.6 4.4 6.6

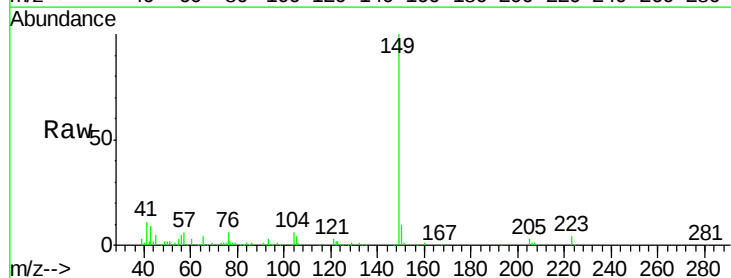

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 104.00 (103.70 to 104.70): E

