

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006366.D
 Acq On : 09 Jul 2016 00:43
 Operator : UM/SJ
 Sample : H3861-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.816	712	719	734	rBV	550904	945279	22.36%	2.048%
2	6.975	737	746	759	rBV	386713	628681	14.87%	1.362%
3	7.169	772	779	791	rBV	529372	877360	20.75%	1.901%
4	7.640	852	859	874	rVB	766934	1269535	30.03%	2.751%
5	8.346	972	979	995	rVB	652063	1108737	26.23%	2.403%
6	8.793	1048	1055	1065	rBV	534531	916310	21.68%	1.986%
7	9.510	1169	1177	1193	rBV	448694	785013	18.57%	1.701%
8	10.046	1261	1268	1281	rBV	656580	1149101	27.18%	2.490%
9	10.416	1324	1331	1346	rBV	1092494	1940363	45.90%	4.205%
10	10.557	1348	1355	1370	rBV	613358	1156692	27.36%	2.507%
11	13.698	1883	1889	1894	rBV	1226352	1786124	42.25%	3.871%
12	13.745	1894	1897	1907	rVB	457116	658538	15.58%	1.427%
13	13.981	1930	1937	1948	rVB	1318281	2138904	50.60%	4.635%
14	14.286	1982	1989	1998	rBV2	1600894	2662998	62.99%	5.771%
15	14.504	2019	2026	2041	rBV	457607	845222	19.99%	1.832%
16	15.151	2132	2136	2142	rVB2	35875	49137	1.16%	0.106%
17	15.286	2152	2159	2166	rBV	1803373	2671312	63.19%	5.789%
18	15.416	2175	2181	2193	rBV	427378	645055	15.26%	1.398%
19	16.010	2278	2282	2290	rBV3	52494	92814	2.20%	0.201%
20	16.804	2413	2417	2423	rBV2	45806	72062	1.70%	0.156%
21	17.039	2450	2457	2462	rBV	2159187	3286657	77.74%	7.122%
22	17.080	2462	2464	2468	rVV	153432	179298	4.24%	0.389%
23	17.133	2468	2473	2485	rVB2	1901774	2998873	70.94%	6.499%
24	17.910	2600	2605	2610	rBV	34185	55522	1.31%	0.120%
25	18.110	2634	2639	2652	rVB3	81297	161634	3.82%	0.350%
26	18.839	2758	2763	2768	rBV	41907	74587	1.76%	0.162%
27	19.104	2799	2808	2813	rBV	512804	736332	17.42%	1.596%
28	19.257	2829	2834	2837	rBV	39000	55241	1.31%	0.120%
29	19.333	2842	2847	2849	rVV	27072	49133	1.16%	0.106%
30	19.439	2859	2865	2879	rVV2	2471165	4227494	100.00%	9.161%
31	19.792	2919	2925	2933	rBV4	38785	105184	2.49%	0.228%
32	19.962	2951	2954	2963	rVB	105094	155616	3.68%	0.337%
33	20.068	2968	2972	2976	rVV	81312	112188	2.65%	0.243%
34	20.127	2977	2982	2985	rVB2	50371	76718	1.81%	0.166%

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006366.D
Acq On : 09 Jul 2016 00:43
Operator : UM/SJ
Sample : H3861-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ11

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Title : SVOA CALIBRATION

35	20.262	3002	3005	3009	rBV	37045	49941	1.18%	0.108%
36	20.310	3010	3013	3017	rVV2	41028	56414	1.33%	0.122%
37	20.374	3020	3024	3027	rVB	58924	76790	1.82%	0.166%
38	20.957	3120	3123	3128	rBV3	85849	144178	3.41%	0.312%
39	21.151	3153	3156	3160	rVB	153389	168994	4.00%	0.366%
40	21.233	3163	3170	3175	rVV	2491726	3712067	87.81%	8.044%
41	21.268	3175	3176	3183	rVB	228110	238922	5.65%	0.518%
42	21.386	3193	3196	3200	rBV2	40880	61957	1.47%	0.134%
43	22.274	3344	3347	3352	rVB3	62069	89648	2.12%	0.194%
44	22.774	3427	3432	3438	rBV2	213168	520164	12.30%	1.127%
45	23.251	3509	3513	3516	rBV	95775	165111	3.91%	0.358%
46	23.303	3516	3522	3537	rVB2	1354190	3004024	71.06%	6.510%
47	23.445	3539	3546	3553	rBV	1363950	2681543	63.43%	5.811%
48	23.950	3627	3632	3642	rVB	115535	246374	5.83%	0.534%
49	24.680	3751	3756	3767	rBV2	105487	255967	6.05%	0.555%


Sum of corrected areas: 46145808

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006366.D
Acq On : 09 Jul 2016 00:43
Operator : UM/SJ
Sample : H3861-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BDJ11

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

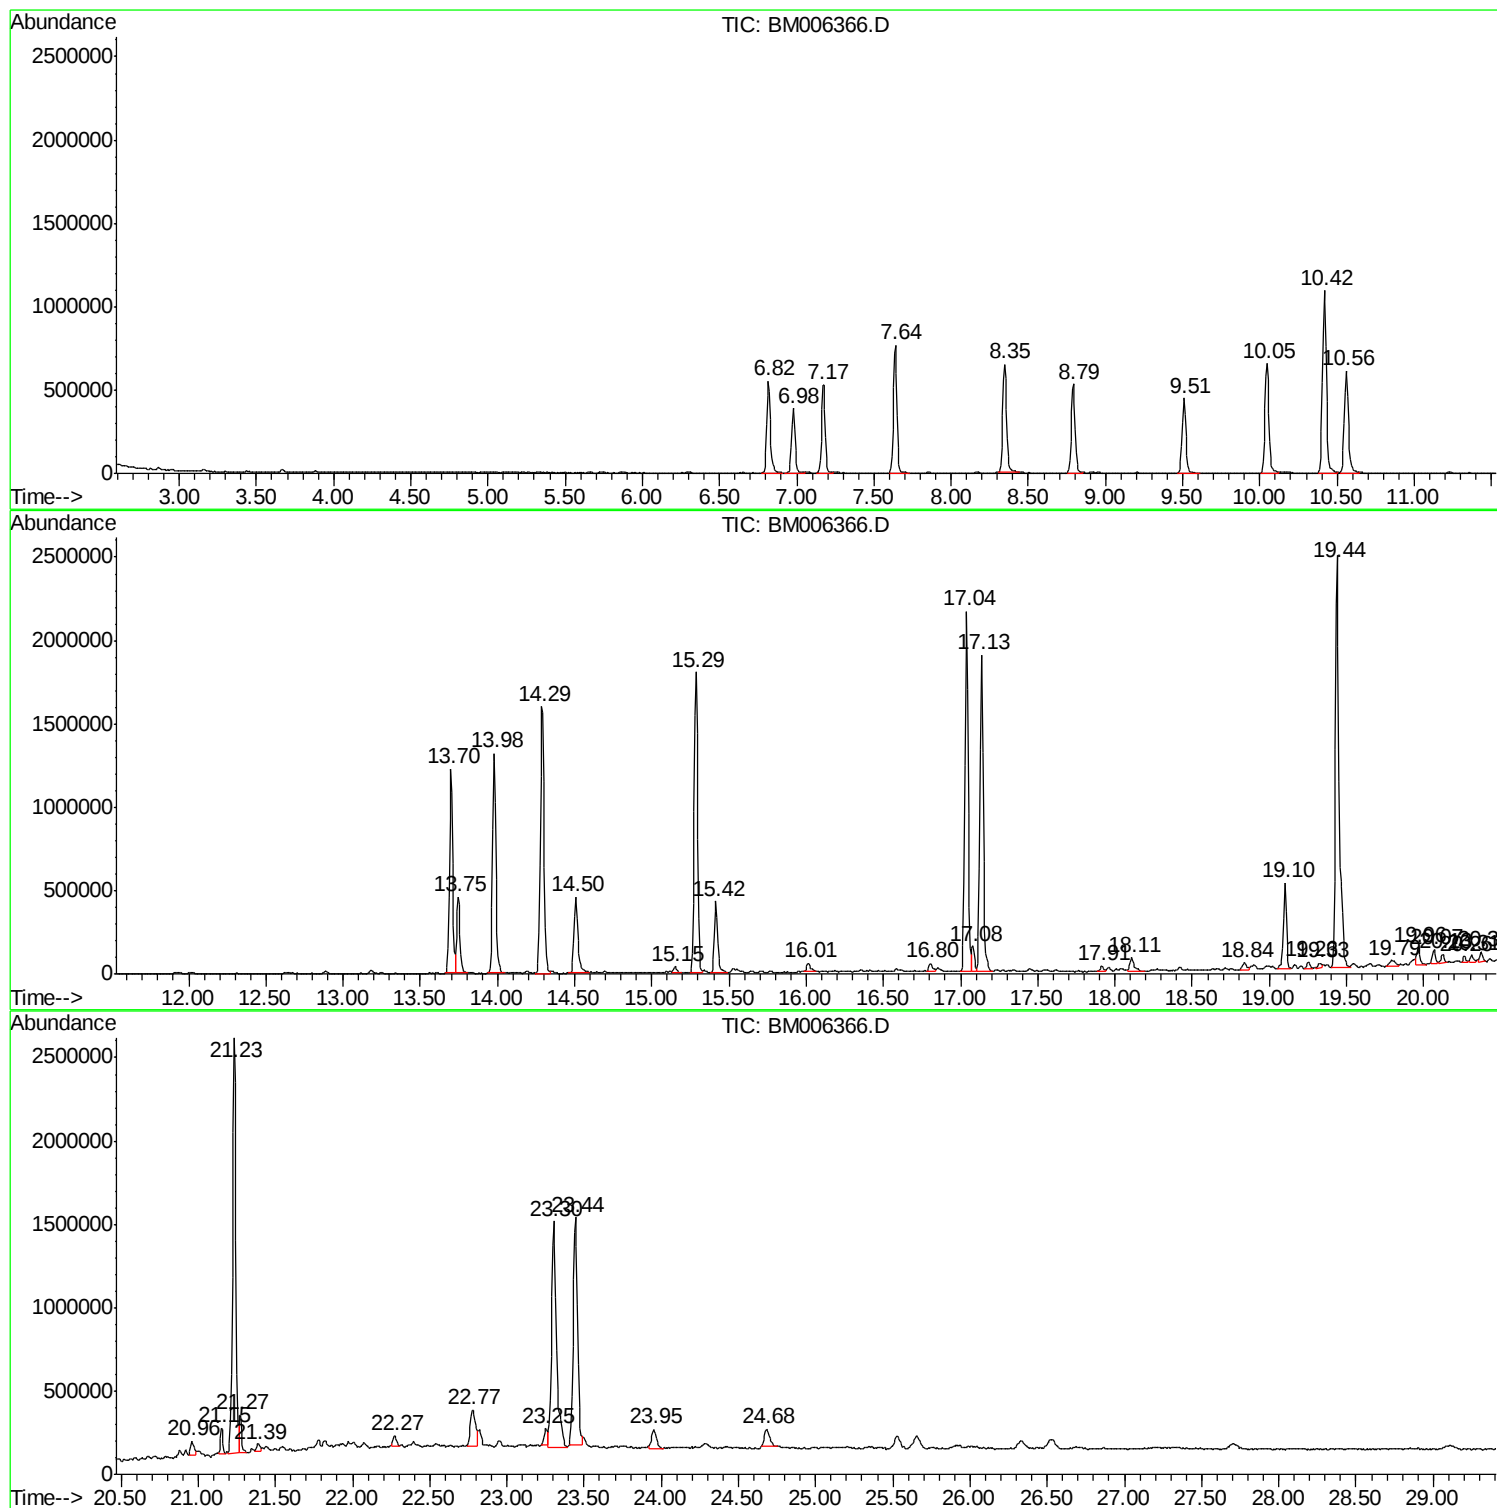

Data Path : V:\HPCHEM1\BNA_M\DATA\BM070916\
Data File : BM006366.D
Acq On : 09 Jul 2016 00:43
Operator : UM/SJ
Sample : H3861-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ11

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : V:\HPCHEM1\BNA_M\DATA\BM070916\
Data File : BM006366.D
Acq On : 09 Jul 2016 00:43
Operator : UM/SJ
Sample : H3861-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ11

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc