

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
 Data File : BM006381.D
 Acq On : 09 Jul 2016 16:39
 Operator : UM/SJ
 Sample : H3914-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TR4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.810	712	718	726	rVB	202662	325435	6.41%	0.757%
2	6.969	738	745	754	rBV	587850	918801	18.09%	2.138%
3	7.163	771	778	790	rBV	687733	1116850	21.98%	2.599%
4	7.628	850	857	866	rBV	526047	864703	17.02%	2.012%
5	8.340	972	978	997	rVB	546842	930135	18.31%	2.164%
6	8.787	1046	1054	1061	rBV	781492	1354568	26.66%	3.152%
7	9.498	1168	1175	1189	rBV	698614	1220959	24.03%	2.841%
8	10.039	1256	1267	1286	rBV	880975	1589471	31.29%	3.698%
9	10.410	1322	1330	1343	rBV	703278	1247005	24.55%	2.901%
10	13.698	1882	1889	1906	rBV	1664021	2659528	52.35%	6.188%
11	13.974	1927	1936	1947	rBV	1705674	2828764	55.68%	6.582%
12	14.127	1955	1962	1972	rBV2	21293	53159	1.05%	0.124%
13	14.280	1982	1988	2001	rVB2	963619	1561830	30.74%	3.634%
14	14.504	2020	2026	2039	rBV	220371	382473	7.53%	0.890%
15	15.280	2151	2158	2169	rBV	2432589	3687355	72.58%	8.579%
16	15.410	2174	2180	2194	rVV	1058029	1511368	29.75%	3.516%
17	17.033	2449	2456	2466	rBV	1214748	1816872	35.76%	4.227%
18	17.133	2466	2473	2488	rVB	2824426	4262337	83.90%	9.917%
19	19.433	2858	2864	2876	rVB	3285588	4873922	95.94%	11.340%
20	21.233	3164	3170	3177	rBV	1686272	2209675	43.49%	5.141%
21	22.268	3344	3346	3351	rVB	42551	51235	1.01%	0.119%
22	22.768	3428	3431	3436	rVB2	60101	74172	1.46%	0.173%
23	23.303	3514	3522	3533	rVB2	2602269	5080403	100.00%	11.821%
24	23.439	3538	3545	3555	rVB	1104229	2194537	43.20%	5.106%
25	23.944	3627	3631	3640	rVB3	76874	163879	3.23%	0.381%


Sum of corrected areas: 42979436

Data Path : V:\HPCHEM1\BNA M\DATA\BM070916\
Data File : BM006381.D
Acq On : 09 Jul 2016 16:39
Operator : UM/SJ
Sample : H3914-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TR4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

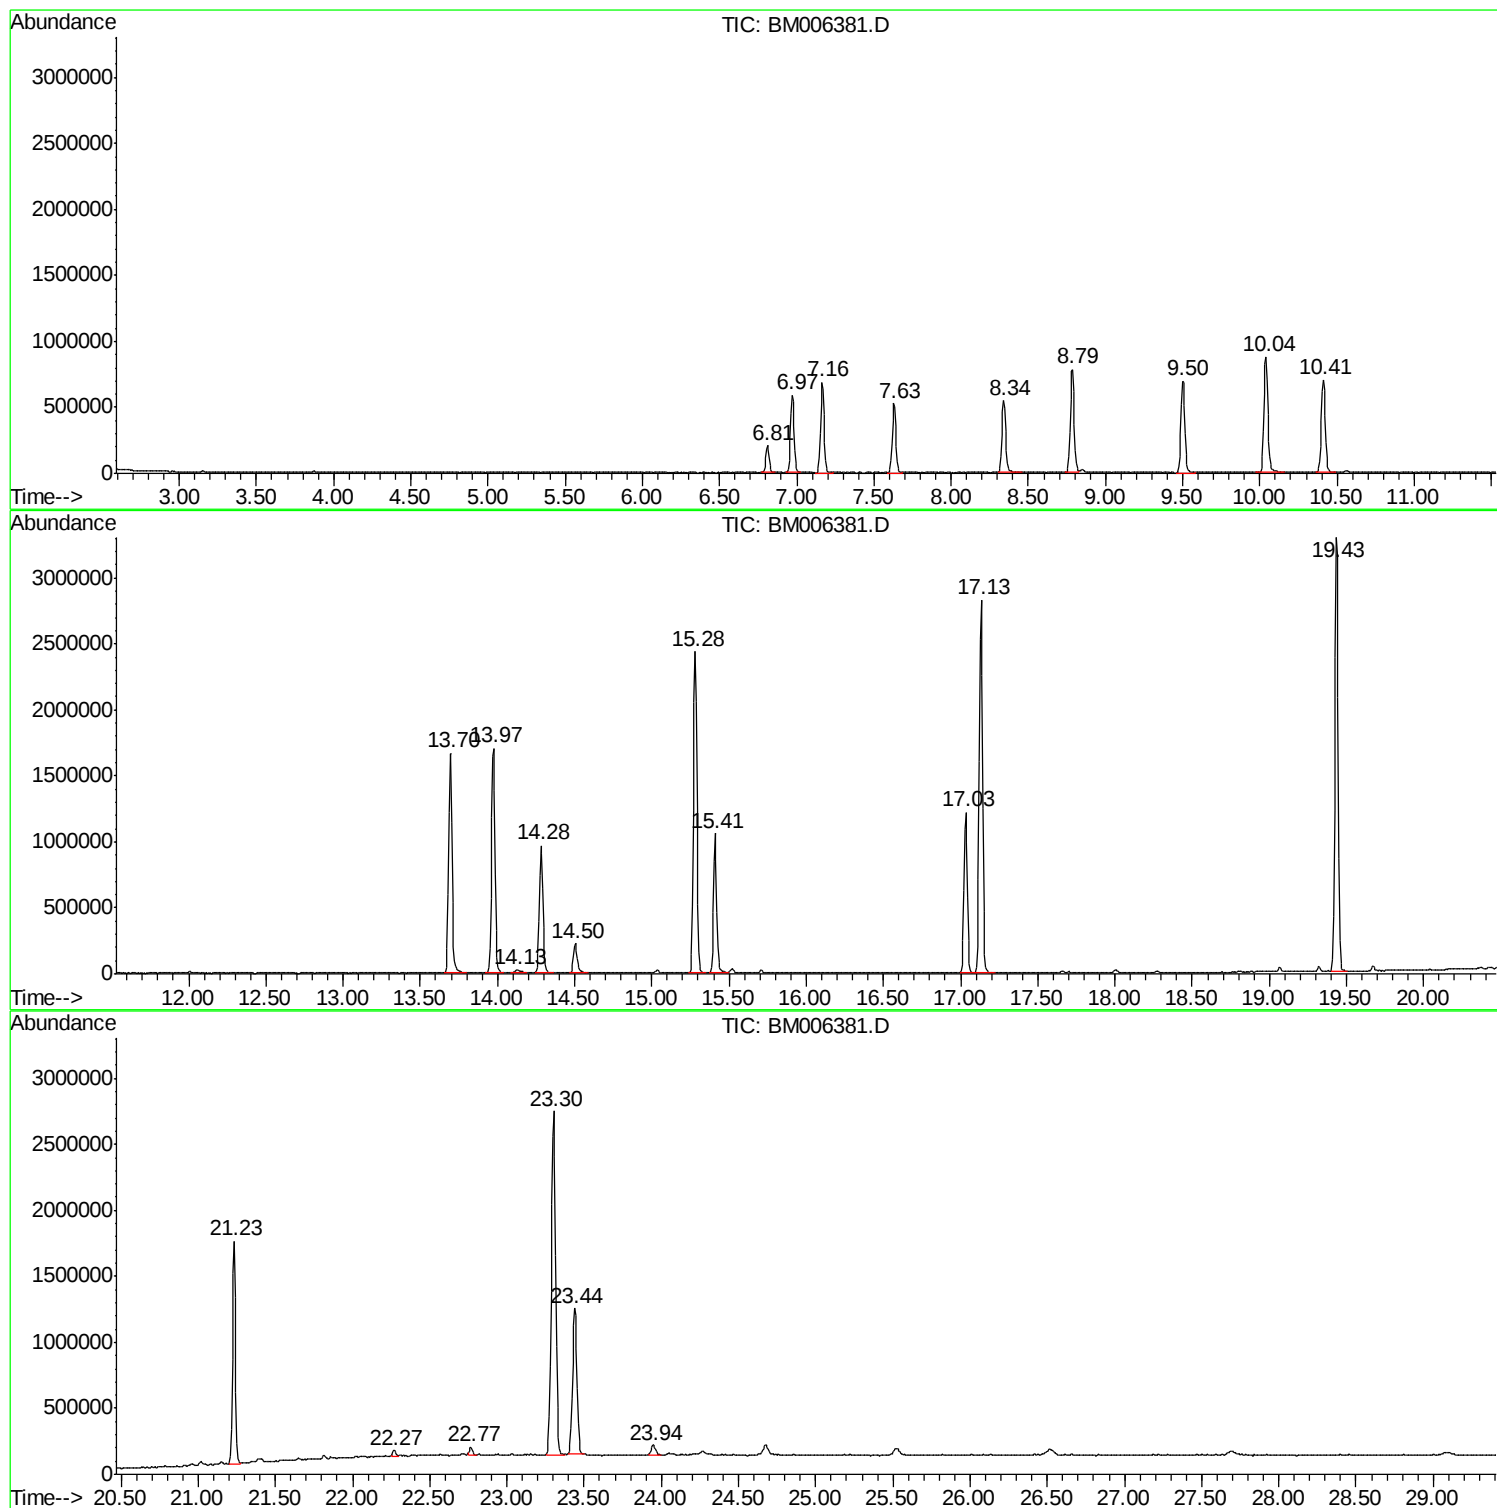

Data Path : V:\HPCHEM1\BNA_M\DATA\BM070916\
Data File : BM006381.D
Acq On : 09 Jul 2016 16:39
Operator : UM/SJ
Sample : H3914-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TR4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : V:\HPCHEM1\BNA_M\DATA\BM070916\
Data File : BM006381.D
Acq On : 09 Jul 2016 16:39
Operator : UM/SJ
Sample : H3914-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TR4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc