
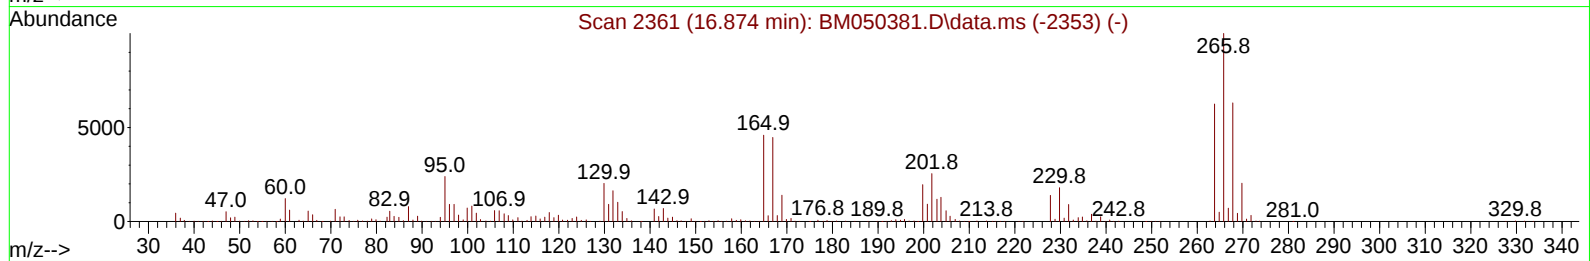
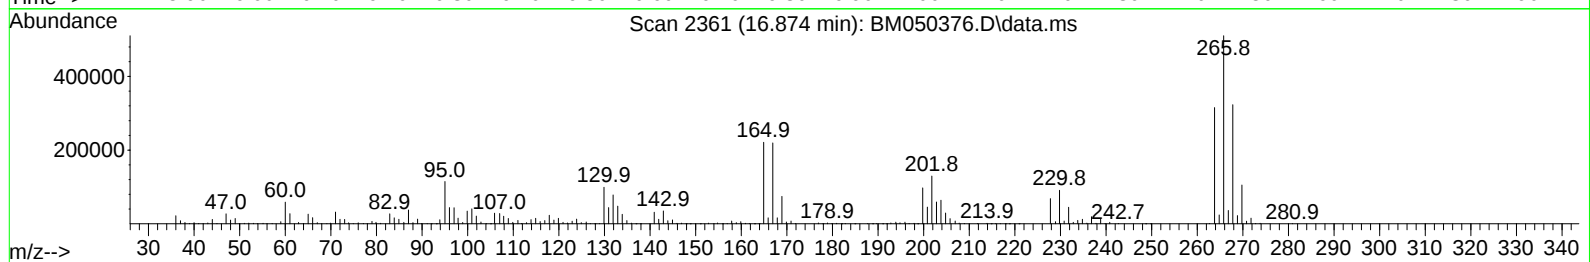


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070925\
Data File : BM050376.D
Acq On : 08 Jul 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 17:14:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 15:59:58 2025
Response via : Initial Calibration

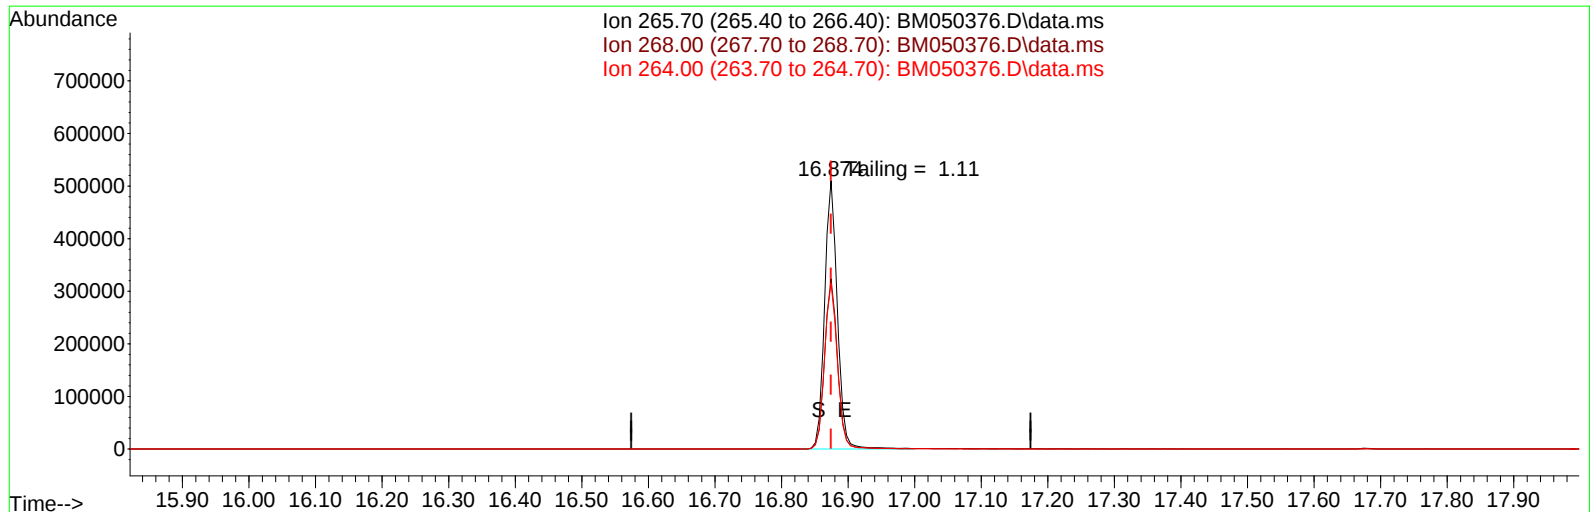

TIC: BM050376.D\data.ms

(70) Pentachlorophenol (C)




16.874min (+ 0.000) 0.00 ng

response 680595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.37
264.00	62.40	61.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070925\
Data File : BM050376.D
Acq On : 08 Jul 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 17:14:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 15:59:58 2025
Response via : Initial Calibration

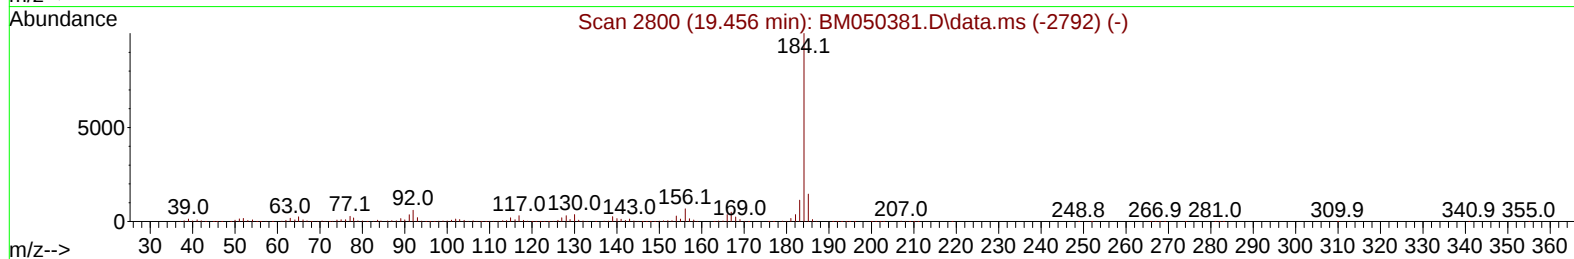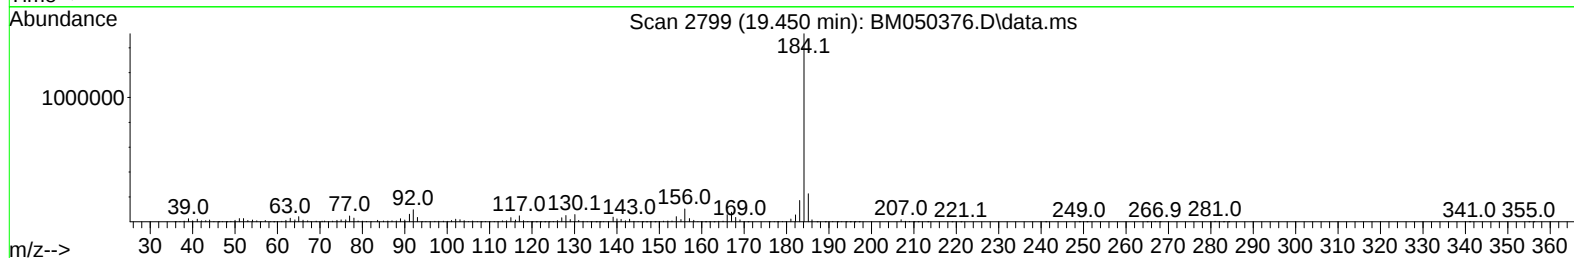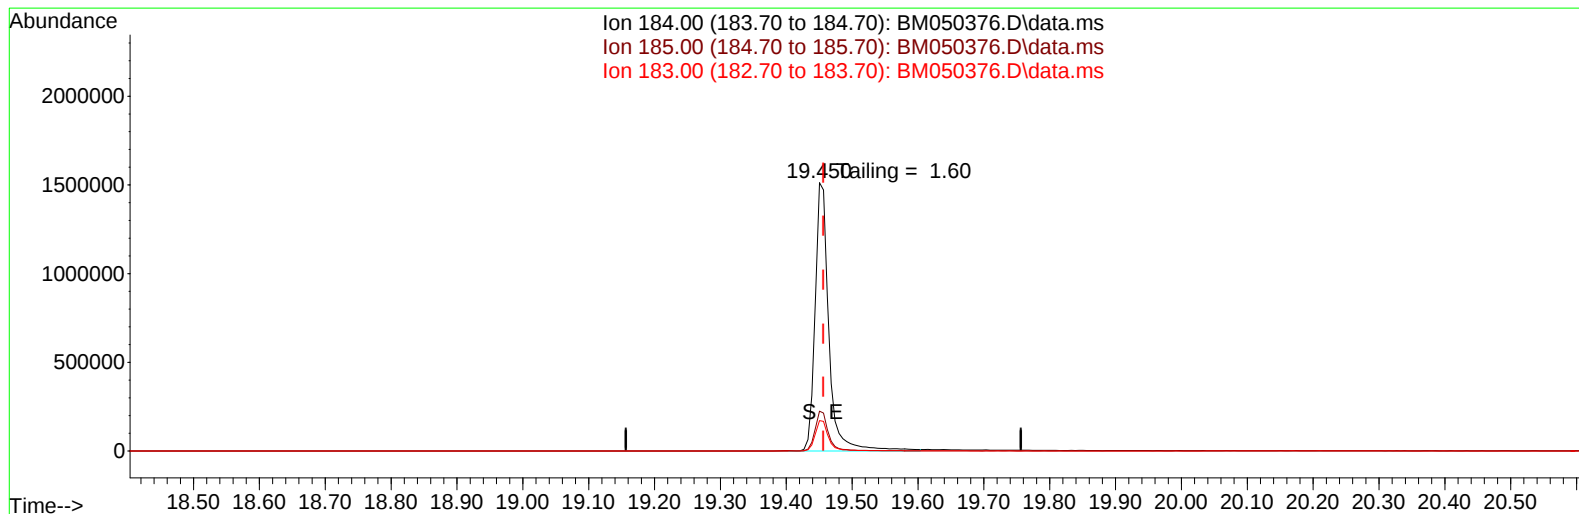

TIC: BM050376.D\data.ms

(77) Benzidine**19.450min (-0.006) 78341.13 ng****response 2201890**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.87
183.00	11.30	11.33
0.00	0.00	0.00