


Data Path : Z:\HPCHEM1\BNA_M\Data\BM071015\
 Data File : BM001890.D
 Acq On : 10 Jul 2015 12:33
 Operator : TP/UM
 Sample : DFTPP71
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP71

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041515.M
 Title : SVOA CALIBRATION
 Last Update : Thu Apr 16 05:47:45 2015

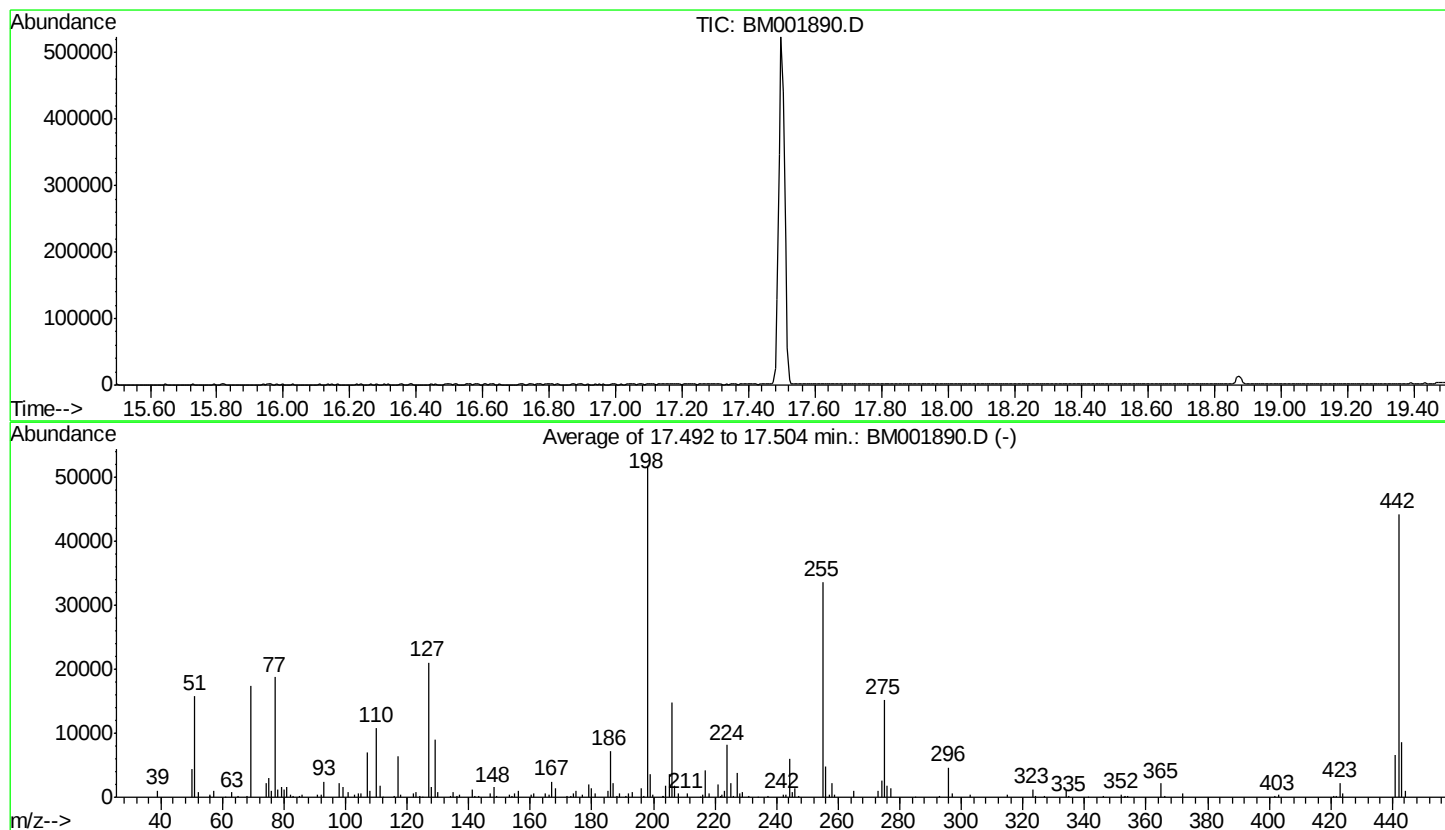

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	15823	PASS
68	69	0.00	2	0.9	158	PASS
69	198	0.00	100	33.7	17449	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.7	21080	PASS
197	198	0.00	2	0.3	166	PASS
198	198	100	100	100.0	51810	PASS
199	198	5	9	6.9	3580	PASS
275	198	10	60	29.4	15234	PASS
365	198	1	100	4.1	2113	PASS
441	443	0.01	100	76.0	6531	PASS
442	198	50	100	85.4	44256	PASS
443	442	15	24	19.4	8592	PASS

m/z	Abundance
39.10	1013.0
44.00	748.0
50.00	3969.0
51.00	15088.0
52.00	885.0
55.90	430.0
56.90	1060.0
63.00	638.0
69.00	16384.0
74.10	2048.0
75.00	2828.0
76.00	833.0
77.00	17664.0
78.00	1296.0
79.00	1632.0
80.00	1043.0
81.00	1562.0
82.00	428.0
86.00	405.0
91.00	453.0
92.00	330.0
93.00	2267.0
98.00	2022.0
99.00	1525.0
100.90	658.0
103.00	320.0
103.90	493.0
105.00	625.0
107.00	6564.0
108.00	913.0
110.00	9917.0
111.00	1754.0
117.00	5564.0
117.90	365.0
122.00	452.0
122.90	740.0
124.00	372.0
124.90	306.0
127.00	18320.0
128.00	1635.0
129.00	7904.0
130.00	682.0
135.00	760.0
137.10	416.0
140.90	928.0
143.00	337.0
146.90	589.0
148.00	1396.0
153.00	368.0
154.90	583.0
156.00	970.0
160.00	395.0
161.00	545.0
164.90	446.0
167.00	1994.0
168.00	1320.0
173.90	467.0
175.00	1018.0
176.80	377.0
179.00	1548.0
180.00	1055.0
181.10	491.0
185.10	767.0
186.00	5999.0
187.00	1810.0
189.00	404.0
191.90	388.0
193.00	709.0
196.00	1169.0
198.00	41488.0
198.90	2933.0
199.90	312.0
202.90	334.0
204.00	1479.0
205.00	3008.0
206.00	11867.0
207.00	2066.0
208.00	474.0
211.00	420.0
216.00	423.0
216.90	3547.0
218.00	480.0
221.10	1644.0
223.00	845.0
224.00	6739.0
225.00	1568.0
227.00	2974.0
228.00	470.0
229.00	755.0
237.00	334.0
242.00	336.0

Instrument :
BNA_M
ClientSampleId :
DFTPP71

242.90	319.0
244.10	4835.0
245.10	691.0
245.90	1198.0
255.00	25592.0
255.90	3263.0
258.00	1374.0
258.90	335.0
265.00	621.0
273.00	690.0
274.00	1981.0
275.00	11090.0
276.00	1624.0
276.90	965.0
296.00	3813.0
296.90	447.0
314.90	400.0
323.00	899.0
334.10	599.0
352.00	352.0
364.90	1593.0
372.10	431.0
423.00	1488.0
424.00	458.0
441.00	3828.0
442.10	26936.0
443.00	5164.0
444.00	610.0

Instrument :
BNA_M
ClientSampleId :
DFTPP71

m/z	Abundance
39.00	1106.0
43.90	714.0
50.00	3902.0
51.00	13335.0
52.00	633.0
56.00	444.0
57.00	956.0
63.00	631.0
65.00	322.0
69.00	15436.0
74.00	1670.0
75.00	2472.0
76.00	987.0
77.10	16248.0
78.10	1135.0
79.00	1625.0
80.00	1006.0
80.90	1261.0
82.10	340.0
85.10	346.0
91.90	409.0
93.00	2152.0
98.00	1942.0
99.00	1481.0
100.90	834.0
102.90	346.0
104.00	561.0
105.00	548.0
107.00	5874.0
107.90	975.0
110.00	9923.0
111.00	1594.0
116.00	474.0
117.00	5969.0
118.00	373.0
122.00	653.0
123.00	650.0
127.00	19488.0
128.00	1578.0
129.00	8395.0
130.00	753.0
135.00	593.0
137.00	462.0
140.90	1326.0
142.00	373.0
147.00	519.0
148.00	1481.0
153.00	524.0
154.00	363.0
155.00	605.0
156.00	821.0
160.10	484.0
160.90	574.0
165.00	464.0
165.90	453.0
167.00	2590.0
168.00	1279.0
171.90	402.0
172.90	347.0
174.00	373.0
175.00	993.0
176.90	564.0
179.00	2131.0
180.00	1452.0
181.00	713.0
185.00	1009.0
186.00	7476.0
187.00	1907.0
188.00	413.0
188.90	563.0
191.90	665.0
193.00	732.0
195.90	1418.0
198.00	50600.0
198.90	3444.0
199.90	304.0
203.00	432.0
204.00	1796.0
205.00	3869.0
206.00	15123.0
207.00	2370.0
207.90	591.0
211.00	525.0
216.00	394.0
216.90	4131.0
218.00	718.0
221.00	1983.0
222.00	449.0
223.00	989.0
224.00	8202.0
225.00	2274.0

Instrument :
BNA_M
ClientSampleId :
DFTPP71

227.00	4013.0
227.90	725.0
228.90	676.0
230.90	355.0
242.10	459.0
243.10	516.0
244.00	6061.0
245.10	817.0
246.00	1535.0
255.00	35248.0
256.00	5005.0
256.90	566.0
258.00	2538.0
259.00	329.0
264.90	997.0
272.90	897.0
274.00	2512.0
275.00	16372.0
276.00	1851.0
276.90	1628.0
284.90	315.0
292.90	368.0
296.00	5012.0
297.00	631.0
302.90	638.0
315.00	435.0
323.10	1480.0
323.90	354.0
334.00	1073.0
341.00	310.0
346.00	444.0
351.90	486.0
353.00	325.0
354.10	382.0
365.00	2261.0
366.00	335.0
372.00	916.0
402.00	354.0
403.00	655.0
421.00	461.0
421.90	480.0
423.10	2968.0
424.10	702.0
441.10	7540.0
442.10	55096.0
443.10	10414.0
444.00	1226.0

Instrument :

BNA_M

ClientSampleId :

DFTPP71

m/z	Abundance
39.00	1071.0
44.00	676.0
50.10	5080.0
51.10	19048.0
52.00	924.0
56.10	575.0
57.00	1245.0
61.00	315.0
63.00	1013.0
65.00	338.0
68.10	474.0
69.00	20528.0
74.00	2840.0
75.00	3656.0
76.10	1184.0
77.10	22392.0
78.00	1491.0
79.00	1817.0
80.00	1405.0
81.00	1723.0
81.90	506.0
82.90	440.0
85.00	406.0
86.00	647.0
91.00	519.0
92.10	445.0
93.00	3075.0
98.00	2648.0
99.00	1967.0
101.00	972.0
103.10	304.0
103.90	968.0
105.00	729.0
107.00	8329.0
108.00	1076.0
110.00	12690.0
111.00	2157.0
111.90	304.0
115.90	410.0
117.00	7475.0
118.00	553.0
122.00	592.0
123.00	828.0
127.00	25432.0
128.00	1767.0
129.00	10962.0
129.90	818.0
134.00	380.0
135.00	976.0
136.00	475.0
137.10	407.0
141.00	1415.0
142.00	403.0
147.00	837.0
148.00	1811.0
149.00	368.0
153.00	576.0
154.00	302.0
155.00	817.0
156.00	1464.0
160.00	392.0
161.00	818.0
165.00	703.0
166.00	504.0
167.00	2868.0
168.00	1461.0
171.90	422.0
173.00	509.0
174.00	842.0
175.00	1290.0
176.90	508.0
179.00	2501.0
180.00	1648.0
180.90	639.0
185.00	1160.0
186.00	8167.0
187.00	2698.0
188.00	304.0
189.10	717.0
191.10	325.0
192.00	838.0
193.00	864.0
195.90	1672.0
197.00	500.0
198.00	63344.0
199.00	4364.0
200.00	337.0
203.10	453.0
204.00	2391.0
205.10	4056.0
206.00	17576.0

Instrument :
BNA_M
ClientSampleId :
DFTPP71

207.00	2295.0
207.90	836.0
210.90	704.0
215.00	318.0
216.00	451.0
217.00	4763.0
217.90	583.0
221.00	2581.0
221.70	626.0
222.00	631.0
223.00	1112.0
224.00	9586.0
225.00	2642.0
225.90	384.0
227.00	4356.0
228.00	564.0
229.00	1049.0
230.90	398.0
233.90	317.0
237.00	376.0
242.00	652.0
243.00	473.0
244.00	7233.0
244.90	798.0
246.00	1667.0
247.00	383.0
255.00	40040.0
256.00	5987.0
257.00	528.0
258.00	2639.0
259.00	469.0
265.00	1179.0
273.00	1322.0
274.00	3282.0
275.00	18240.0
276.00	2246.0
276.90	1692.0
293.10	437.0
296.00	5064.0
297.00	866.0
302.90	604.0
314.90	508.0
323.10	1417.0
327.00	363.0
334.00	1146.0
335.00	404.0
346.00	385.0
351.90	443.0
352.80	306.0
354.00	500.0
365.00	2487.0
366.00	360.0
372.10	751.0
403.10	451.0
420.90	369.0
421.90	326.0
423.10	2281.0
423.90	745.0
441.10	8226.0
442.10	50736.0
443.10	10199.0
444.10	900.0

Instrument :
BNA_M
ClientSampleId :
DFTPP71

m/z	Abundance
44.00	853.0
207.10	501.0

Instrument :
BNA_M
ClientSampleId :
DFTPP71