
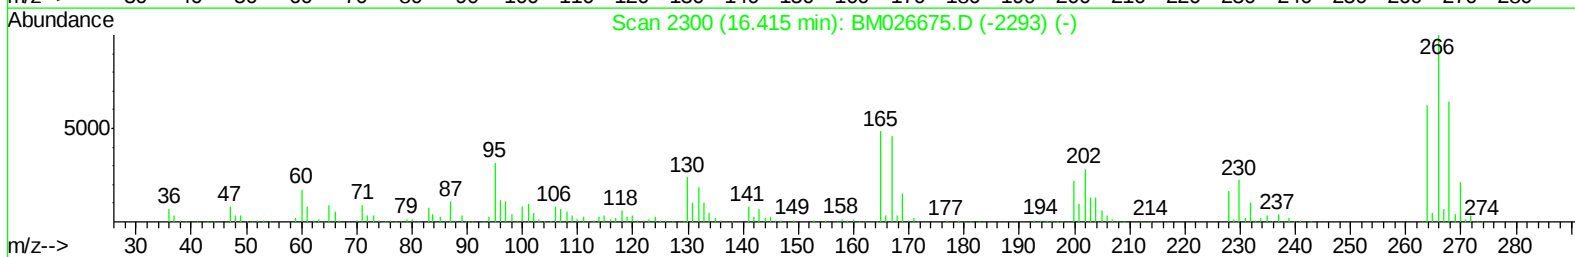
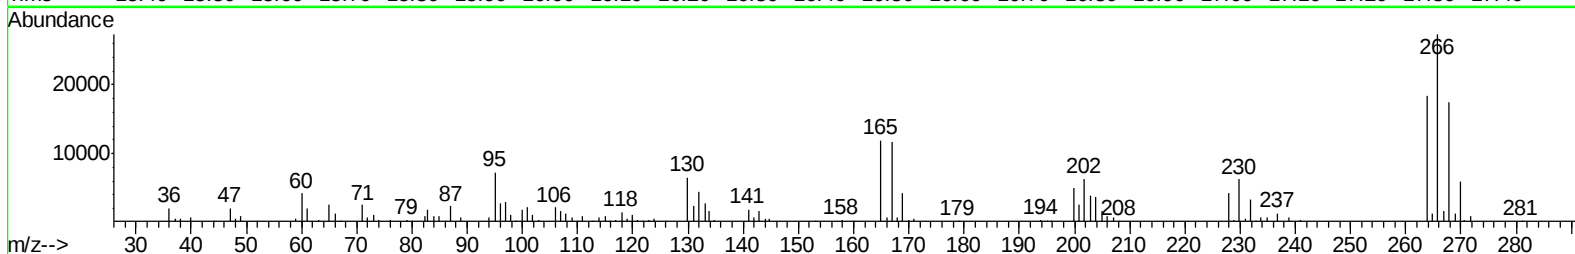


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071020\
Data File : BM026723.D
Acq On : 10 Jul 2020 08:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 00:37:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 10 10:38:33 2020
Response via : Initial Calibration

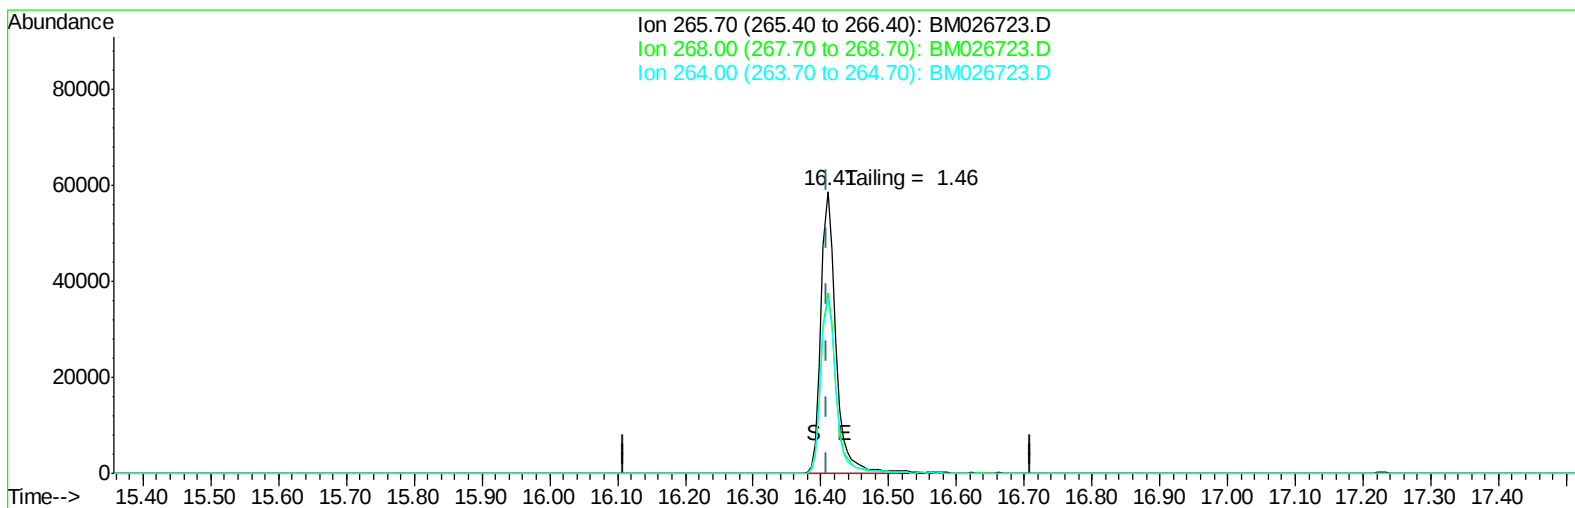

TIC: BM026723.D

(70) Pentachlorophenol (C)




16.410min (+0.000) 8111.30ng

response 88066

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	64.32
264.00	62.60	62.41
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071020\
 Data File : BM026723.D
 Acq On : 10 Jul 2020 08:15
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 00:37:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 10 10:38:33 2020
 Response via : Initial Calibration

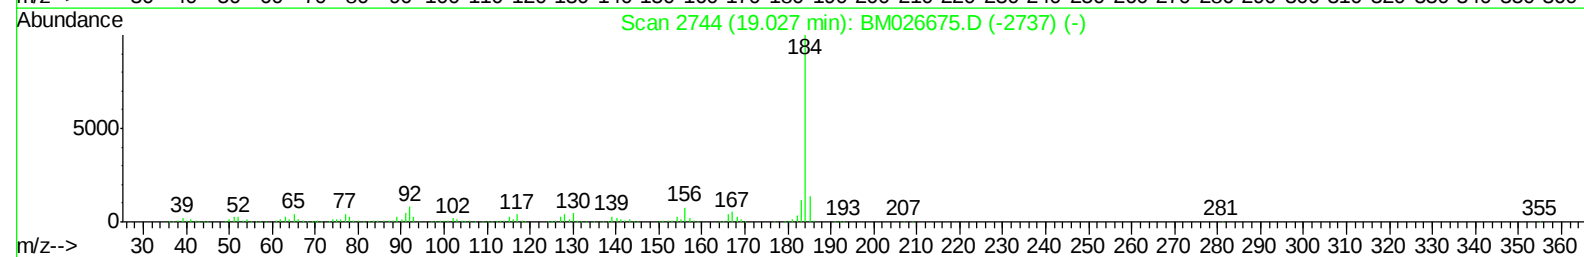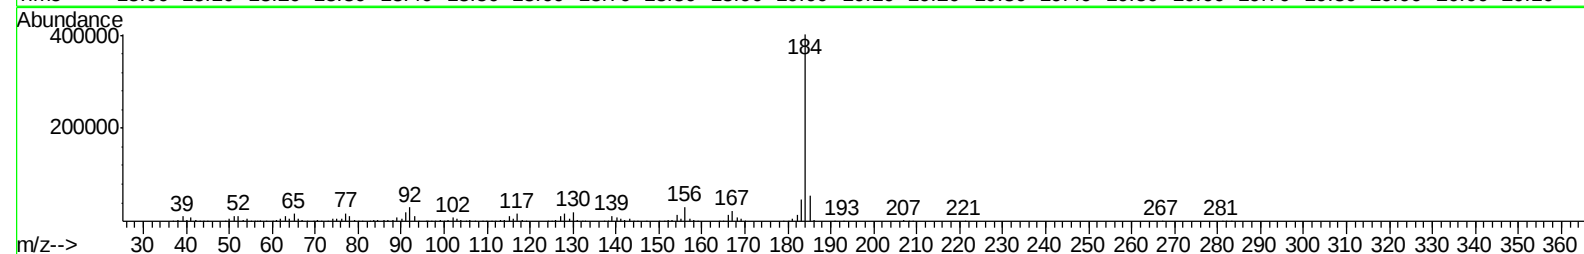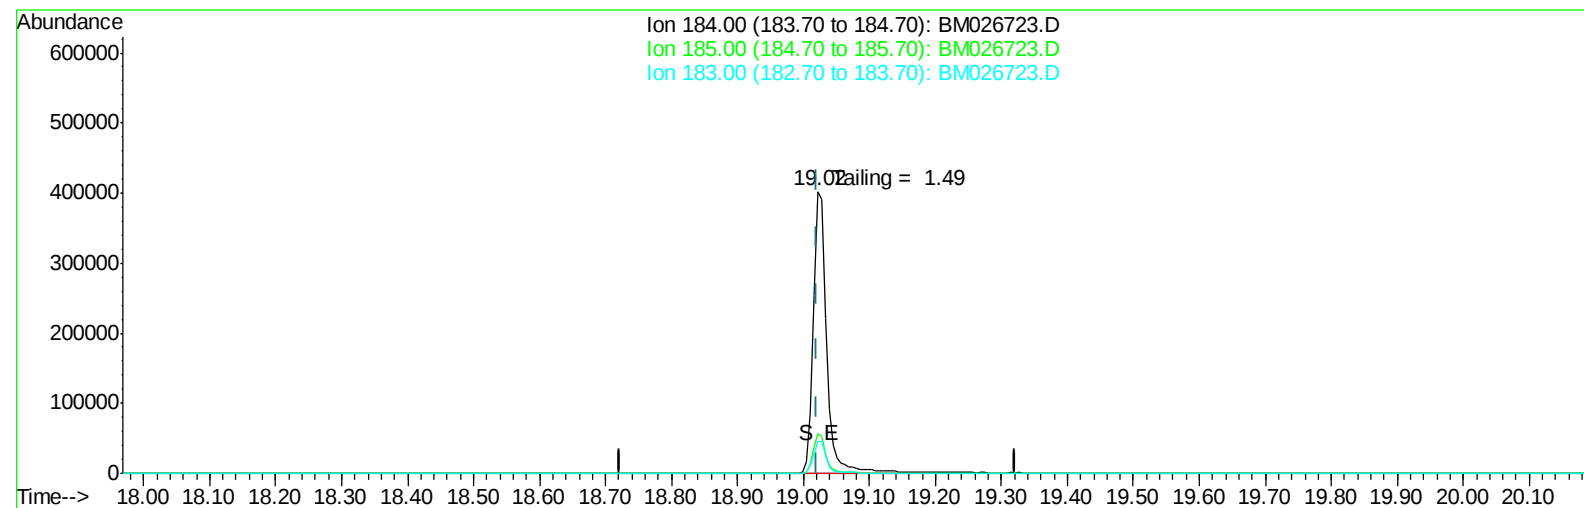

TIC: BM026723.D

(77) Benzidine

19.021min (+0.000) 11480.31ng

response 579415

Ion	Exp%	Act%
184.00	100	100
185.00	13.60	13.90
183.00	11.60	11.43
0.00	0.00	0.00