


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071020\
 Data File : BM026711.D
 Acq On : 09 Jul 2020 08:52
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 09 11:30:08 2020

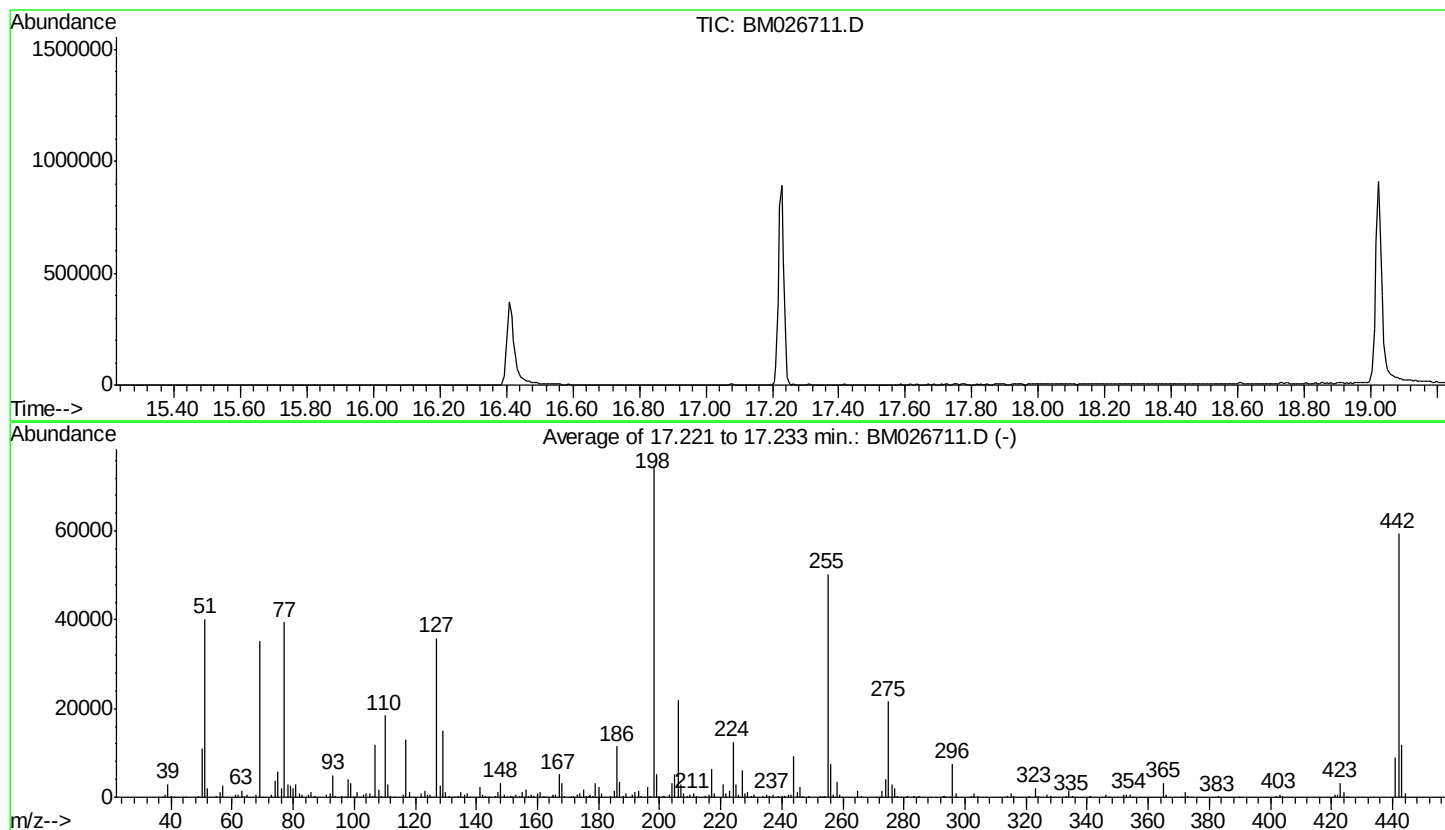

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.7	40162	PASS
68	69	0.00	2	1.9	655	PASS
69	198	0.00	100	47.0	35138	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	48.0	35893	PASS
197	198	0.00	2	0.4	283	PASS
198	198	100	100	100.0	74773	PASS
199	198	5	9	7.0	5253	PASS
275	198	10	60	28.9	21624	PASS
365	198	1	100	4.4	3273	PASS
441	198	0.01	100	12.0	8951	PASS
442	198	50	100	79.4	59370	PASS
443	442	15	24	19.9	11791	PASS