


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071020\
 Data File : BM026723.D
 Acq On : 10 Jul 2020 08:15
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 10 10:38:33 2020

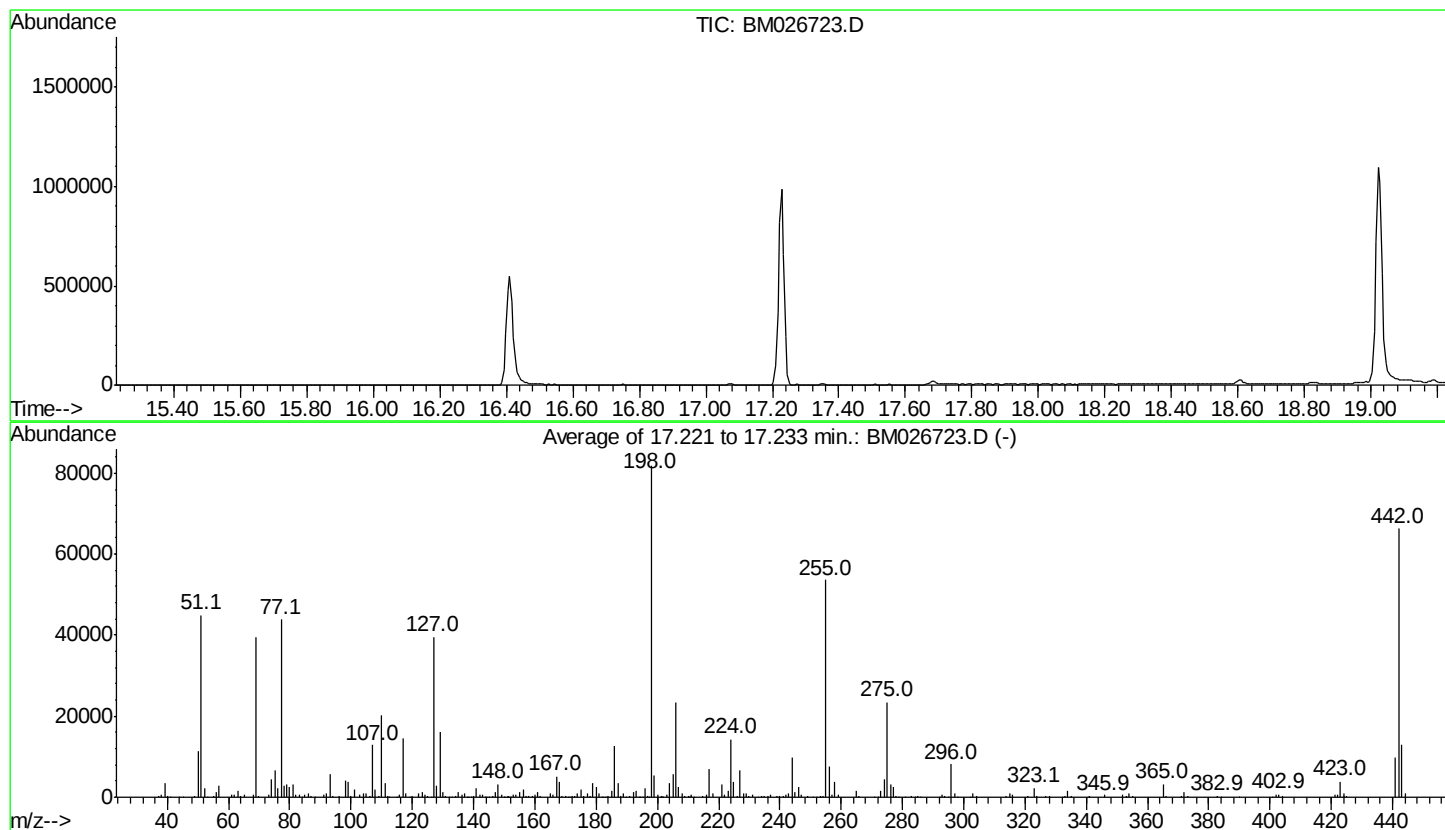

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	45024	PASS
68	69	0.00	2	1.9	740	PASS
69	198	0.00	100	48.3	39570	PASS
70	69	0.00	2	0.6	235	PASS
127	198	10	80	48.3	39520	PASS
197	198	0.00	2	0.5	431	PASS
198	198	100	100	100.0	81856	PASS
199	198	5	9	6.7	5521	PASS
275	198	10	60	28.8	23536	PASS
365	198	1	100	4.0	3315	PASS
441	198	0.01	100	12.2	9960	PASS
442	198	50	100	81.0	66325	PASS
443	442	15	24	19.5	12917	PASS