

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
 Data File : BM050400.D
 Acq On : 10 Jul 2025 21:59
 Operator : RC/JU
 Sample : Q2489-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G4(6-12)

Quant Time: Jul 11 01:28:32 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	597253	20.000	ng	0.00
21) Naphthalene-d8	10.657	136	2214714	20.000	ng	0.00
39) Acenaphthene-d10	14.492	164	1423764	20.000	ng	0.00
64) Phenanthrene-d10	17.221	188	2875413	20.000	ng	0.00
76) Chrysene-d12	21.445	240	3102697	20.000	ng	-0.01
86) Perylene-d12	24.485	264	3090701	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	2036105	58.682	ng	0.00
7) Phenol-d6	7.016	99	1552751	35.500	ng	0.00
23) Nitrobenzene-d5	9.016	82	3621257	83.419	ng	0.00
42) 2,4,6-Tribromophenol	15.968	330	2750567	159.003	ng	0.00
45) 2-Fluorobiphenyl	13.116	172	9537442	82.725	ng	0.00
79) Terphenyl-d14	19.833	244	13090846	74.235	ng	-0.01
Target Compounds						
31) Naphthalene	10.710	128	3023594	26.878	ng	Qvalue 100
32) Benzoic acid	9.922	122	148	5.981	ng	# 1
33) 4-Chloroaniline	10.710	127	391311	8.228	ng	# 33
37) 2-Methylnaphthalene	12.316	142	306779	4.319	ng	97
38) 1-Methylnaphthalene	12.533	142	303775	4.041	ng	98
50) Dimethylphthalate	13.939	163	277947	2.836	ng	100
57) 2,4-Dinitrotoluene	14.839	165	446	2.739	ng	# 36
62) 4-Nitroaniline	15.533	138	732	2.617	ng	# 44
63) Azobenzene	15.839	77	195277	2.271	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050400.D
Acq On : 10 Jul 2025 21:59
Operator : RC/JU
Sample : Q2489-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Quant Time: Jul 11 01:28:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

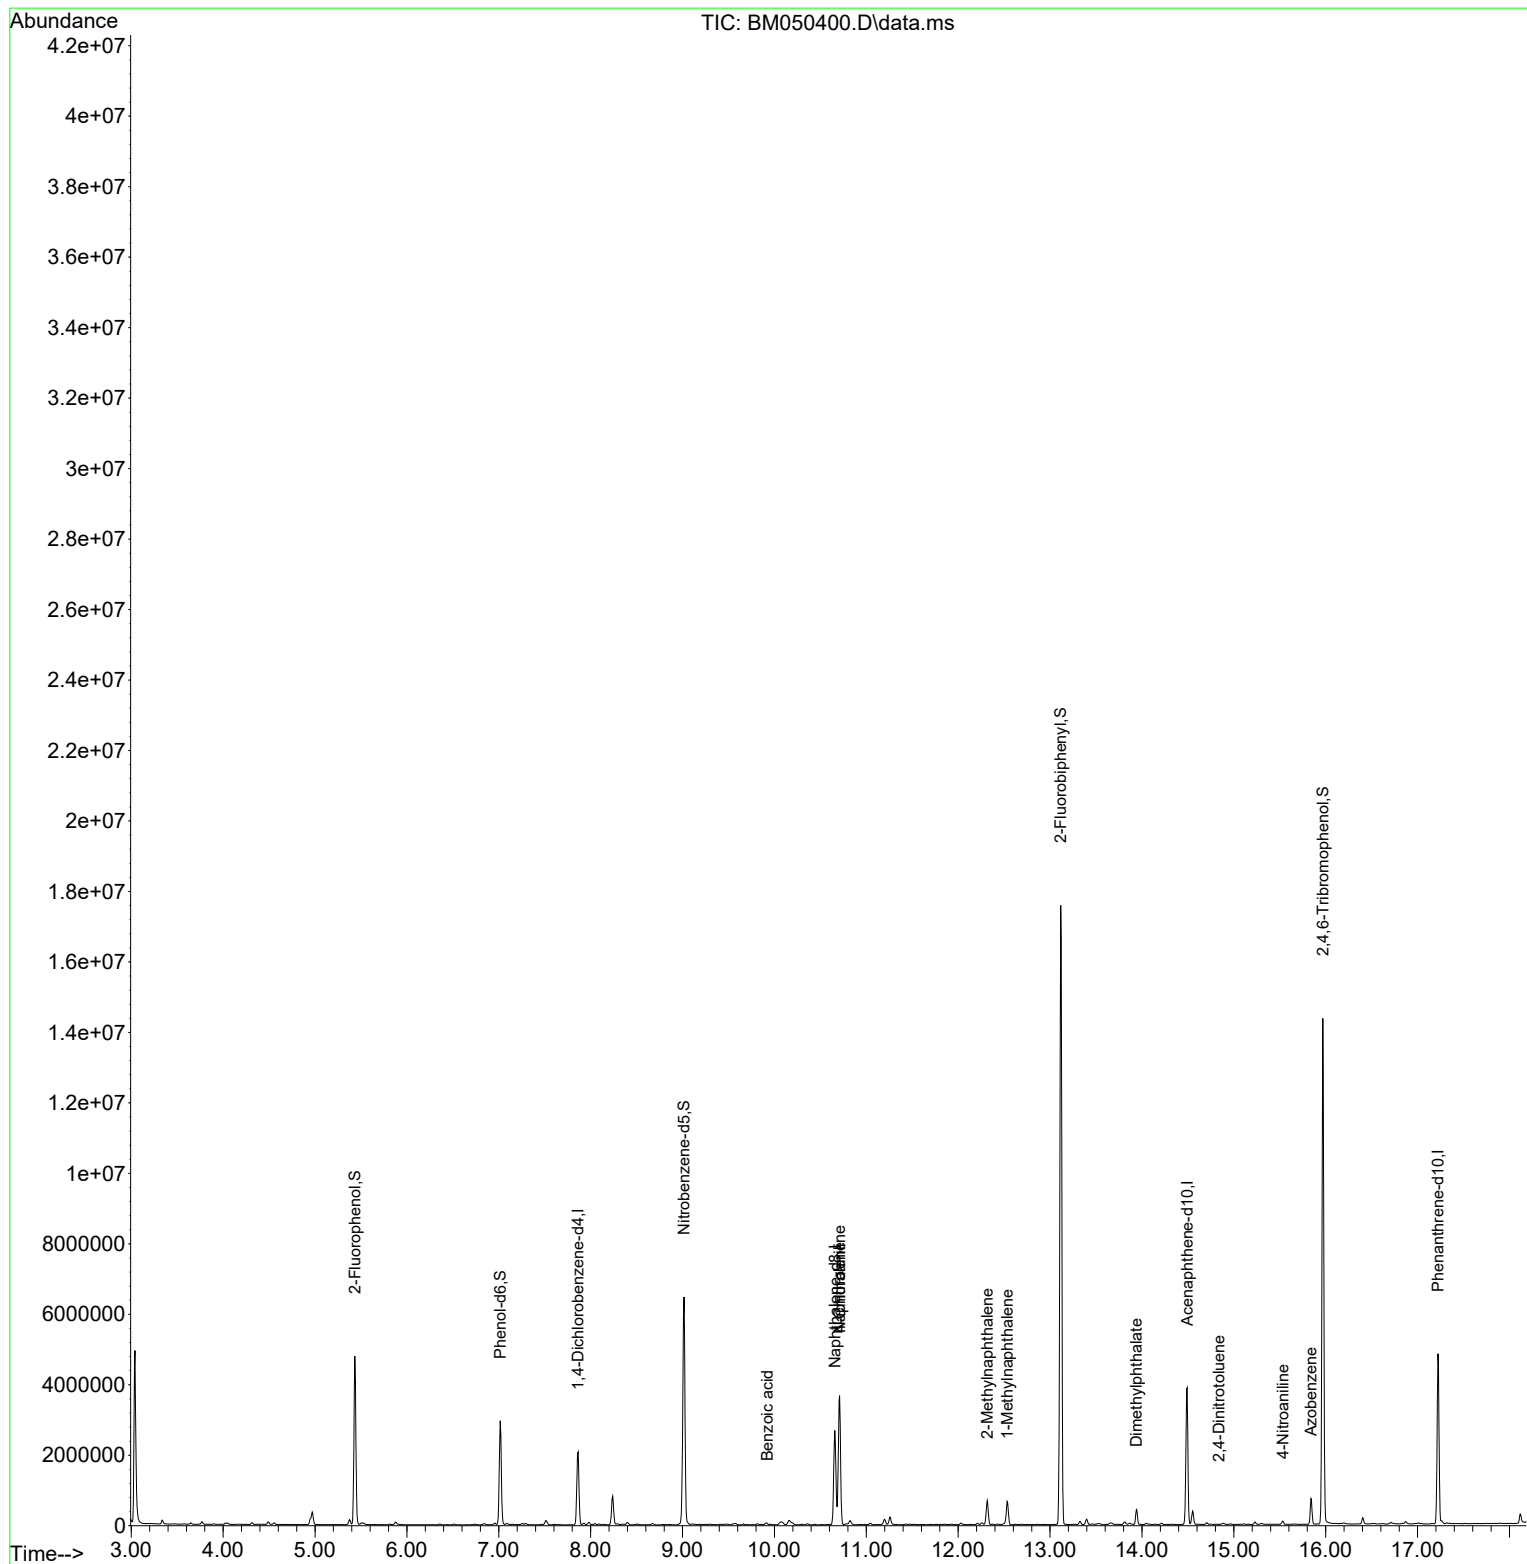


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050400.D
Acq On : 10 Jul 2025 21:59
Operator : RC/JU
Sample : Q2489-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G4(6-12)

Quant Time: Jul 11 01:28:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration




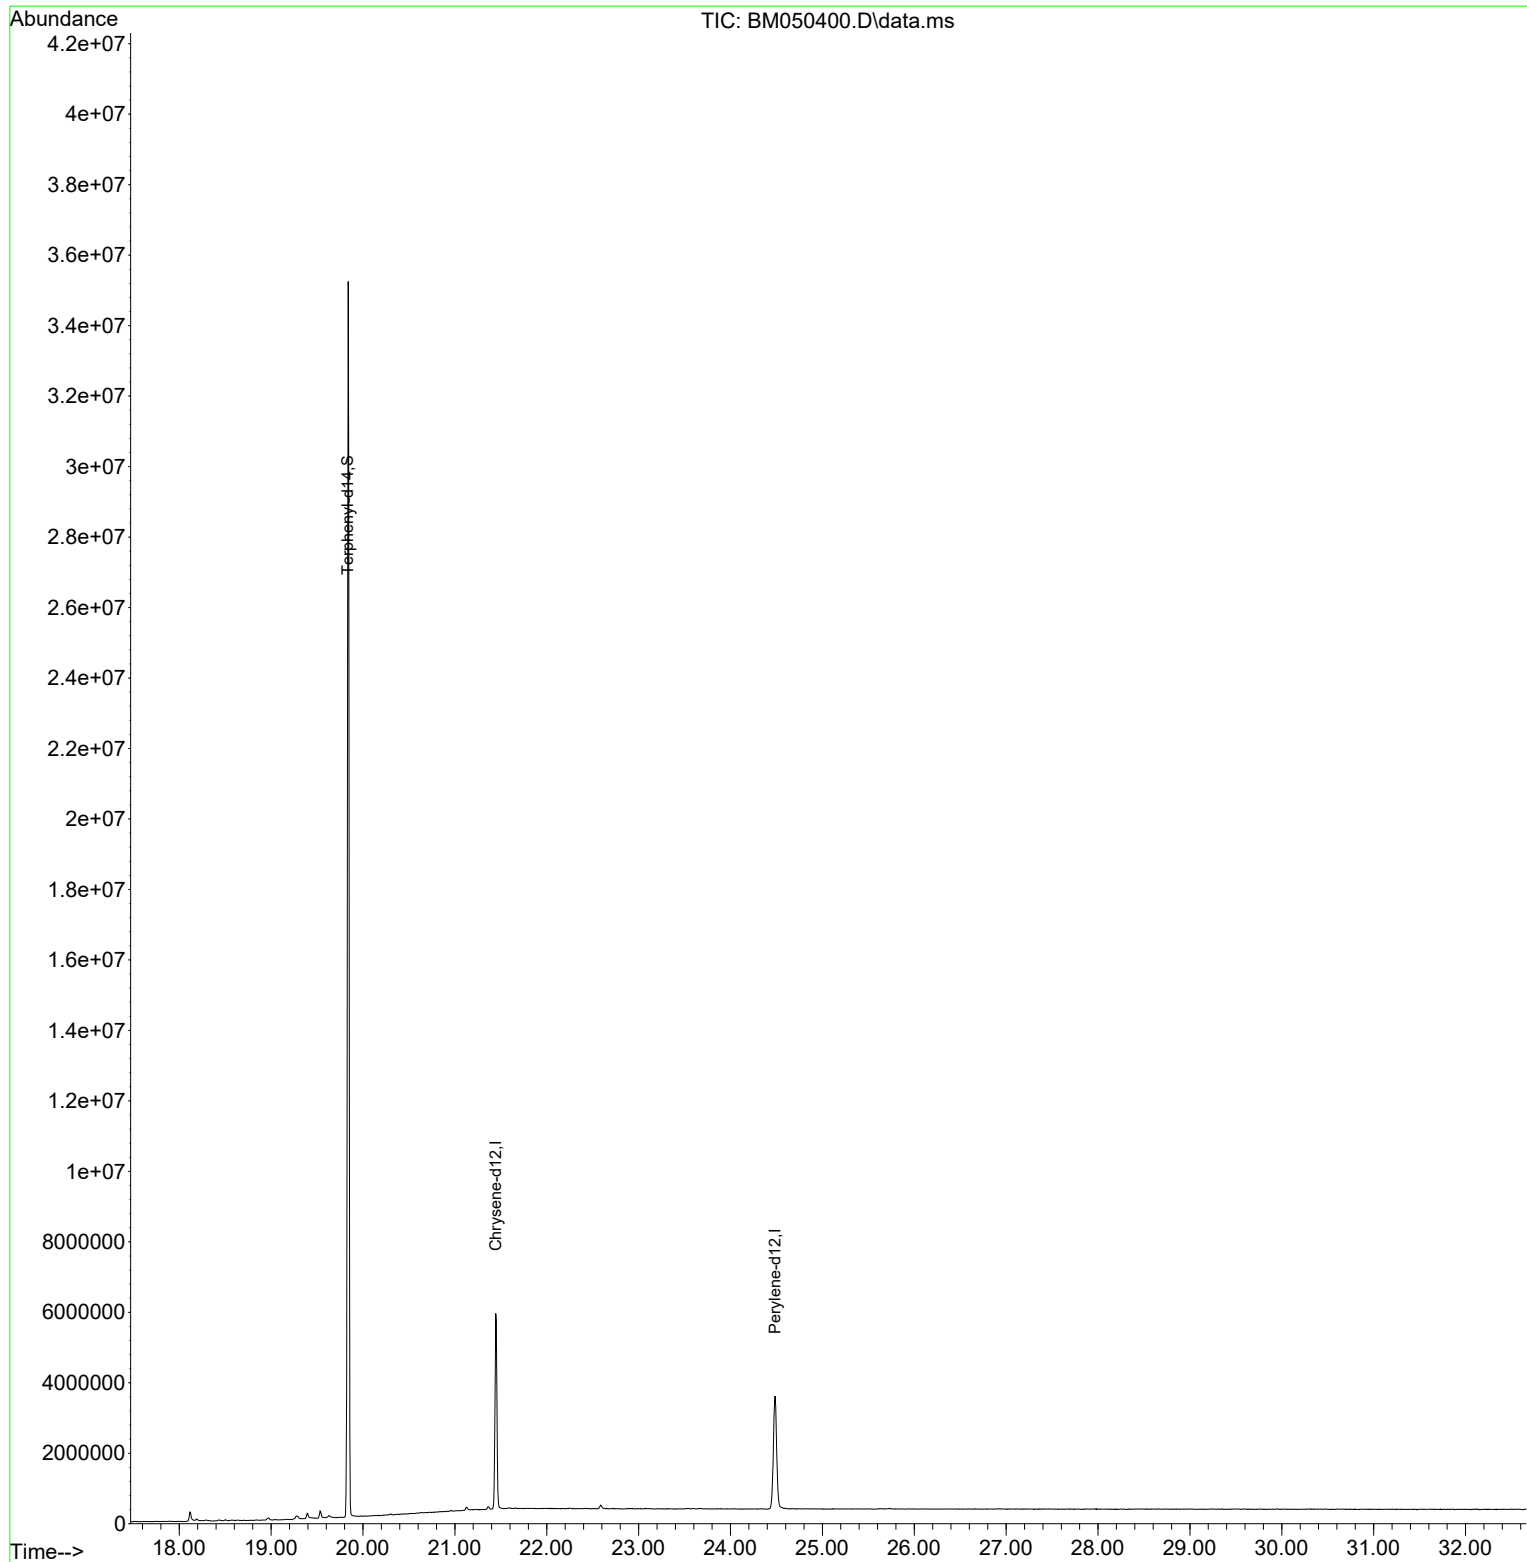


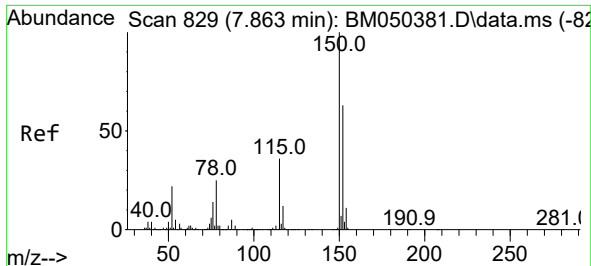

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.863 min Scan# 829
Delta R.T. 0.000 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59




Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Tgt Ion:152 Resp: 597253
Ion Ratio Lower Upper
152 100
150 152.7 126.2 189.4
115 53.9 45.8 68.8

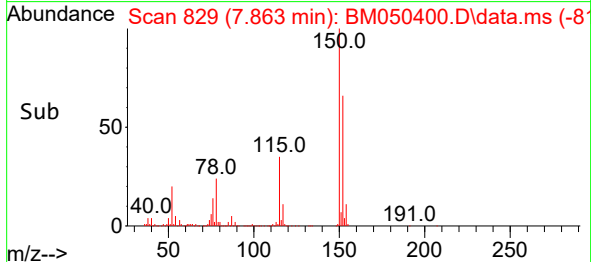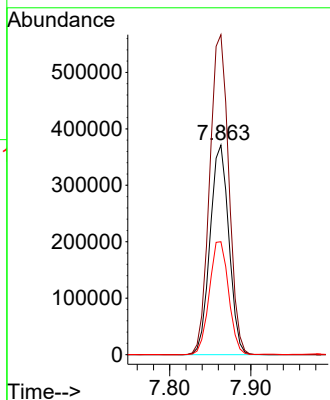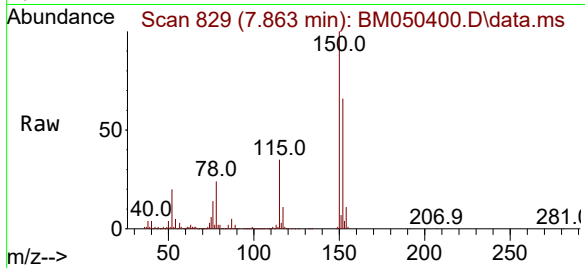

#5
2-Fluorophenol
Concen: 58.682 ng
RT: 5.434 min Scan# 416
Delta R.T. 0.000 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59

Tgt Ion:112 Resp: 2036105
Ion Ratio Lower Upper
112 100
64 55.8 45.5 68.3
63 29.7 24.2 36.4


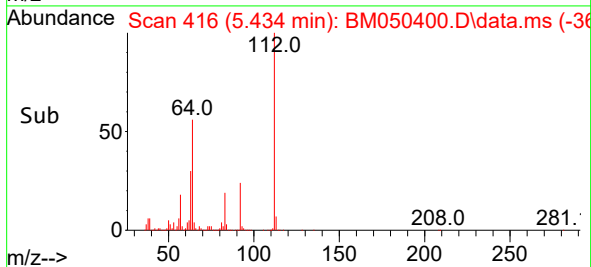
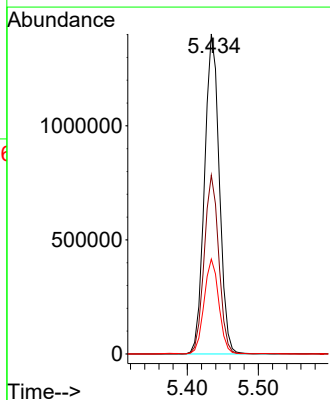
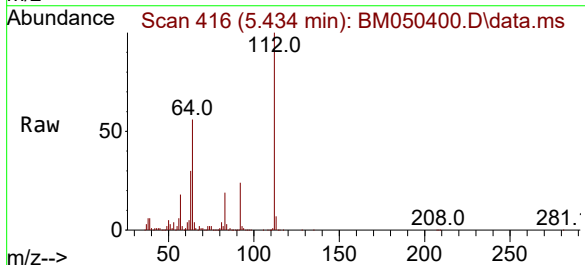


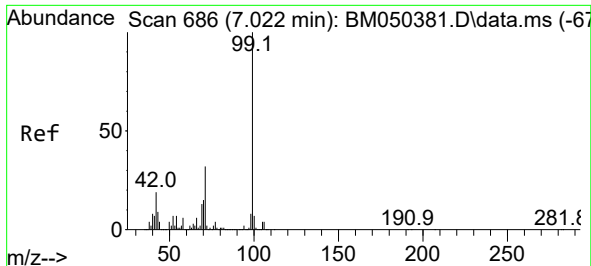

#7
Phenol-d6
Concen: 35.500 ng
RT: 7.016 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59




Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Tgt Ion: 99 Resp: 1552751
Ion Ratio Lower Upper
99 100
42 18.8 15.0 22.6
71 32.4 25.9 38.9

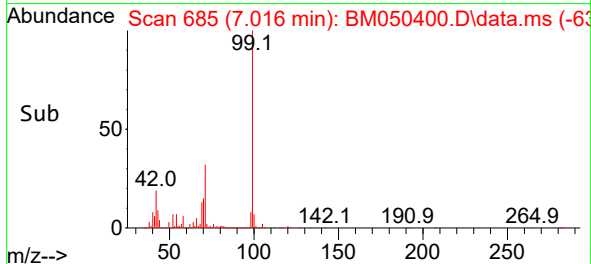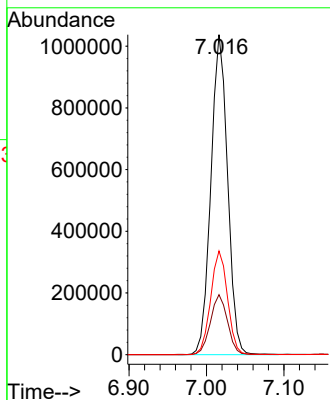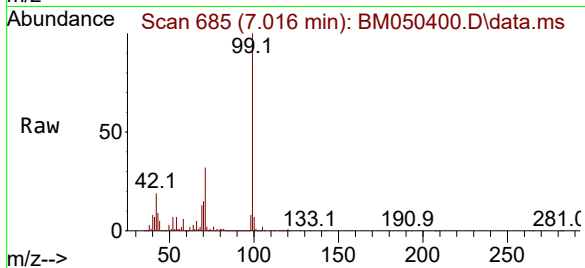

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.657 min Scan# 1304
Delta R.T. -0.006 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59

Tgt Ion: 136 Resp: 2214714
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 7.7 6.3 9.5
68 5.3 4.2 6.2

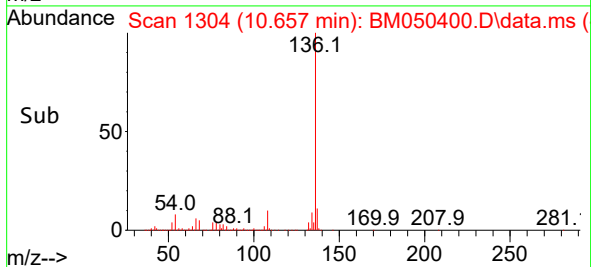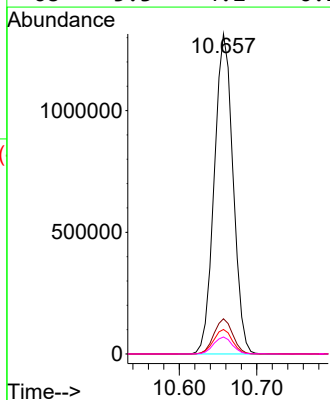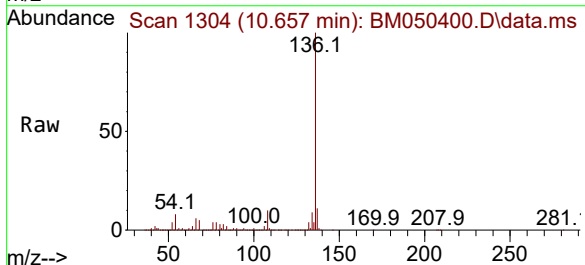

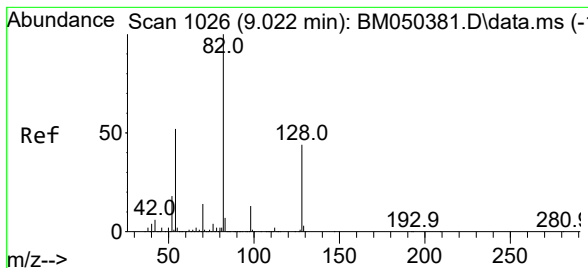

#23

Nitrobenzene-d5

Concen: 83.419 ng

RT: 9.016 min Scan# 1025

Delta R.T. -0.006 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59

Instrument :





BNA_M

ClientSampleId :

G4(6-12)

Tgt Ion: 82 Resp: 3621257

Ion	Ratio	Lower	Upper
82	100		
128	44.0	35.2	52.8
54	49.8	41.5	62.3

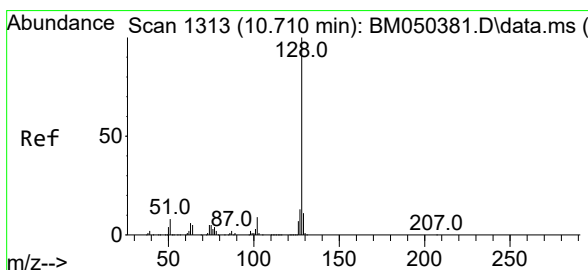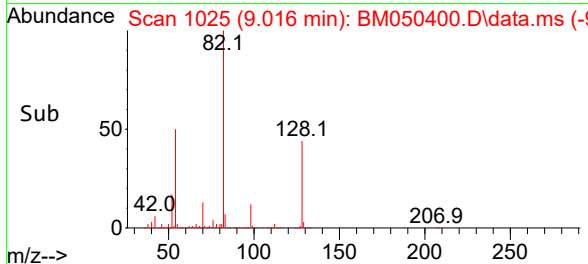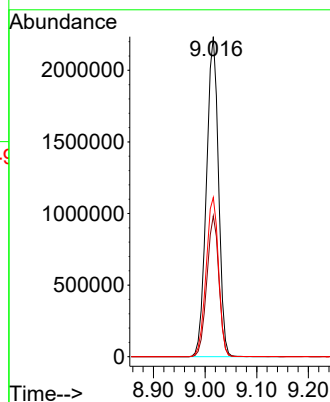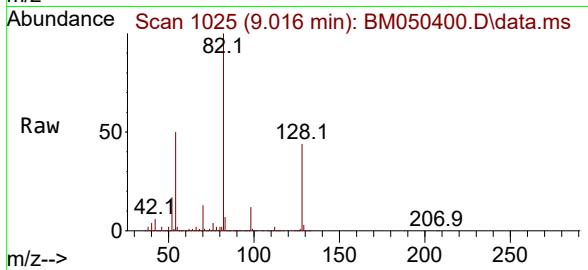

#31

Naphthalene

Concen: 26.878 ng

RT: 10.710 min Scan# 1313




Delta R.T. 0.000 min


Lab File: BM050400.D

Acq: 10 Jul 2025 21:59

Tgt Ion: 128 Resp: 3023594

Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.8	13.2
127	13.0	10.4	15.6

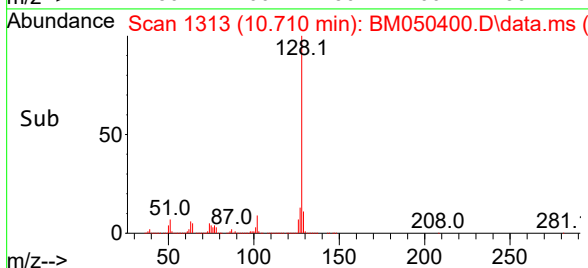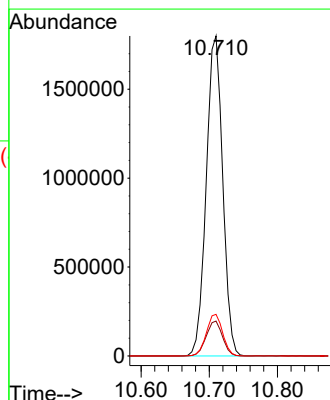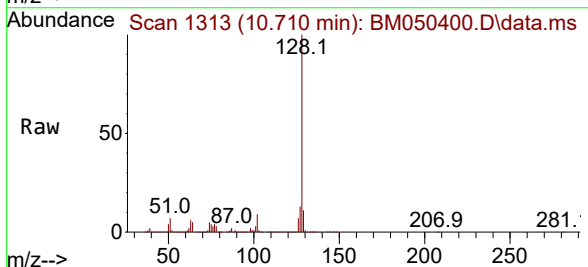



#32

Benzoic acid

Concen: 5.981 ng

RT: 9.922 min Scan# 1183

Delta R.T. -0.023 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59

Instrument :

BNA_M

ClientSampleId :

G4(6-12)





Tgt Ion:122 Resp: 148

Ion Ratio Lower Upper

122 100

105 218.0 104.0 144.0#

77 432.9 73.8 113.8#

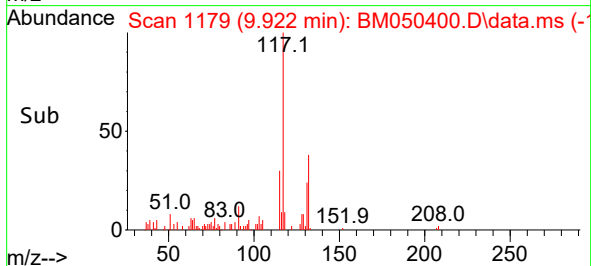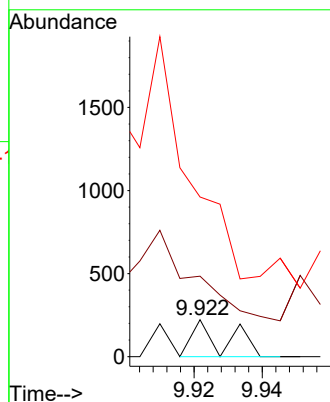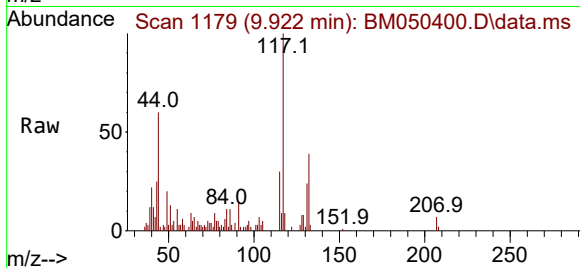

#33

4-Chloroaniline

Concen: 8.228 ng

RT: 10.710 min Scan# 1313

Delta R.T. -0.100 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59

Tgt Ion:127 Resp: 391311




Ion Ratio Lower Upper


127 100

129 84.0 25.5 38.3#

65 0.0 23.9 35.9#

92 0.1 14.6 21.8#

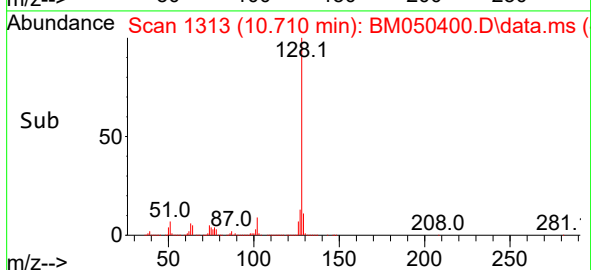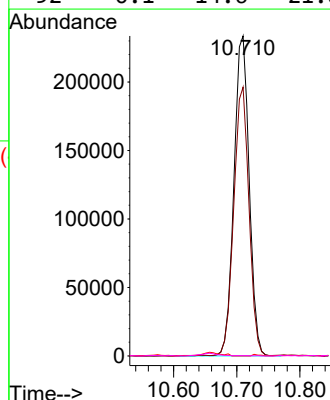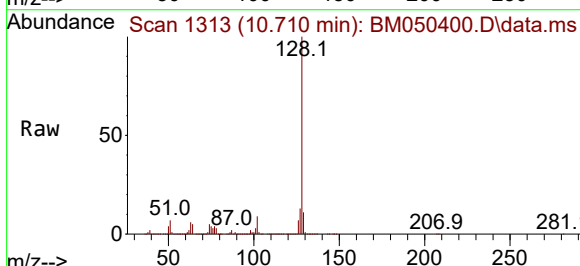

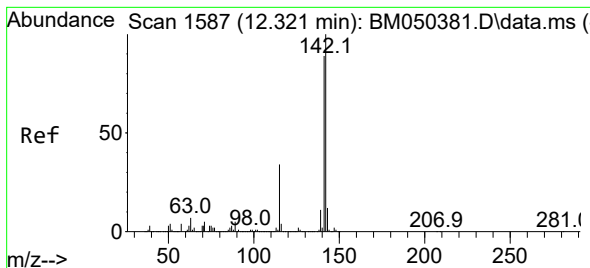

#37

2-Methylnaphthalene

Concen: 4.319 ng

RT: 12.316 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59

Instrument :

BNA_M

ClientSampleId :

G4(6-12)





Tgt Ion:142 Resp: 306779

Ion Ratio Lower Upper

142 100

141 85.0 70.8 106.2

115 35.3 27.0 40.4

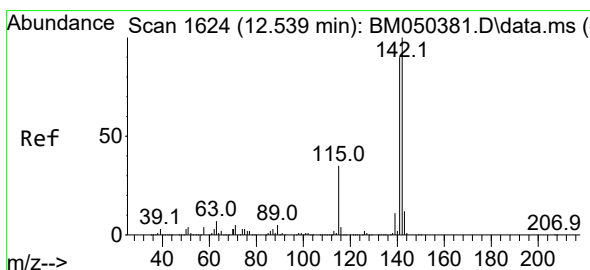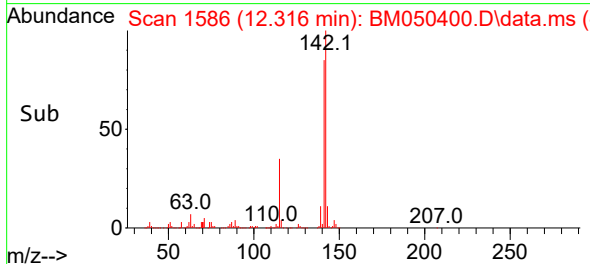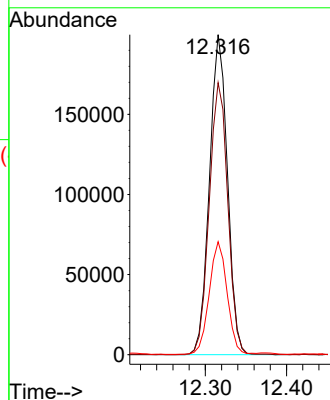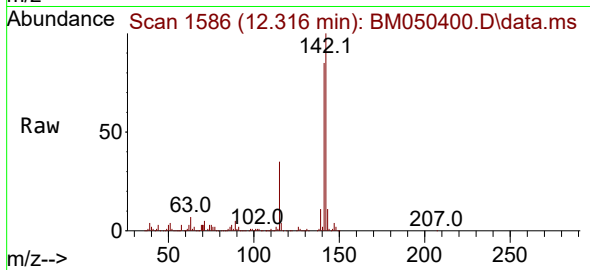

#38

1-Methylnaphthalene

Concen: 4.041 ng

RT: 12.533 min Scan# 1623

Delta R.T. -0.006 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59




Tgt Ion:142 Resp: 303775


Ion Ratio Lower Upper

142 100

141 88.4 71.9 107.9

116 3.4 3.0 4.6


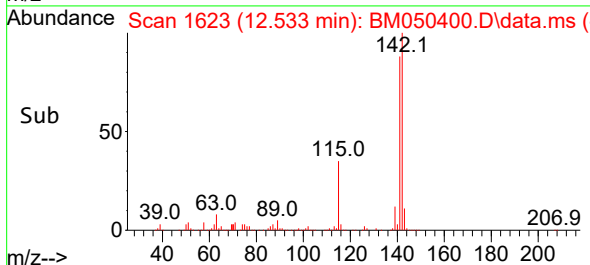
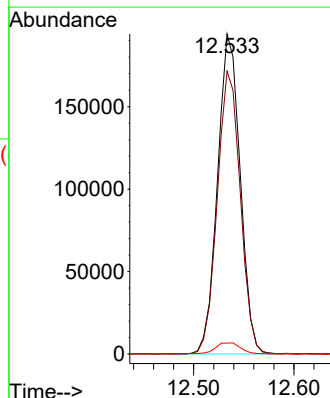
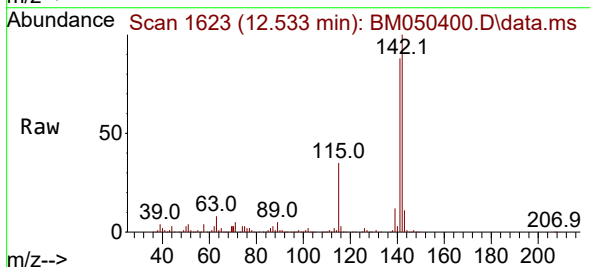


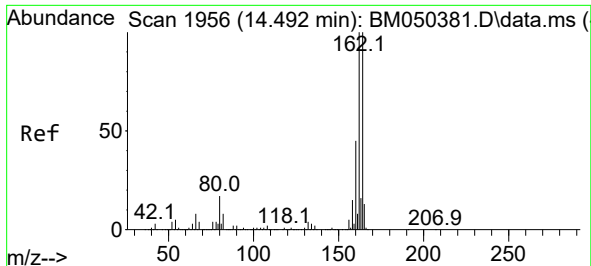

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.492 min Scan# 1956
Delta R.T. 0.000 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59




Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Tgt Ion:164 Resp: 1423764
Ion Ratio Lower Upper
164 100
162 99.5 79.9 119.9
160 45.6 36.2 54.4

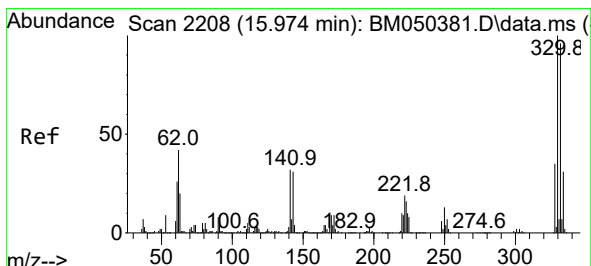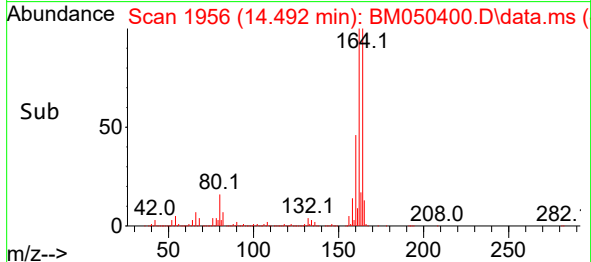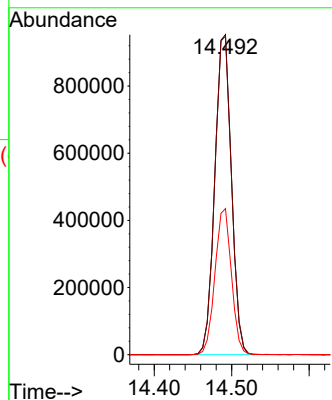

#42
2,4,6-Tribromophenol
Concen: 159.003 ng
RT: 15.968 min Scan# 2207
Delta R.T. -0.006 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59

Tgt Ion:330 Resp: 2750567
Ion Ratio Lower Upper
330 100
332 96.5 76.9 115.3
141 30.5 27.4 41.0


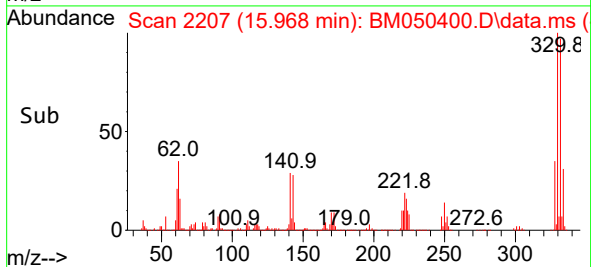
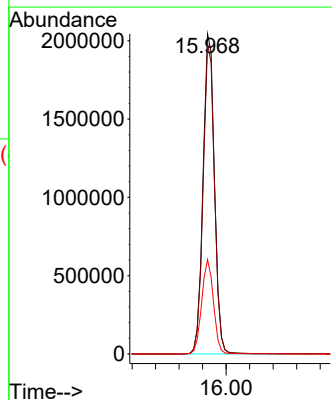
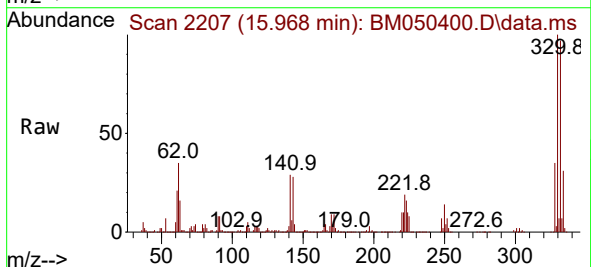


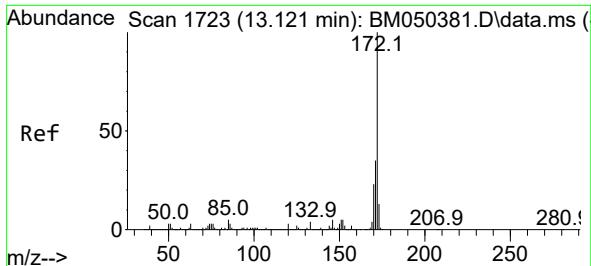

#45
2-Fluorobiphenyl
Concen: 82.725 ng
RT: 13.116 min Scan# 1722
Delta R.T. -0.006 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59




Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Tgt Ion:172 Resp: 9537442
Ion Ratio Lower Upper
172 100
171 34.9 27.7 41.5
170 23.5 18.8 28.2

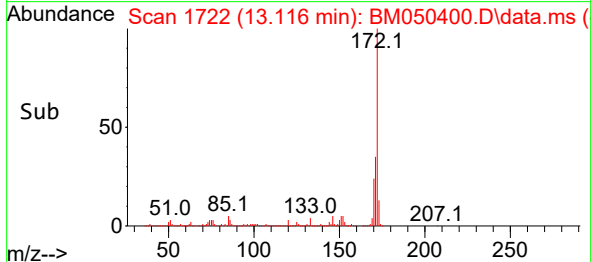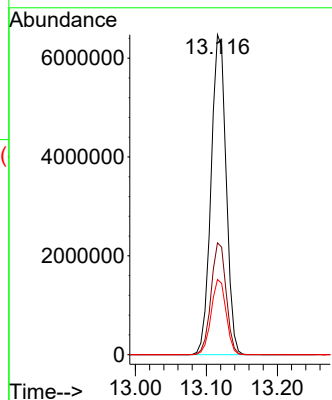

#50
Dimethylphthalate
Concen: 2.836 ng
RT: 13.939 min Scan# 1862
Delta R.T. -0.012 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59

Tgt Ion:163 Resp: 277947
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.2
164 10.3 8.2 12.2


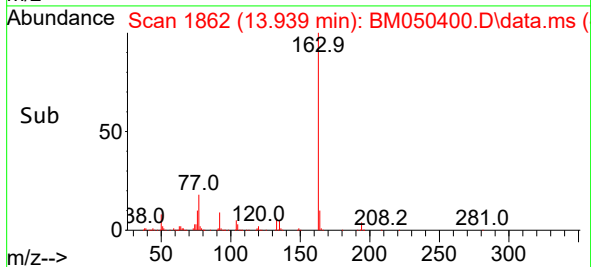
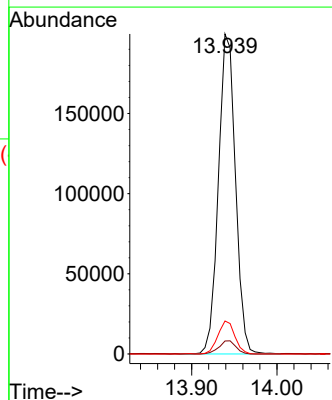
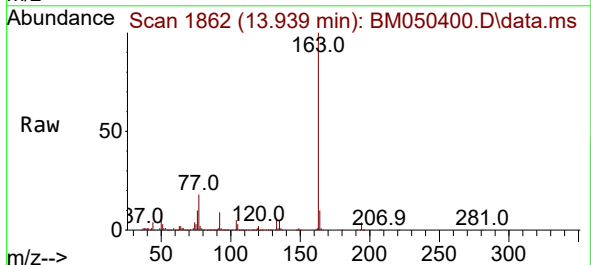


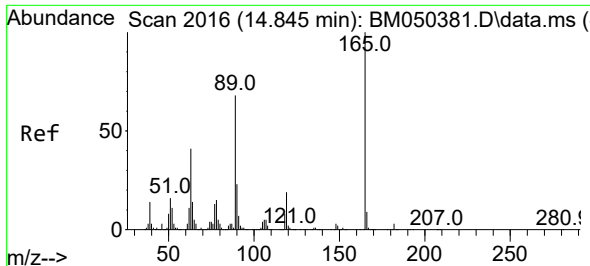

#57
2,4-Dinitrotoluene
Concen: 2.739 ng
RT: 14.839 min Scan# 2016
Delta R.T. -0.006 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59




Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Tgt Ion:165 Resp: 446
Ion Ratio Lower Upper
165 100
63 62.8 32.5 48.7#
89 0.0 54.0 81.0#
182 0.0 2.0 3.0#

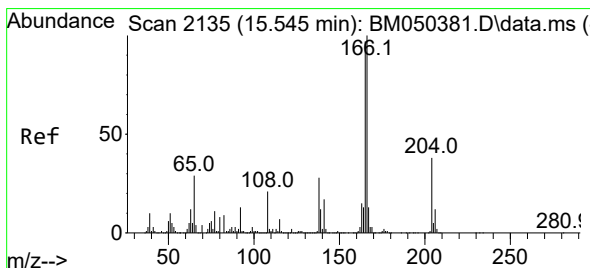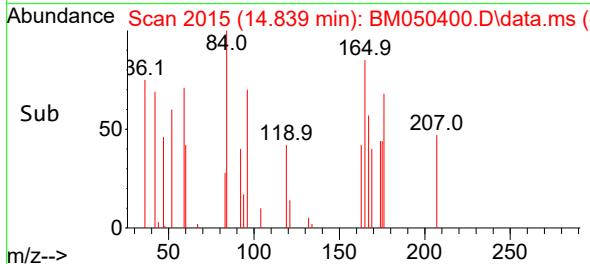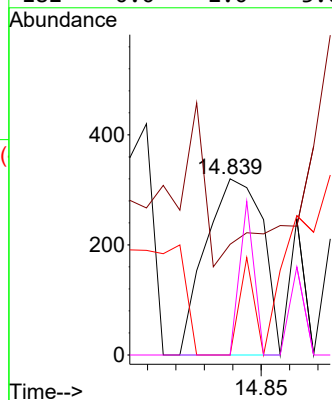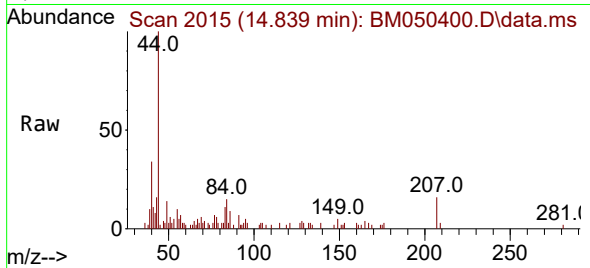

#62
4-Nitroaniline
Concen: 2.617 ng
RT: 15.533 min Scan# 2133
Delta R.T. -0.012 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59

Tgt Ion:138 Resp: 732
Ion Ratio Lower Upper
138 100
92 0.0 24.5 64.5#
108 32.4 52.5 92.5#


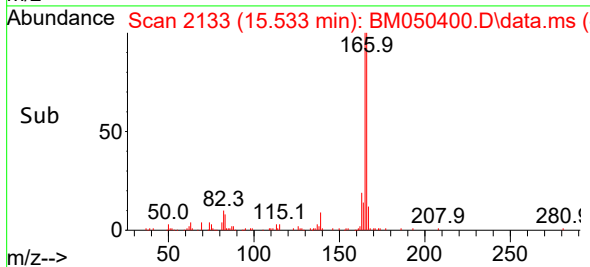
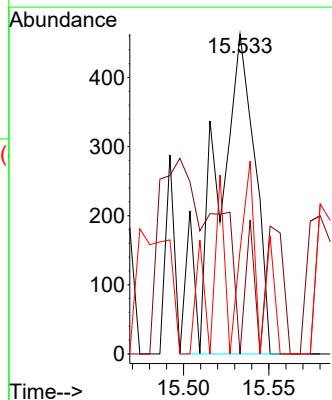
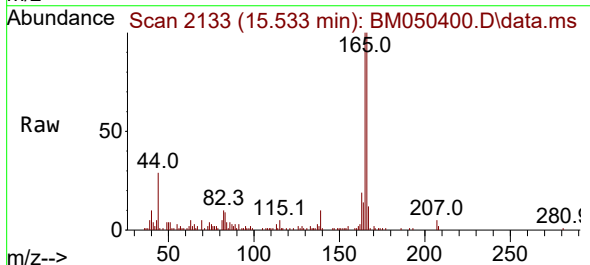




#63
Azobenzene
Concen: 2.271 ng
RT: 15.839 min Scan# 2185
Delta R.T. 0.012 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59




Instrument :
BNA_M
ClientSampleId :
G4(6-12)


Tgt Ion: 77 Resp: 195277
Ion Ratio Lower Upper
77 100
182 84.1 10.0 50.0#
105 145.5 2.0 42.0#
51 43.8 11.7 51.7

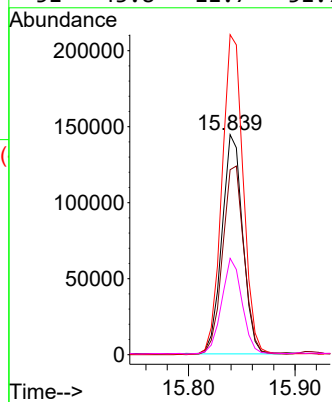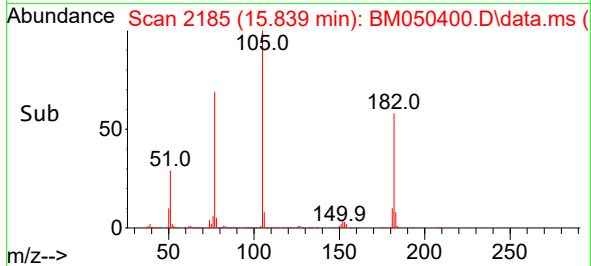

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.221 min Scan# 2420
Delta R.T. -0.006 min
Lab File: BM050400.D
Acq: 10 Jul 2025 21:59

Tgt Ion:188 Resp: 2875413
Ion Ratio Lower Upper
188 100
94 7.7 6.0 9.0
80 8.3 6.5 9.7

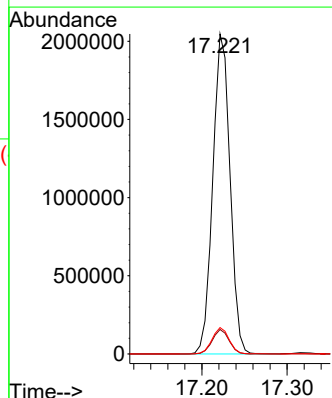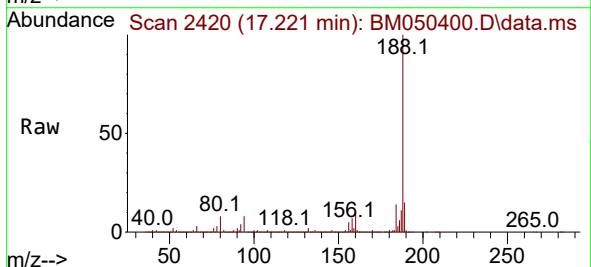



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.445 min Scan# 3140

Delta R.T. -0.012 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59

Instrument :

BNA_M

ClientSampleId :

G4(6-12)





Tgt Ion:240 Resp: 3102697

Ion Ratio Lower Upper

240 100

120 8.8 6.7 10.1

236 26.5 20.7 31.1

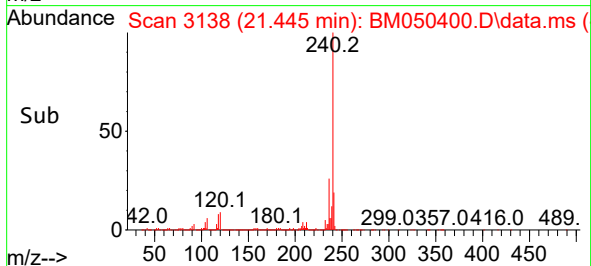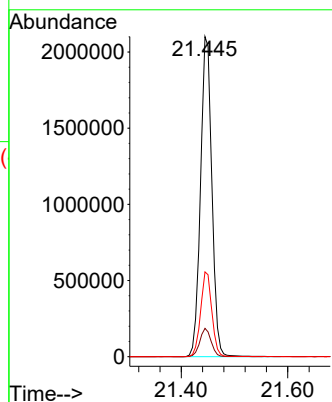

#79

Terphenyl-d14

Concen: 74.235 ng

RT: 19.833 min Scan# 2864

Delta R.T. -0.012 min

Lab File: BM050400.D

Acq: 10 Jul 2025 21:59




Tgt Ion:244 Resp:13090846


Ion Ratio Lower Upper

244 100

212 8.6 5.7 8.5#

122 10.6 6.2 9.2#

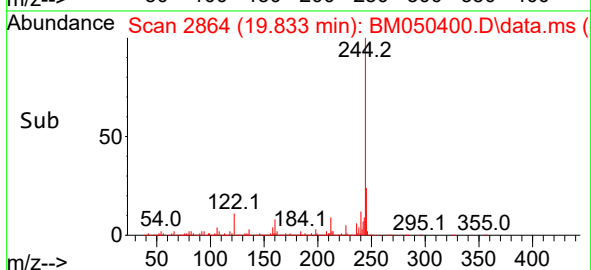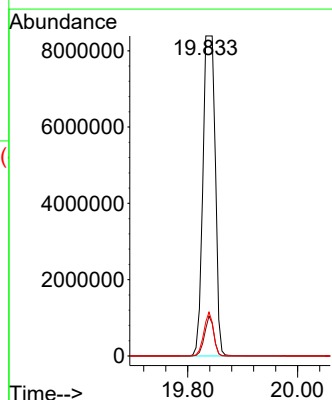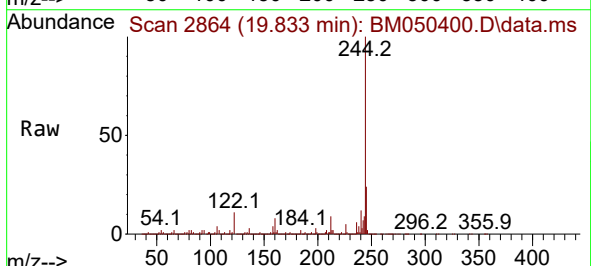



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.485 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: BM050400.D
 Acq: 10 Jul 2025 21:59

Instrument :
 BNA_M
 ClientSampleId :
 G4(6-12)

Tgt Ion:264 Resp: 3090701
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.2 28.8
 265 21.7 17.8 26.6

