

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
 Data File : BM050401.D
 Acq On : 10 Jul 2025 22:39
 Operator : RC/JU
 Sample : Q2489-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G3(0-6)

Quant Time: Jul 11 01:28:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	538062	20.000	ng	0.00
21) Naphthalene-d8	10.657	136	2010300	20.000	ng	0.00
39) Acenaphthene-d10	14.486	164	1320616	20.000	ng	0.00
64) Phenanthrene-d10	17.221	188	2672284	20.000	ng	0.00
76) Chrysene-d12	21.445	240	2968688	20.000	ng	-0.01
86) Perylene-d12	24.486	264	3080582	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	1883570	60.257	ng	0.00
7) Phenol-d6	7.016	99	1441309	36.577	ng	0.00
23) Nitrobenzene-d5	9.016	82	3335262	84.643	ng	0.00
42) 2,4,6-Tribromophenol	15.968	330	2552013	159.047	ng	0.00
45) 2-Fluorobiphenyl	13.116	172	8561125	80.057	ng	0.00
79) Terphenyl-d14	19.833	244	12530171	74.263	ng	-0.01
Target Compounds						
50) Dimethylphthalate	13.939	163	914525	10.058	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050401.D
Acq On : 10 Jul 2025 22:39
Operator : RC/JU
Sample : Q2489-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G3(0-6)

Quant Time: Jul 11 01:28:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

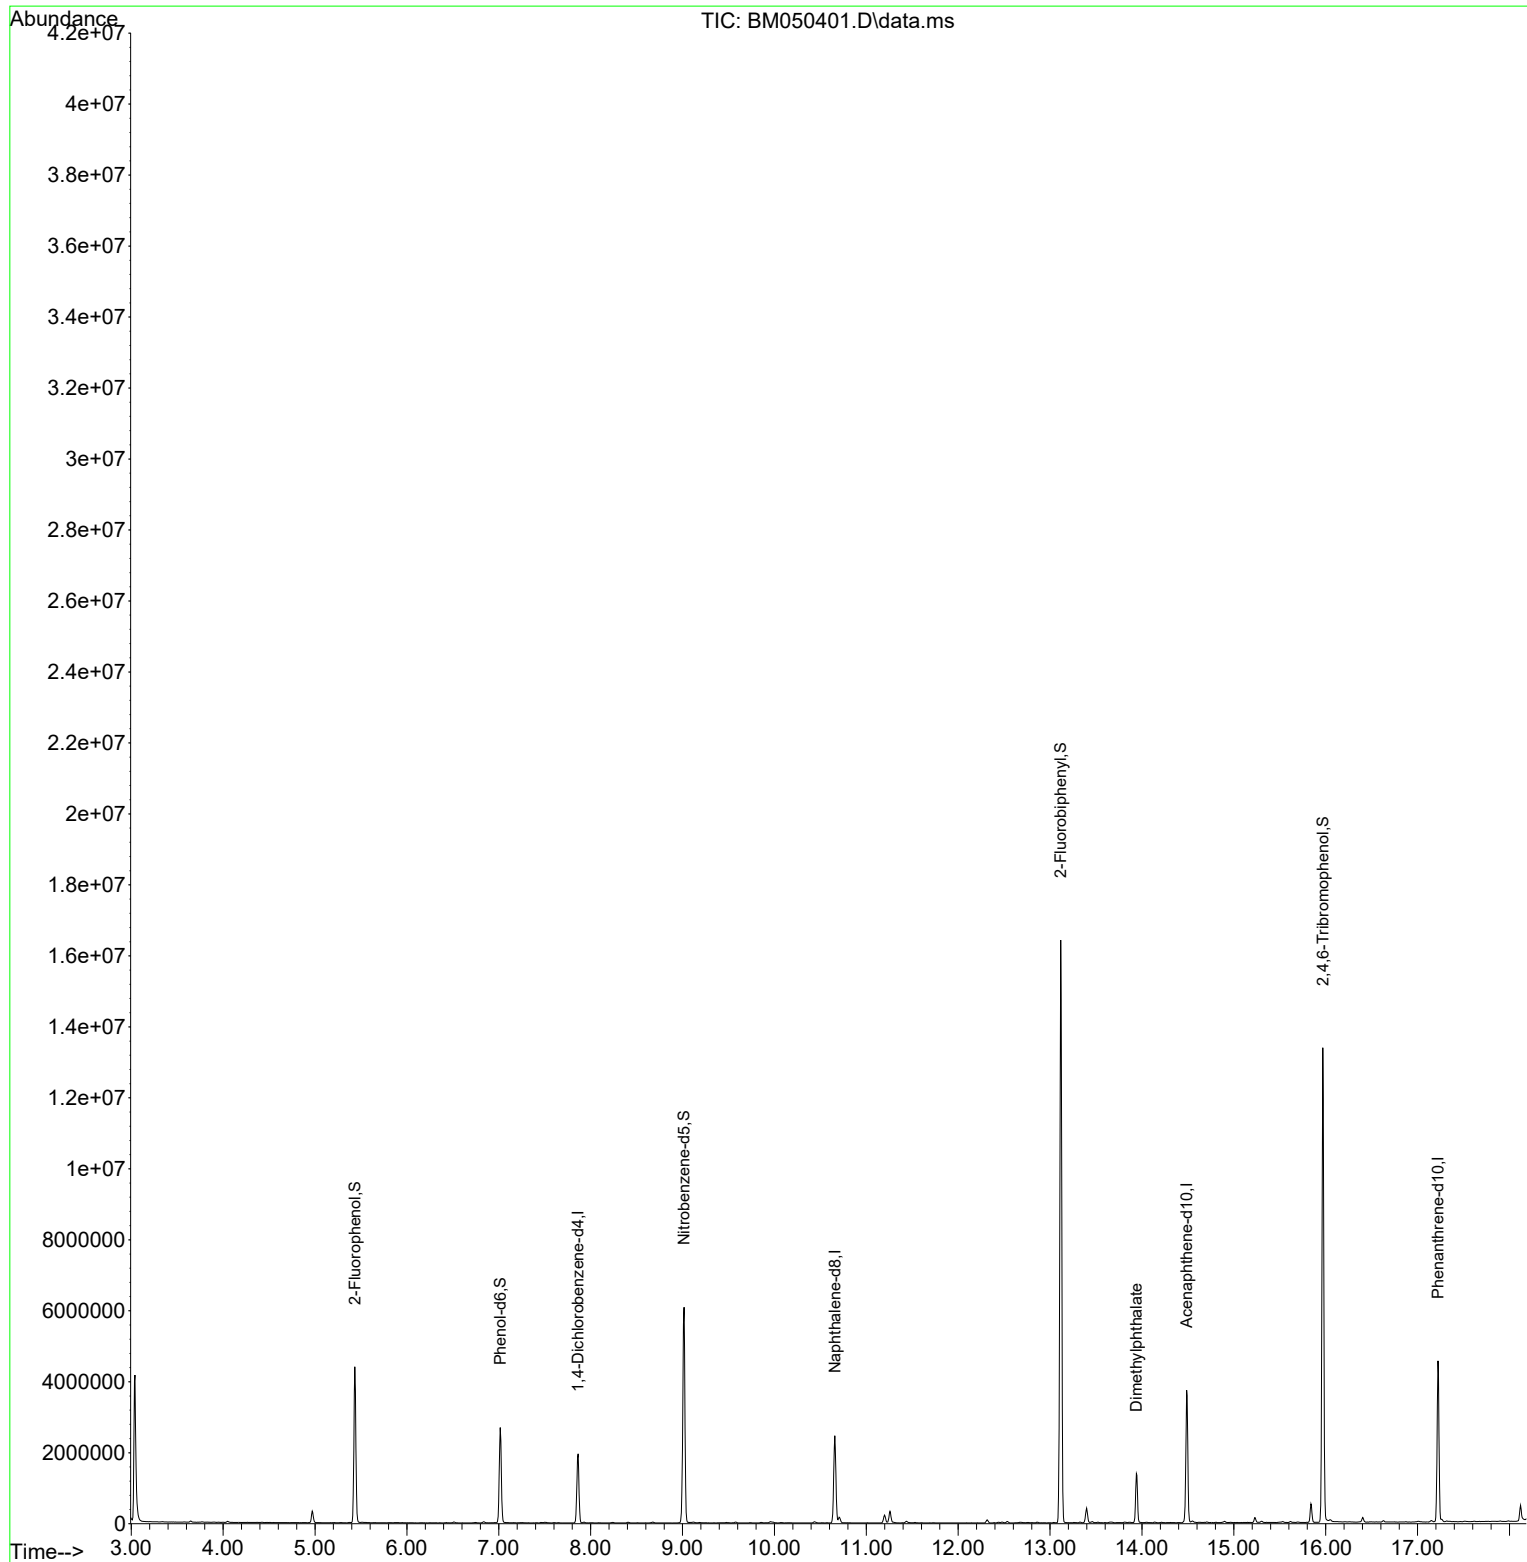

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050401.D
Acq On : 10 Jul 2025 22:39
Operator : RC/JU
Sample : Q2489-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G3(0-6)

Quant Time: Jul 11 01:28:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

