
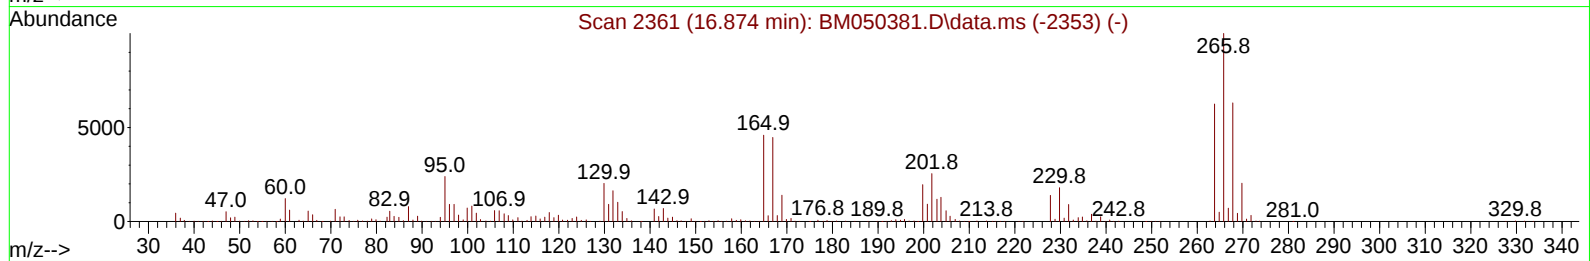
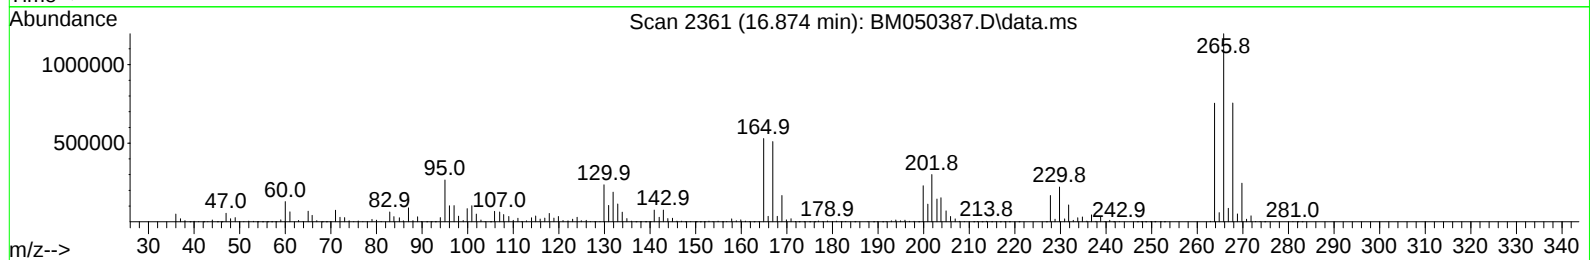


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050387.D
Acq On : 10 Jul 2025 13:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 14:36:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

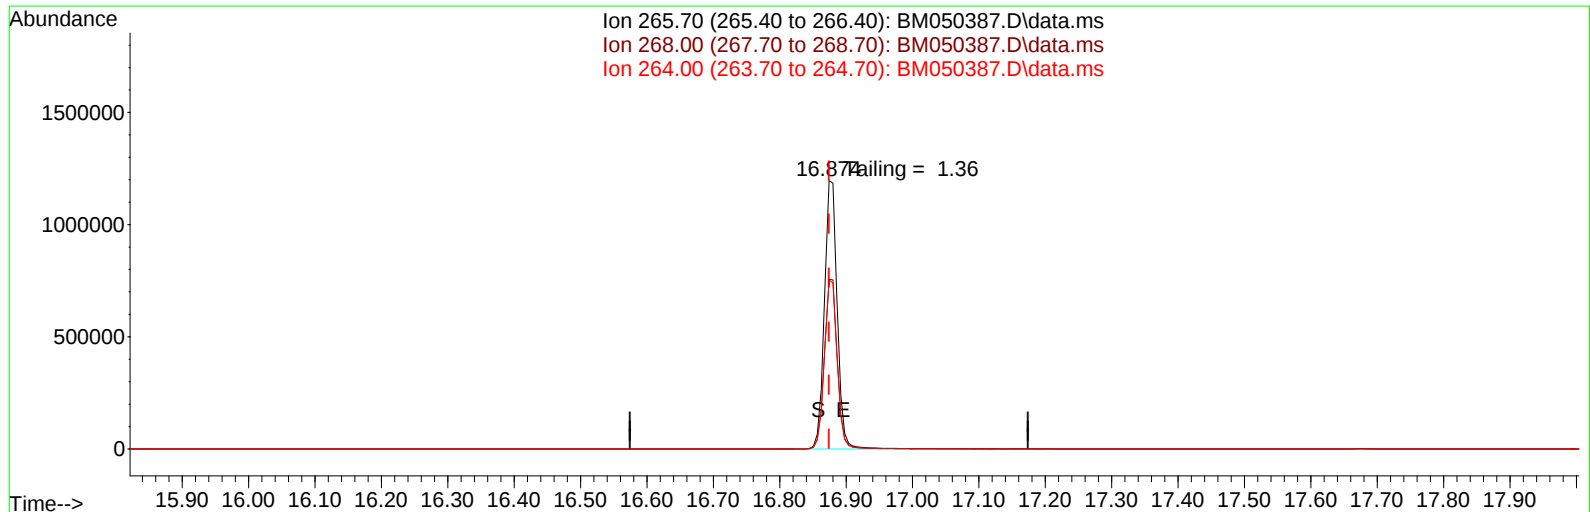

TIC: BM050387.D\data.ms

(70) Pentachlorophenol (C)




16.874min (+ 0.000) 1991582.93 ng

response 1613299

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.20
264.00	62.40	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050387.D
Acq On : 10 Jul 2025 13:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 14:36:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

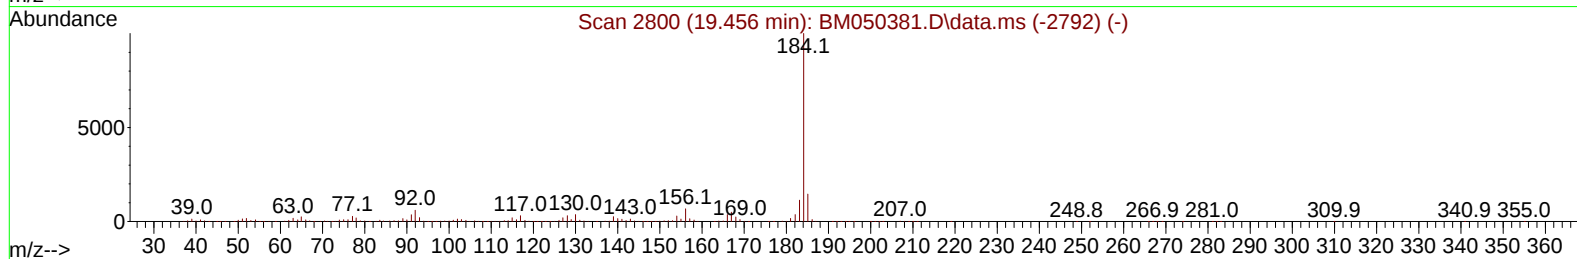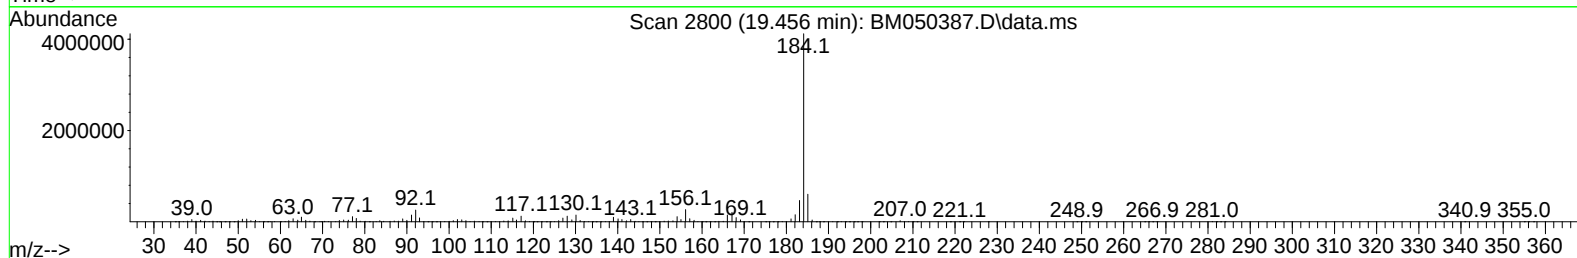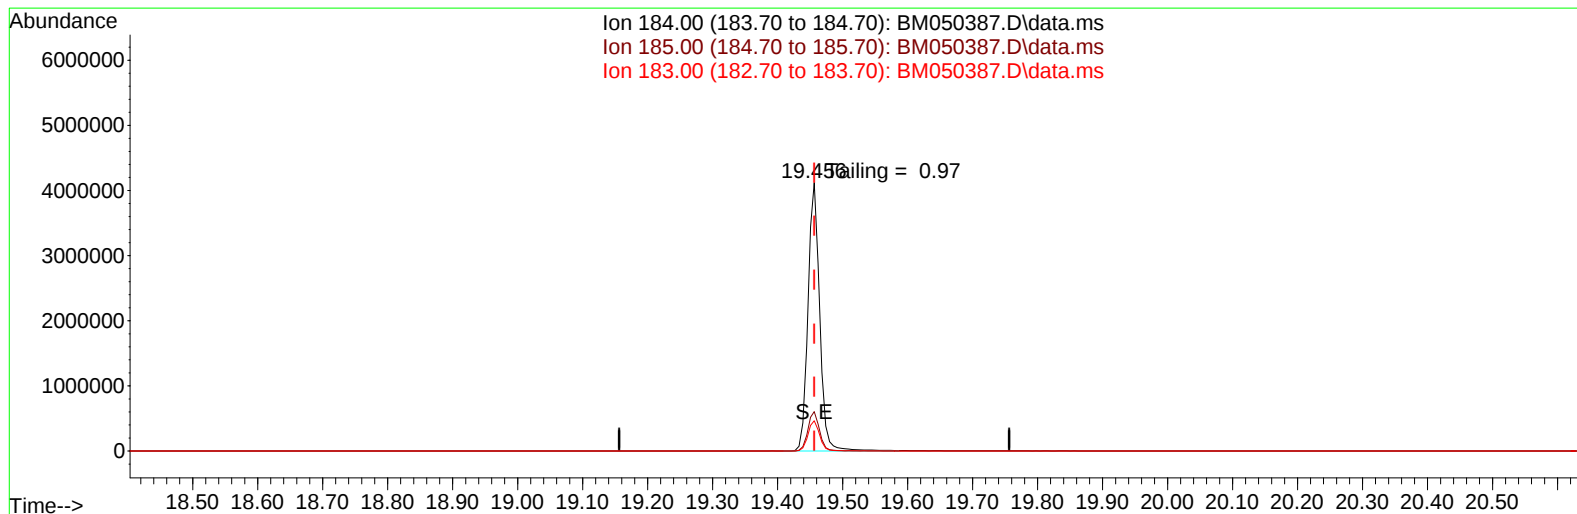

TIC: BM050387.D\data.ms

(77) Benzidine**19.456min (+ 0.000) 4529.57 ng****response 5211463**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.67
183.00	11.30	11.30
0.00	0.00	0.00