

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071116\
 Data File : BM006400.D
 Acq On : 11 Jul 2016 18:12
 Operator : UM/SJ
 Sample : PB91936BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK36

Quant Time: Jul 12 00:59:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 12 00:59:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	104595	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	427566	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	242982	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	576075	20.00	ng/ul	0.00
75) Chrysene-d12	21.23	240	718711	20.00	ng/ul	0.00
83) Perylene-d12	23.43	264	762632	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	16130	6.59	ng/uL	0.00
5) Phenol-d5	6.81	99	351362	35.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	216928	37.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	278449	37.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	274563	34.64	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	132166	38.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	150036	38.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	256505	36.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	350793	48.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	841002	41.48	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1033981	41.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	144320	37.55	ng/ul	0.00
57) Fluorene-d10	15.28	176	730620	41.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	107867	31.96	ng/ul	0.00
70) Anthracene-d10	17.13	188	1146731	41.72	ng/ul	0.00
76) Pyrene-d10	19.43	212	1311015	38.25	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.30	264	1467659	41.42	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.34	70	8093	1.17	ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071116\
Data File : BM006400.D
Acq On : 11 Jul 2016 18:12
Operator : UM/SJ
Sample : PB91936BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Quant Time: Jul 12 00:59:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 12 00:59:35 2016
Response via : Initial Calibration

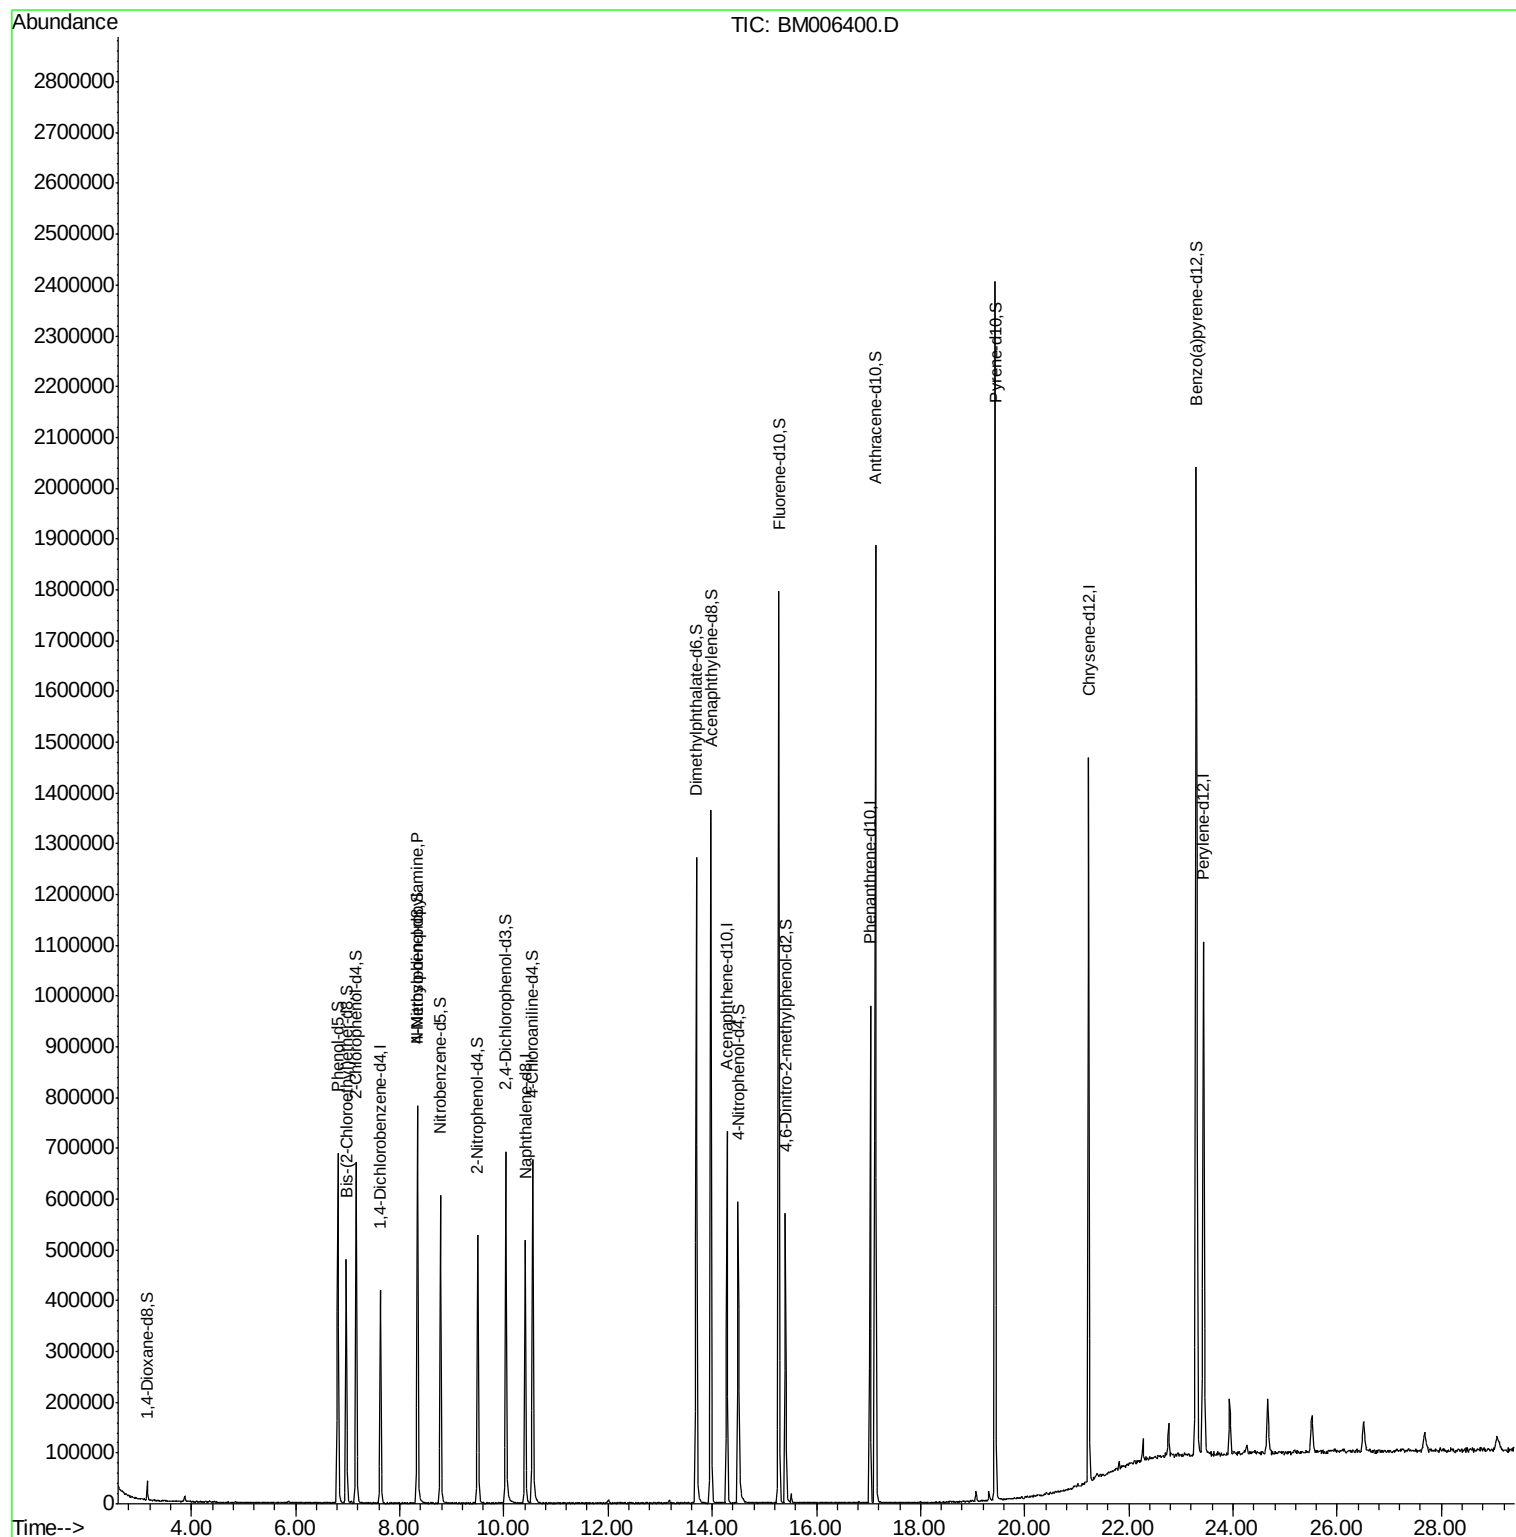

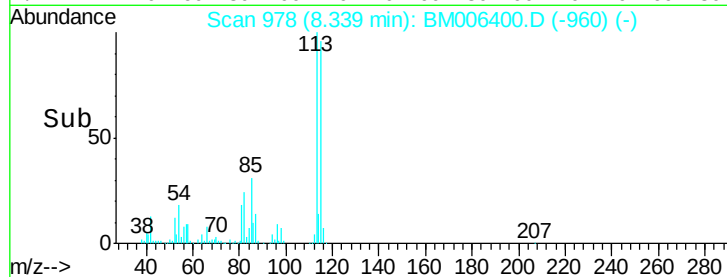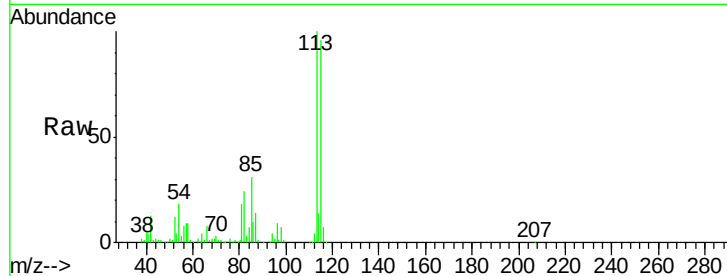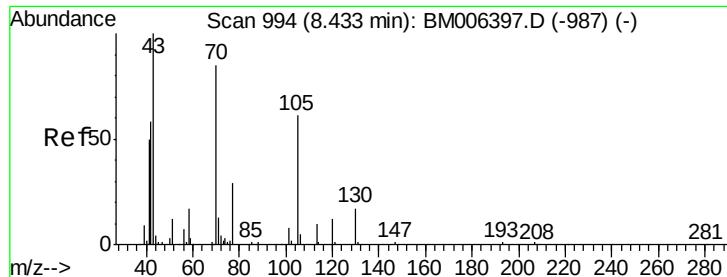

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.17 ng/ul
 RT: 8.34 min Scan# 978
 Delta R.T. -0.09 min
 Lab File: BM006400.D
 Acq: 11 Jul 2016 18:12

Instrument :
 BNA_M
 ClientSampleId :
 SBLK36

Tgt Ion: 70 Resp: 8093
 Ion Ratio Lower Upper
 70 100
 42 445.4 50.6 75.8#
 101 0.0 7.9 11.9#
 130 0.0 15.8 23.6#

