

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
 Data File : BM046526.D
 Acq On : 11 Jul 2024 20:57
 Operator : MA/JU
 Sample : PB161917BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK917

Quant Time: Jul 12 05:10:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 05:09:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	1886	0.400	ng/ul	0.00
4) Naphthalene-d8	10.277	136	4933	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.160	164	3635	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.91
17) Chrysene-d12	21.114	240	6681	0.400	ng/ul #	0.00
23) Perylene-d12	23.256	264	9249	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.118	96	7478	4.826	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.877	152	2051	0.258	ng/ul	0.00
18) Fluoranthene-d10	18.946	212	5262	0.259	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.159	166	844	0.062	ng/ul#	20
20) Pyrene	19.314	202	926	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.124	252	2339	0.077	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046526.D
Acq On : 11 Jul 2024 20:57
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK917

Quant Time: Jul 12 05:10:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration




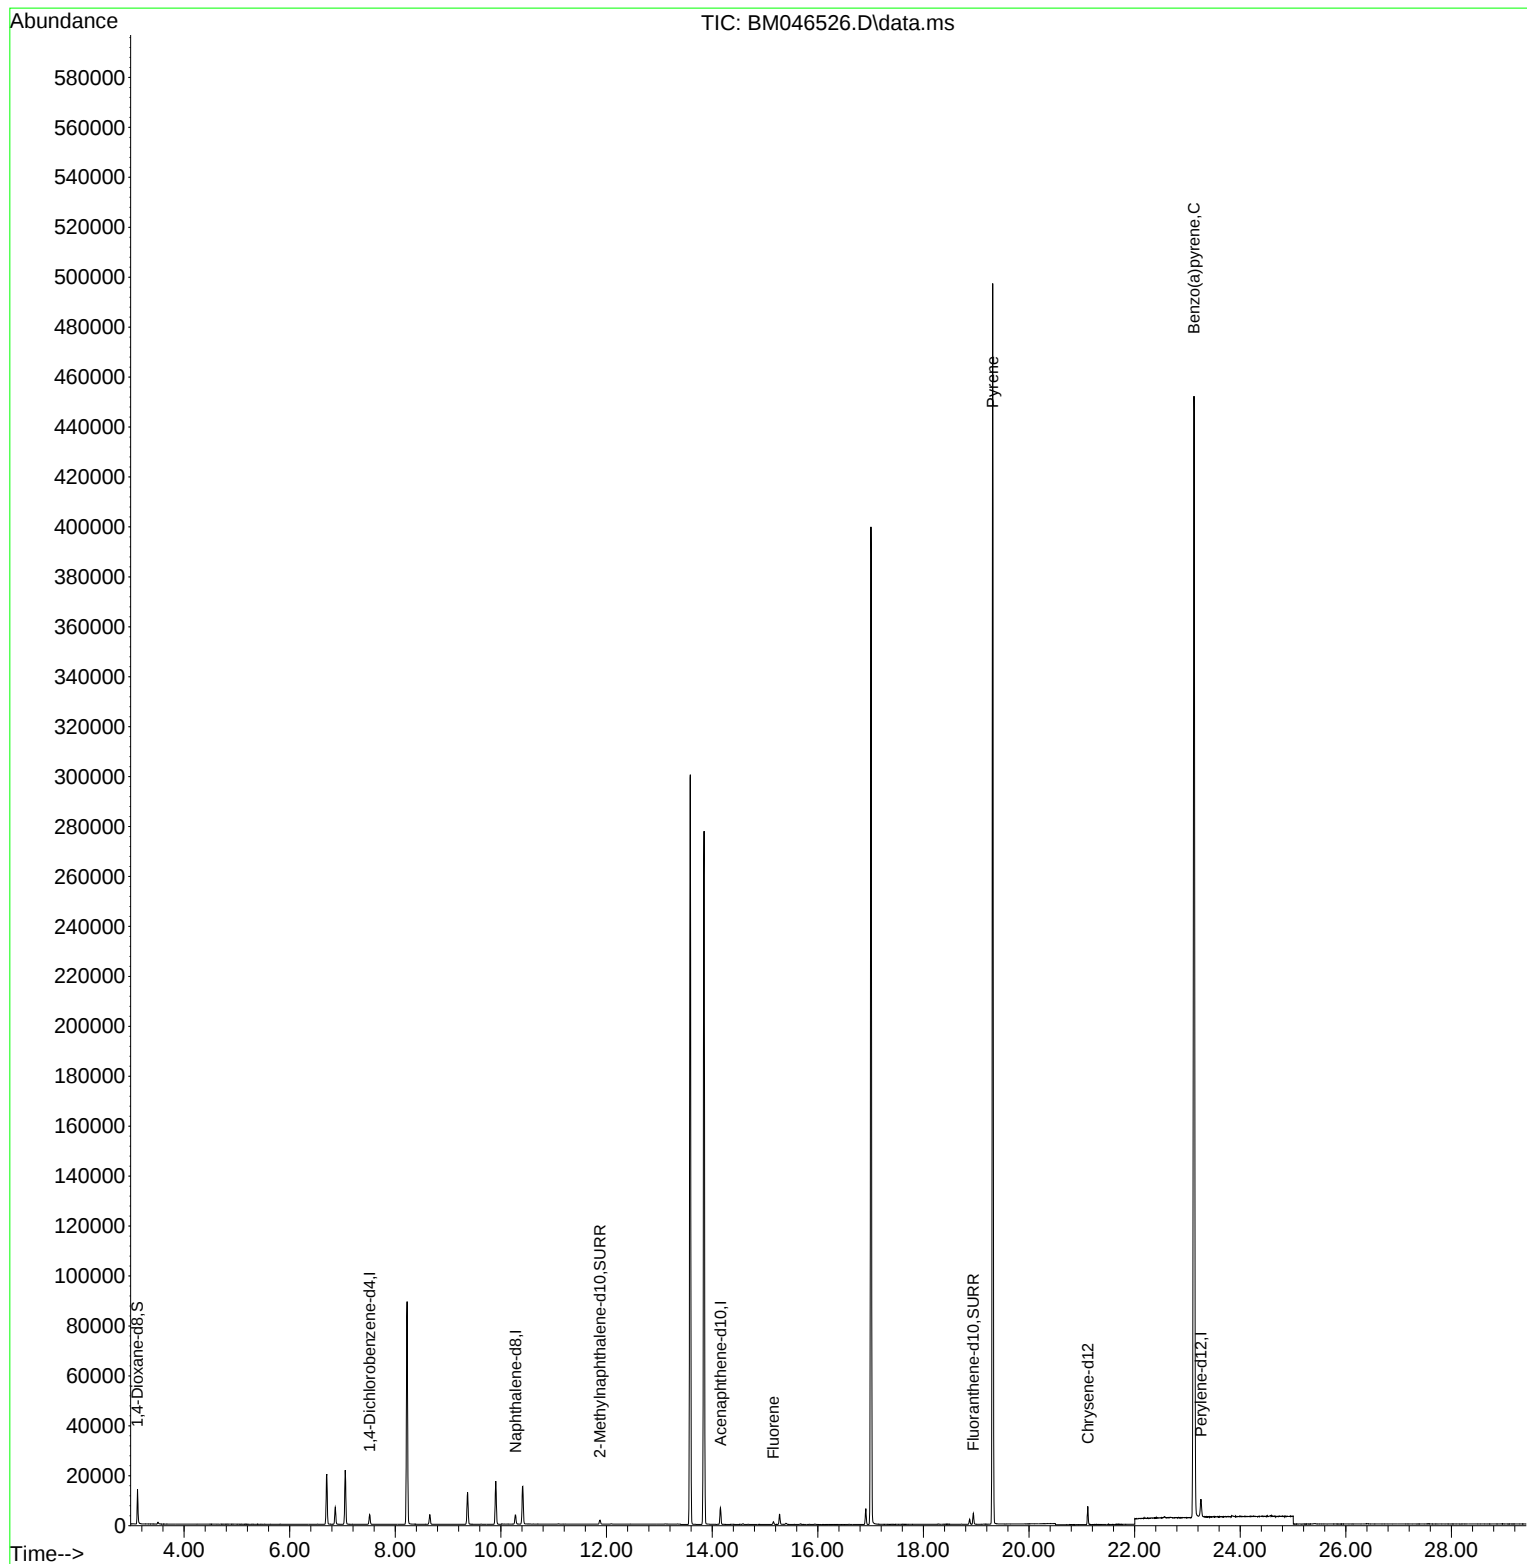


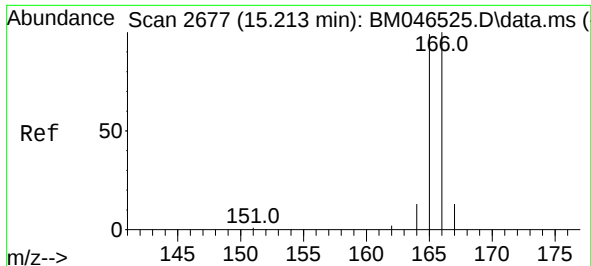

#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.159 min Scan# 2665
Delta R.T. -0.054 min
Lab File: BM046526.D
Acq: 11 Jul 2024 20:57




Instrument :
BNA_M
ClientSampleId :
SBLK917


Tgt Ion:166 Resp: 844
Ion Ratio Lower Upper
166 100
165 11.4 76.1 114.1#
167 34.8 12.5 18.7#

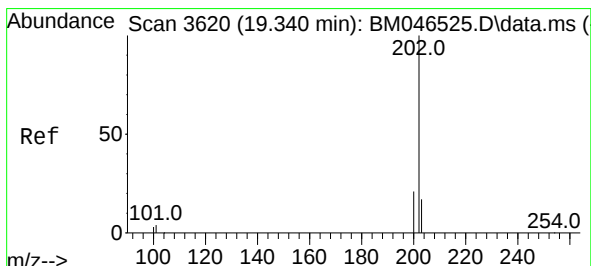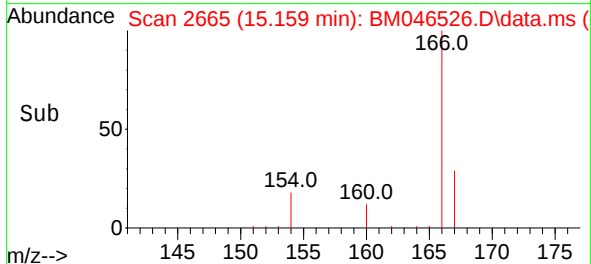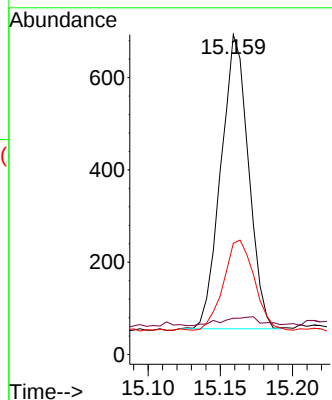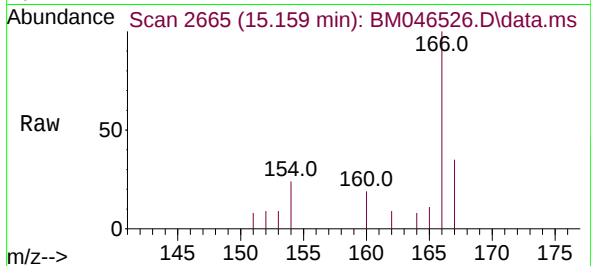

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.314 min Scan# 3614
Delta R.T. -0.026 min
Lab File: BM046526.D
Acq: 11 Jul 2024 20:57


Tgt Ion:202 Resp: 926
Ion Ratio Lower Upper
202 100
101 164.0 5.1 7.7#
100 1334.6 3.8 5.6#

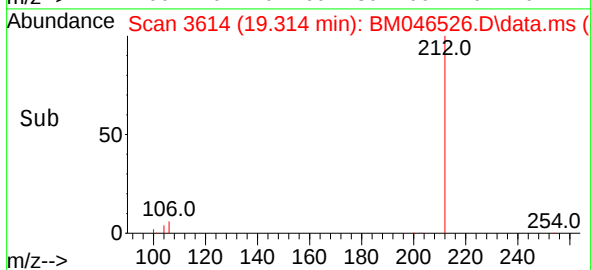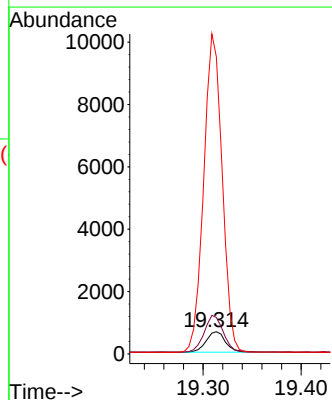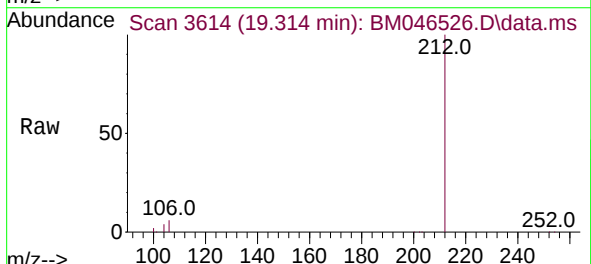

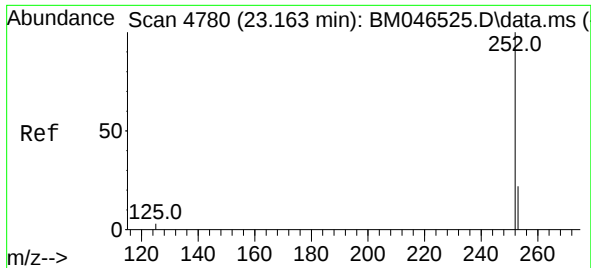

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.124 min Scan# 41
Delta R.T. -0.038 min
Lab File: BM046526.D
Acq: 11 Jul 2024 20:57

Instrument :
BNA_M
ClientSampleId :
SBLK917

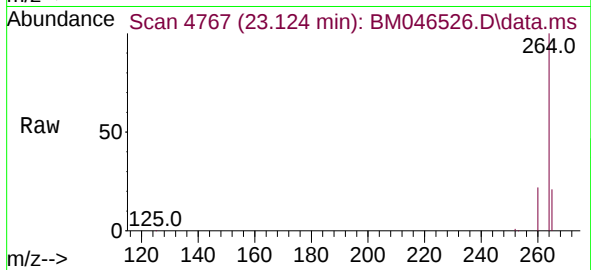

Tgt Ion:252 Resp: 2339
Ion Ratio Lower Upper
252 100
253 50.2 24.0 36.0#
125 32.3 8.2 12.2#

