




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046510.D
Acq On : 11 Jul 2024 10:27
Operator : MA/JU
Sample : PB161755BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK755

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:19:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 04:18:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

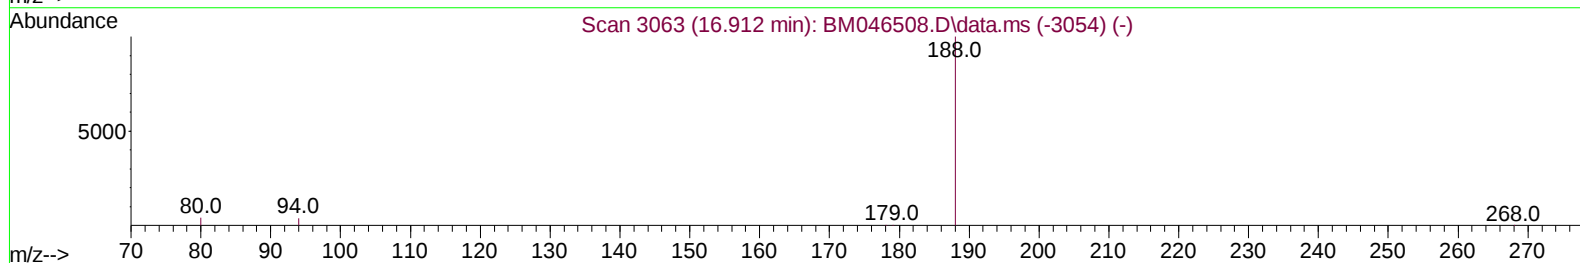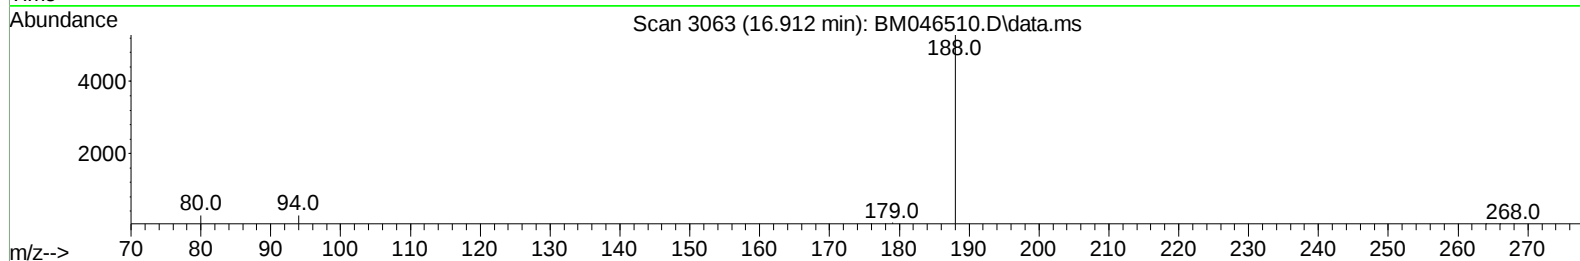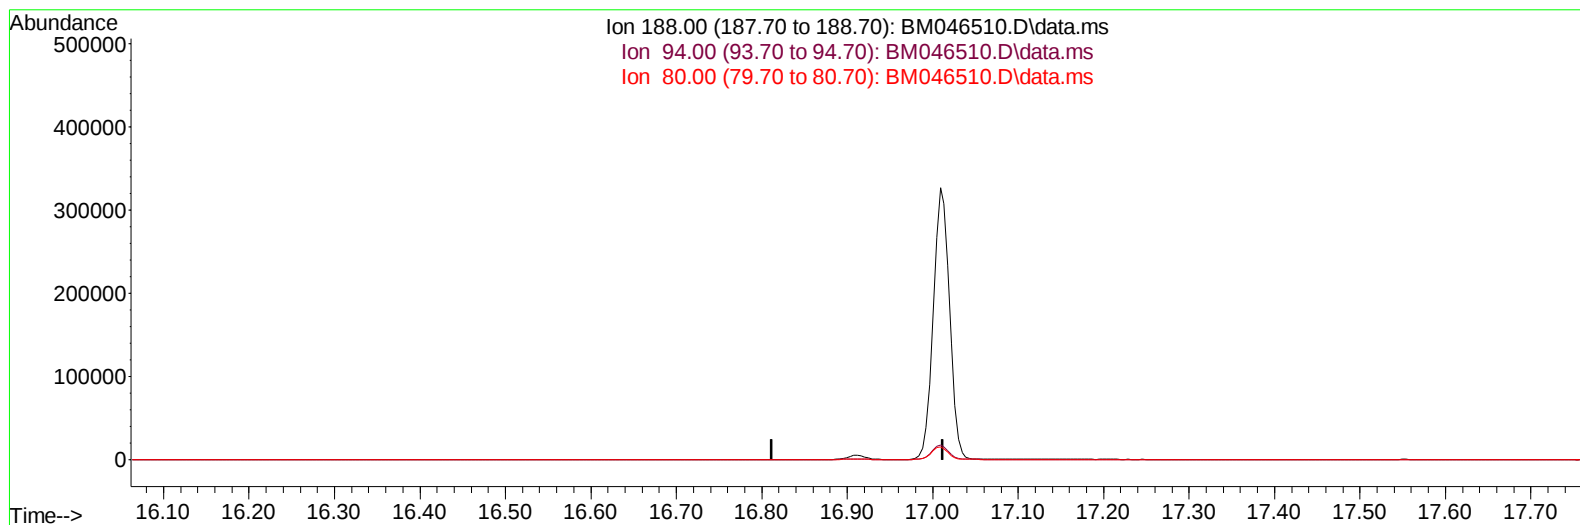

TIC: BM046510.D\data.ms

(13) Phenanthrene-d10 (I)

16.912min (-16.912) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.40	0.00#
80.00	6.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046510.D
Acq On : 11 Jul 2024 10:27
Operator : MA/JU
Sample : PB161755BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK755

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:19:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 04:18:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

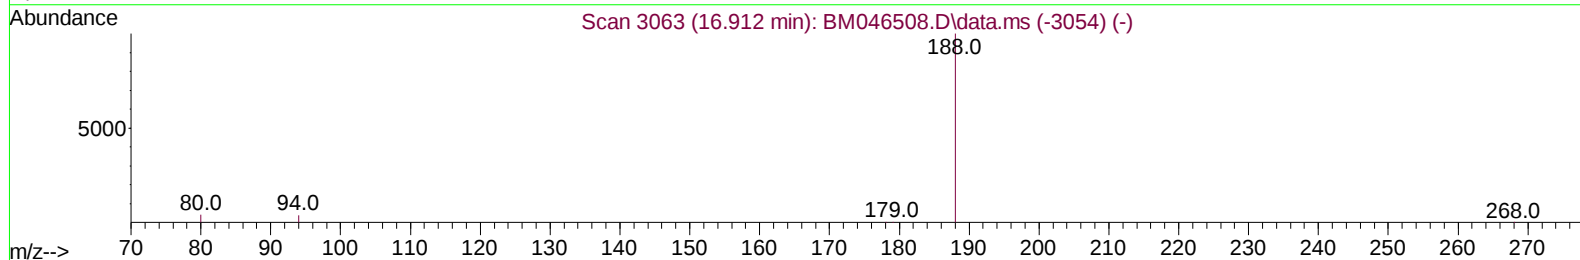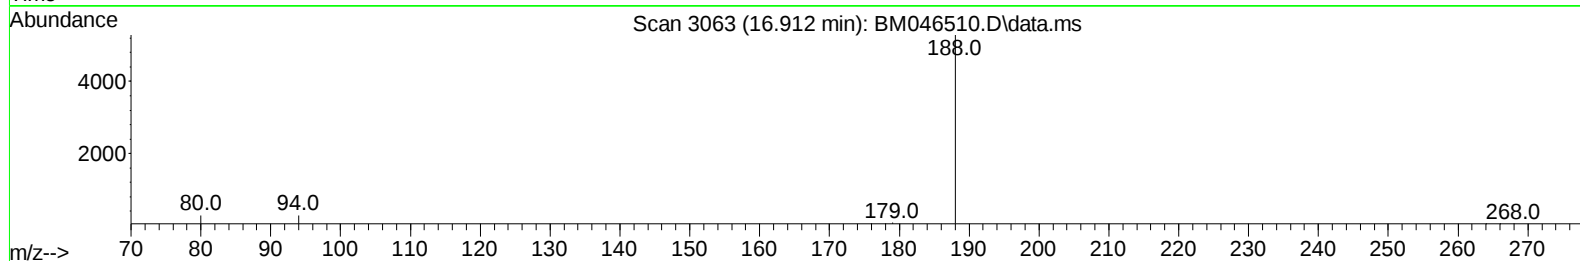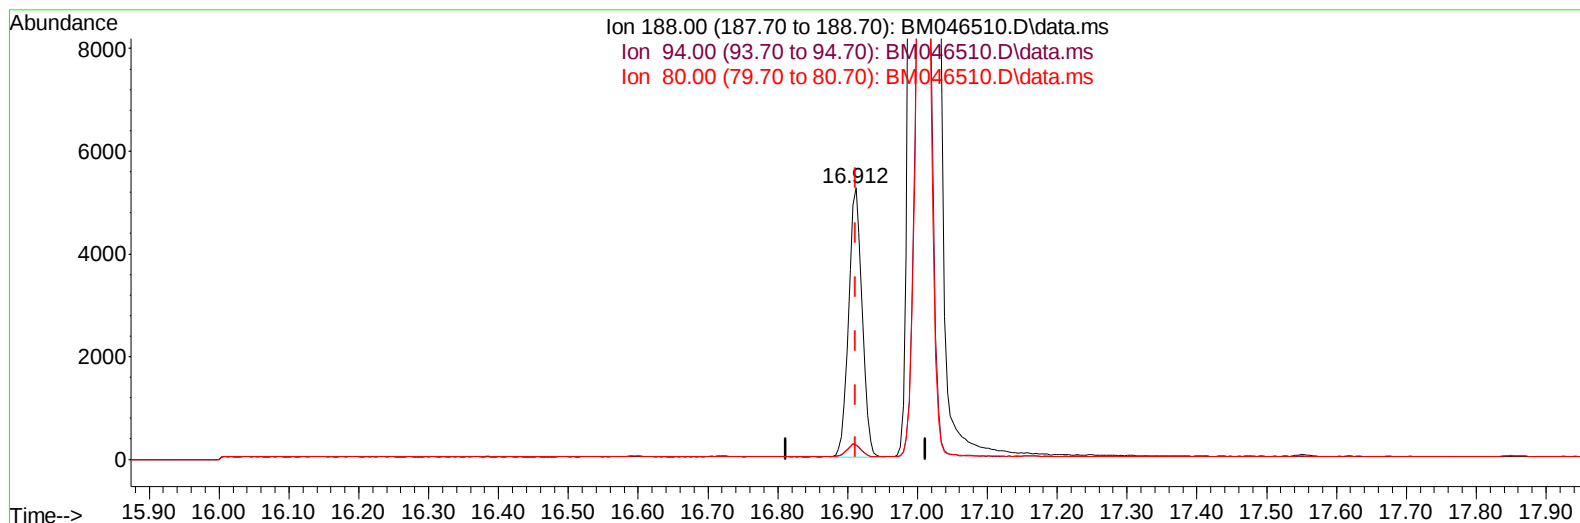

TIC: BM046510.D\data.ms

(13) Phenanthrene-d10 (I)

16.912min (+ 0.000) 0.40 ng/ul m

response 7018

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.40	5.35
80.00	6.60	5.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046510.D
Acq On : 11 Jul 2024 10:27
Operator : MA/JU
Sample : PB161755BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK755

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:19:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 04:18:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

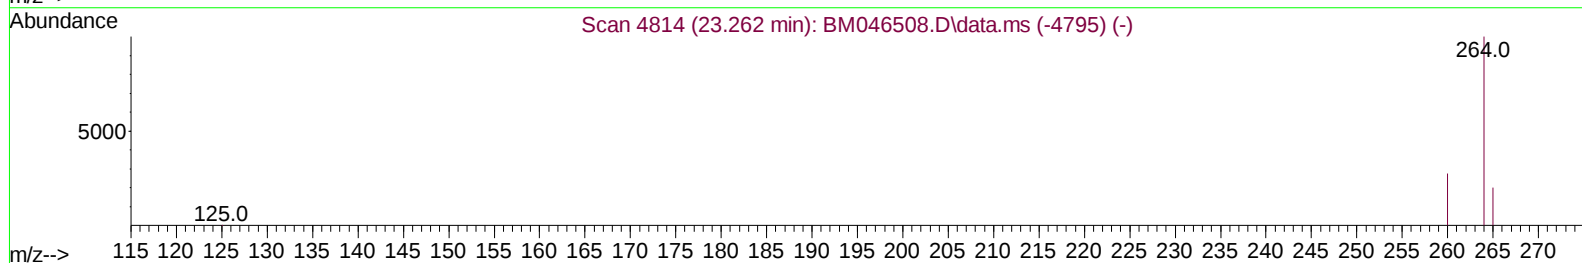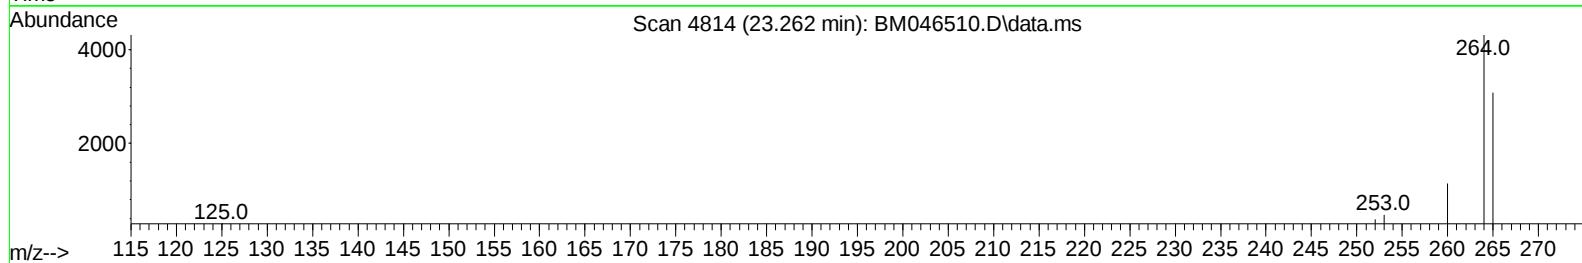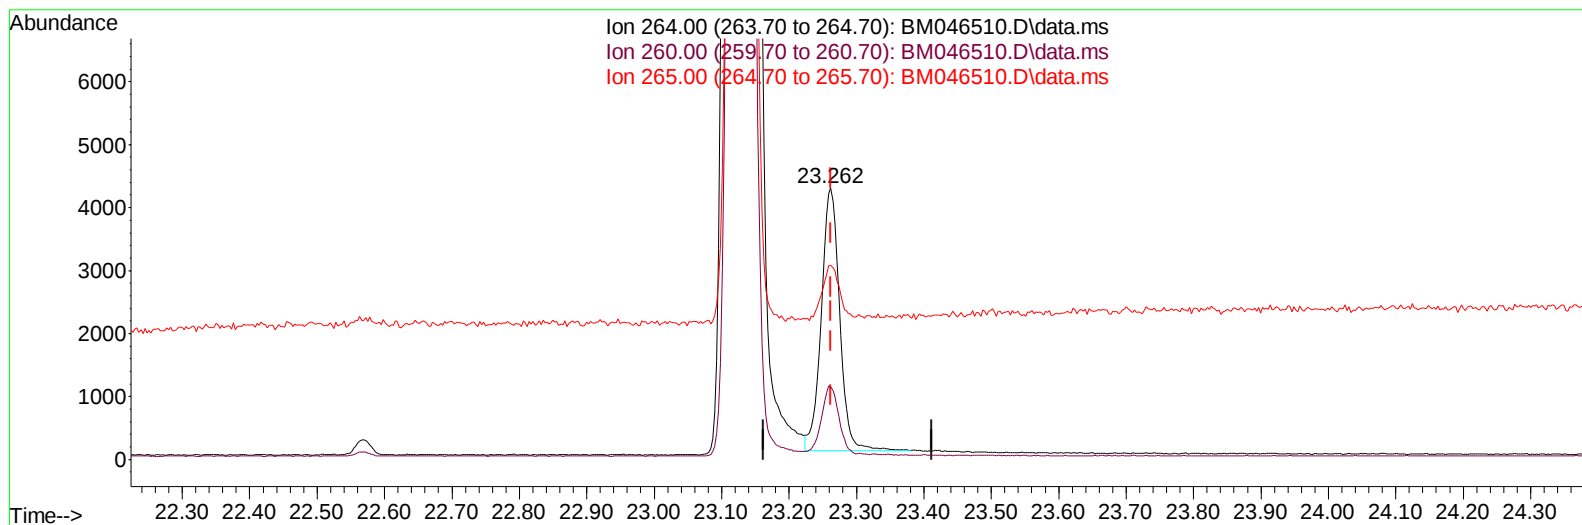

TIC: BM046510.D\data.ms

(23) Perylene-d12 (I)

23.262min (+ 0.000) 0.40 ng/ul

response 7853

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.71
265.00	88.90	71.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046510.D
Acq On : 11 Jul 2024 10:27
Operator : MA/JU
Sample : PB161755BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK755

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:19:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 04:18:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

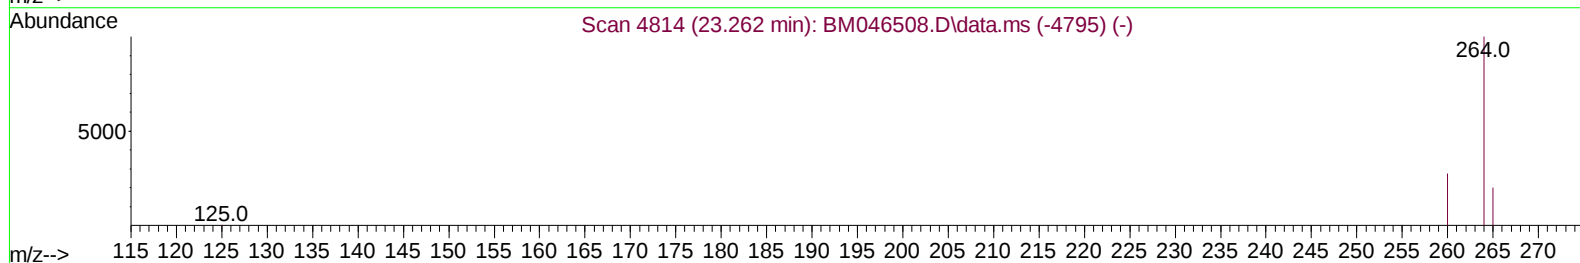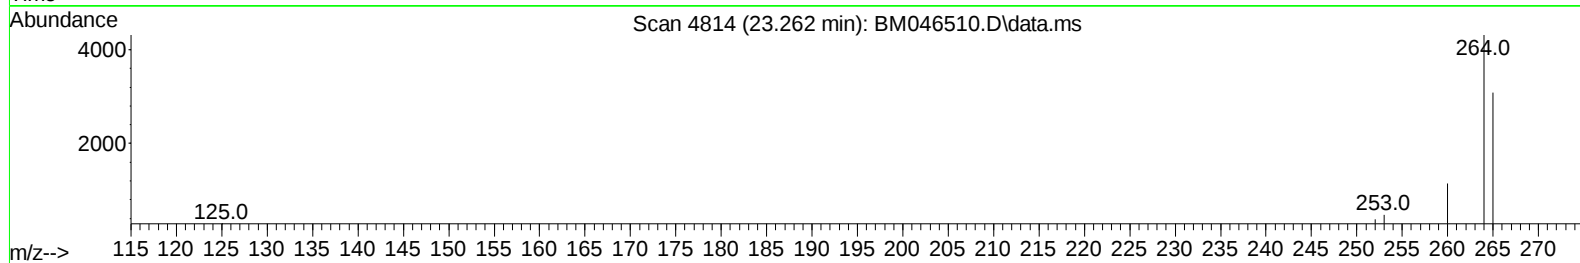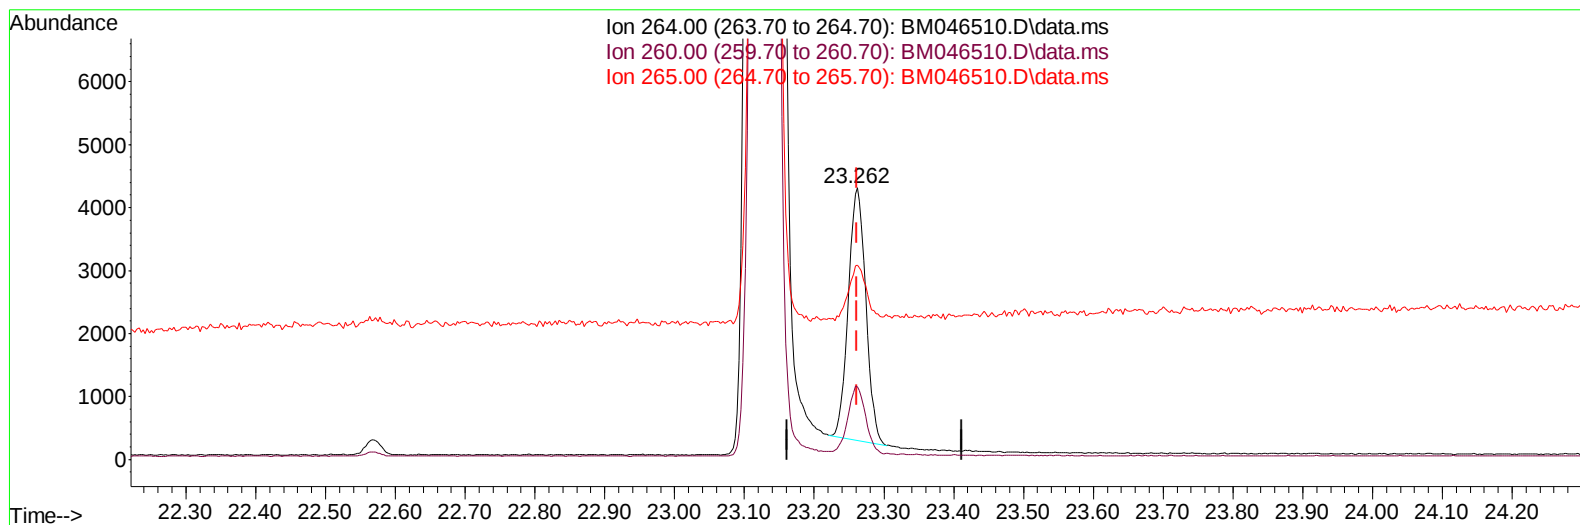

TIC: BM046510.D\data.ms

(23) Perylene-d12 (I)

23.262min (+ 0.000) 0.40 ng/ul m

response 6954

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.71
265.00	88.90	71.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
 Data File : BM046510.D
 Acq On : 11 Jul 2024 10:27
 Operator : MA/JU
 Sample : PB161755BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK755

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/13/2024

Quant Time: Jul 12 04:19:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 04:18:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	1825	0.400	ng/ul	0.00
4) Naphthalene-d8	10.275	136	4453	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.158	164	3107	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.912	188	7018m	0.400	ng/ul	0.00
17) Chrysene-d12	21.117	240	5886	0.400	ng/ul #	0.00
23) Perylene-d12	23.262	264	6954m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.117	96	7058	4.707	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.875	152	1881	0.262	ng/ul	0.00
18) Fluoranthene-d10	18.950	212	4852	0.271	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046510.D
Acq On : 11 Jul 2024 10:27
Operator : MA/JU
Sample : PB161755BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK755

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:19:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 04:18:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

