




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046526.D
Acq On : 11 Jul 2024 20:57
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK917

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:10:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

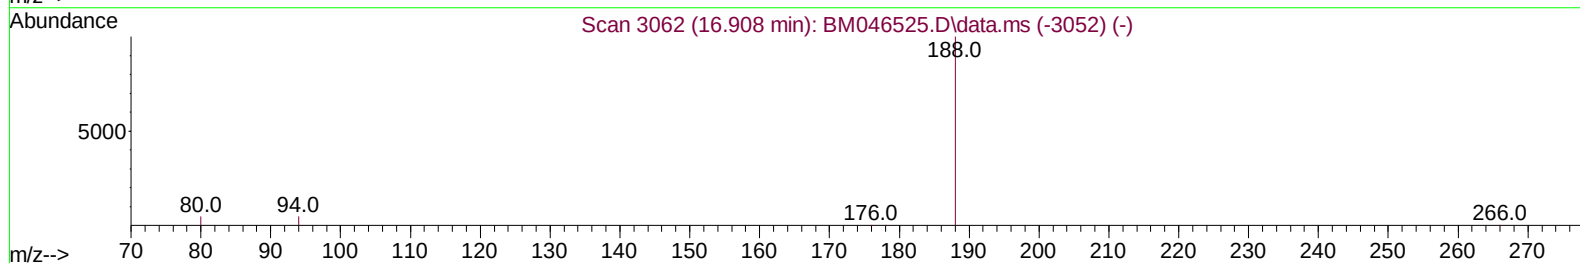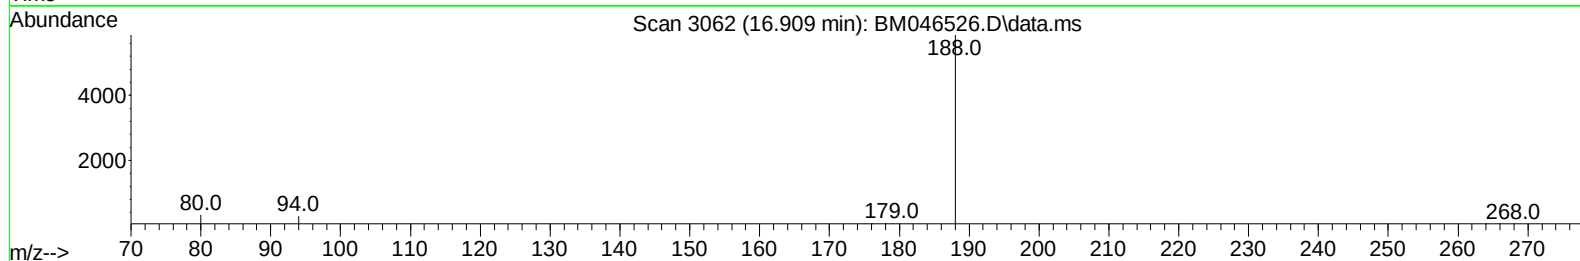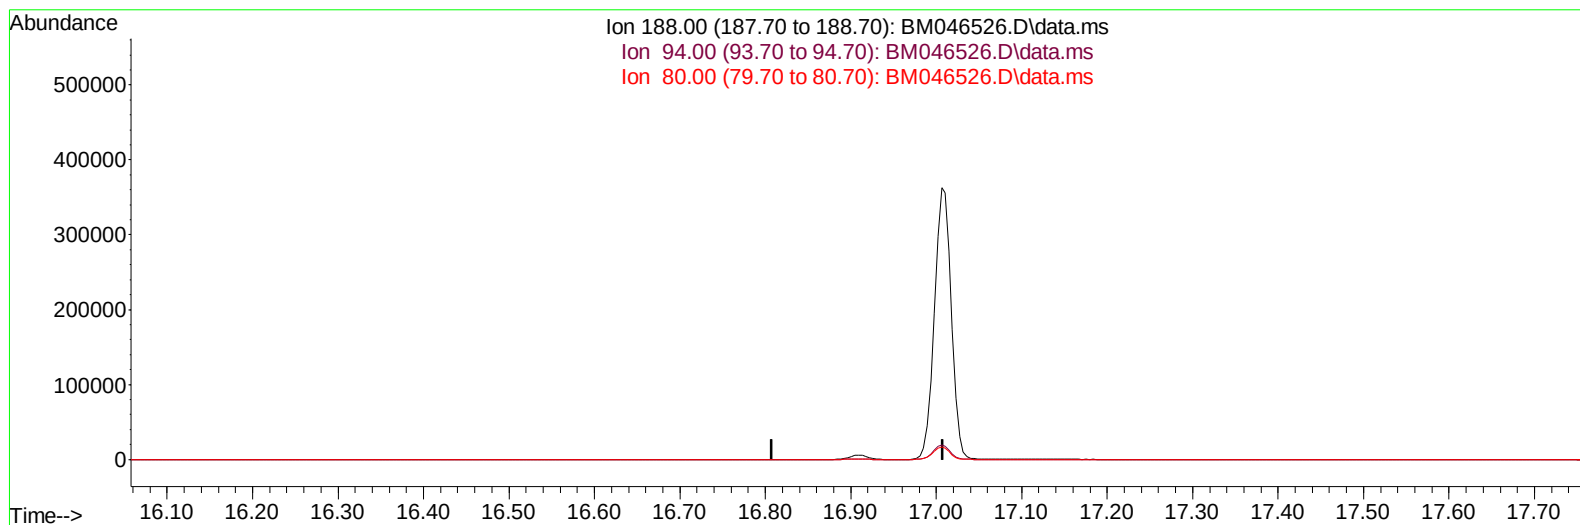

TIC: BM046526.D\data.ms

(13) Phenanthrene-d10 (I)

16.908min (-16.908) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.40	0.00#
80.00	6.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046526.D
Acq On : 11 Jul 2024 20:57
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK917

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:10:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

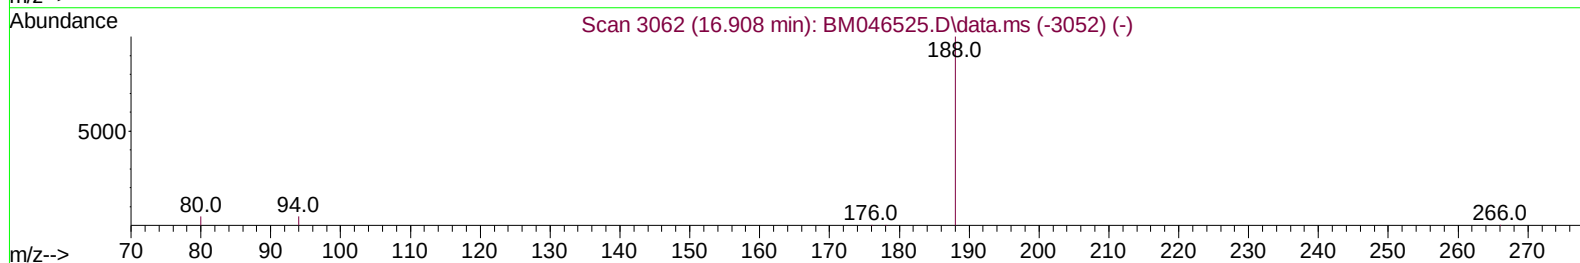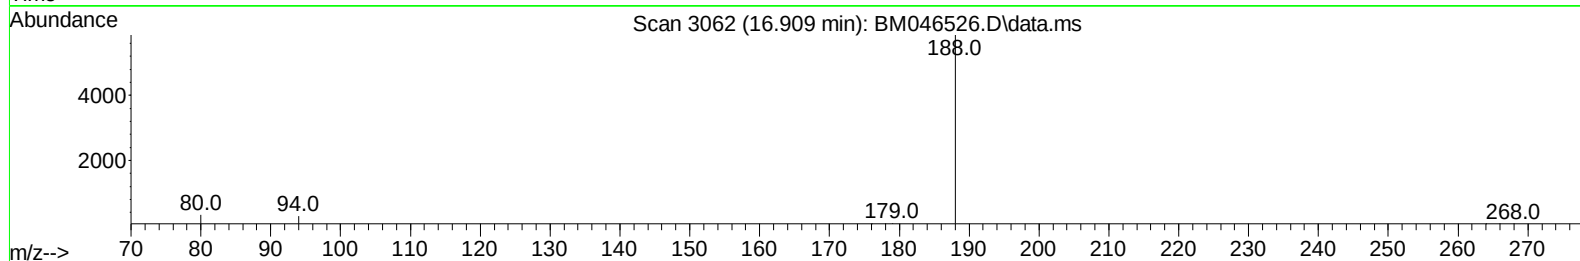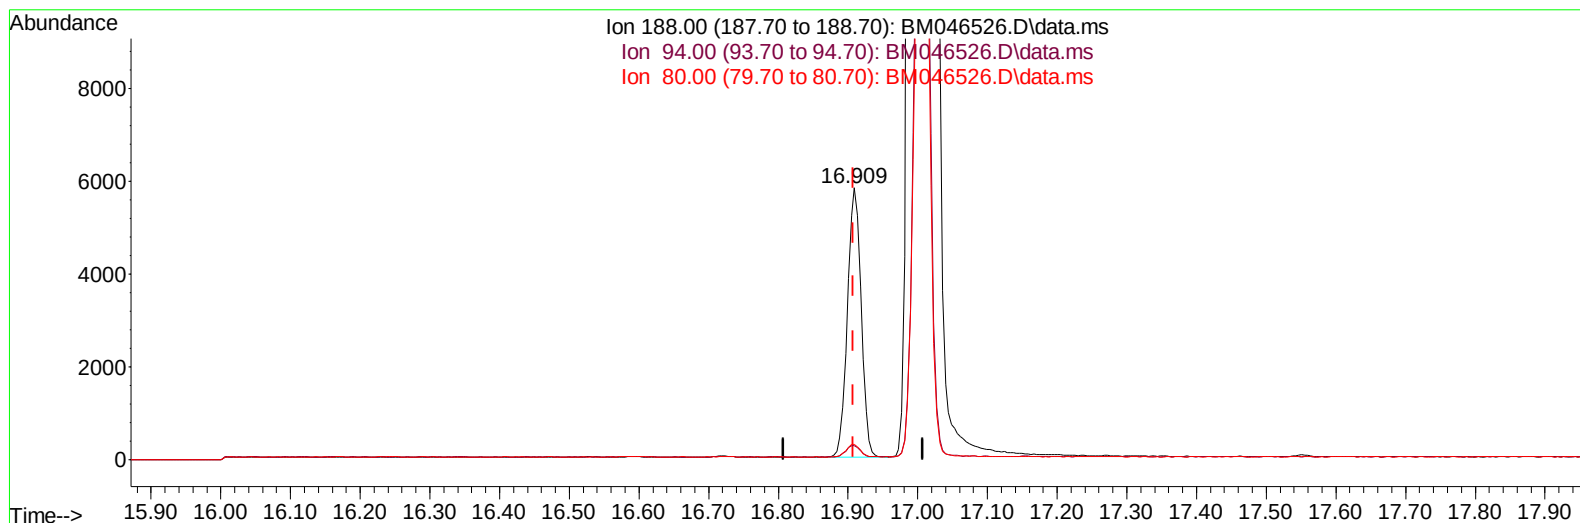

TIC: BM046526.D\data.ms

(13) Phenanthrene-d10 (I)

16.909min (+ 0.001) 0.40 ng/ul m

response 7927

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.40	5.07#
80.00	6.60	5.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046526.D
Acq On : 11 Jul 2024 20:57
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK917

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

Quant Time: Jul 12 05:10:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

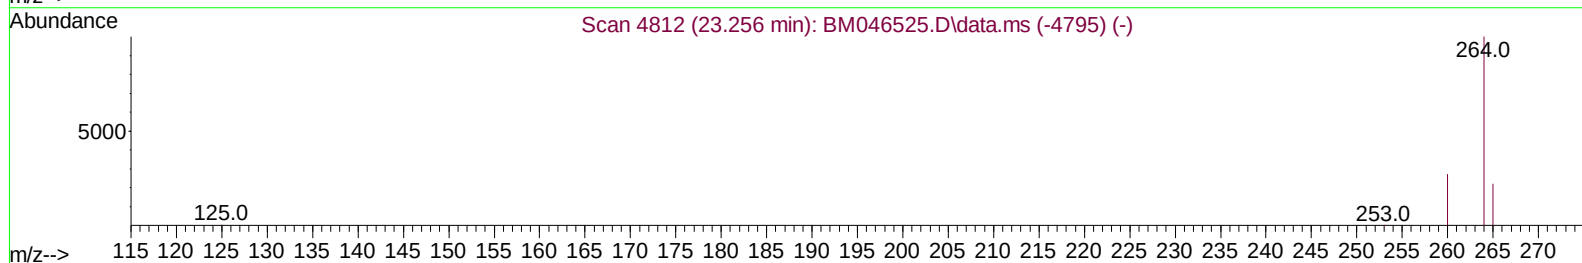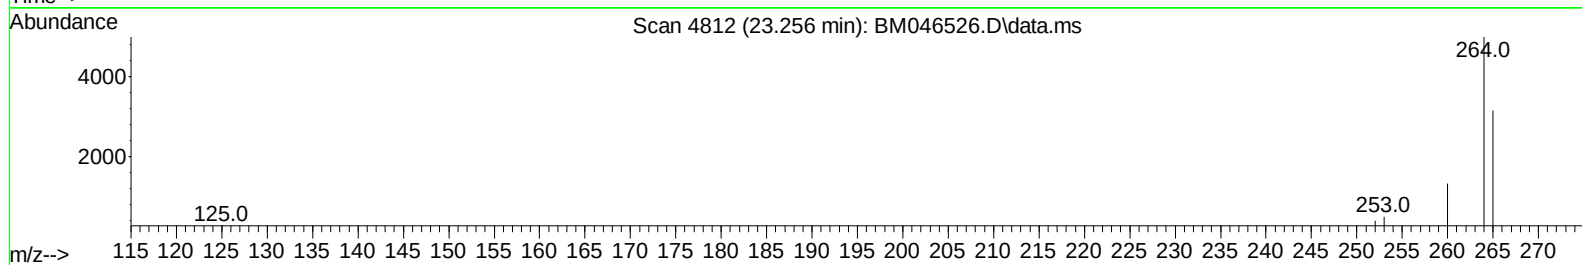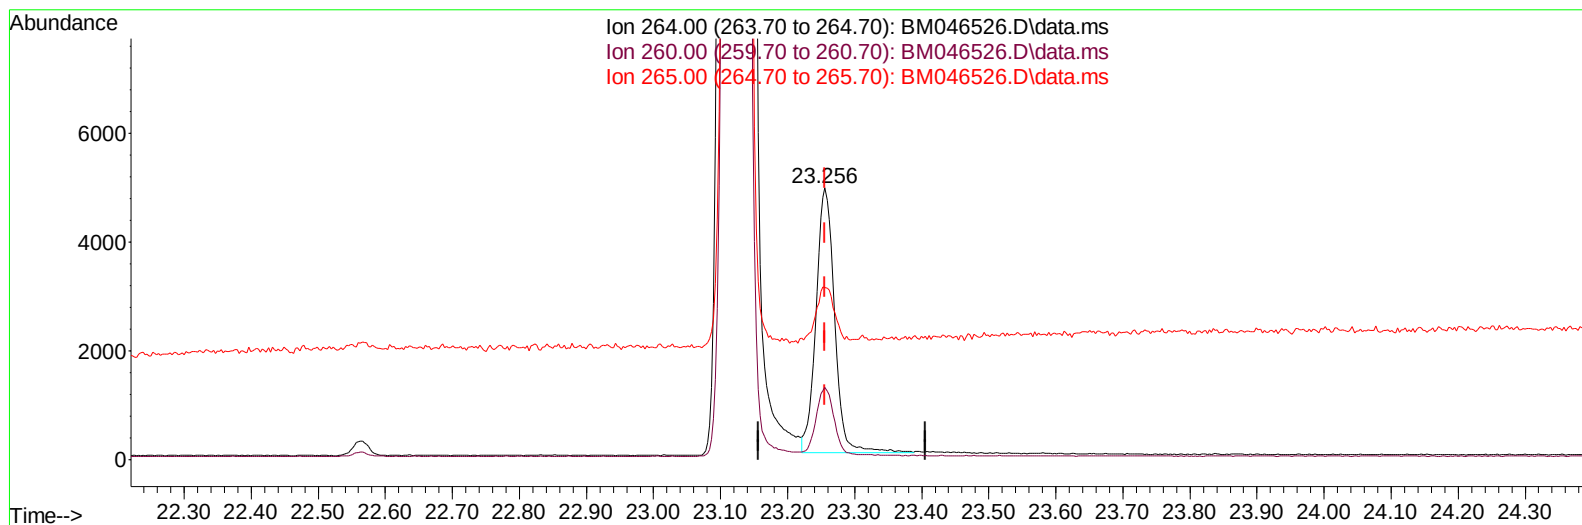

TIC: BM046526.D\data.ms

(23) Perylene-d12 (I)

23.256min (-0.000) 0.40 ng/u1

response 9249

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.56
265.00	88.90	63.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046526.D
Acq On : 11 Jul 2024 20:57
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK917

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:10:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

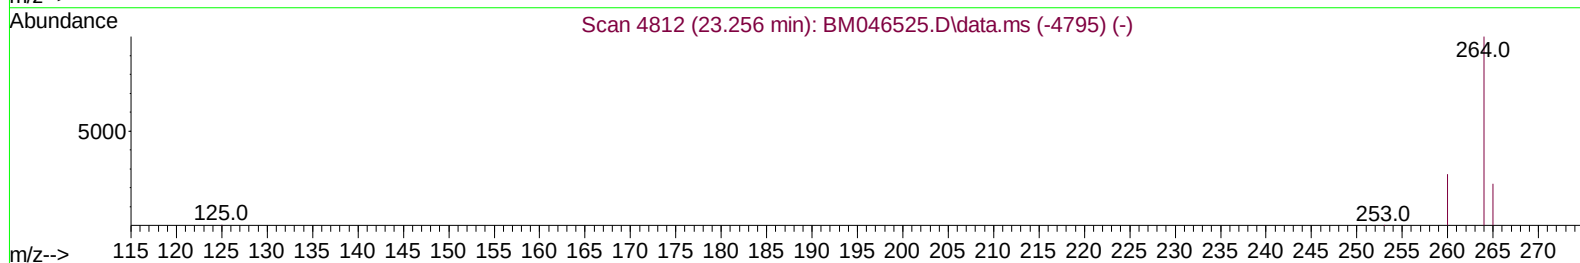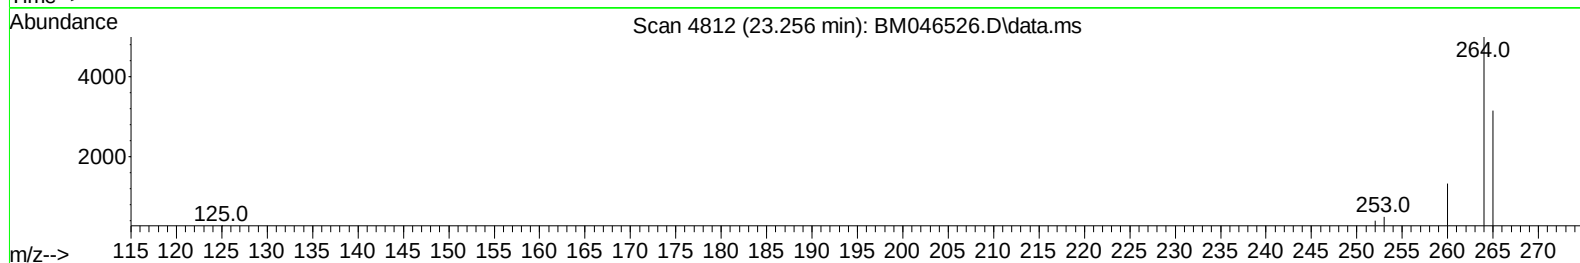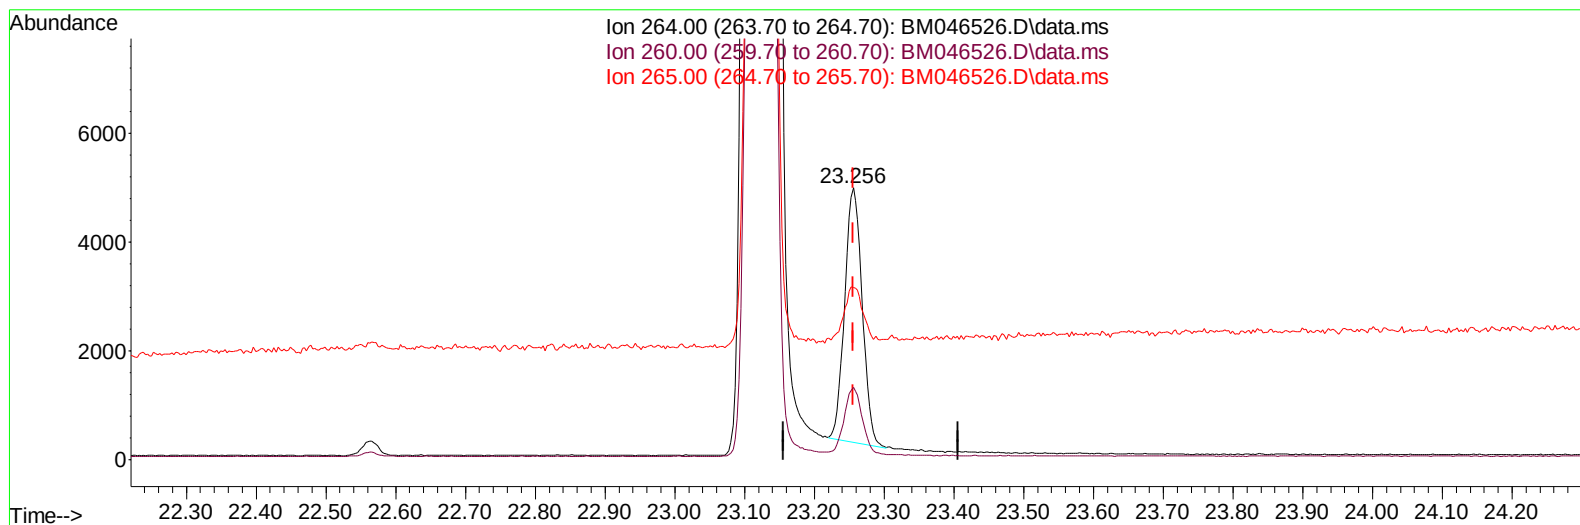

TIC: BM046526.D\data.ms

(23) Perylene-d12 (I)

23.256min (-0.000) 0.40 ng/ul m

response 8164

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.56
265.00	88.90	63.24#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
 Data File : BM046526.D
 Acq On : 11 Jul 2024 20:57
 Operator : MA/JU
 Sample : PB161917BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK917

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/13/2024

Quant Time: Jul 12 05:10:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 05:09:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	1886	0.400	ng/ul	0.00
4) Naphthalene-d8	10.277	136	4933	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.160	164	3635	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.909	188	7927m	0.400	ng/ul	0.00
17) Chrysene-d12	21.114	240	6681	0.400	ng/ul #	0.00
23) Perylene-d12	23.256	264	8164m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.118	96	7478	4.826	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.877	152	2051	0.258	ng/ul	0.00
18) Fluoranthene-d10	18.946	212	5262	0.259	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046526.D
Acq On : 11 Jul 2024 20:57
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK917

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:10:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

