




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046531.D
Acq On : 12 Jul 2024 00:02
Operator : MA/JU
Sample : P3109-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0HC2

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:11:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

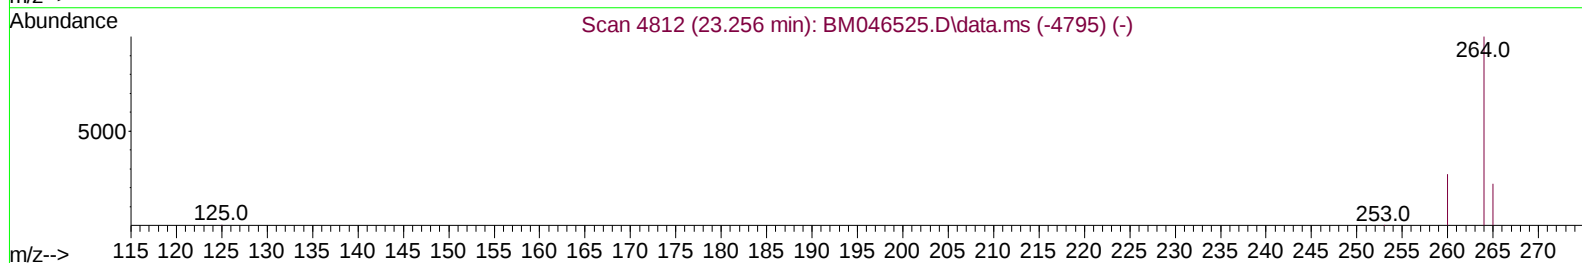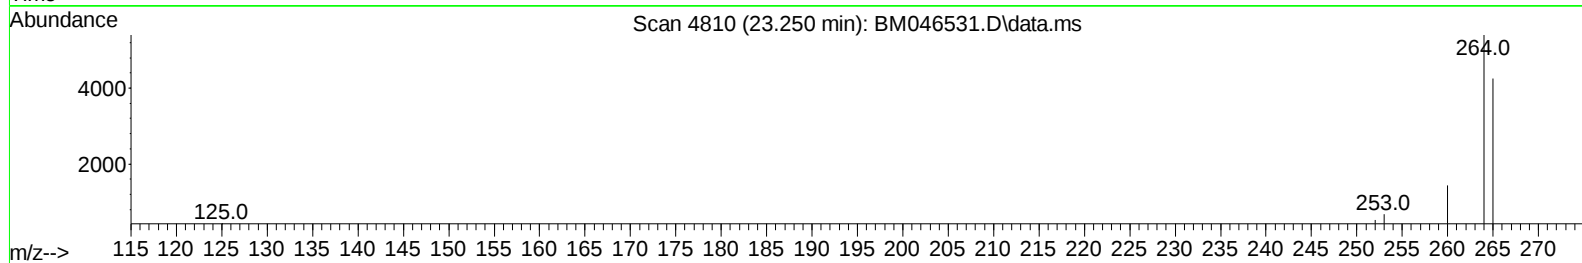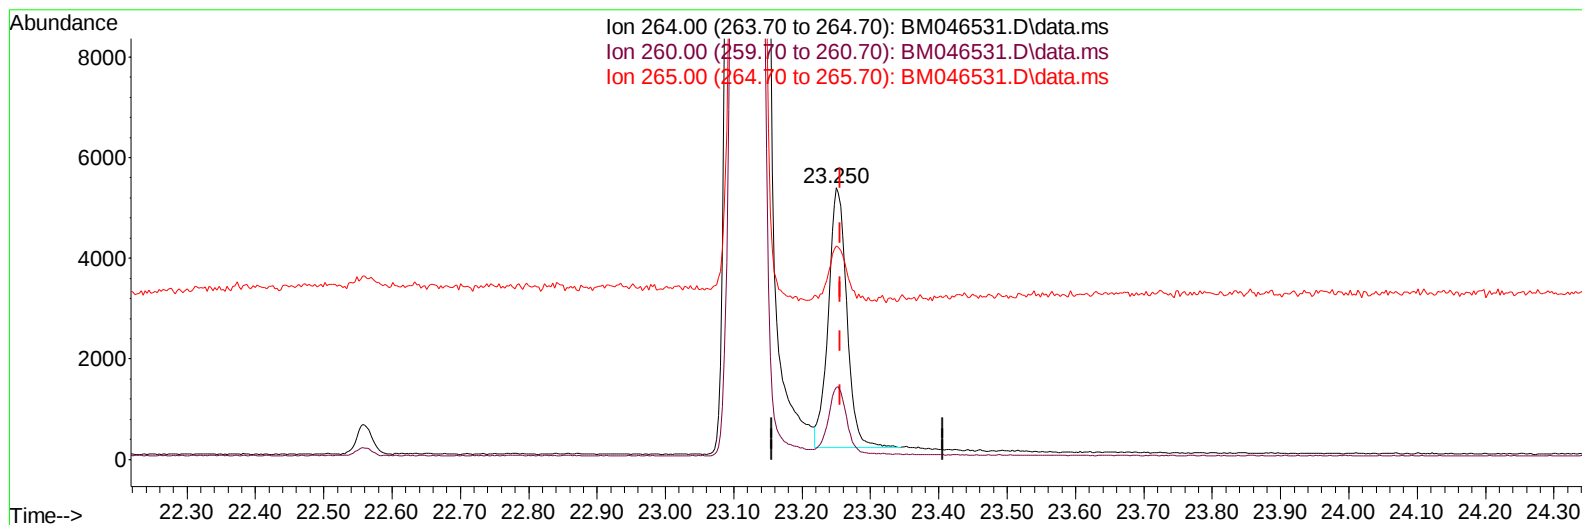

TIC: BM046531.D\data.ms

(23) Perylene-d12 (I)

23.250min (-0.006) 0.40 ng/u1

response 9686

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.57
265.00	88.90	78.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046531.D
Acq On : 12 Jul 2024 00:02
Operator : MA/JU
Sample : P3109-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0HC2

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:11:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

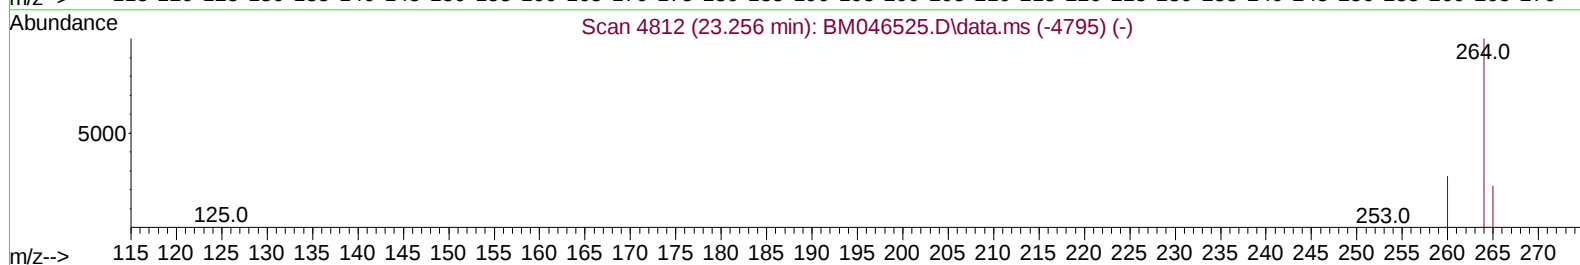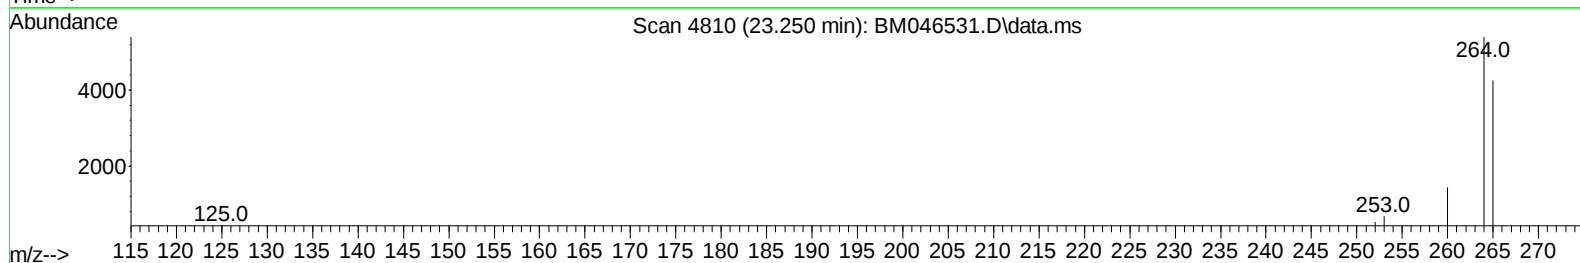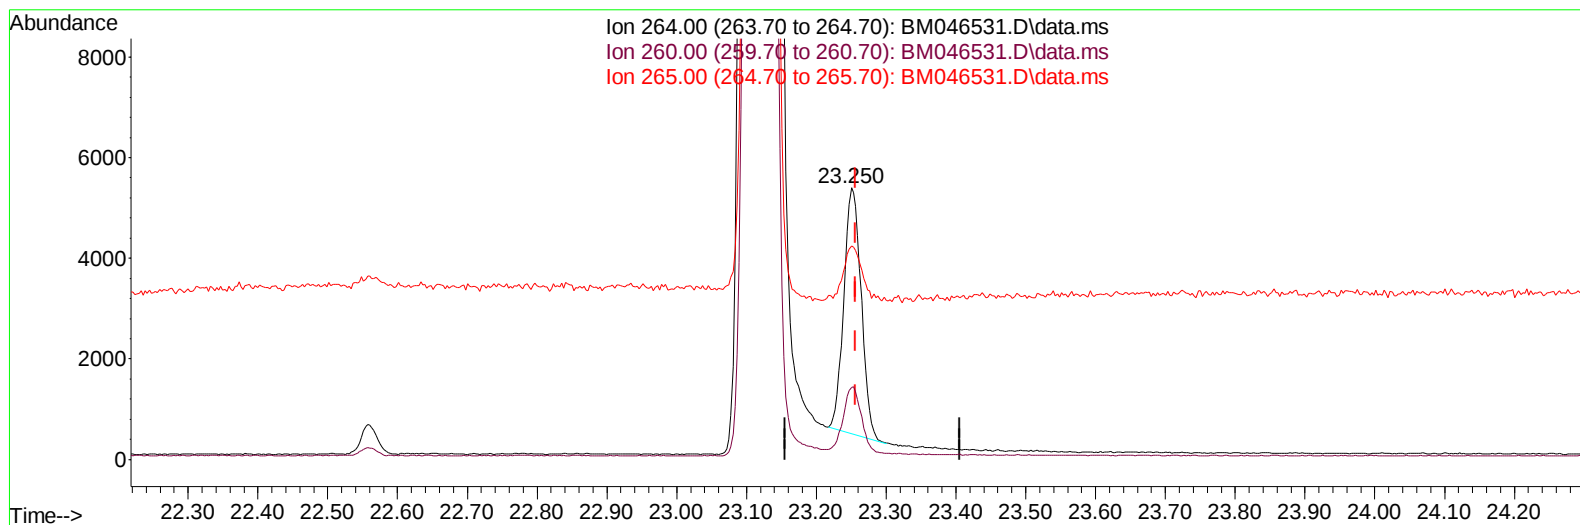

TIC: BM046531.D\data.ms

(23) Perylene-d12 (I)

23.250min (-0.006) 0.40 ng/ul m

response 8388

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.57
265.00	88.90	78.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
 Data File : BM046531.D
 Acq On : 12 Jul 2024 00:02
 Operator : MA/JU
 Sample : P3109-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0HC2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/13/2024

Quant Time: Jul 12 05:11:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 05:09:19 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.514	152		1558	0.400	ng/ul	0.00
4) Naphthalene-d8	10.275	136		4246	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.149	164		7408	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.908	188		9716	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.108	240		8852	0.400	ng/ul	0.00
23) Perylene-d12	23.250	264		8388m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.117	96		5674	4.432	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.870	152		2368	0.346	ng/ul	0.00
18) Fluoranthene-d10	18.959	212		9978	0.370	ng/ul	0.01
Target Compounds							
							Qvalue
5) Naphthalene	10.325	128		1085	0.100	ng/ul#	64
8) 1-Methylnaphthalene	12.172	142		1751	0.226	ng/ul	98
11) Acenaphthene	14.218	153		530	0.023	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046531.D
Acq On : 12 Jul 2024 00:02
Operator : MA/JU
Sample : P3109-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0HC2

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:11:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

