

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
 Data File : BM046530.D
 Acq On : 11 Jul 2024 23:25
 Operator : MA/JU
 Sample : P3084-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GC9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/13/2024

Quant Time: Jul 12 05:11:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 05:09:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	1383	0.400	ng/ul	0.00
4) Naphthalene-d8	10.275	136	3602	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.154	164	2730	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.908	188	5767m	0.400	ng/ul	0.00
17) Chrysene-d12	21.111	240	4829	0.400	ng/ul	0.00
23) Perylene-d12	23.253	264	5410m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.117	96	6820	6.002	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.875	152	2235	0.385	ng/ul	0.00
18) Fluoranthene-d10	18.945	212	6143	0.418	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.325	128	342	0.037	ng/ul#	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071124\
Data File : BM046530.D
Acq On : 11 Jul 2024 23:25
Operator : MA/JU
Sample : P3084-09
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E1GC9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024


Quant Time: Jul 12 05:11:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

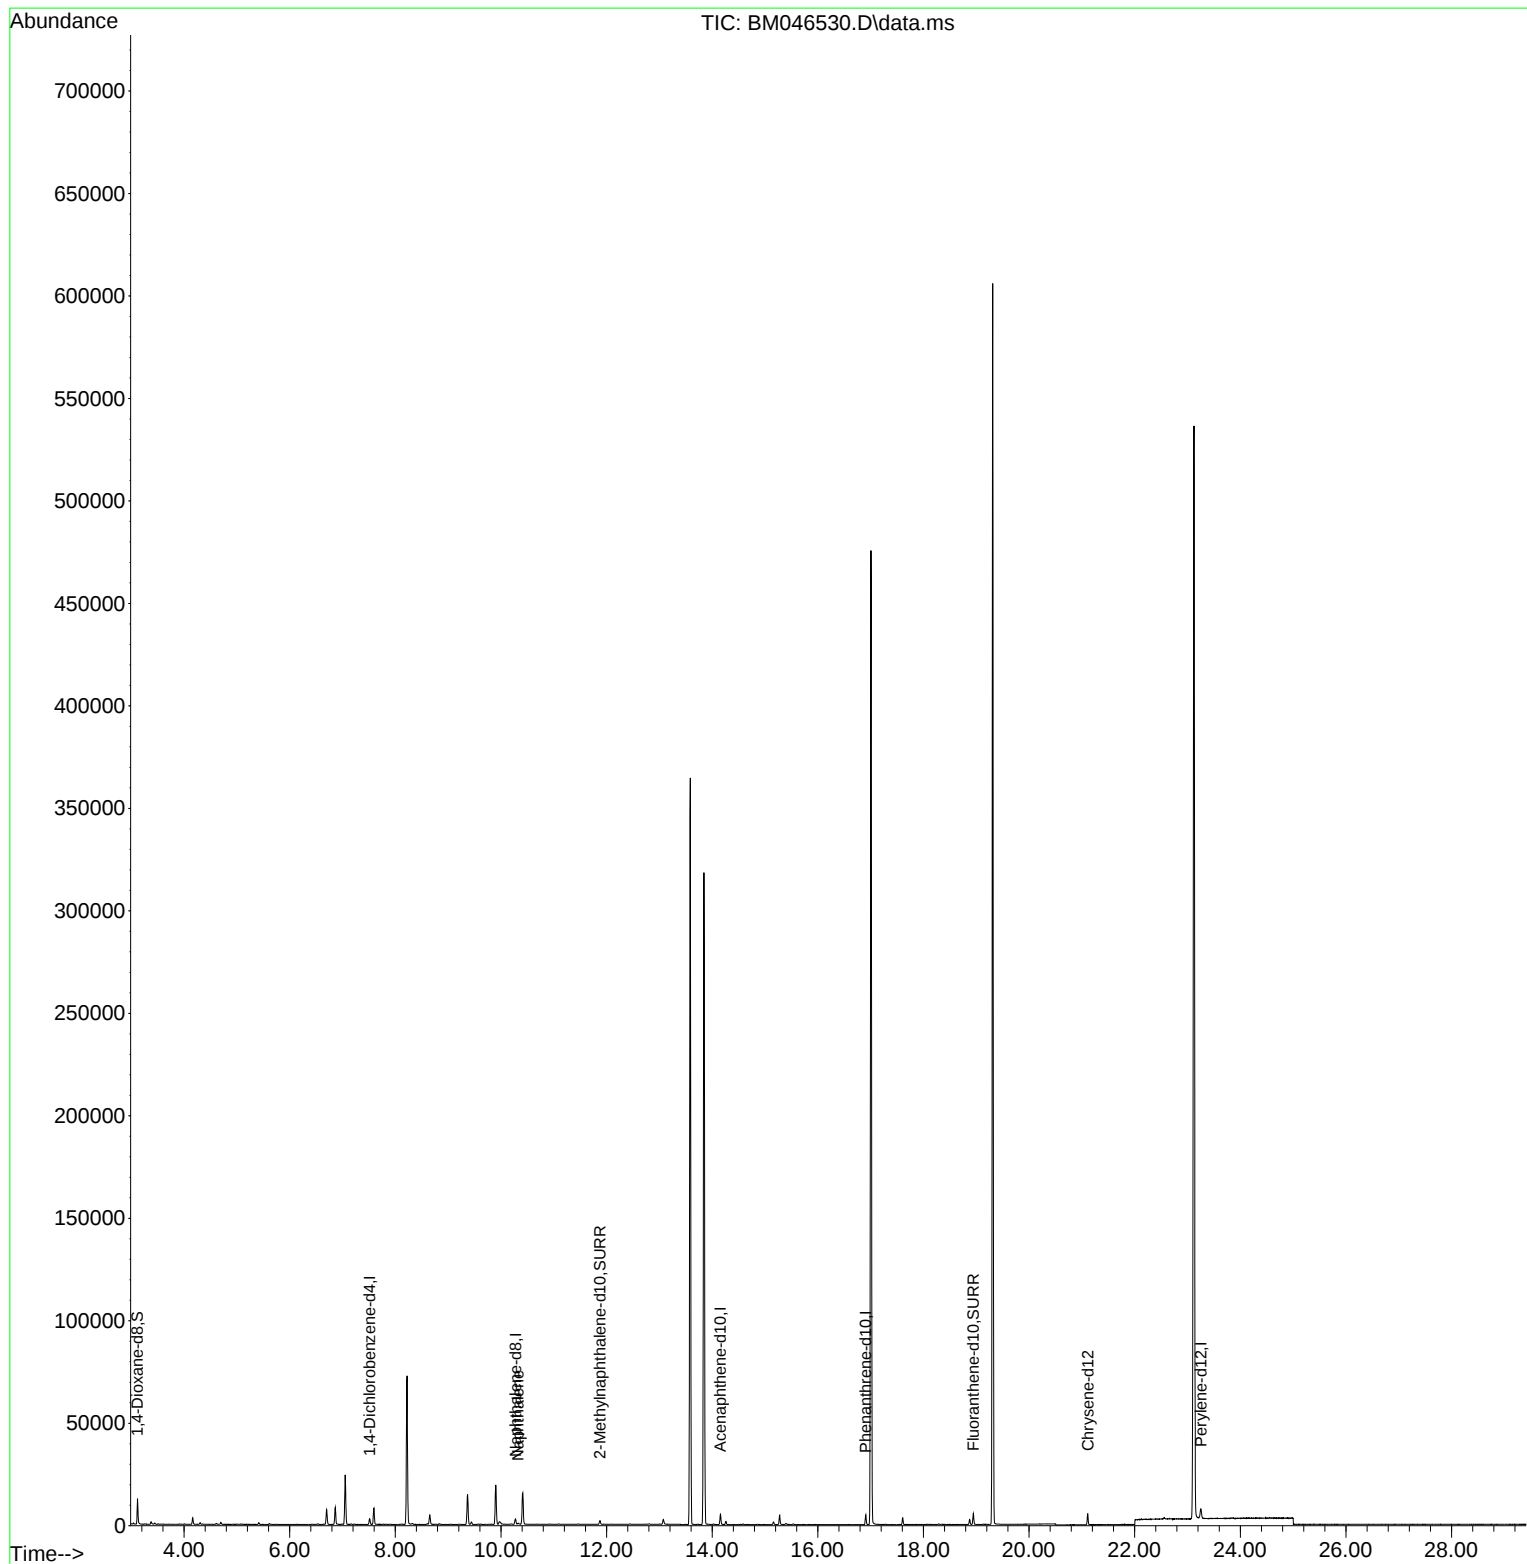

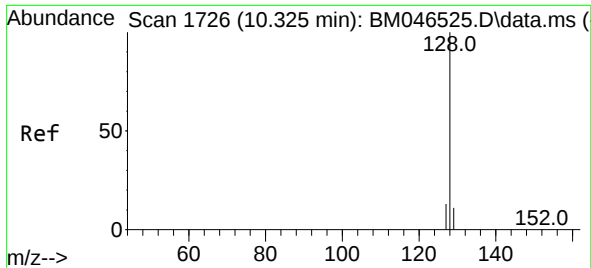

#5
Naphthalene
Concen: 0.037 ng/ul
RT: 10.325 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM046530.D
Acq: 11 Jul 2024 23:25

Instrument :
BNA_M
ClientSampleId :
E1GC9

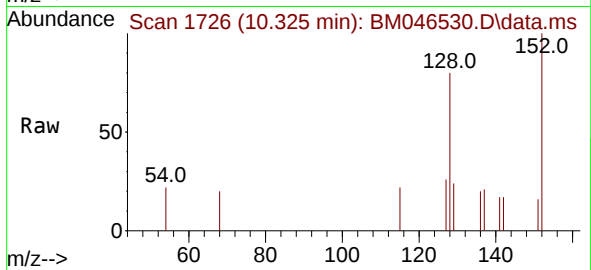

Tgt Ion:128 Resp: 342
Ion Ratio Lower Upper
128 100
129 30.6 10.3 15.5
127 32.2 12.2 18.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

