
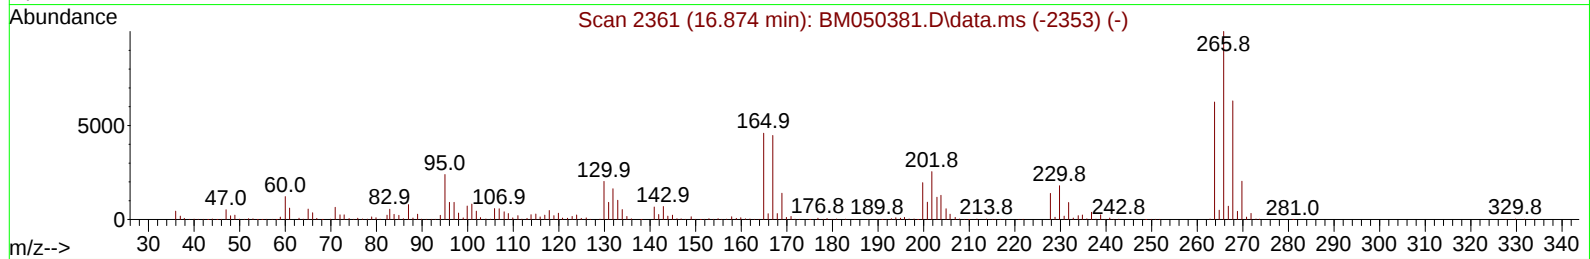
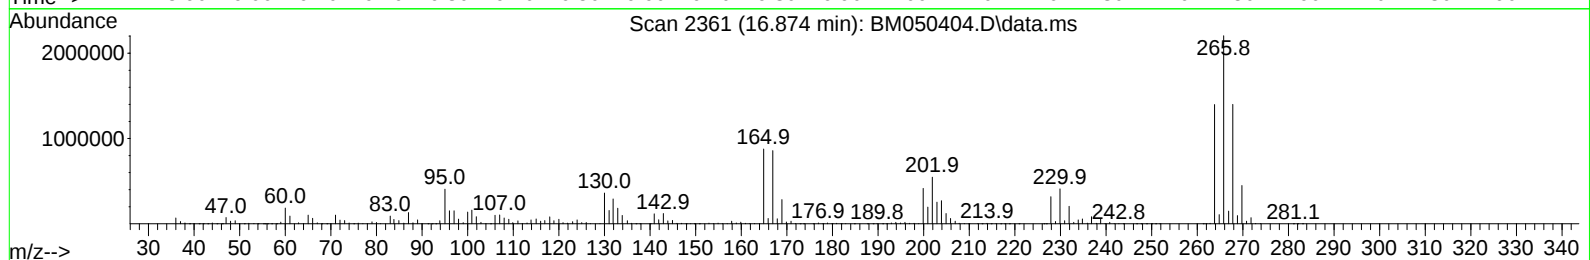


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071125\
Data File : BM050404.D
Acq On : 11 Jul 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 11:15:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

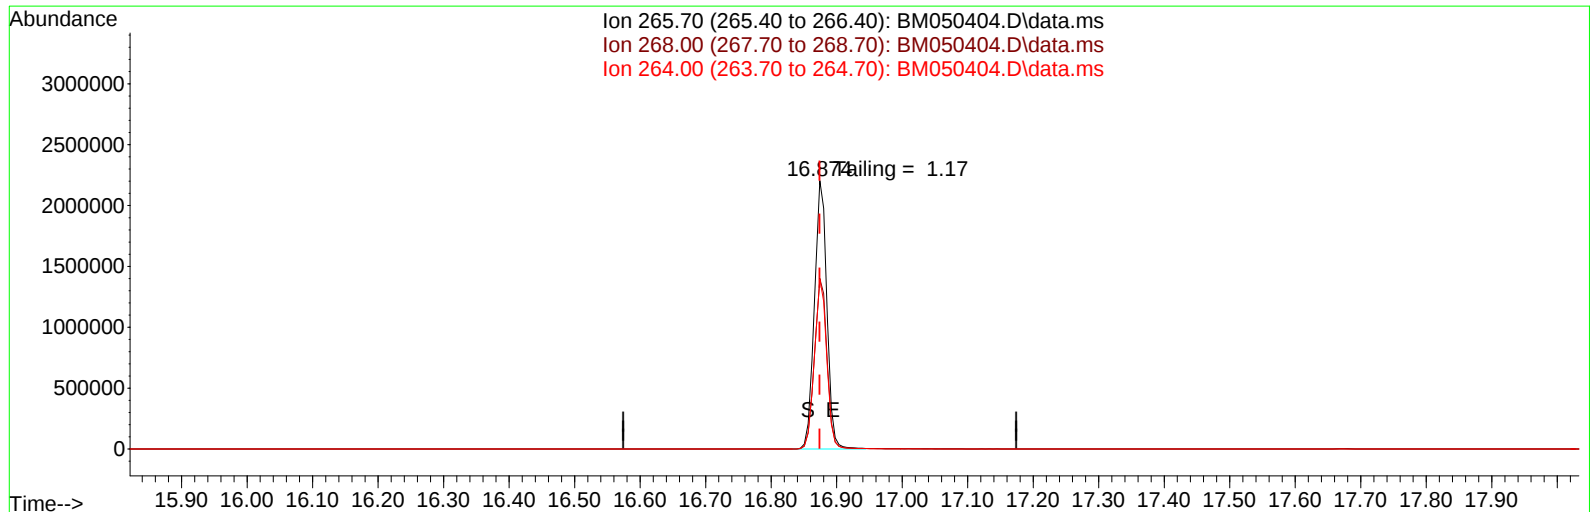

TIC: BM050404.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.000) 979981.22 ng

response 2929278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.49
264.00	62.40	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071125\
Data File : BM050404.D
Acq On : 11 Jul 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 11:15:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

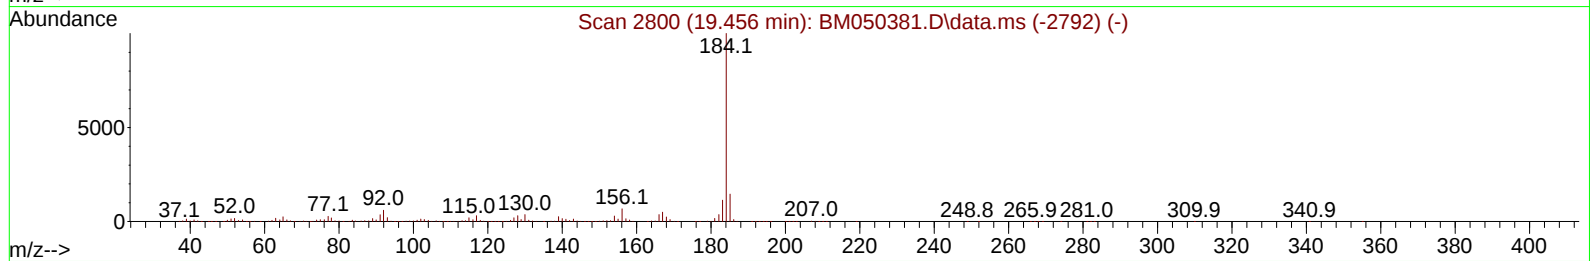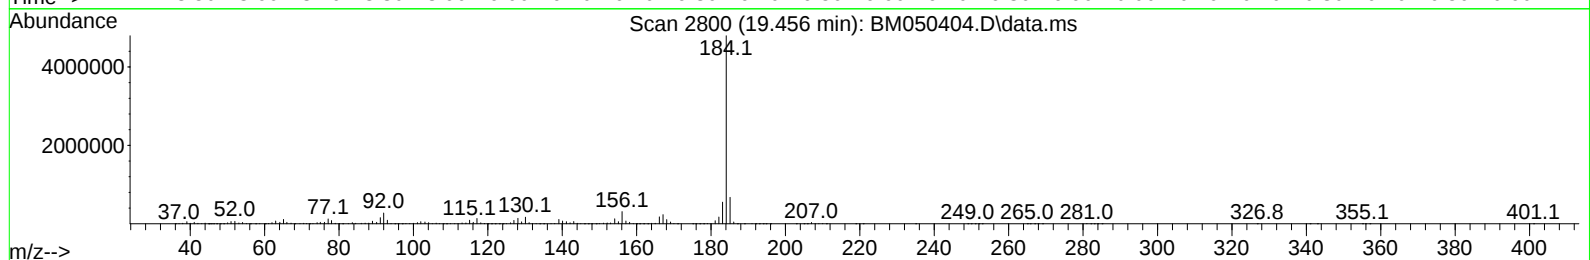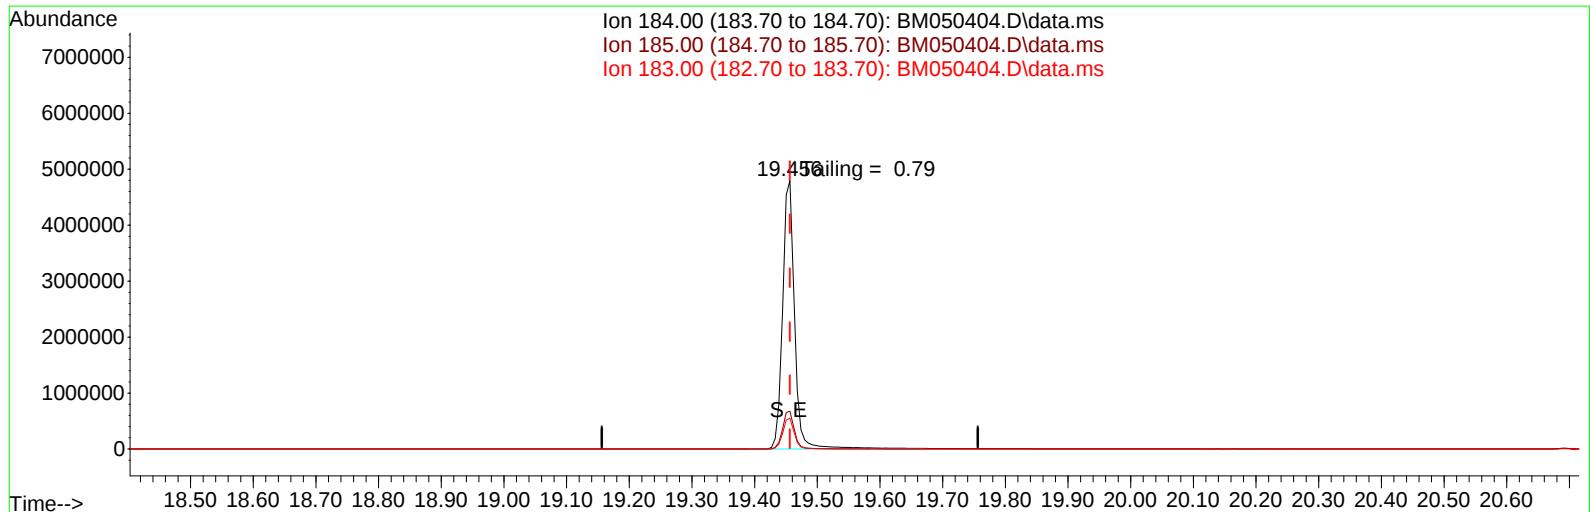

TIC: BM050404.D\data.ms

(77) Benzidine

19.456min (0.000) 235287.94 ng

response 6445446

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.09
183.00	11.30	11.49
0.00	0.00	0.00