


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071125\
Data File : BM050404.D
Acq On : 11 Jul 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 08 18:32:25 2025

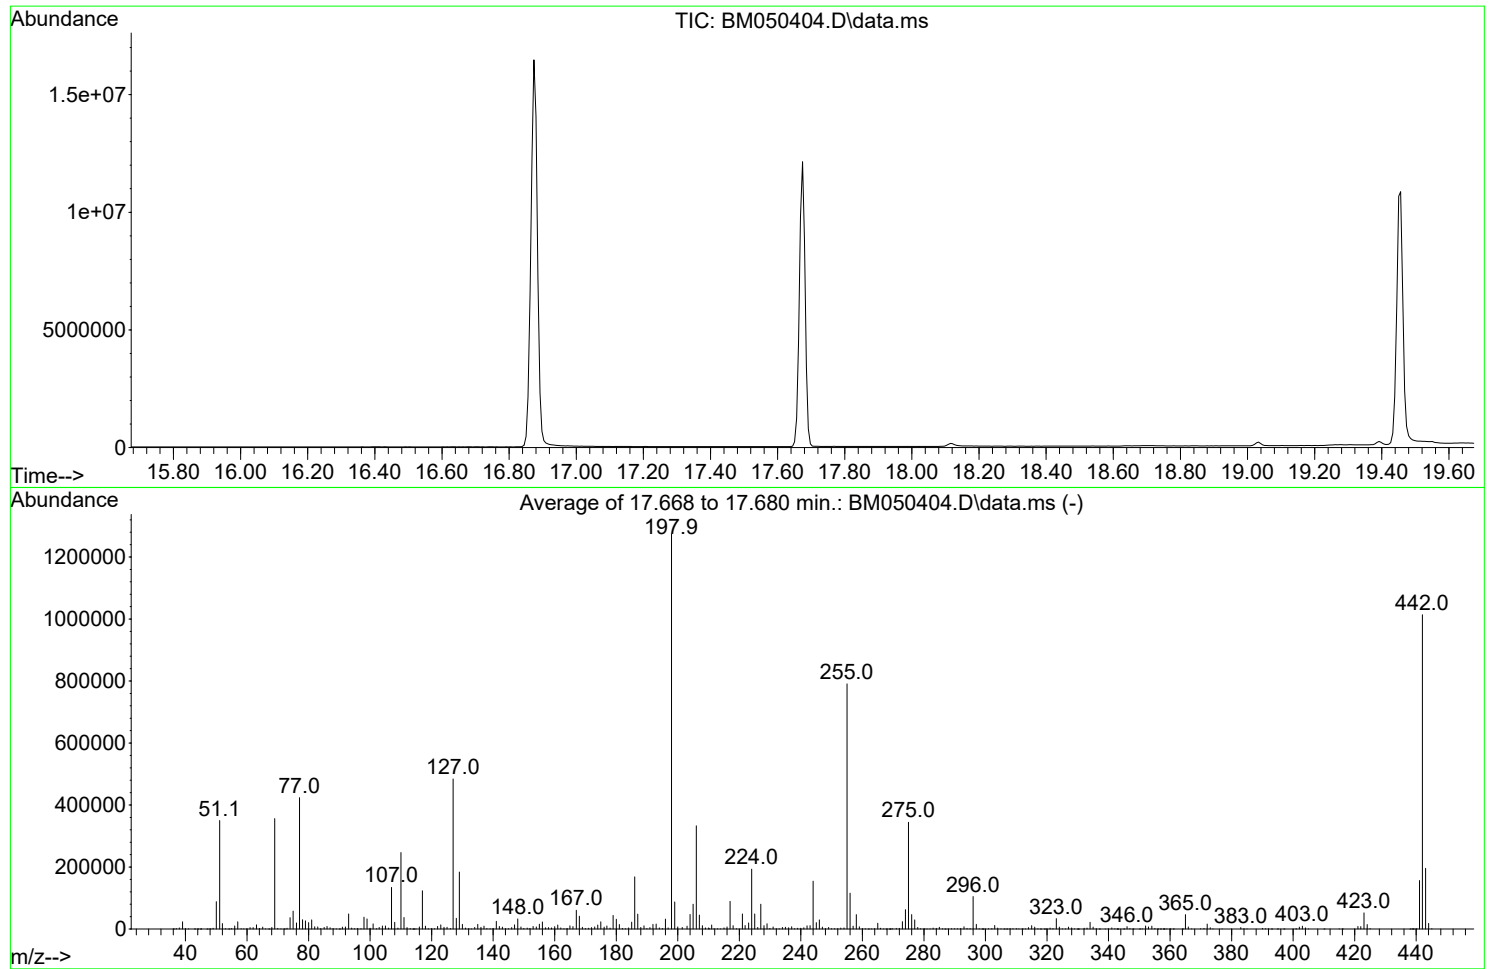

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	5317	PASS
69	69	100	100	100.0	356328	PASS
70	69	0.00	2	0.5	1930	PASS
197	198	0.00	2	0.3	3619	PASS
198	198	100	100	100.0	1273685	PASS
199	198	5	9	6.9	87397	PASS
365	198	1	100	3.6	46325	PASS
441	443	0.01	150	79.9	156275	PASS
442	442	100	100	100.0	1013803	PASS
443	442	15	24	19.3	195541	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/11/2025	BNA_M	<u>BM050404.D</u>
Compound Name	Response	Retention Time
DDT	3699626	20.692
DDD	35194	20.309
DDE	1870	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37064	3736690	0.99

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071125\
Data File : BM050404.D
Acq On : 11 Jul 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 11 11:15:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

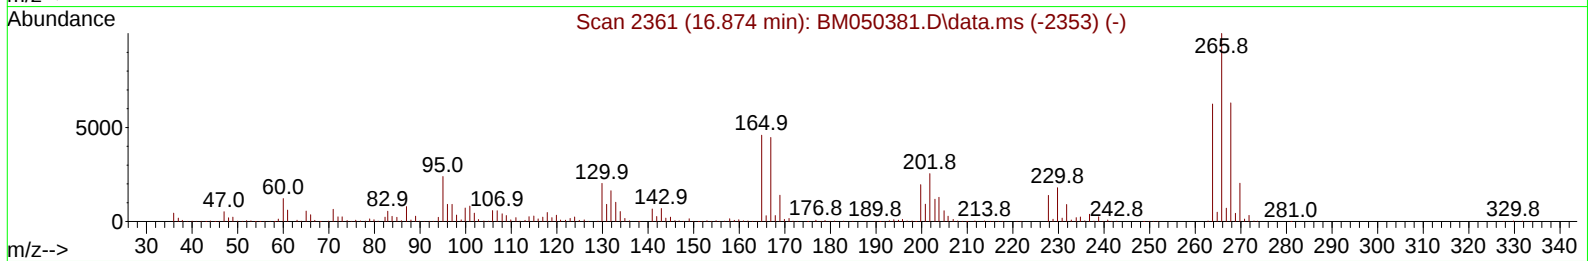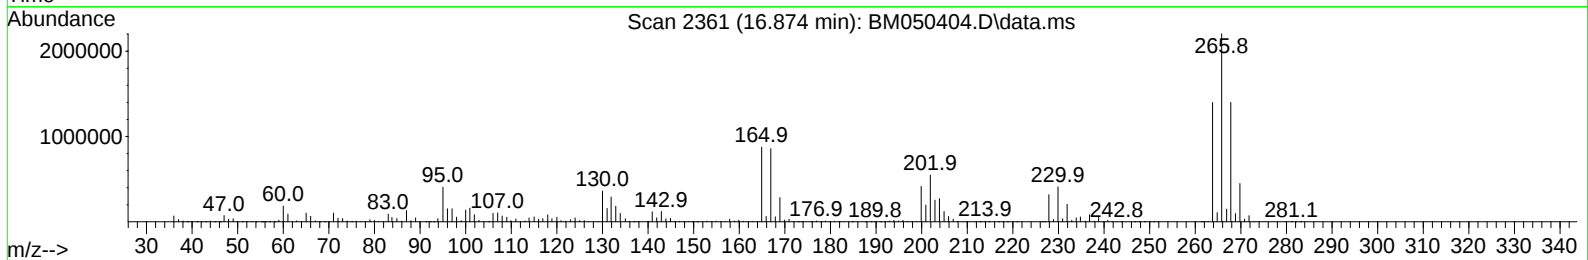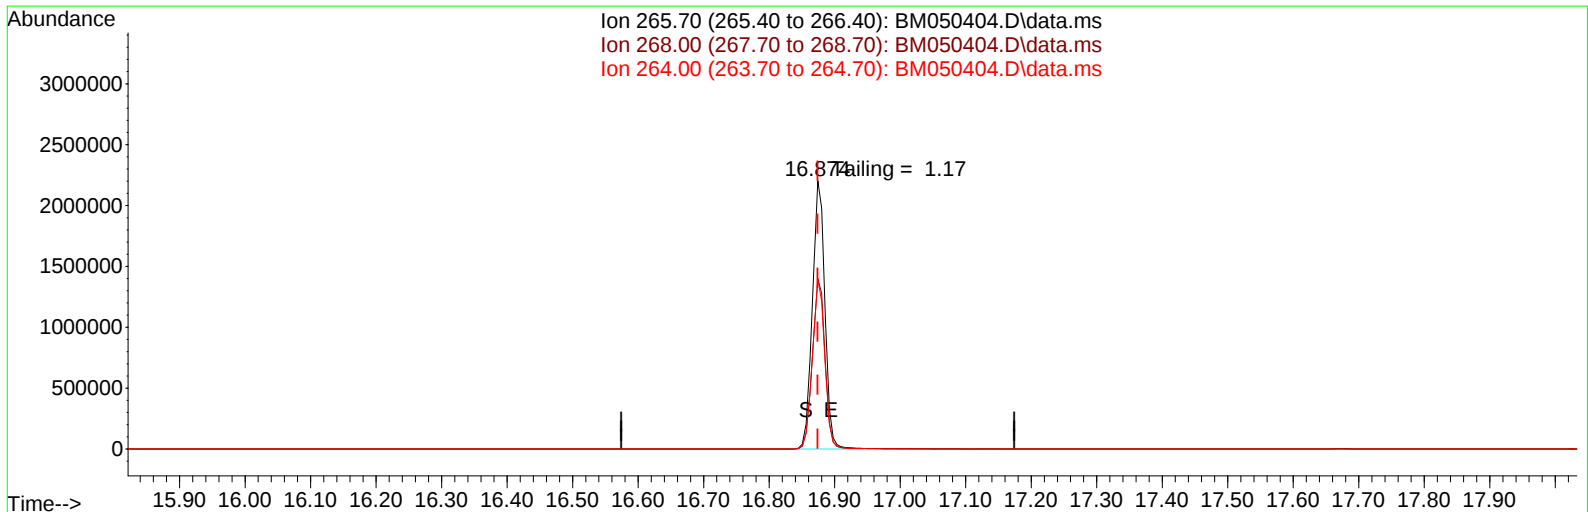

TIC: BM050404.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.000) 979981.22 ng




response 2929278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.49
264.00	62.40	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071125\
Data File : BM050404.D
Acq On : 11 Jul 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 11 11:15:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

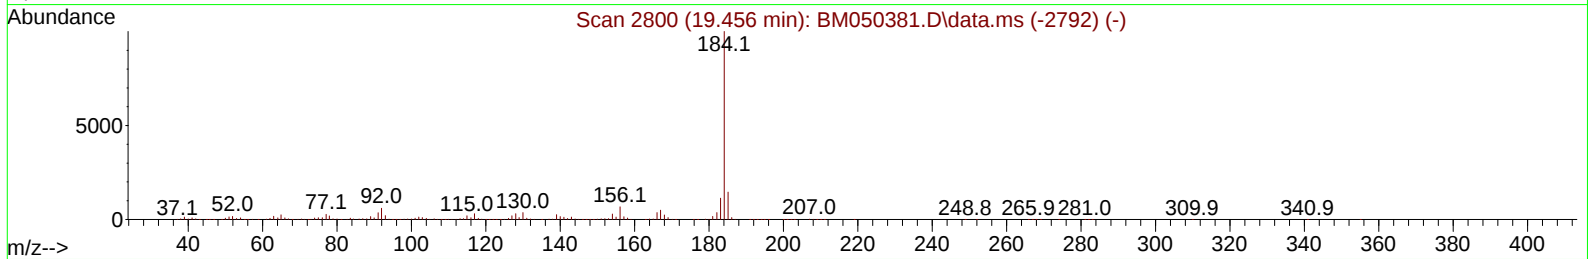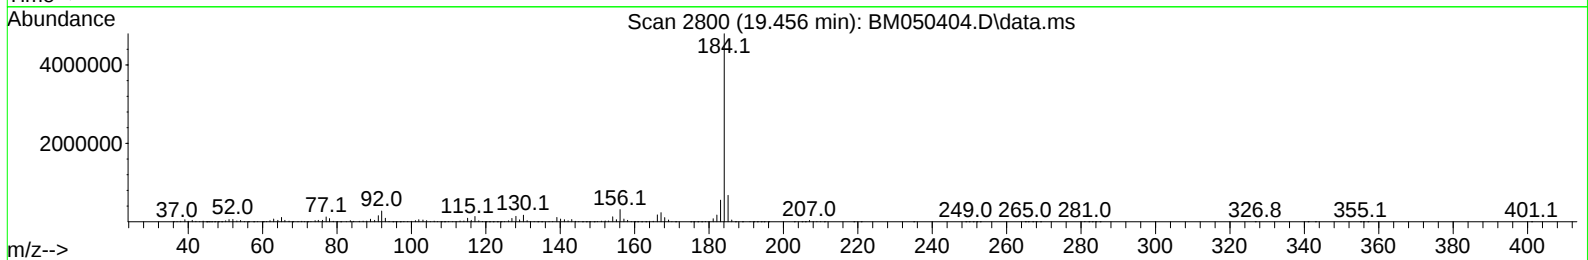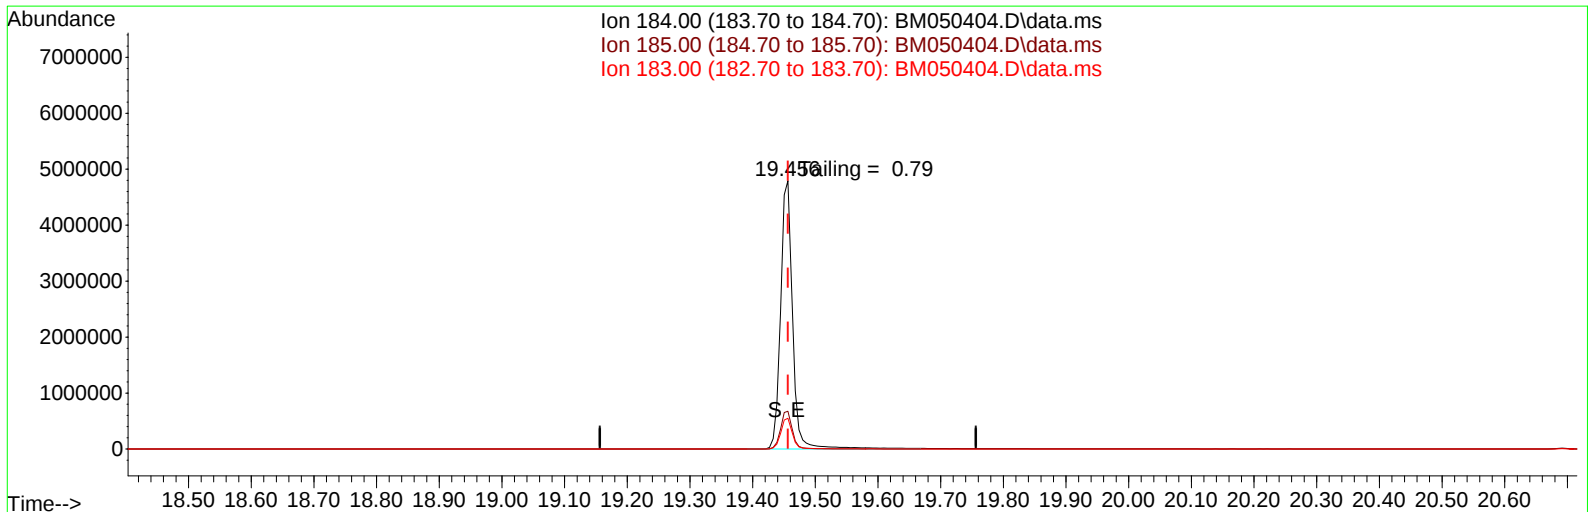

TIC: BM050404.D\data.ms

(77) Benzidine

19.456min (0.000) 235287.94 ng

response 6445446

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.09
183.00	11.30	11.49
0.00	0.00	0.00