
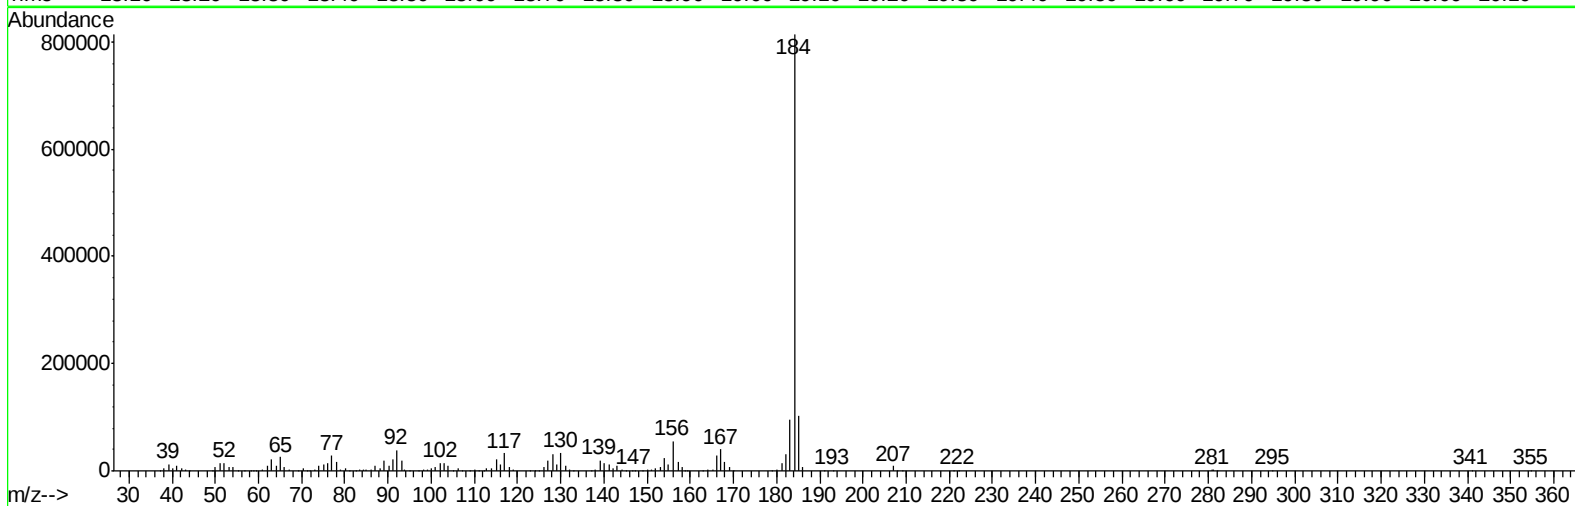


Data Path : Z:\HPCHEM1\BNA M\DATA\BM071217\
Data File : BM010801.D
Acq On : 12 Jul 2017 15:02
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 08:57:33 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

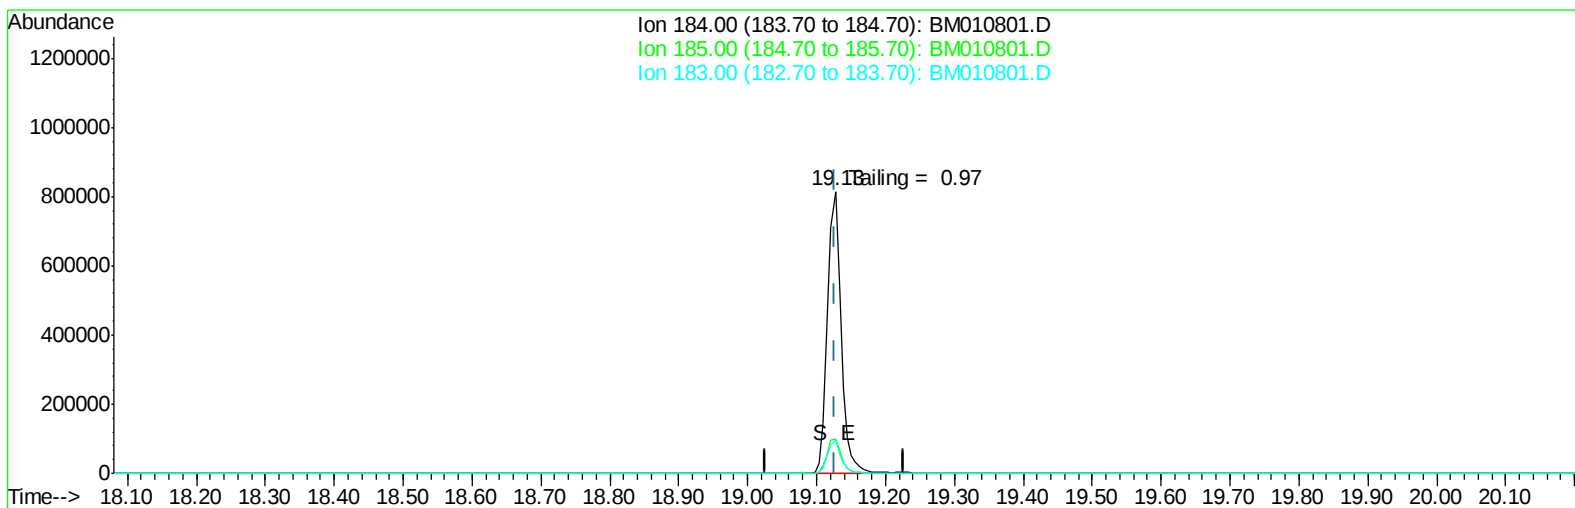

TIC: BM010801.D

(76) Benzidine

19.127min (+0.000) 11413.40ng

response 1116328

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	12.51
183.00	11.10	11.74
0.00	0.00	0.00