
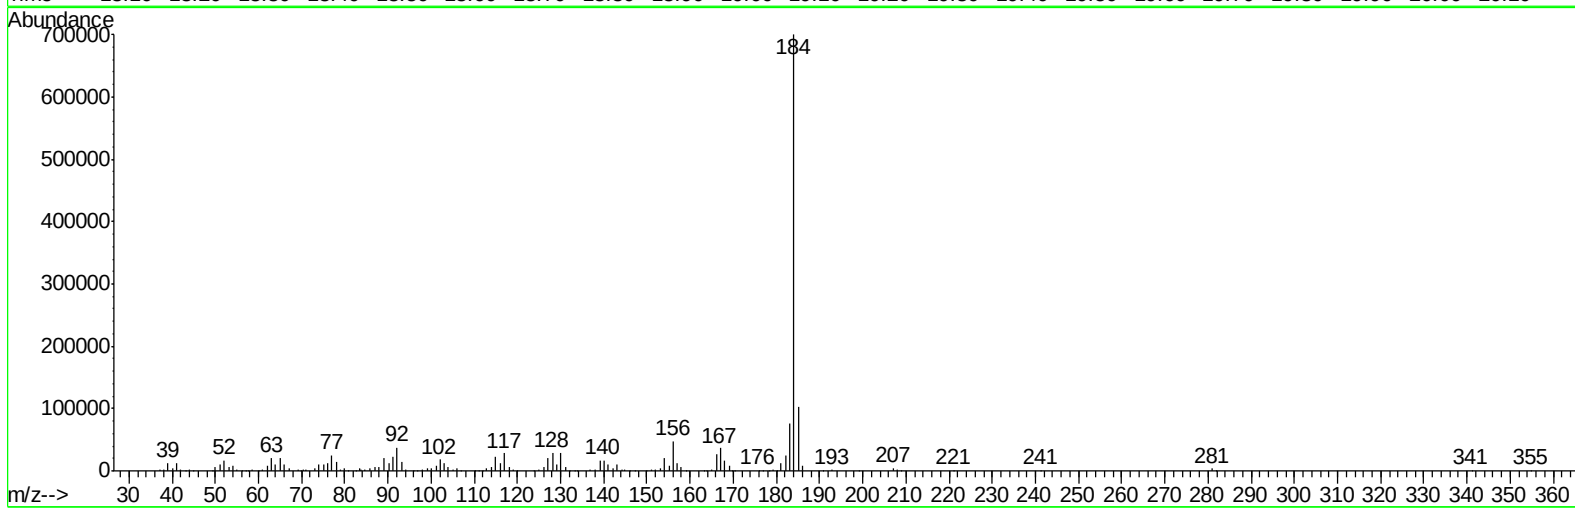


Data Path : Z:\HPCHEM1\BNA M\DATA\BM071217\
Data File : BM010792.D
Acq On : 12 Jul 2017 09:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 08:56:14 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

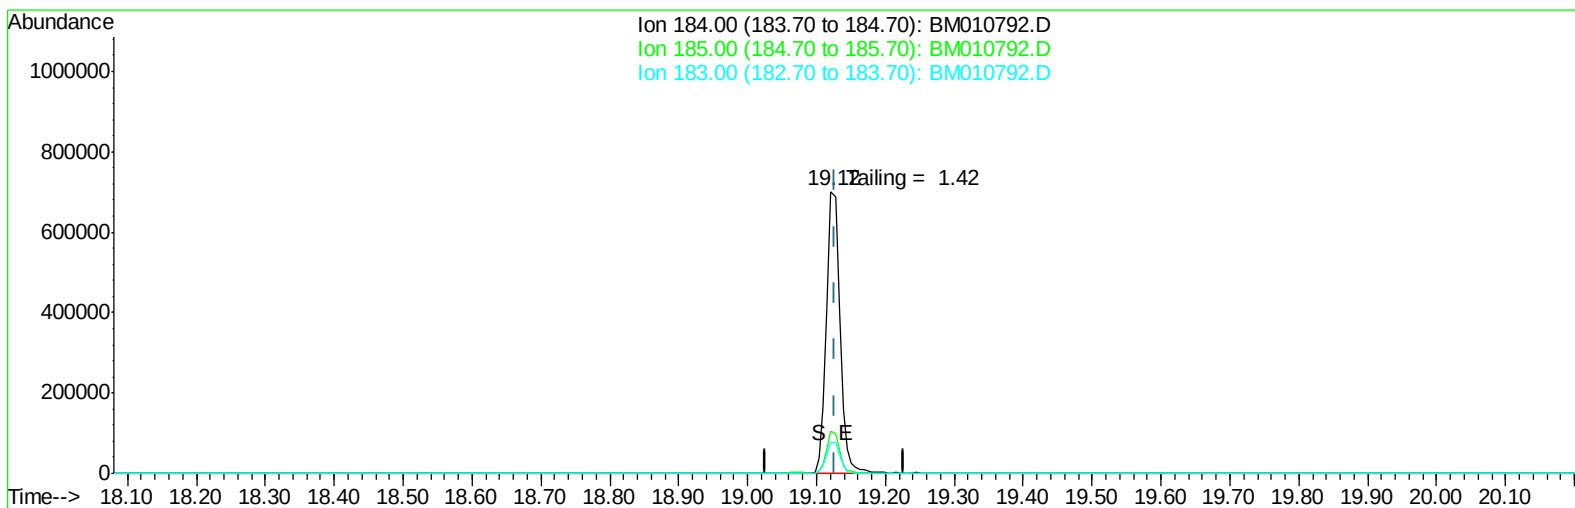

TIC: BM010792.D

(76) Benzidine



19.121min (-0.006) 18087.37ng

response 953523

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.82
183.00	11.10	10.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071217\
Data File : BM010792.D
Acq On : 12 Jul 2017 09:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 08:53:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

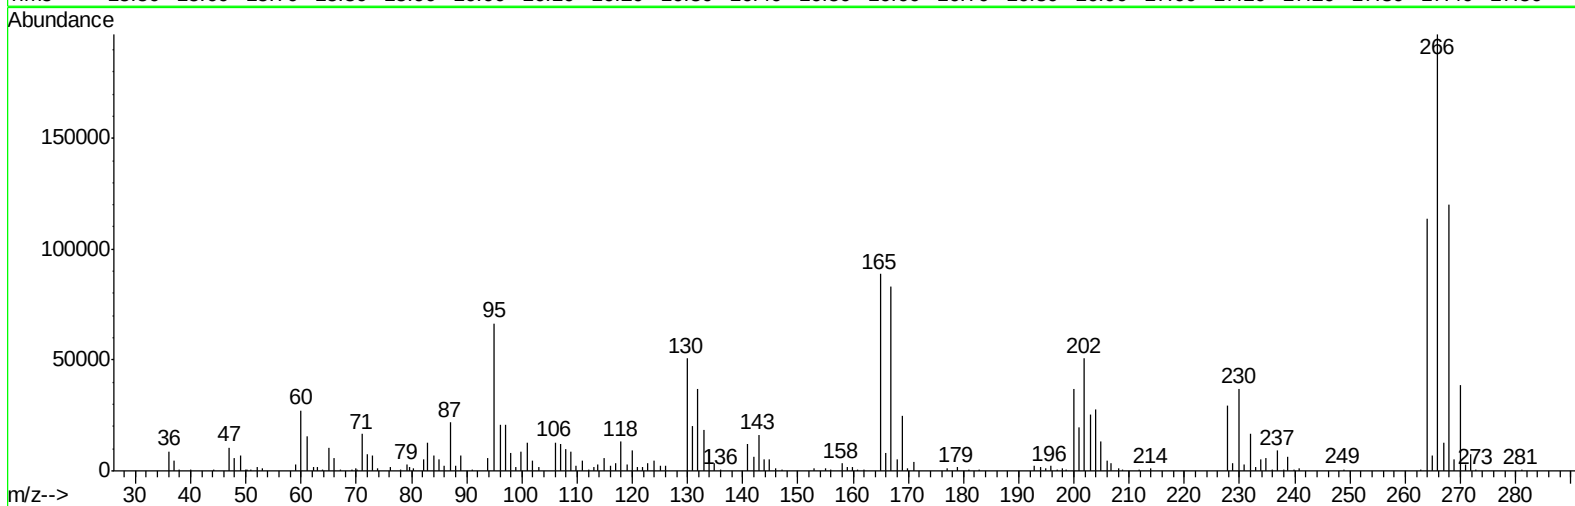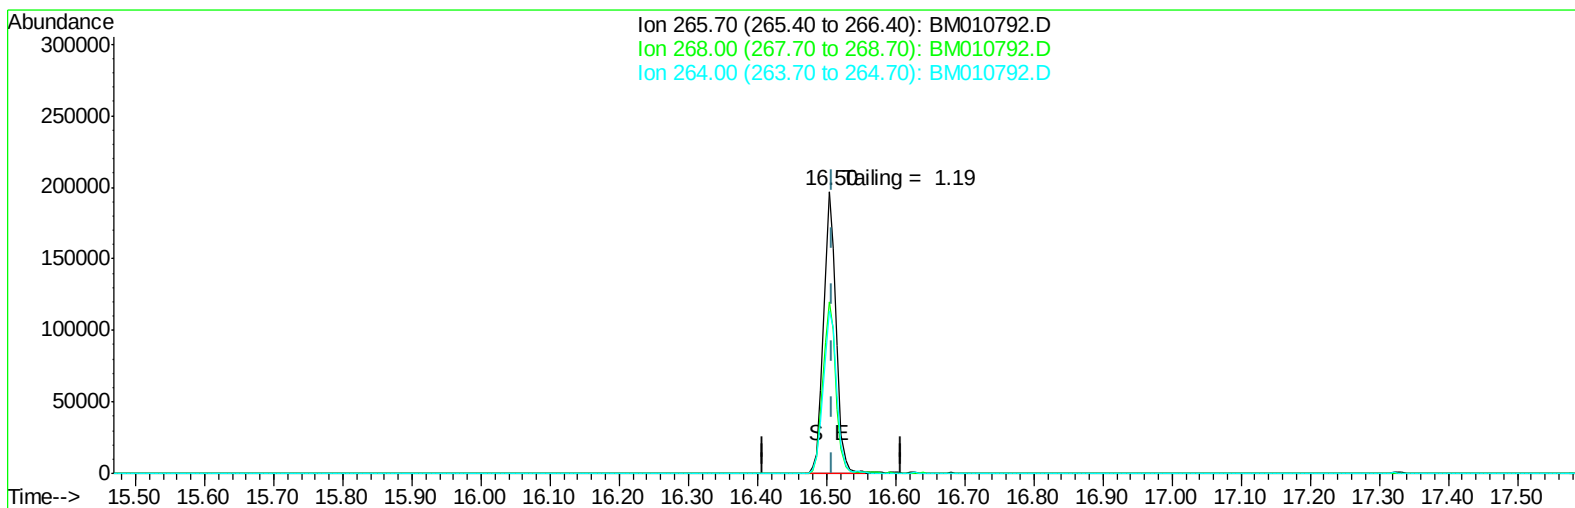

TIC: BM010792.D

(69) Pentachlorophenol (C)

16.504min (-0.006) 0.00ng

response 249038

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.10
264.00	61.20	57.68
0.00	0.00	0.00