


Data Path : Z:\HPCHEM1\BNA_M\Data\BM071217\
 Data File : BM010792.D
 Acq On : 12 Jul 2017 09:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

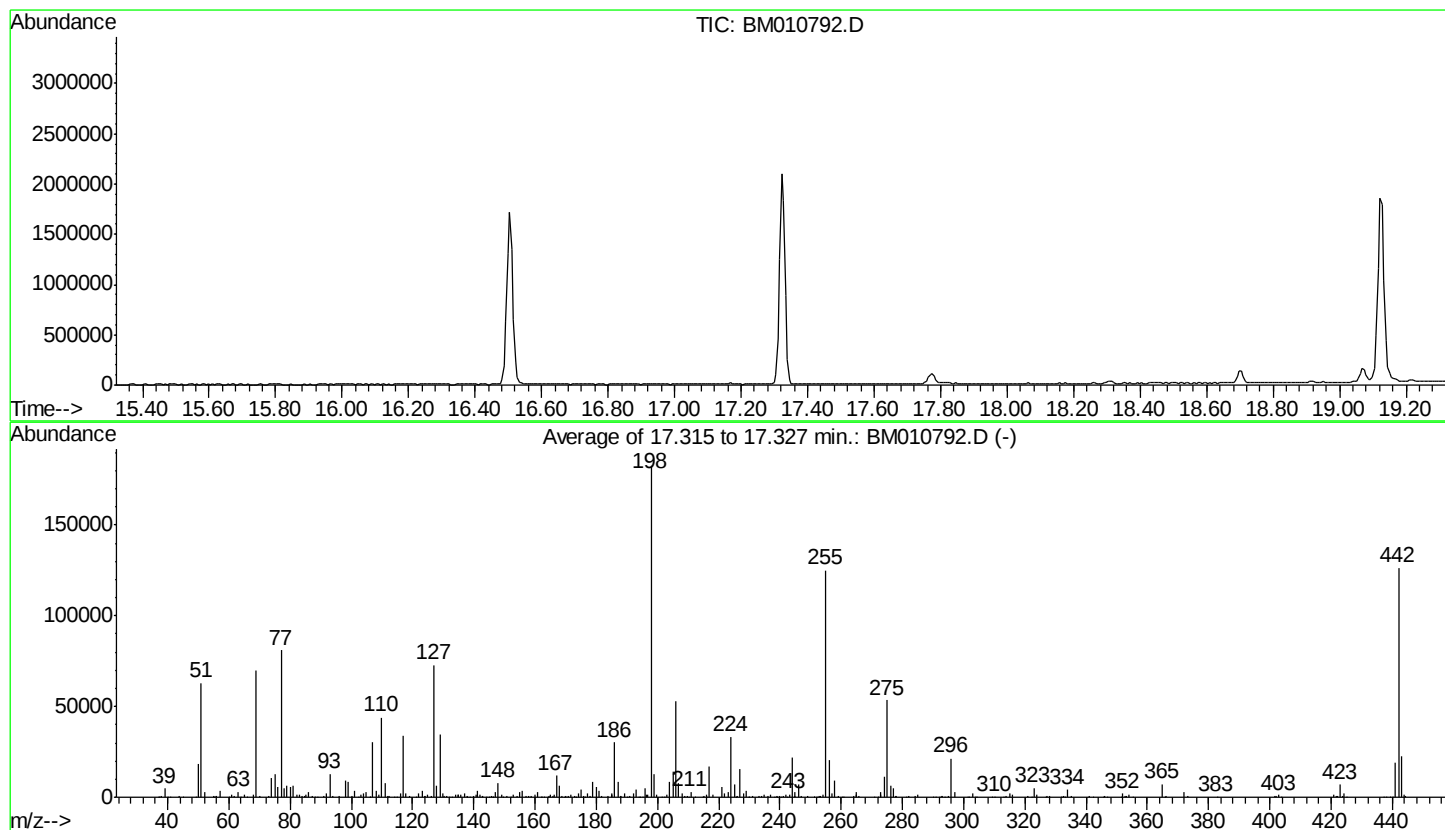

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	63131	PASS
68	69	0.00	2	1.8	1277	PASS
69	198	0.00	100	38.4	70232	PASS
70	69	0.00	2	0.6	404	PASS
127	198	10	80	39.9	72962	PASS
197	198	0.00	2	0.9	1661	PASS
198	198	100	100	100.0	182805	PASS
199	198	5	9	7.0	12809	PASS
275	198	10	60	29.3	53501	PASS
365	198	1	100	3.9	7204	PASS
441	443	0.01	100	84.1	19238	PASS
442	198	50	100	69.2	126589	PASS
443	442	15	24	18.1	22865	PASS