


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071315\
Data File : BM001897.D
Acq On : 13 Jul 2015 09:35
Operator : TP/UM
Sample : DFTPP72
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP72

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
Title : SVOA CALIBRATION
Last Update : Tue Apr 28 06:36:34 2015

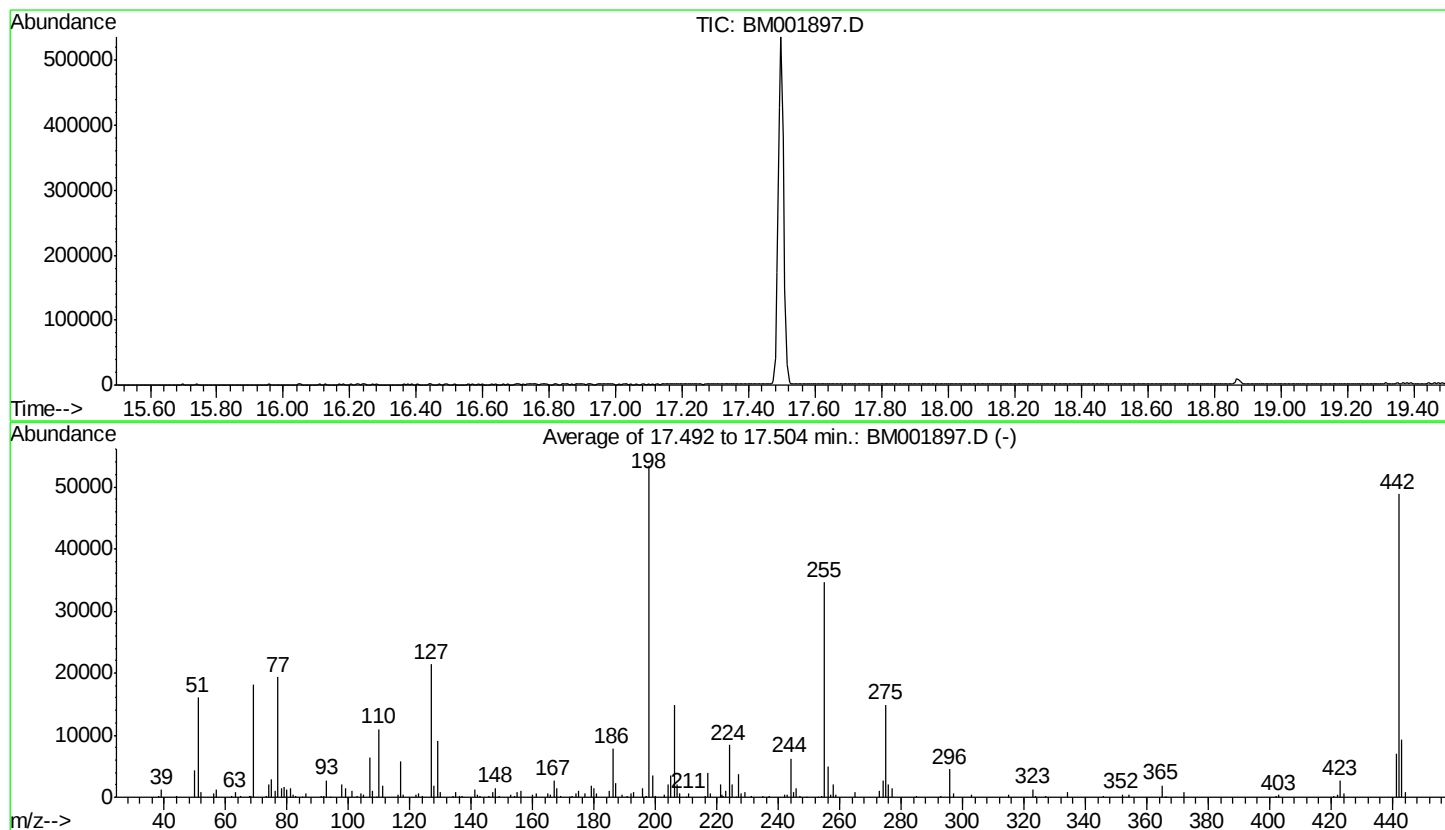

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	16035	PASS
68	69	0.00	2	0.8	148	PASS
69	198	0.00	100	33.9	18084	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.0	21384	PASS
197	198	0.00	2	0.4	187	PASS
198	198	100	100	100.0	53410	PASS
199	198	5	9	6.5	3460	PASS
275	198	10	60	27.9	14885	PASS
365	198	1	100	3.5	1887	PASS
441	443	0.01	100	74.6	6988	PASS
442	198	50	100	91.5	48850	PASS
443	442	15	24	19.2	9371	PASS

m/z	Abundance
38.00	331.0
39.10	1431.0
44.00	1019.0
50.00	4898.0
51.00	18408.0
52.00	973.0
55.90	619.0
56.90	1401.0
62.00	405.0
63.00	806.0
64.90	424.0
67.90	394.0
69.00	20080.0
73.00	351.0
74.00	2354.0
75.00	3224.0
76.00	1046.0
77.10	20704.0
78.10	1618.0
79.00	1804.0
80.00	1218.0
81.00	1716.0
81.90	401.0
82.90	355.0
85.90	603.0
91.00	361.0
92.10	388.0
93.00	3031.0
98.00	2274.0
99.00	1532.0
101.00	1067.0
102.90	340.0
104.00	529.0
105.00	575.0
107.00	7085.0
108.00	1100.0
109.00	316.0
110.00	11668.0
111.00	2046.0
115.90	448.0
117.00	6086.0
118.00	564.0
121.90	453.0
123.00	753.0
123.90	306.0
127.00	22632.0
128.00	1927.0
129.00	9226.0
129.90	759.0
135.00	788.0
136.00	338.0
136.90	395.0
141.00	1341.0
142.10	447.0
143.00	345.0
147.00	805.0
148.00	1651.0
149.00	438.0
153.00	479.0
153.90	343.0
154.90	699.0
156.00	1252.0
160.00	509.0
161.00	575.0
164.90	559.0
166.00	408.0
167.00	2441.0
168.00	1407.0
168.90	317.0
172.00	308.0
174.00	672.0
175.00	1195.0
177.00	632.0
179.00	1827.0
180.00	1428.0
180.90	507.0
185.00	778.0
186.10	7389.0
187.00	2205.0
188.90	532.0
191.90	626.0
193.00	819.0
196.00	1212.0
197.10	563.0
197.90	52888.0
199.00	3672.0
202.90	477.0
204.00	2173.0
205.00	3425.0
206.00	14248.0
207.10	2281.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72

208.10	618.0
211.10	431.0
216.10	345.0
217.00	4132.0
218.00	422.0
221.00	1973.0
221.80	678.0
223.00	969.0
224.00	7955.0
225.00	2079.0
227.00	3432.0
228.00	681.0
228.90	610.0
241.90	526.0
243.00	419.0
244.00	5605.0
245.00	758.0
245.90	1348.0
255.00	30056.0
256.00	4763.0
257.00	356.0
257.90	1889.0
258.80	361.0
265.10	608.0
273.00	886.0
274.00	2566.0
275.00	13064.0
276.00	1741.0
277.00	1317.0
296.00	3618.0
297.00	553.0
303.10	369.0
314.90	503.0
323.10	1092.0
333.90	576.0
352.00	356.0
354.00	420.0
365.00	1512.0
372.00	651.0
422.10	321.0
423.00	1820.0
424.10	432.0
441.10	5023.0
442.10	35192.0
443.10	6964.0
444.10	661.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72

m/z	Abundance
39.00	1216.0
43.90	864.0
50.10	5036.0
51.00	18264.0
52.00	1034.0
56.00	686.0
57.00	1287.0
63.00	877.0
64.90	468.0
68.10	445.0
69.00	20840.0
74.00	2370.0
75.00	3510.0
76.00	1196.0
77.10	22816.0
78.10	1415.0
78.90	1743.0
80.00	1295.0
81.00	1964.0
82.00	448.0
83.00	321.0
85.00	327.0
86.00	608.0
90.90	436.0
92.00	528.0
93.00	3323.0
94.00	309.0
98.00	2137.0
98.90	2068.0
101.00	1224.0
103.00	386.0
103.90	733.0
105.00	598.0
107.00	7623.0
108.00	1226.0
110.00	12666.0
111.00	1836.0
116.00	483.0
117.00	6660.0
118.10	535.0
122.00	533.0
122.90	925.0
124.00	371.0
127.00	24128.0
128.00	2069.0
129.00	11018.0
130.00	1053.0
133.90	462.0
135.00	931.0
136.00	371.0
137.00	317.0
141.00	1697.0
142.00	363.0
142.90	302.0
145.90	398.0
147.00	869.0
148.00	1711.0
148.90	357.0
153.00	602.0
153.90	419.0
155.00	1131.0
156.00	1275.0
160.00	543.0
161.00	762.0
165.00	551.0
166.00	486.0
167.00	3051.0
168.00	1551.0
169.00	376.0
173.00	355.0
173.90	816.0
175.10	1034.0
176.90	658.0
179.00	2382.0
179.90	1641.0
181.00	666.0
185.00	1356.0
186.00	9293.0
187.00	2763.0
189.00	490.0
190.90	415.0
191.90	664.0
193.00	792.0
195.90	1624.0
198.00	63472.0
198.90	4163.0
199.90	333.0
202.90	489.0
204.00	2433.0
205.00	4215.0
206.10	18016.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72

207.00	2880.0
207.90	825.0
210.00	327.0
210.90	905.0
216.00	336.0
217.00	4447.0
218.00	819.0
220.90	2489.0
221.80	796.0
223.00	1119.0
224.00	10138.0
225.00	2345.0
226.00	325.0
227.00	4681.0
228.00	734.0
229.00	1022.0
231.00	430.0
234.90	499.0
236.90	347.0
242.00	419.0
243.10	538.0
244.00	7384.0
245.00	963.0
245.90	1550.0
247.00	332.0
249.10	327.0
252.90	308.0
254.00	351.0
255.00	42312.0
256.00	5793.0
256.90	580.0
258.00	2720.0
258.90	489.0
264.90	1069.0
273.00	1379.0
274.00	3028.0
275.00	18024.0
276.00	2382.0
277.00	1676.0
285.00	463.0
292.90	322.0
296.00	5887.0
297.00	760.0
303.00	426.0
314.90	563.0
323.00	1620.0
323.90	359.0
326.90	453.0
334.00	1023.0
346.00	360.0
352.00	540.0
354.00	402.0
365.00	2163.0
365.90	321.0
372.00	790.0
402.00	410.0
403.10	513.0
421.00	395.0
422.00	358.0
423.00	3294.0
424.10	730.0
441.10	7894.0
442.10	58152.0
443.10	11510.0
444.00	962.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72

m/z	Abundance
39.00	958.0
44.00	1072.0
50.00	3077.0
51.10	11435.0
52.00	558.0
55.90	442.0
57.00	796.0
63.00	535.0
69.00	13334.0
74.00	1306.0
75.00	2006.0
76.10	673.0
77.10	14495.0
78.00	1138.0
79.00	1147.0
80.00	935.0
81.00	954.0
82.00	324.0
85.90	453.0
93.00	1962.0
98.00	1581.0
99.00	1043.0
100.90	599.0
103.90	389.0
104.90	392.0
107.00	4720.0
108.00	669.0
110.00	8686.0
110.90	1547.0
115.90	363.0
117.00	4520.0
117.90	325.0
123.10	414.0
127.00	17392.0
128.00	1419.0
129.00	7252.0
130.00	535.0
135.00	486.0
140.90	820.0
142.00	443.0
147.00	549.0
147.90	1101.0
152.90	364.0
155.00	429.0
156.00	807.0
159.90	345.0
161.00	476.0
165.00	501.0
165.90	336.0
167.00	2383.0
168.00	1158.0
173.00	326.0
174.00	362.0
175.00	732.0
176.80	366.0
178.90	1446.0
180.00	1017.0
181.00	455.0
185.00	821.0
186.10	6614.0
187.00	1669.0
189.00	503.0
191.90	566.0
193.00	608.0
195.90	1244.0
196.60	319.0
198.00	43872.0
198.90	2545.0
202.90	447.0
204.00	1763.0
205.00	2966.0
206.00	12204.0
207.00	2324.0
207.90	528.0
211.00	509.0
217.00	3392.0
218.00	384.0
221.10	1711.0
222.00	475.0
223.00	788.0
224.00	7195.0
225.00	1747.0
227.00	3114.0
227.90	445.0
228.90	731.0
242.00	424.0
243.10	401.0
244.00	5873.0
245.00	715.0
245.90	1226.0
255.00	31352.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72

256.00	4391.0
256.90	349.0
257.90	1433.0
258.90	310.0
265.10	761.0
273.00	1029.0
274.00	2498.0
275.00	13567.0
276.00	1869.0
276.90	1306.0
293.00	305.0
296.00	3957.0
297.00	651.0
302.90	440.0
315.00	467.0
323.00	1318.0
334.00	934.0
346.00	300.0
352.00	383.0
354.10	486.0
365.00	1987.0
366.10	311.0
372.00	824.0
401.90	303.0
403.00	440.0
421.00	325.0
422.00	436.0
423.10	2750.0
424.00	542.0
441.10	8049.0
442.10	53208.0
443.00	9641.0
444.10	946.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72

m/z	Abundance
44.00	832.0
206.90	443.0

Instrument :
BNA_M
ClientSampleId :
DFTPP72