
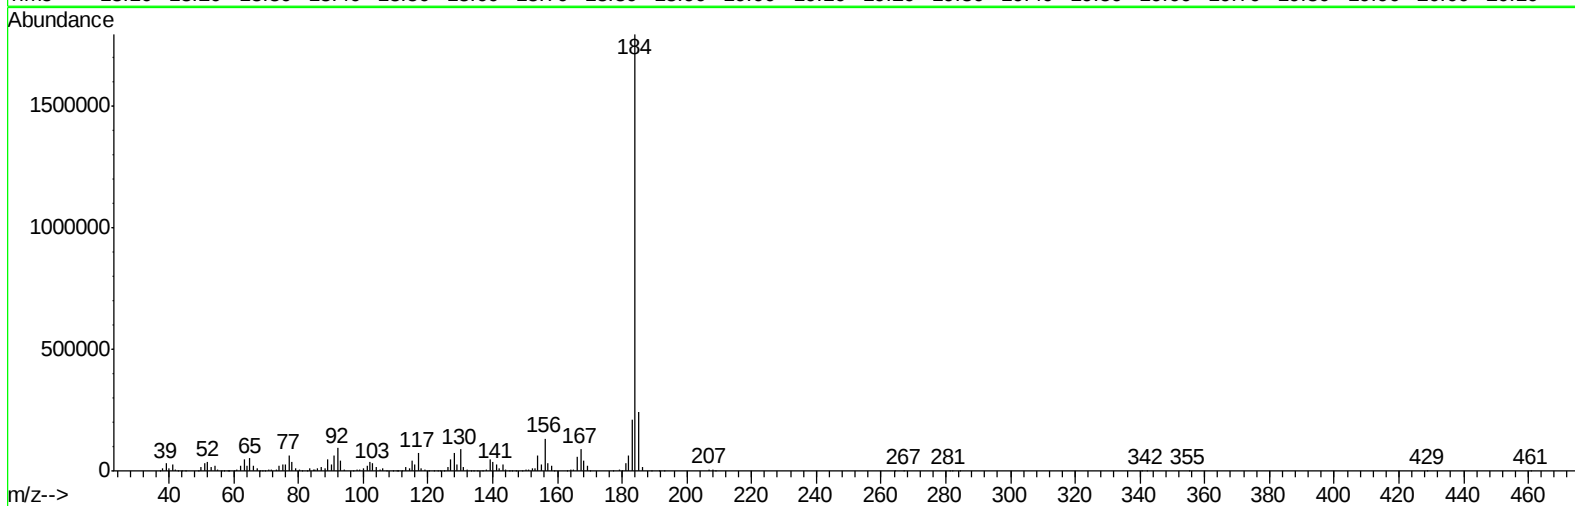


Data Path : Z:\HPCHEM1\BNA M\Data\BM071317\
Data File : BM010801.D
Acq On : 13 Jul 2017 08:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 09:16:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

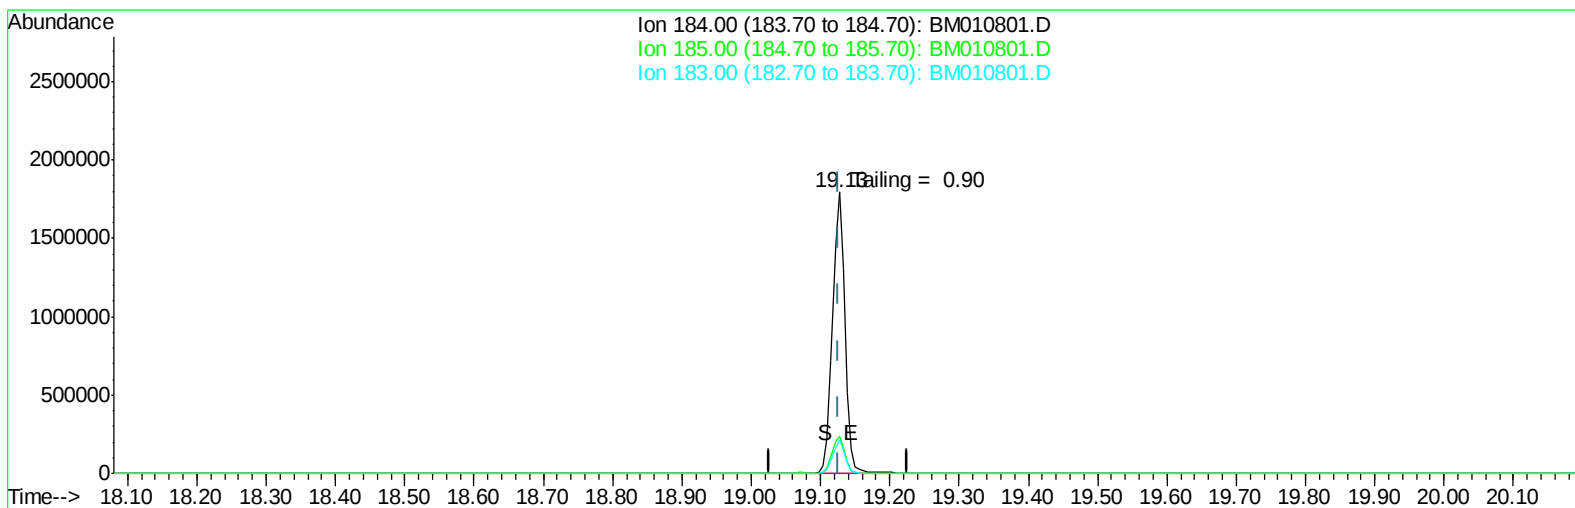

TIC: BM010801.D

(76) Benzidine



19.127min (+0.000) 2686.93ng

response 2243439

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.39
183.00	11.10	11.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM071317\
Data File : BM010801.D
Acq On : 13 Jul 2017 08:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 09:16:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

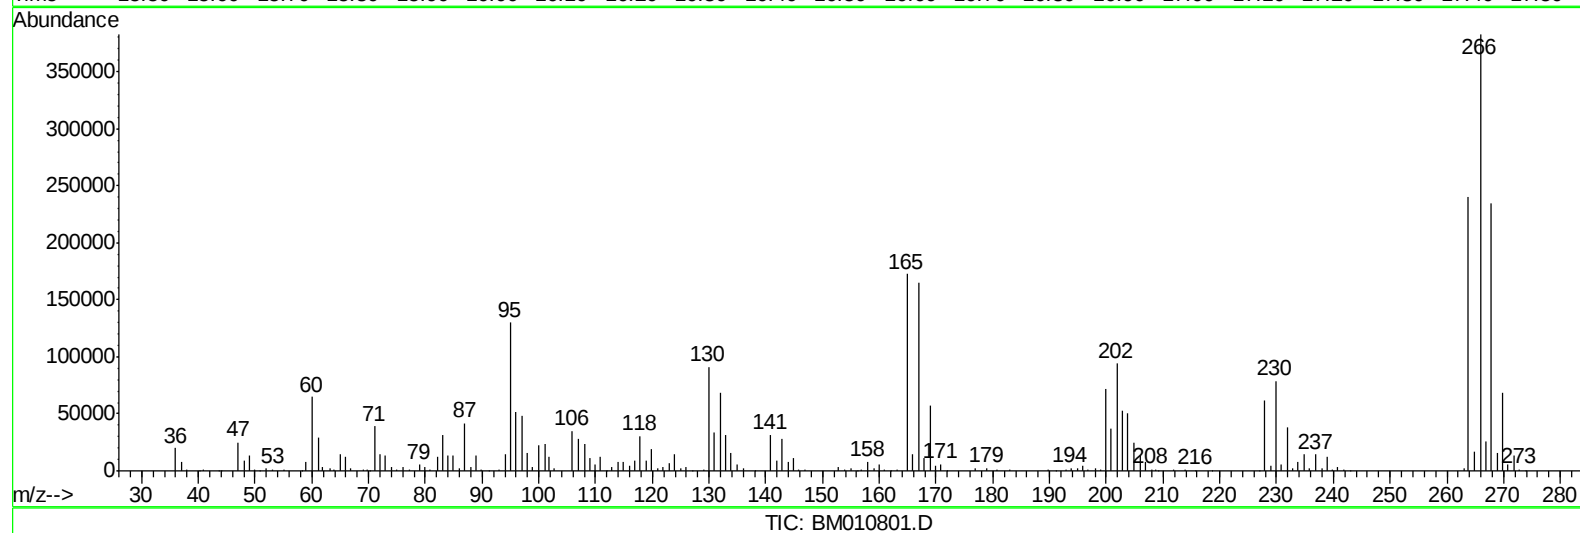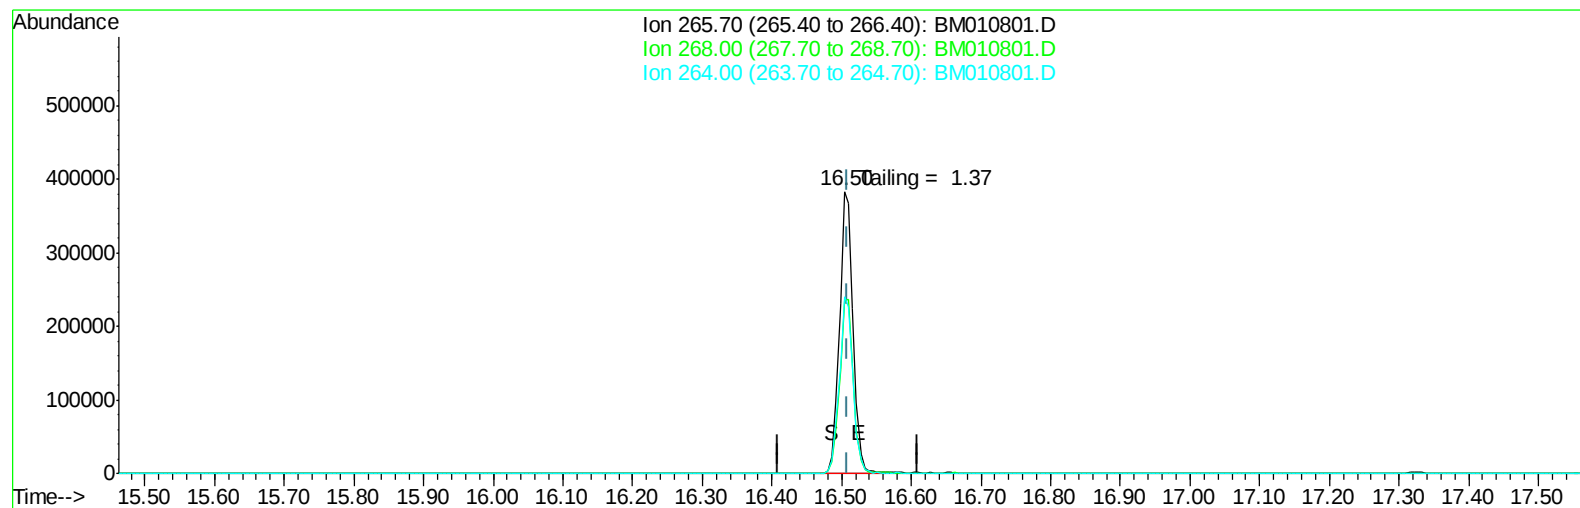

(69) Pentachlorophenol (C)

16.504min (-0.006) 456276.80ng

response 517134

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.43
264.00	61.20	62.87
0.00	0.00	0.00