
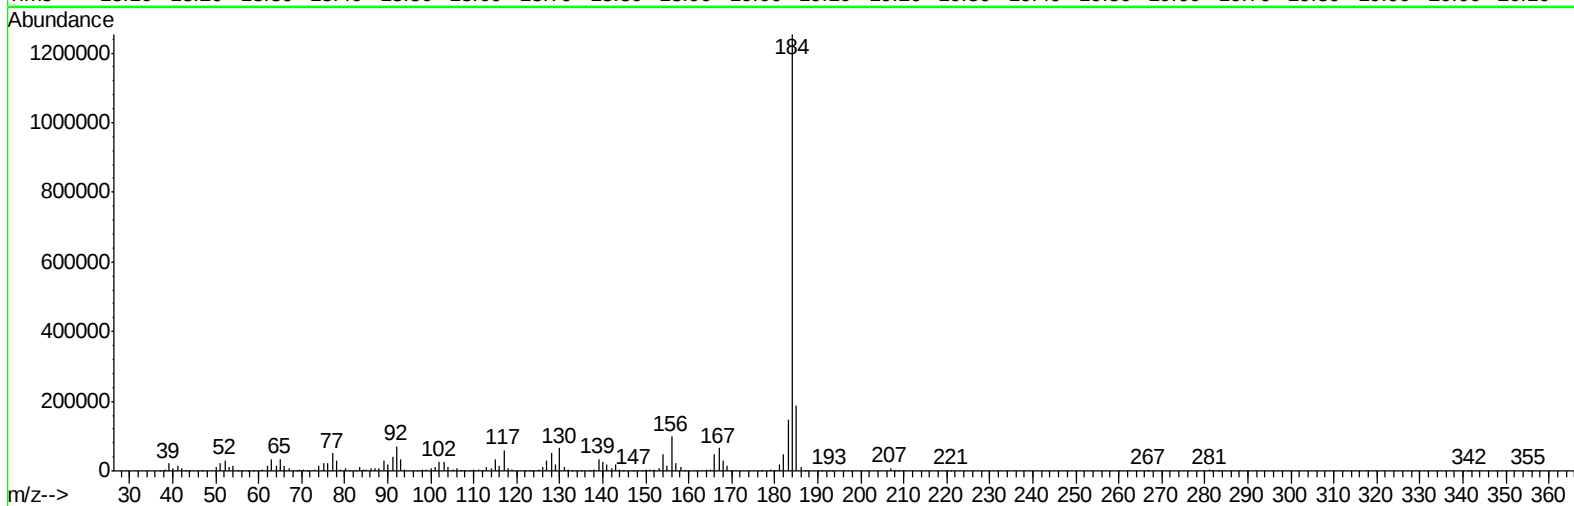


Data Path : Z:\HPCHEM1\BNA M\Data\BM071317\
 Data File : BM010818.D
 Acq On : 13 Jul 2017 18:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 09:18:36 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 14:21:16 2017
 Response via : Initial Calibration

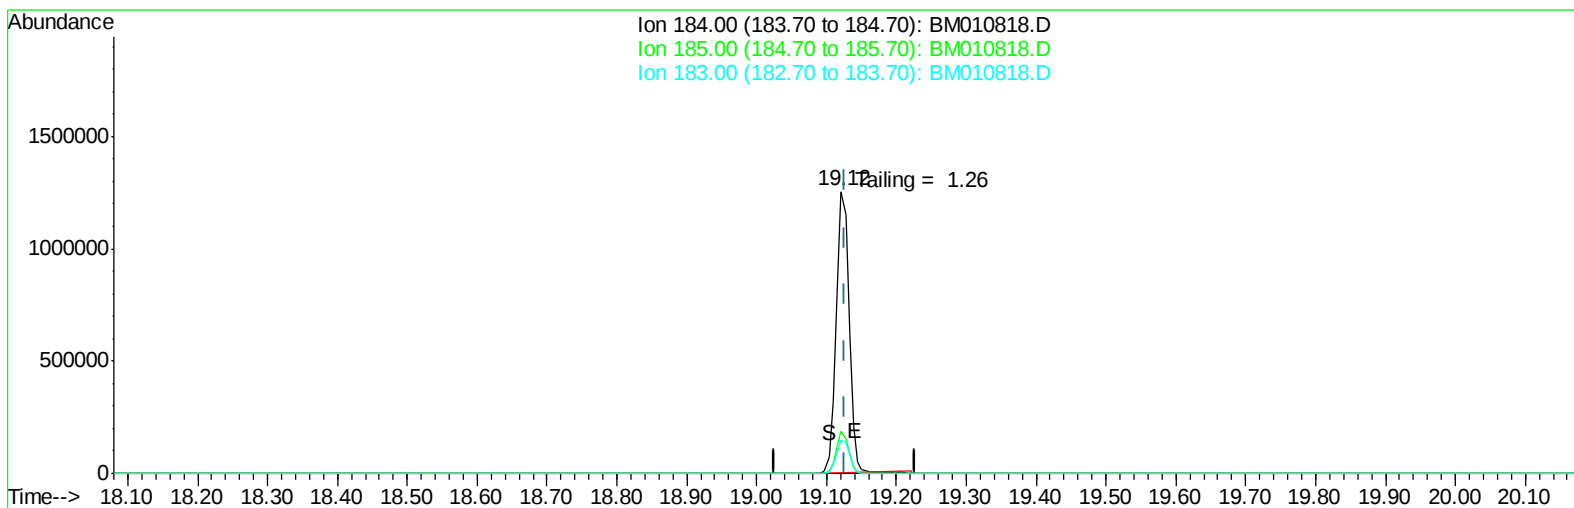

TIC: BM010818.D

(76) Benzidine



19.121min (-0.006) 66137.49ng

response 1598177

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.88
183.00	11.10	11.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM071317\
Data File : BM010818.D
Acq On : 13 Jul 2017 18:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 09:18:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

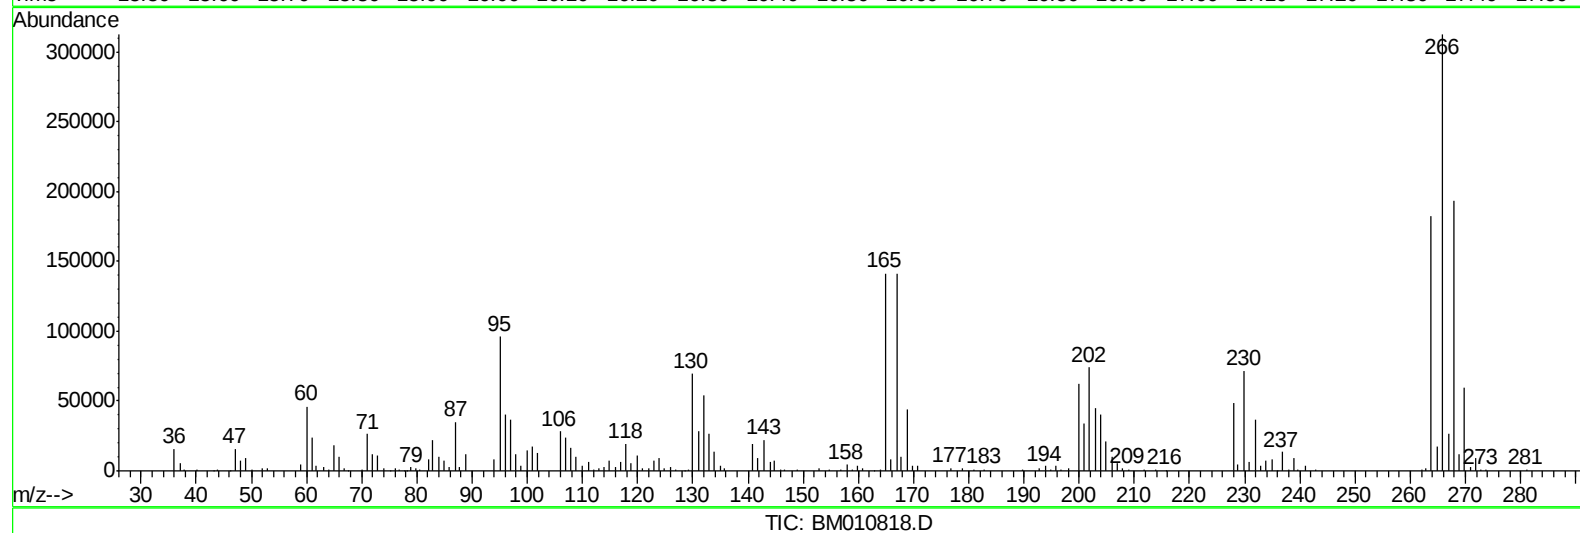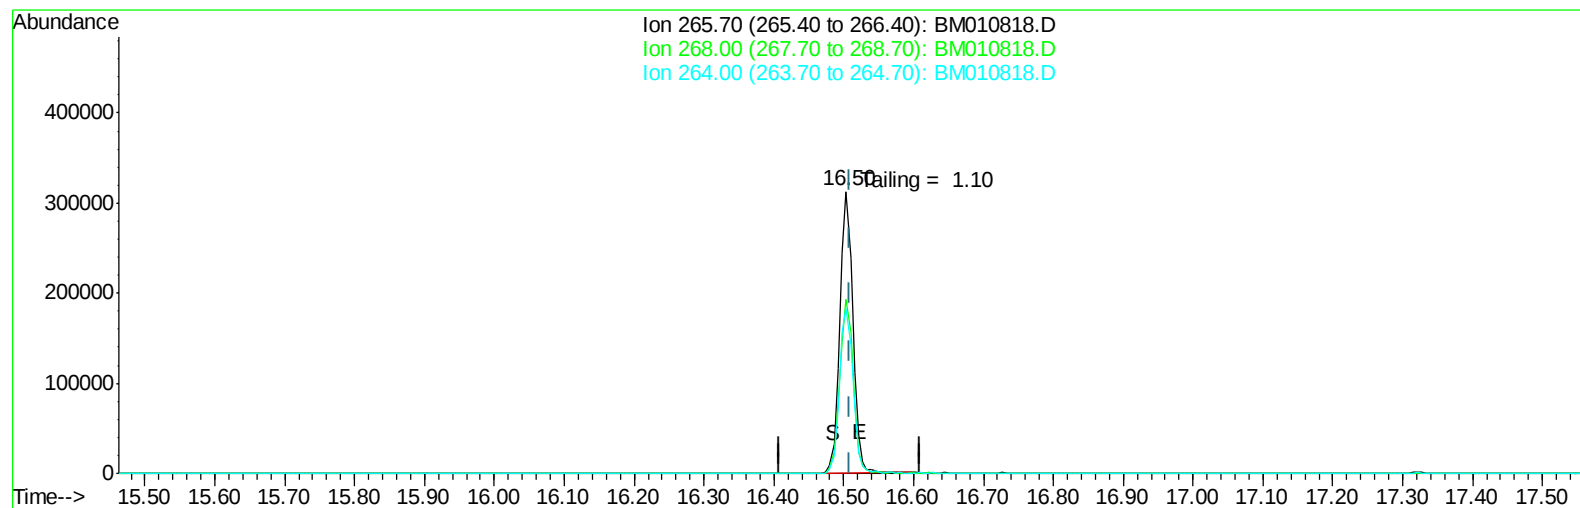

(69) Pentachlorophenol (C)

16.504min (-0.006) 229826.04ng

response 401395

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.83
264.00	61.20	58.45
0.00	0.00	0.00