


Data Path : Z:\HPCHEM1\BNA_M\Data\BM071317\
 Data File : BM010801.D
 Acq On : 13 Jul 2017 08:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

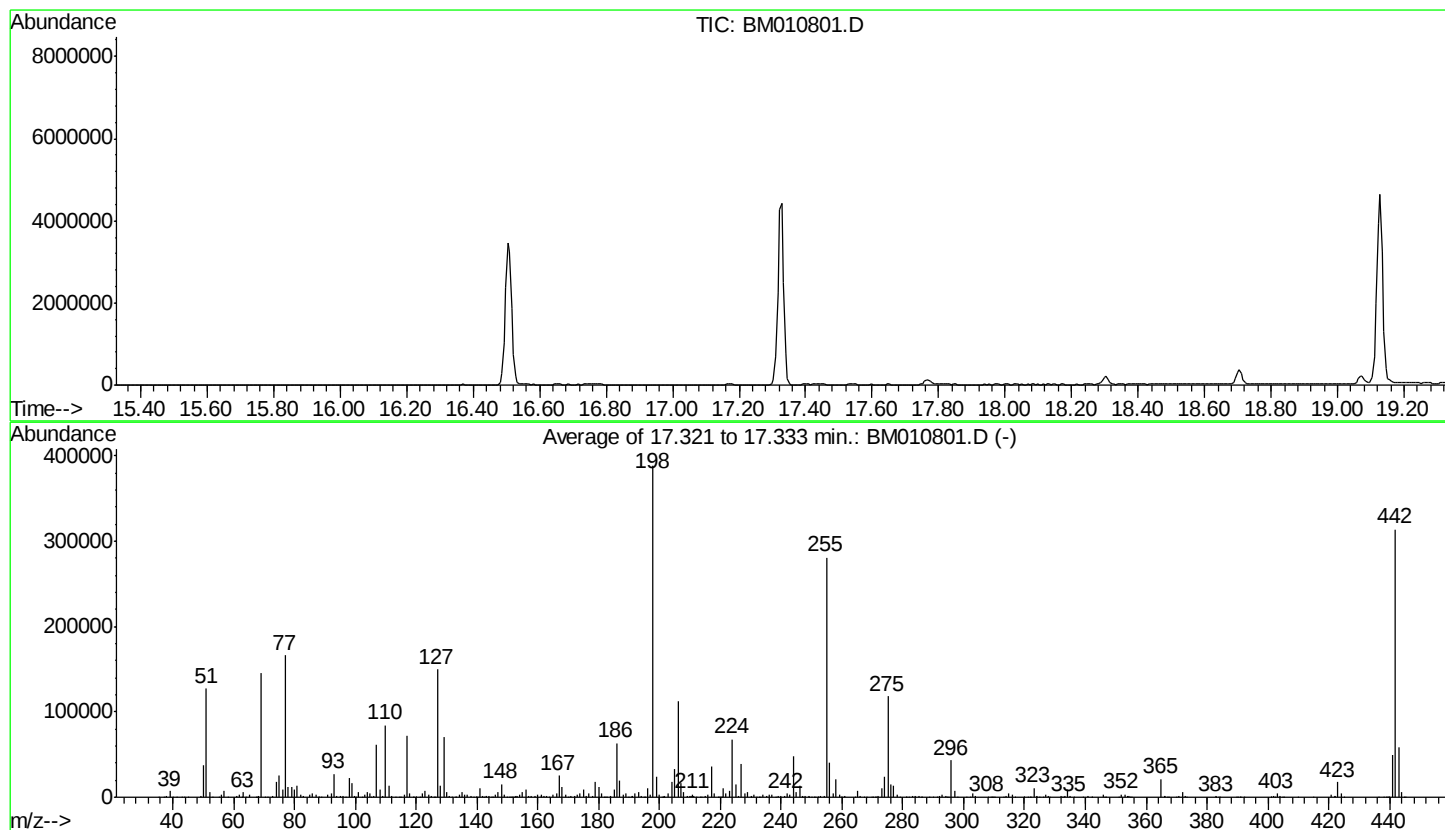

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	127120	PASS
68	69	0.00	2	1.3	1949	PASS
69	198	0.00	100	37.6	146301	PASS
70	69	0.00	2	0.5	722	PASS
127	198	10	80	38.5	149456	PASS
197	198	0.00	2	0.7	2749	PASS
198	198	100	100	100.0	388672	PASS
199	198	5	9	6.4	24757	PASS
275	198	10	60	30.4	118101	PASS
365	198	1	100	5.6	21746	PASS
441	442	0.01	24	15.9	49880	PASS
442	198	50	100	80.9	314304	PASS
443	442	15	24	18.4	57930	PASS