


Data Path : Z:\HPCHEM1\BNA_M\Data\BM071317\
 Data File : BM010818.D
 Acq On : 13 Jul 2017 18:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

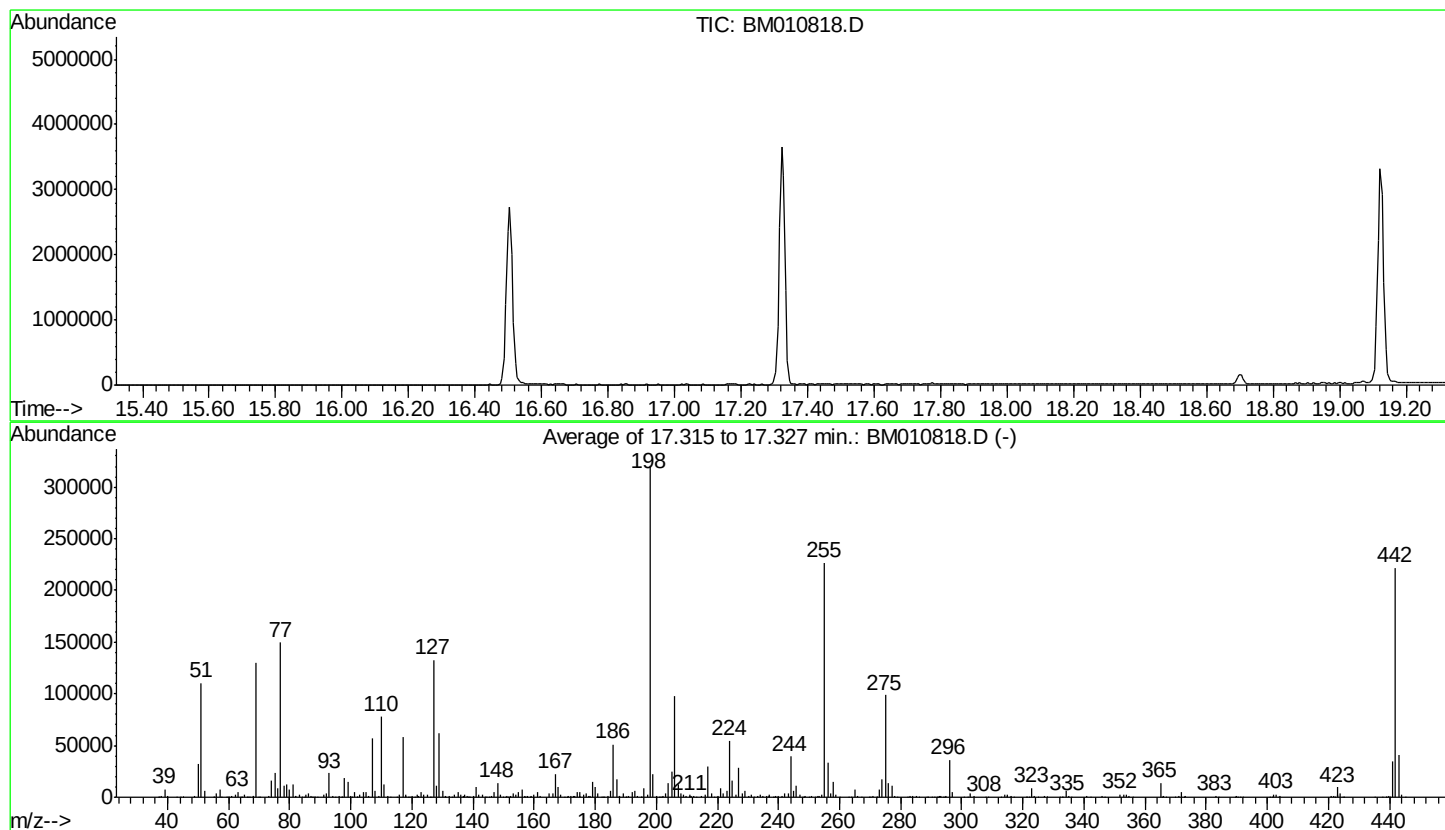

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	110565	PASS
68	69	0.00	2	1.4	1871	PASS
69	198	0.00	100	40.5	129856	PASS
70	69	0.00	2	0.5	659	PASS
127	198	10	80	41.4	132874	PASS
197	198	0.00	2	0.8	2420	PASS
198	198	100	100	100.0	320682	PASS
199	198	5	9	7.1	22890	PASS
275	198	10	60	30.8	98730	PASS
365	198	1	100	4.3	13882	PASS
441	442	0.01	24	15.8	35064	PASS
442	198	50	100	69.3	222229	PASS
443	442	15	24	18.3	40653	PASS