

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
 Data File : BM035796.D
 Acq On : 13 Jul 2022 14:48
 Operator : CG/JU
 Sample : PB146151BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146151BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.464	397	404	414	rBV	5270396	7193995	49.72%	10.468%
2	7.069	669	677	688	rBV	4936999	7499748	51.83%	10.913%
3	7.905	812	819	830	rVB	1191891	1831602	12.66%	2.665%
4	9.069	1009	1017	1026	rBV	3012687	4835373	33.42%	7.036%
5	10.710	1289	1296	1306	rVB	1568414	2584362	17.86%	3.761%
6	13.175	1707	1715	1722	rBV	8137398	11746292	81.18%	17.092%
7	14.539	1940	1947	1954	rBV	2226719	3105997	21.47%	4.520%
8	16.022	2192	2199	2221	rBV	5160814	7010654	48.45%	10.201%
9	17.275	2405	2412	2420	rBV	2437361	3266126	22.57%	4.753%
10	19.904	2853	2859	2873	rBV	12152825	14468813	100.00%	21.054%
11	21.451	3117	3122	3129	rBV	2240921	2749086	19.00%	4.000%
12	23.833	3520	3527	3538	rVB2	1280556	2430231	16.80%	3.536%




Sum of corrected areas: 68722279

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
Data File : BM035796.D
Acq On : 13 Jul 2022 14:48
Operator : CG/JU
Sample : PB146151BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146151BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

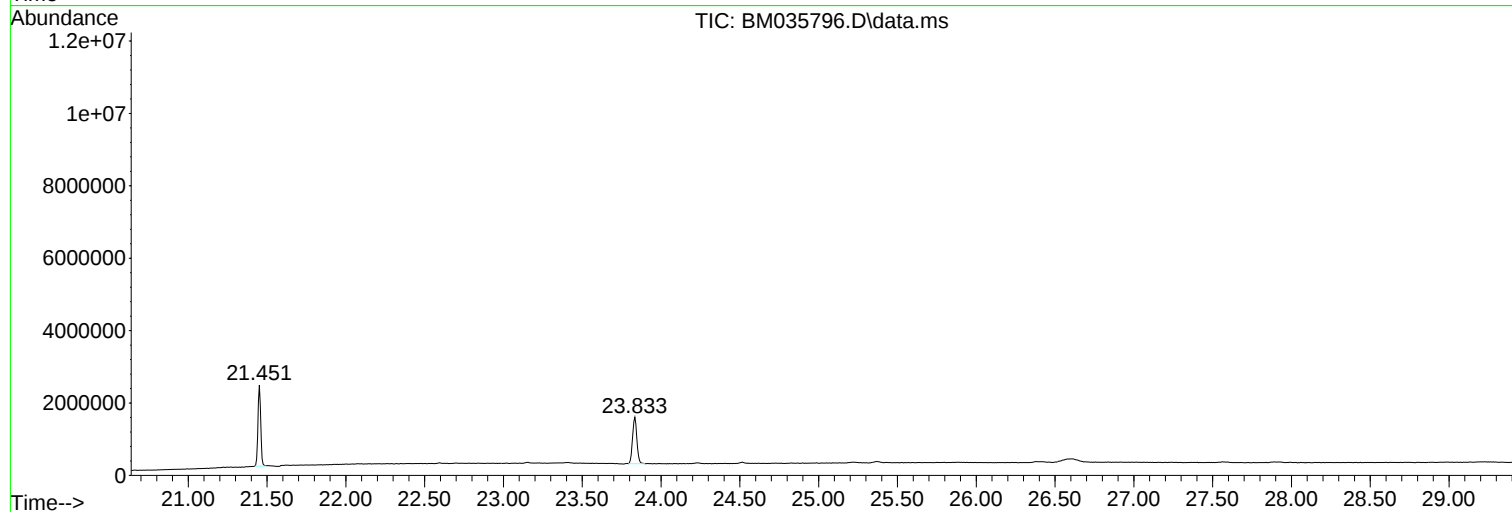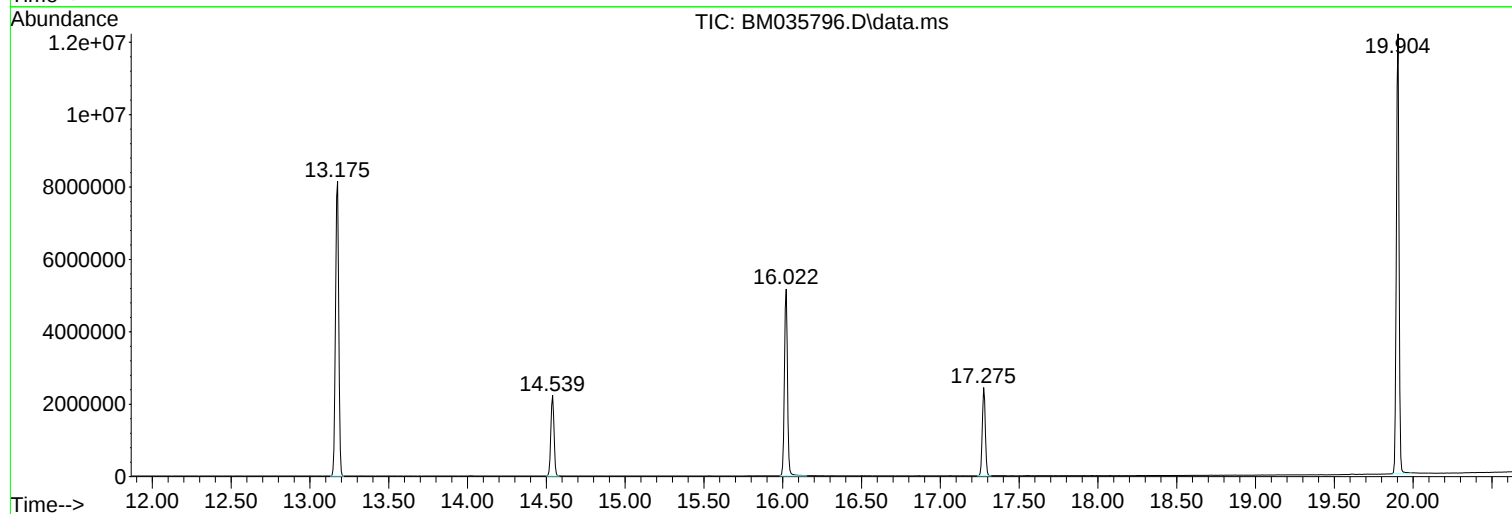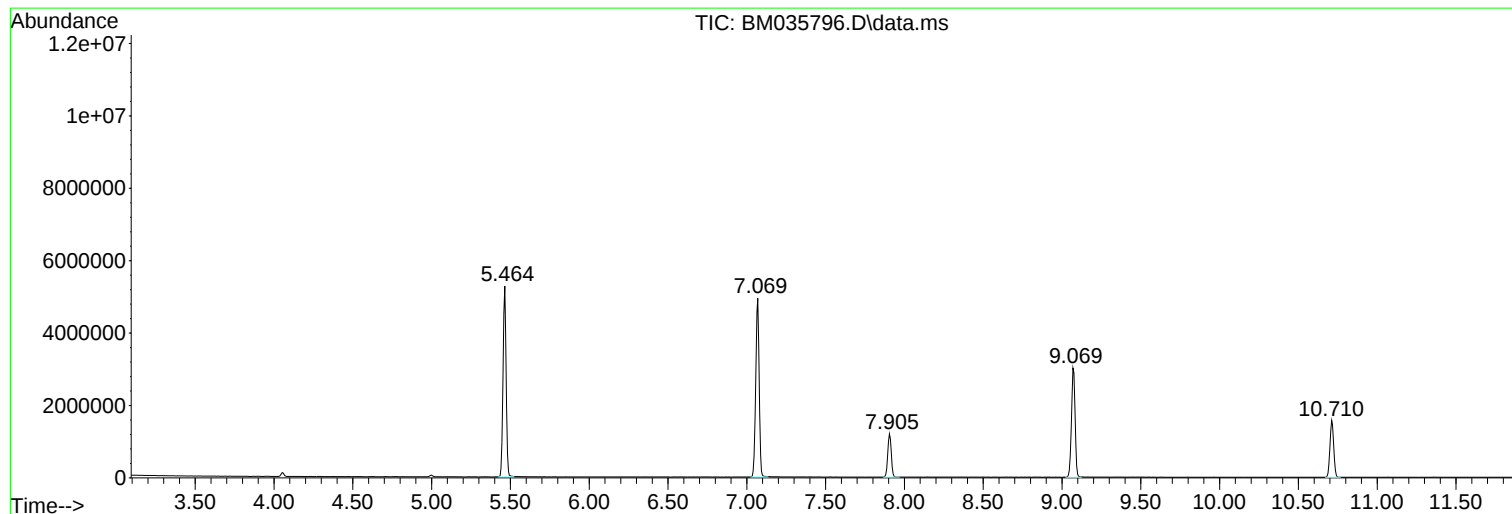

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
Data File : BM035796.D
Acq On : 13 Jul 2022 14:48
Operator : CG/JU
Sample : PB146151BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146151BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
Data File : BM035796.D
Acq On : 13 Jul 2022 14:48
Operator : CG/JU
Sample : PB146151BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146151BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------