
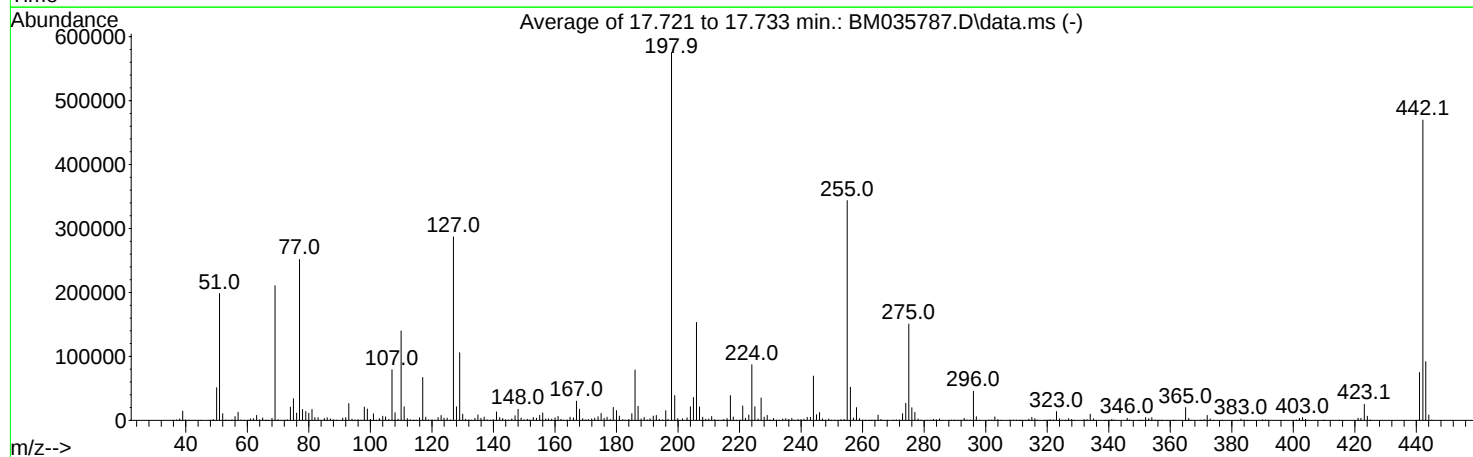


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
 Data File : BM035787.D
 Acq On : 13 Jul 2022 09:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 14 01:21:21 2022

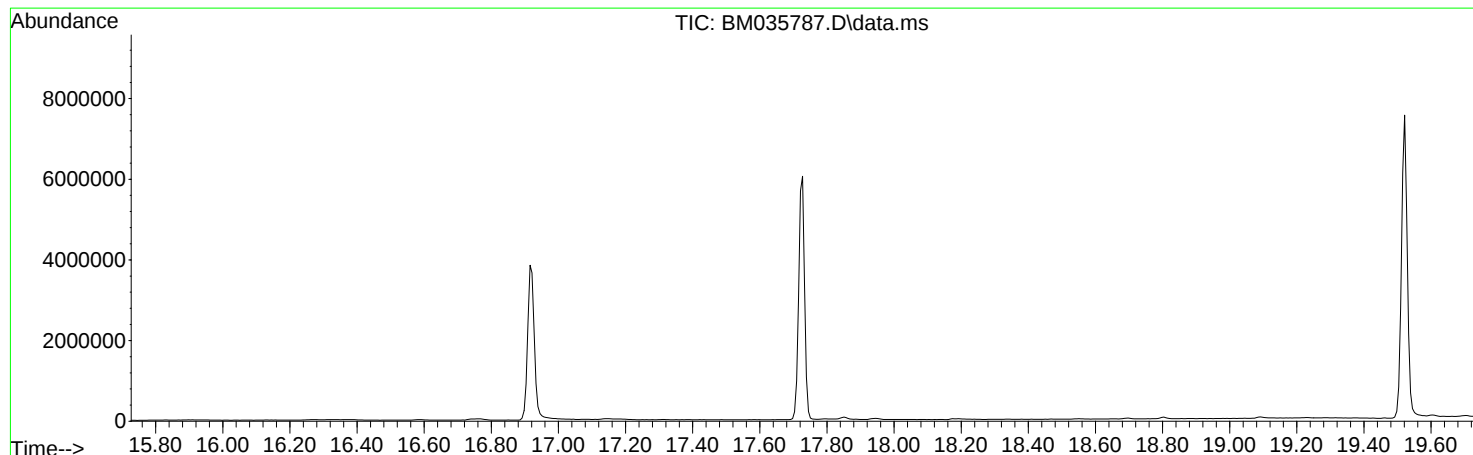

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	198492	PASS
68	69	0.00	2	1.5	3169	PASS
69	198	0.00	100	36.6	210614	PASS
70	69	0.00	2	0.5	956	PASS
127	198	10	80	49.9	287104	PASS
197	198	0.00	2	0.3	1524	PASS
198	198	100	100	100.0	575253	PASS
199	198	5	9	6.7	38755	PASS
275	198	10	60	26.2	150605	PASS
365	198	1	100	3.5	20126	PASS
441	198	0.01	100	13.0	74800	PASS
442	442	50	100	100.0	469675	PASS
443	442	15	24	19.5	91781	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/13/2022	BNA_M	<u>BM035787.D</u>
Compound Name	Response	Retention Time
DDT	1764457	20.75
DDD	2401	20.31
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2401	1766858	0.14

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
 Data File : BM035787.D
 Acq On : 13 Jul 2022 09:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 13 19:02:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 13 14:50:43 2022
 Response via : Initial Calibration

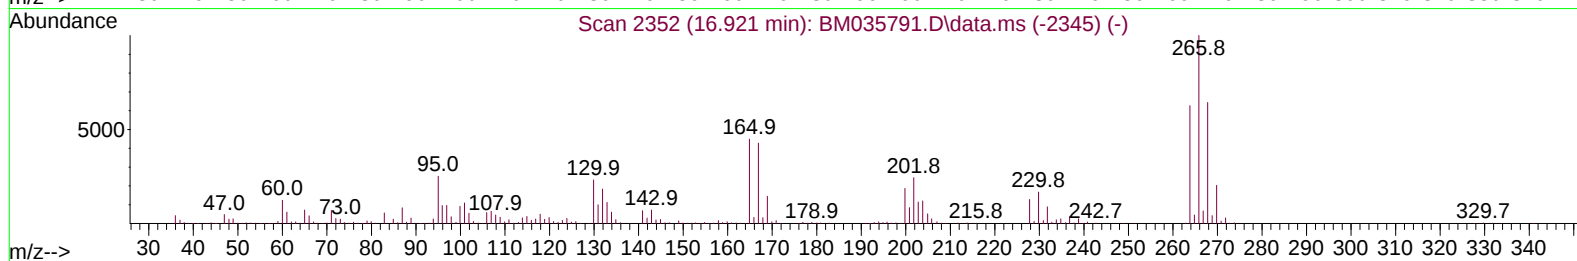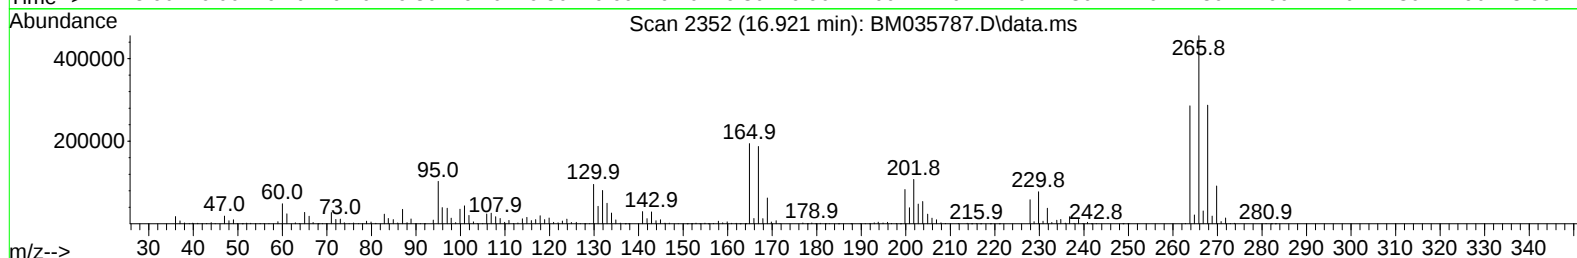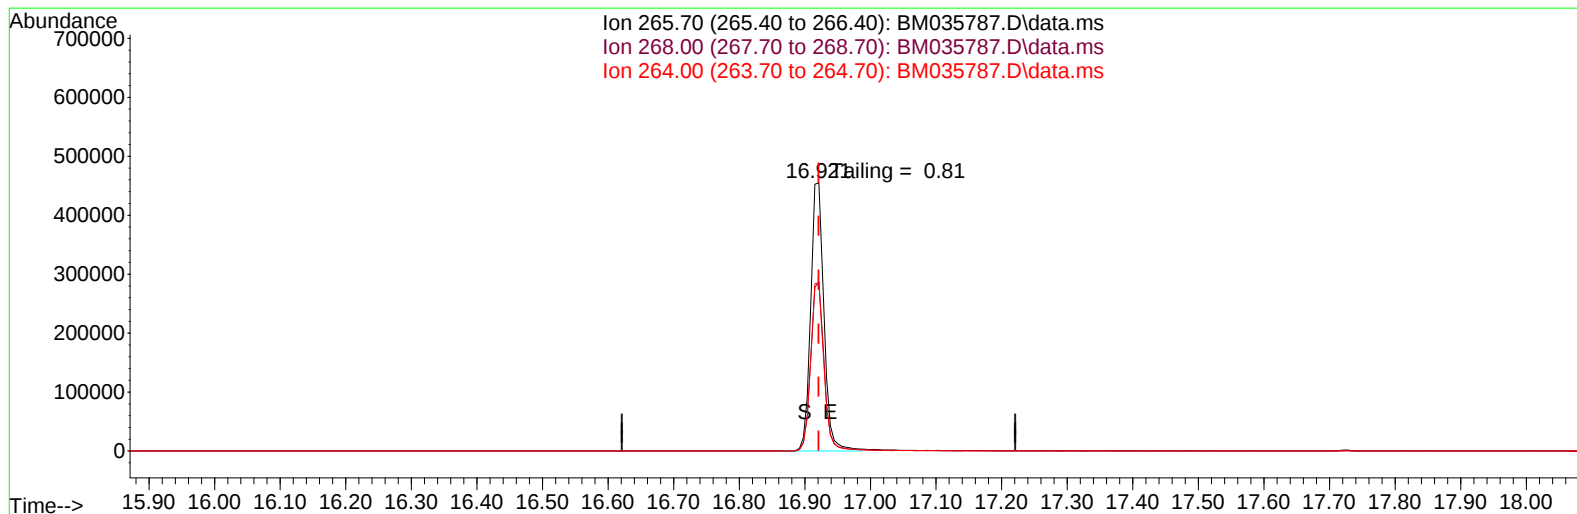

TIC: BM035787.D\data.ms

(70) Pentachlorophenol (C)

16.921min (+ 0.000) 0.00 ng




response 647103

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.10
264.00	63.30	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071322\
Data File : BM035787.D
Acq On : 13 Jul 2022 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 13 19:02:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 13 14:50:43 2022
Response via : Initial Calibration

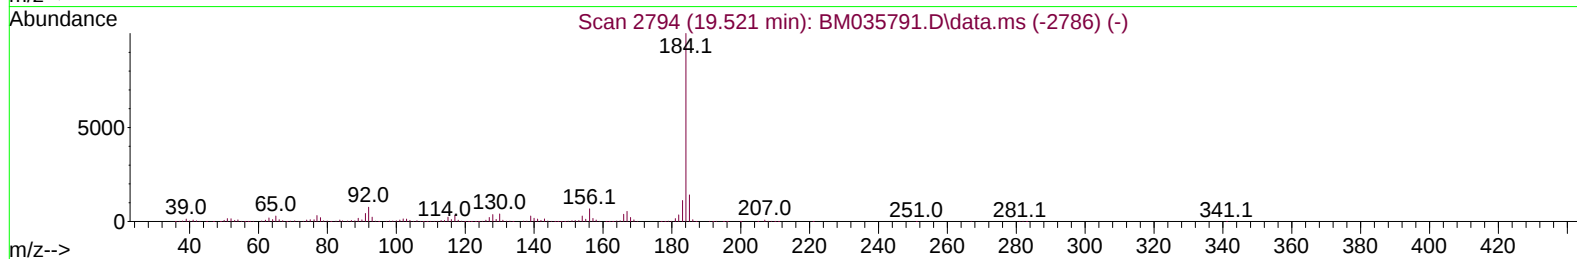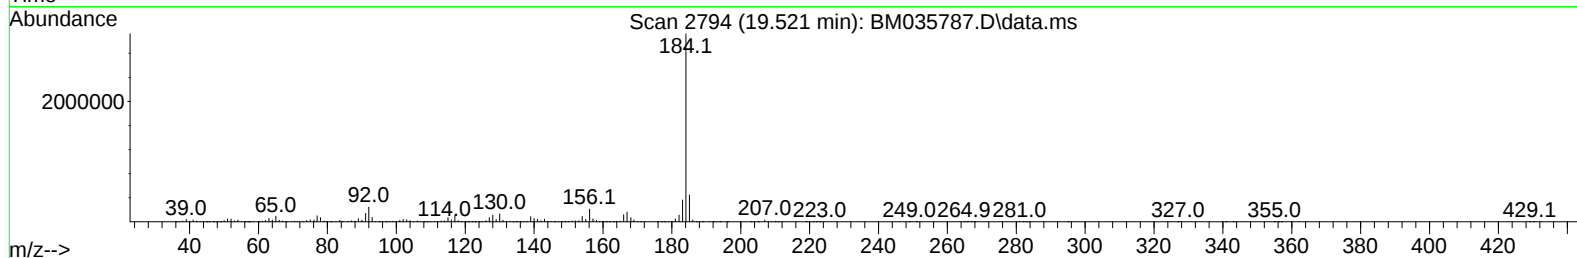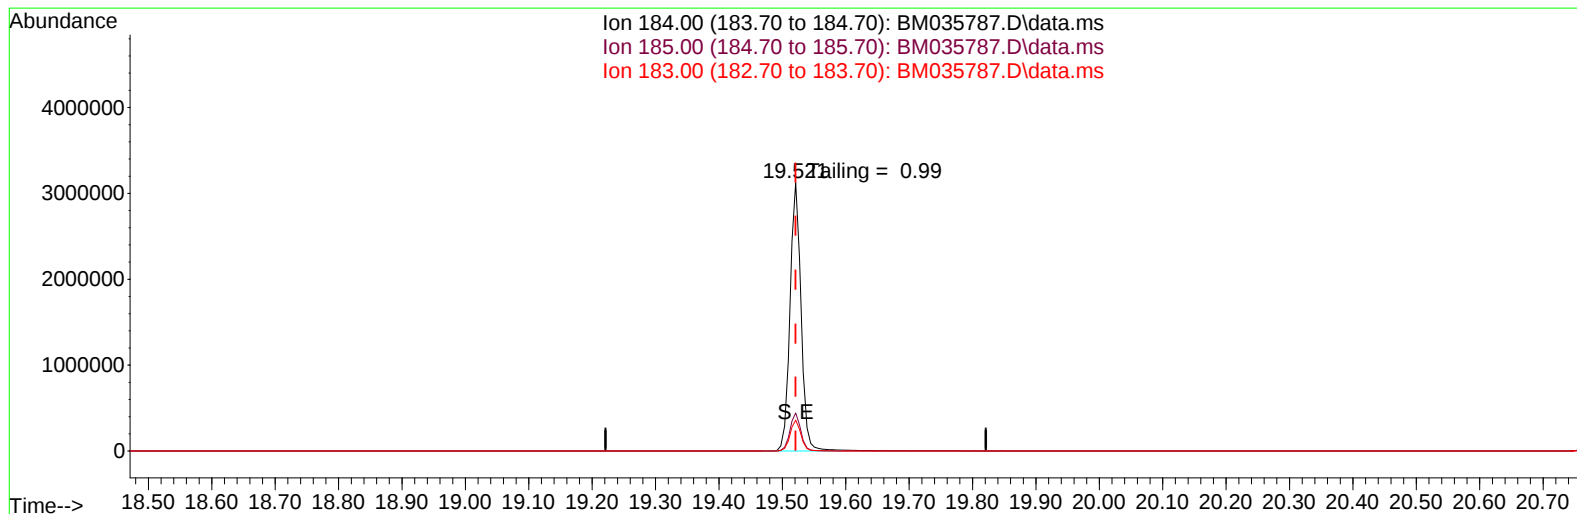

TIC: BM035787.D\data.ms

(77) Benzidine

19.521min (+ 0.000) 450009.57 ng

response 3811549

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.90	11.55
0.00	0.00	0.00