


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071415\
 Data File : BM001911.D
 Acq On : 14 Jul 2015 10:28
 Operator : TP/UM
 Sample : DFTPP74
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP74

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 08 10:41:47 2015

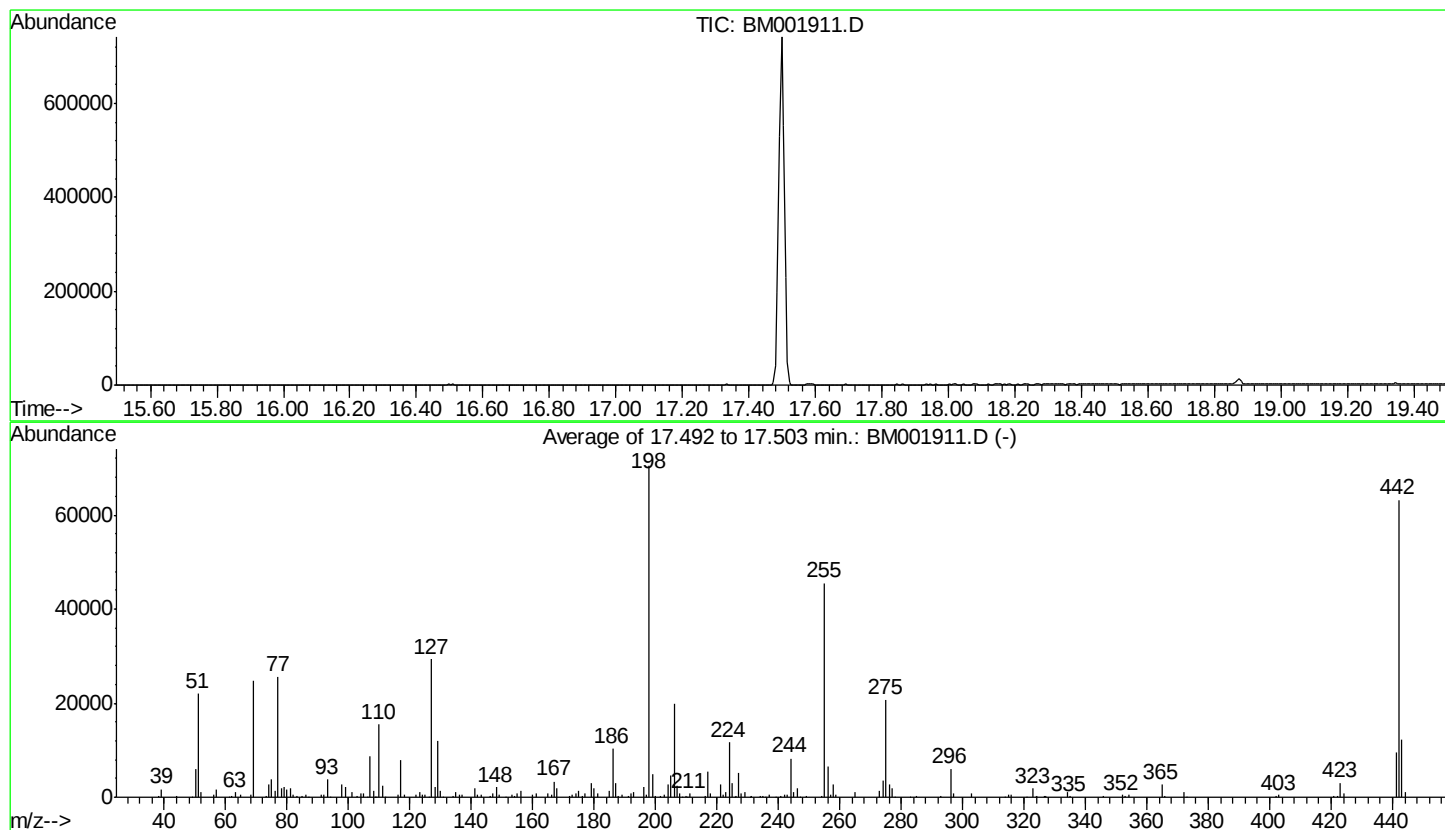

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	21981	PASS
68	69	0.00	2	1.9	466	PASS
69	198	0.00	100	35.1	24728	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.5	29274	PASS
197	198	0.00	2	0.9	611	PASS
198	198	100	100	100.0	70501	PASS
199	198	5	9	7.1	5014	PASS
275	198	10	60	29.3	20685	PASS
365	198	1	100	3.8	2675	PASS
441	443	0.01	100	76.8	9403	PASS
442	198	50	100	89.7	63237	PASS
443	442	15	24	19.4	12244	PASS

m/z	Abundance
38.00	436.0
39.00	1699.0
44.00	776.0
49.00	319.0
50.10	6219.0
51.10	22576.0
52.00	1079.0
56.00	627.0
57.00	1455.0
62.00	386.0
63.00	1061.0
65.00	496.0
68.20	500.0
69.00	25304.0
73.00	336.0
74.00	2671.0
75.00	3974.0
76.10	1083.0
77.10	24976.0
78.00	1726.0
79.10	2162.0
80.00	1605.0
81.00	2055.0
82.00	619.0
83.00	506.0
84.90	532.0
86.00	642.0
90.90	471.0
92.00	587.0
93.00	3649.0
93.90	394.0
98.00	2582.0
99.00	2141.0
101.00	988.0
102.90	434.0
104.00	957.0
105.00	704.0
106.00	314.0
107.00	8774.0
108.00	1326.0
110.00	14420.0
111.00	2272.0
116.00	466.0
117.00	7152.0
118.00	642.0
121.90	572.0
123.00	909.0
124.00	389.0
124.90	337.0
126.20	334.0
127.00	28512.0
128.00	2372.0
129.00	11325.0
130.00	1319.0
133.90	396.0
135.00	975.0
135.90	467.0
137.00	658.0
141.00	1807.0
142.00	596.0
143.00	396.0
147.00	906.0
148.00	1979.0
149.00	415.0
153.00	378.0
153.90	332.0
154.90	817.0
156.00	1334.0
160.00	568.0
161.00	819.0
165.00	762.0
165.90	527.0
167.00	3020.0
168.00	1957.0
172.00	361.0
172.90	393.0
174.10	715.0
175.00	1253.0
177.00	590.0
179.00	2872.0
180.00	1728.0
181.00	816.0
185.00	1231.0
186.00	9274.0
187.00	2716.0
188.00	374.0
189.00	519.0
191.00	387.0
191.90	756.0
193.00	944.0
196.00	1675.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

197.00	493.0
198.00	63216.0
198.90	4674.0
201.50	339.0
202.90	546.0
204.00	2499.0
205.00	4172.0
206.00	17128.0
207.00	2919.0
207.90	967.0
211.10	825.0
215.90	339.0
217.00	4915.0
218.00	611.0
221.00	2245.0
221.90	544.0
223.00	1078.0
224.00	10151.0
225.00	2544.0
225.90	355.0
227.00	4557.0
228.00	651.0
229.00	891.0
230.90	407.0
235.00	384.0
236.90	444.0
240.80	351.0
242.00	607.0
243.00	564.0
244.10	7058.0
245.00	753.0
246.00	1922.0
249.00	324.0
255.00	36776.0
256.00	5540.0
257.10	524.0
258.00	2160.0
258.90	338.0
265.00	988.0
273.00	1168.0
274.00	2681.0
275.00	16528.0
276.00	2356.0
277.00	1811.0
293.10	336.0
296.00	4317.0
296.90	688.0
303.00	647.0
315.00	450.0
316.00	322.0
323.00	1474.0
323.90	360.0
326.80	348.0
334.10	963.0
346.00	316.0
352.00	307.0
352.90	352.0
354.00	389.0
365.00	1910.0
372.00	939.0
403.00	374.0
423.00	1944.0
424.10	503.0
441.10	6173.0
442.10	39608.0
443.10	8345.0
444.10	893.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

m/z	Abundance
37.90	329.0
39.00	1996.0
44.00	756.0
50.10	6922.0
51.00	26744.0
52.10	1285.0
56.00	743.0
57.00	1783.0
61.10	390.0
61.90	337.0
63.00	1197.0
64.90	596.0
68.00	543.0
69.00	29600.0
74.00	3319.0
75.00	4969.0
76.10	1726.0
77.10	31488.0
78.10	2274.0
79.00	2789.0
80.00	1956.0
81.00	2487.0
82.00	702.0
83.00	584.0
84.90	401.0
86.00	816.0
86.90	369.0
90.90	523.0
91.90	612.0
93.00	4561.0
97.90	3602.0
99.00	2910.0
101.00	1325.0
102.90	467.0
104.00	874.0
105.00	896.0
107.00	10072.0
108.00	1567.0
109.10	380.0
110.00	19048.0
111.00	2858.0
111.90	363.0
116.00	660.0
117.00	9671.0
118.00	689.0
122.00	809.0
123.00	1170.0
123.90	628.0
124.90	570.0
127.00	35696.0
128.00	2784.0
129.00	14178.0
130.00	1598.0
130.90	395.0
134.00	558.0
135.00	1284.0
135.90	524.0
137.10	713.0
141.00	2352.0
141.90	515.0
142.90	542.0
146.00	480.0
147.00	1058.0
147.90	2643.0
149.00	497.0
151.10	333.0
153.00	688.0
153.90	455.0
155.00	1045.0
156.00	1710.0
160.00	622.0
161.00	1062.0
164.90	815.0
166.00	650.0
167.00	3903.0
168.00	2181.0
172.00	322.0
172.90	436.0
174.00	946.0
175.00	1772.0
175.90	512.0
176.90	785.0
178.90	3582.0
179.90	2177.0
181.00	1122.0
185.00	1790.0
186.00	12553.0
187.00	3435.0
188.00	375.0
189.00	701.0
191.00	506.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

191.90	1123.0
193.00	1333.0
196.10	2272.0
197.10	776.0
197.90	87000.0
198.90	5957.0
199.90	507.0
201.50	363.0
202.90	674.0
204.00	3209.0
205.00	6053.0
206.10	24616.0
207.00	3556.0
208.00	844.0
208.80	375.0
210.10	483.0
210.90	774.0
216.00	511.0
217.00	6564.0
217.90	925.0
221.00	3690.0
221.90	780.0
223.00	1367.0
224.00	13920.0
225.00	3585.0
226.10	556.0
227.00	6417.0
228.00	875.0
229.00	1244.0
231.10	616.0
233.90	447.0
234.90	541.0
235.90	300.0
237.00	706.0
239.00	313.0
240.90	322.0
242.00	716.0
243.00	861.0
244.00	10037.0
245.00	1275.0
246.00	2037.0
246.90	426.0
249.00	336.0
254.00	440.0
255.00	56352.0
256.00	8042.0
256.90	723.0
258.00	3558.0
258.90	551.0
265.00	1315.0
272.90	1591.0
274.00	4630.0
275.00	25120.0
276.00	3382.0
277.00	2286.0
278.00	396.0
283.00	327.0
285.00	466.0
293.00	543.0
296.00	7483.0
297.00	1108.0
302.90	767.0
315.00	955.0
316.00	511.0
323.00	2055.0
324.10	395.0
327.00	598.0
334.00	1205.0
334.90	359.0
346.10	401.0
352.10	665.0
353.00	374.0
354.10	619.0
365.00	3514.0
365.90	404.0
372.10	1074.0
373.00	341.0
401.90	371.0
403.00	681.0
421.10	509.0
422.00	557.0
423.00	3888.0
424.00	836.0
441.10	11140.0
442.10	74448.0
443.10	14660.0
444.00	1360.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

m/z	Abundance
39.00	1321.0
44.00	632.0
50.10	4616.0
51.10	16624.0
52.00	795.0
55.90	640.0
57.00	1303.0
63.00	734.0
65.10	384.0
68.10	356.0
69.00	19280.0
73.10	305.0
74.00	2222.0
75.00	2810.0
76.10	967.0
77.10	20448.0
78.00	1579.0
79.00	1707.0
80.00	1125.0
81.00	1492.0
82.00	511.0
85.00	311.0
86.00	598.0
90.90	393.0
91.90	430.0
93.00	3122.0
98.00	2382.0
99.00	1707.0
101.00	913.0
104.00	648.0
105.00	556.0
107.00	7077.0
108.00	1188.0
108.80	352.0
110.00	12743.0
111.00	2064.0
116.00	412.0
117.00	6962.0
118.00	459.0
122.10	440.0
123.00	883.0
124.00	331.0
125.00	389.0
127.00	23616.0
128.00	1550.0
129.00	10064.0
130.00	807.0
135.00	870.0
136.00	347.0
137.10	486.0
141.00	1345.0
141.90	550.0
143.10	330.0
147.10	701.0
148.10	1571.0
149.00	351.0
153.00	507.0
153.90	409.0
155.00	871.0
156.00	1157.0
159.90	475.0
160.90	775.0
165.00	721.0
166.10	405.0
167.00	3113.0
168.00	1506.0
171.90	303.0
172.80	437.0
174.00	669.0
175.00	1378.0
176.00	459.0
177.00	703.0
179.00	2283.0
180.00	1772.0
181.00	836.0
185.00	1160.0
186.00	9045.0
187.10	2465.0
188.00	435.0
188.90	661.0
192.00	744.0
193.00	991.0
195.90	2307.0
197.10	564.0
197.90	61288.0
198.90	4412.0
200.00	324.0
202.90	514.0
204.00	2535.0
205.00	4033.0
206.00	17560.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

207.00	2569.0
207.90	718.0
210.30	354.0
211.00	599.0
217.00	4704.0
218.00	643.0
221.10	2494.0
221.90	586.0
223.00	930.0
224.00	10780.0
225.10	2714.0
226.00	436.0
227.00	4952.0
228.00	582.0
229.00	802.0
231.00	308.0
236.80	345.0
240.90	324.0
242.00	555.0
243.00	531.0
244.00	7432.0
245.10	1059.0
246.00	1818.0
249.00	327.0
254.10	425.0
255.00	43608.0
256.00	6386.0
256.90	575.0
258.00	2707.0
258.80	402.0
264.90	1292.0
272.90	1369.0
274.00	3535.0
275.00	20408.0
276.10	2595.0
277.00	1667.0
285.10	371.0
296.00	6520.0
297.00	802.0
303.00	726.0
313.90	303.0
315.00	519.0
316.00	472.0
321.00	324.0
323.10	2005.0
324.00	455.0
326.80	370.0
334.00	1389.0
334.90	374.0
345.90	434.0
352.10	632.0
353.00	421.0
354.00	556.0
365.00	2601.0
366.00	398.0
372.00	1135.0
402.00	446.0
403.00	502.0
421.00	467.0
422.00	416.0
423.00	3526.0
424.00	921.0
441.10	10896.0
442.10	75656.0
443.10	13727.0
444.00	1130.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

m/z	Abundance
44.00	559.0
206.90	546.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74

m/z	Abundance
44.00	559.0
206.90	546.0

Instrument :
BNA_M
ClientSampleId :
DFTPP74