

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
 Data File : BM006425.D
 Acq On : 15 Jul 2016 03:51
 Operator : UM/SJ
 Sample : H3990-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ68

Quant Time: Jul 15 04:37:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 04:34:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	129333	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	553905	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	329113	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	798500	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1000397	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1062792	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	8495	2.77	ng/uL	0.00
5) Phenol-d5	6.80	99	397848	37.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	242631	37.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	309194	36.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	320019	38.00	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	155196	36.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	178779	37.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	310090	34.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	412808	44.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	989255	36.73	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1207560	36.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	187809	40.14	ng/ul	0.00
57) Fluorene-d10	15.27	176	850291	35.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	156868	33.96	ng/ul	0.00
70) Anthracene-d10	17.12	188	1356861	35.95	ng/ul	0.00
76) Pyrene-d10	19.42	212	1595142	35.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1854772	38.16	ng/ul	0.00

Target Compounds

						Qvalue
4) Benzaldehyde	6.79	77	653	0.10	ng/ul#	4
6) Phenol	6.83	94	11250	1.01	ng/ul#	88
8) Bis(2-Chloroethyl)ether	7.05	93	1380	0.17	ng/ul#	73
12) 2,2'-oxybis(1-Chloropropan	8.33	45	2333	0.17	ng/ul#	76
15) N-Nitroso-di-n-propylamine	8.33	70	9259	1.32	ng/ul#	1
20) Nitrobenzene	8.77	77	1510	0.14	ng/ul#	42
21) Isophorone	9.49	82	18332	0.92	ng/ul#	73
32) Caprolactam	11.38	113	748	0.26	ng/ul#	71
44) Dimethylphthalate	13.73	163	300781	11.01	ng/ul	99
45) 2,6-Dinitrotoluene	13.73	165	3334	0.61	ng/ul#	55
56) Diethylphthalate	15.10	149	1218	0.04	ng/ul#	59
58) Fluorene	15.27	166	1884	0.07	ng/ul#	7
60) 4-Nitroaniline	15.39	138	311	0.05	ng/ul#	1
63) 4,6-Dinitro-2-methylphenol	15.40	198	690	0.14	ng/ul#	1
64) N-Nitrosodiphenylamine	15.40	169	1530	0.07	ng/ul#	29
69) Phenanthrene	17.06	178	619	0.01	ng/ul#	61
71) Anthracene	17.06	178	619	0.01	ng/ul#	61
73) Di-n-butylphthalate	17.99	149	4587	0.09	ng/ul#	90
74) Fluoranthene	19.09	202	614	0.01	ng/ul#	74
77) Pyrene	19.42	202	2222	0.04	ng/ul#	1
78) Butylbenzylphthalate	20.36	149	289	0.01	ng/ul#	86
80) Benzo(a)anthracene	21.21	228	3699	0.06	ng/ul#	55
81) Bis(2-ethylhexyl)phthalate	21.14	149	4267	0.12	ng/ul#	97

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006425.D
Acq On : 15 Jul 2016 03:51
Operator : UM/SJ
Sample : H3990-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ68

Quant Time: Jul 15 04:37:31 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 04:34:07 2016
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
82) Chrysene	21.26	228	2031	0.04	ng/ul	95
84) Di-n-octyl phthalate	22.00	149	404	0.01	ng/ul#	1
85) Benzo(b)fluoranthene	22.76	252	1266	0.02	ng/ul#	1
86) Benzo(k)fluoranthene	22.79	252	56	0.00	ng/ul#	1
88) Benzo(a)pyrene	23.33	252	235	0.00	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006425.D
Acq On : 15 Jul 2016 03:51
Operator : UM/SJ
Sample : H3990-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ68

Quant Time: Jul 15 04:37:31 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 04:34:07 2016
Response via : Initial Calibration

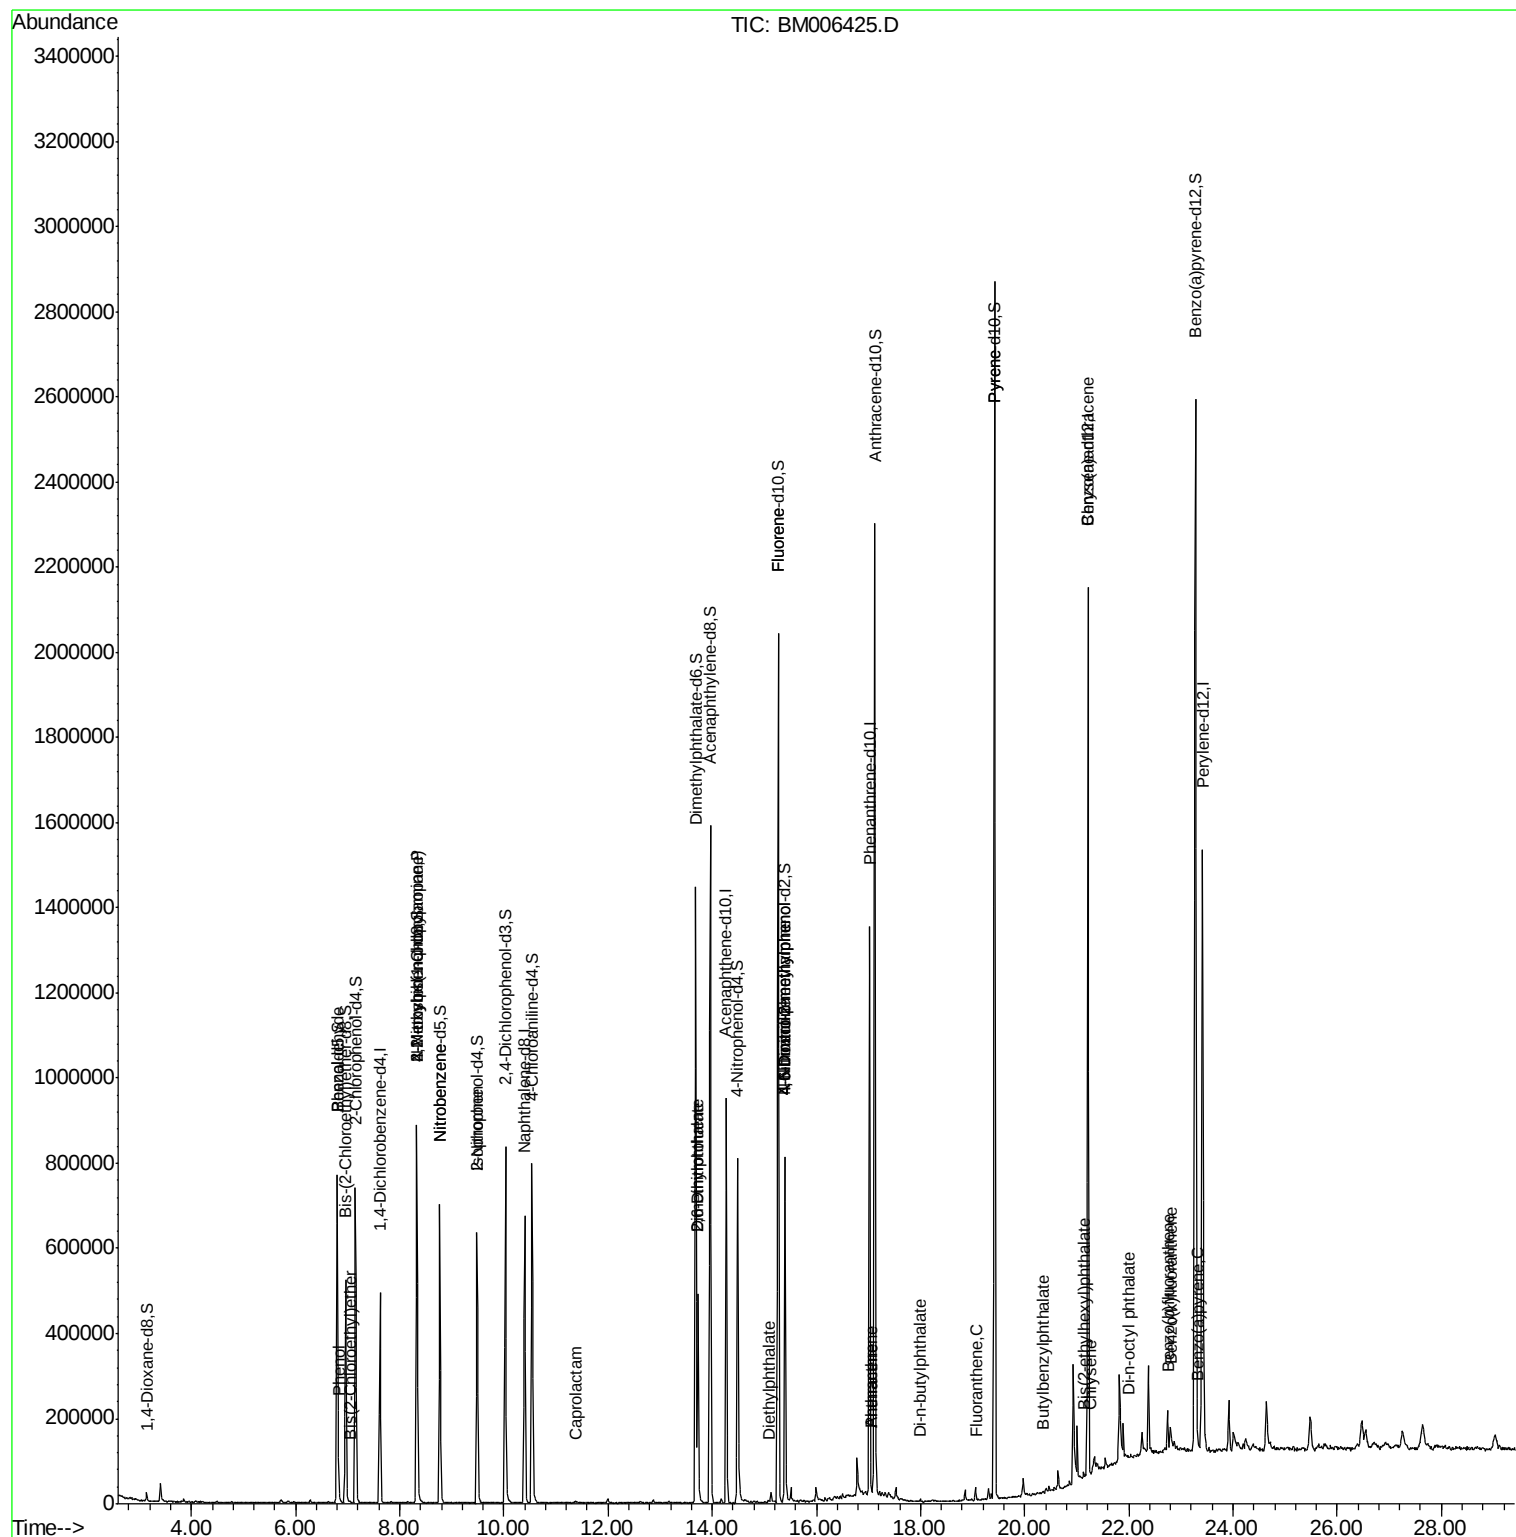

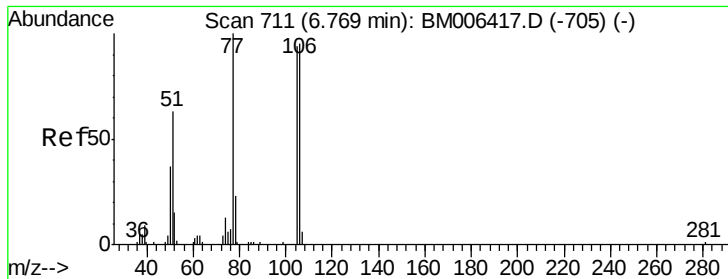

#4

Benzaldehyde

Concen: 0.10 ng/ul

RT: 6.79 min Scan# 715

Delta R.T. 0.02 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68


Tgt Ion: 77 Resp: 653

Ion Ratio Lower Upper

77 100

105 0.0 74.9 112.3#

106 0.0 70.7 106.1#

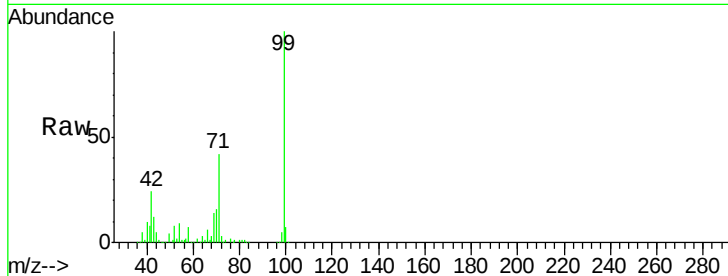

Abundance Ion 77.00 (76.70 to 77.70): BM006417.D (-705) (-)



Ion 105.00 (104.70 to 105.70): BM006417.D (-705) (-)

Ion 106.00 (105.70 to 106.70): BM006417.D (-705) (-)

Time-->

6.79

6.77 6.78 6.79 6.80

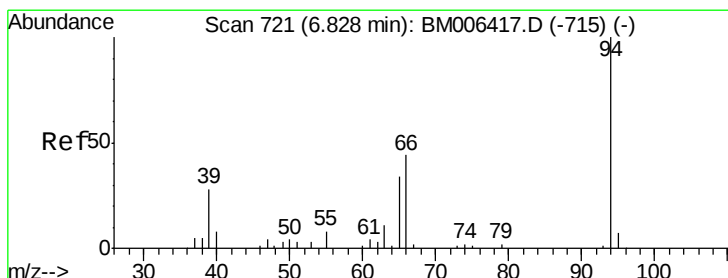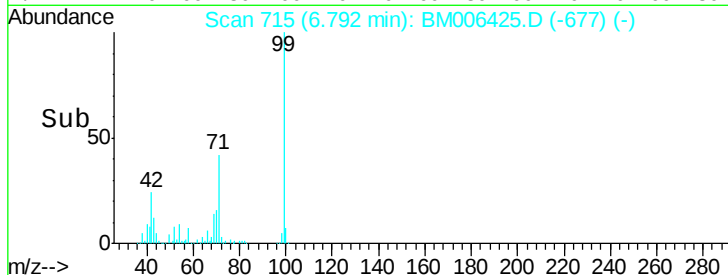

#6

Phenol

Concen: 1.01 ng/ul

RT: 6.83 min Scan# 721

Delta R.T. -0.00 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion: 94 Resp: 11250

Ion Ratio Lower Upper

94 100

65 36.3 25.8 38.8

66 54.3 35.7 53.5#

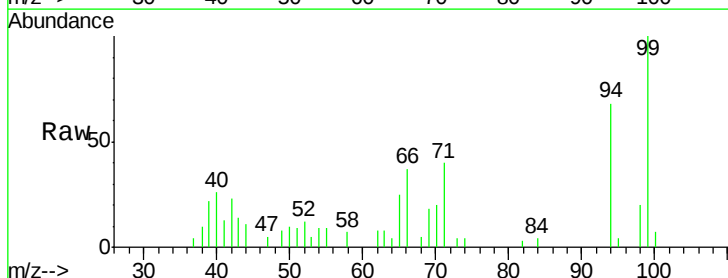

Abundance Ion 94.00 (93.70 to 94.70): BM006417.D (-715) (-)


Ion 65.00 (64.70 to 65.70): BM006417.D (-715) (-)


Ion 66.00 (65.70 to 66.70): BM006417.D (-715) (-)

Time-->

6.83

6.80 6.81 6.82 6.83 6.84 6.85

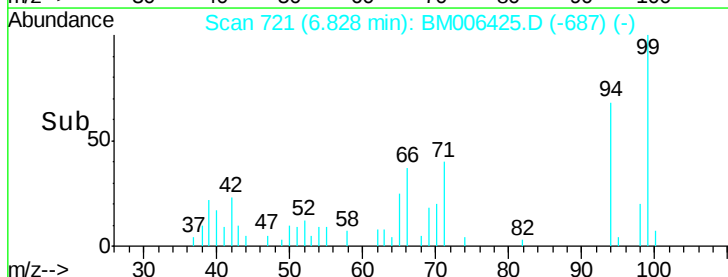



#8

Bis(2-Chloroethyl)ether

Concen: 0.17 ng/ul

RT: 7.05 min Scan# 759

Delta R.T. -0.00 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68


Tgt Ion: 93 Resp: 1380

Ion Ratio Lower Upper

93 100

63 67.5 64.2 96.4




95 0.0 26.0 39.0#



Abundance Ion 93.00 (92.70 to 93.70): BM006417.D (-753) (-)

Ion 63.00 (62.70 to 63.70): BM006417.D (-753) (-)

Ion 95.00 (94.70 to 95.70): BM006417.D (-753) (-)

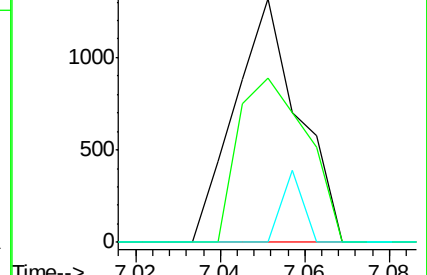

#12

2,2'-oxybis(1-Chloropropane)

Concen: 0.17 ng/ul

RT: 8.33 min Scan# 976

Delta R.T. 0.17 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion: 45 Resp: 2333

Ion Ratio Lower Upper

45 100

77 22.1 11.0 16.4#



79 20.8 8.2 12.4#






Abundance Ion 45.00 (44.70 to 45.70): BM006417.D (-938) (-)

Ion 77.00 (76.70 to 77.70): BM006417.D (-938) (-)

Ion 79.00 (78.70 to 79.70): BM006417.D (-938) (-)

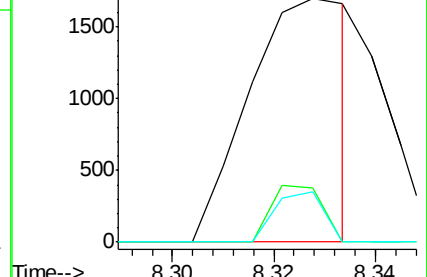

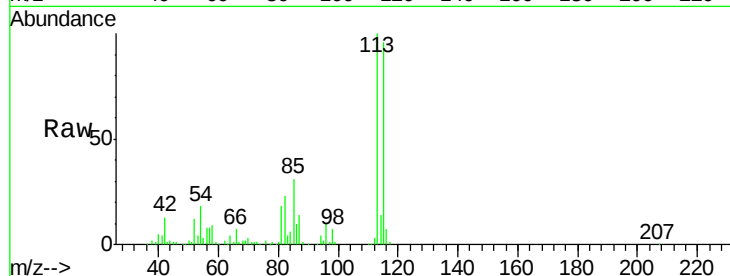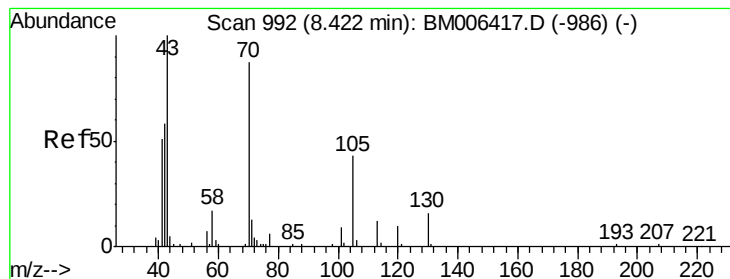

#15

N-Nitroso-di-n-propylamine

Concen: 1.32 ng/ul

RT: 8.33 min Scan# 976

Delta R.T. -0.09 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68

Tgt Ion: 70 Resp: 9259





Ion Ratio Lower Upper

70 100

42 452.1 50.6 75.8#

101 0.0 7.9 11.9#

130 0.0 15.8 23.6#

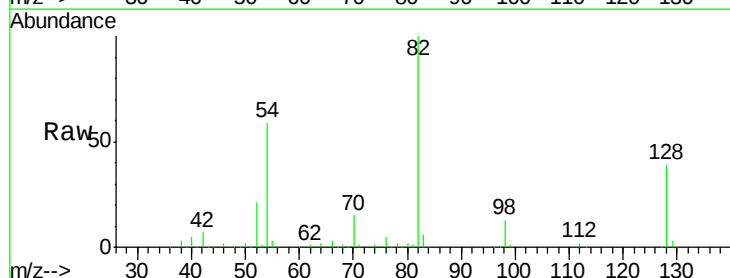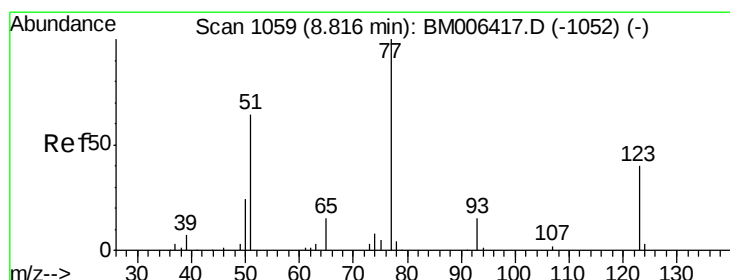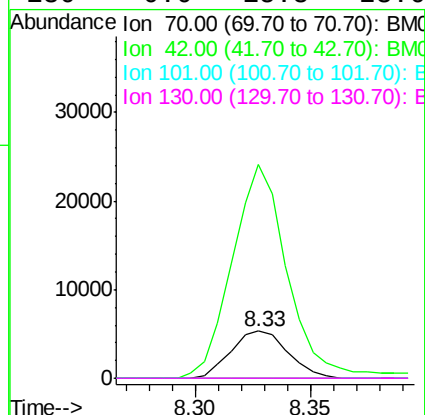

#20

Nitrobenzene

Concen: 0.14 ng/ul

RT: 8.77 min Scan# 1052

Delta R.T. -0.04 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion: 77 Resp: 1510


Ion Ratio Lower Upper

77 100

123 0.0 33.0 49.4#

65 0.0 11.5 17.3#

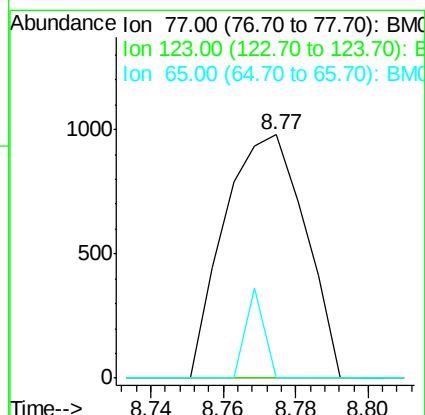



#21

Isophorone

Concen: 0.92 ng/ul

RT: 9.49 min Scan# 1173

Delta R.T. 0.15 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampled :

BDJ68


Tgt Ion: 82 Resp: 18332

Ion Ratio Lower Upper

82 100

95 6.4 6.0 9.0

138 0.0 13.0 19.4#


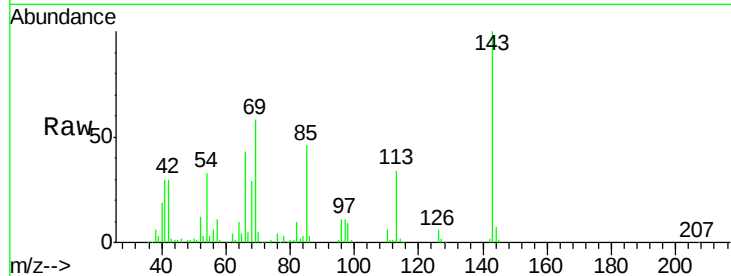


Abundance Ion 82.00 (81.70 to 82.70): BM006417.D (-1140) (-)

Ion 95.00 (94.70 to 95.70): BM006417.D (-1140) (-)

Ion 138.00 (137.70 to 138.70): BM006417.D (-1140) (-)

Time-->

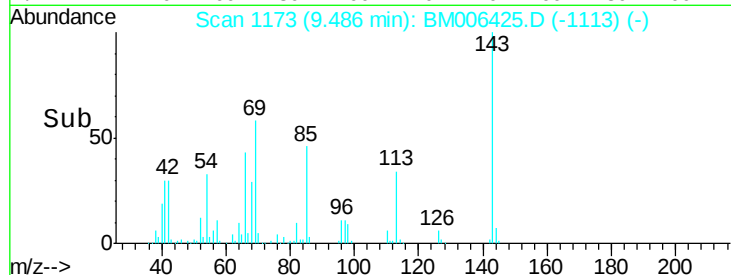

#32

Caprolactam

Concen: 0.26 ng/ul

RT: 11.38 min Scan# 1495

Delta R.T. 0.06 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion: 113 Resp: 748

Ion Ratio Lower Upper

113 100

55 159.3 155.8 233.8

56 106.3 120.5 180.7#





Abundance Ion 113.00 (112.70 to 113.70): BM006417.D (-1478) (-)

Ion 55.00 (54.70 to 55.70): BM006417.D (-1478) (-)

Ion 56.00 (55.70 to 56.70): BM006417.D (-1478) (-)

Time-->



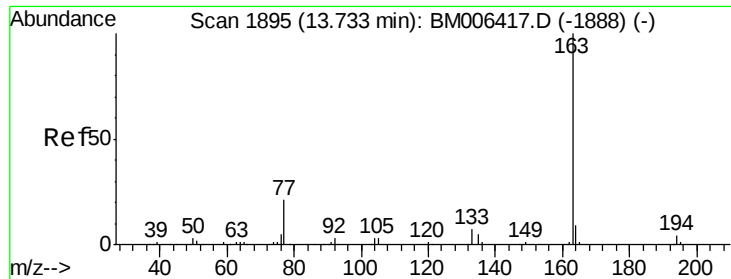

#44

Dimethylphthalate

Concen: 11.01 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampled :

BDJ68


Tgt Ion:163 Resp: 300781

Ion Ratio Lower Upper

163 100

194 3.6 3.4 5.0

164 10.1 7.8 11.8

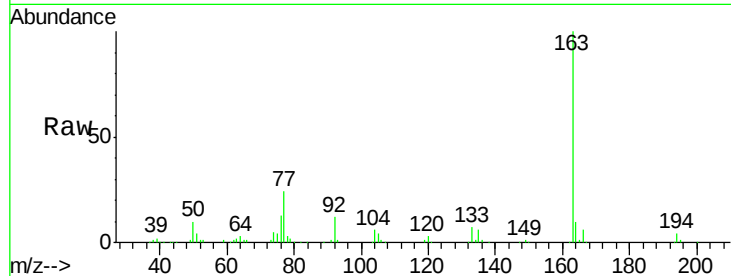


Abundance Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

Time-->

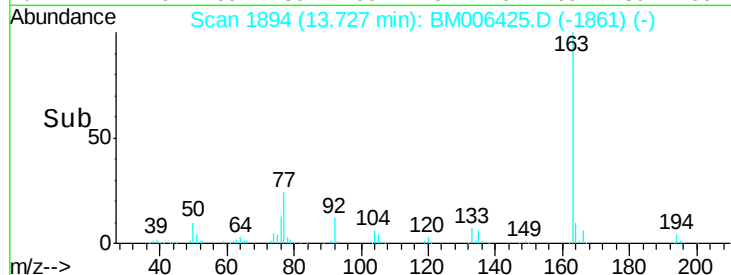

Time-->



#45

2,6-Dinitrotoluene

Concen: 0.61 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.13 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion:165 Resp: 3334

Ion Ratio Lower Upper

165 100

89 18.8 52.1 78.1#

121 18.9 17.3 25.9




Abundance Ion 165.00 (164.70 to 165.70): E


Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

Time-->







Time-->

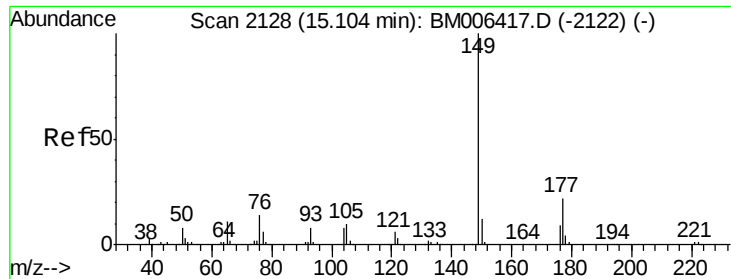

#56
Diethylphthalate
Concen: 0.04 ng/ul
RT: 15.10 min Scan# 2128
Delta R.T. -0.00 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51




Instrument :
BNA_M
ClientSampled :
BDJ68


Tgt Ion:149 Resp: 1218
Ion Ratio Lower Upper
149 100
177 0.0 17.7 26.5#
150 0.0 9.8 14.8#

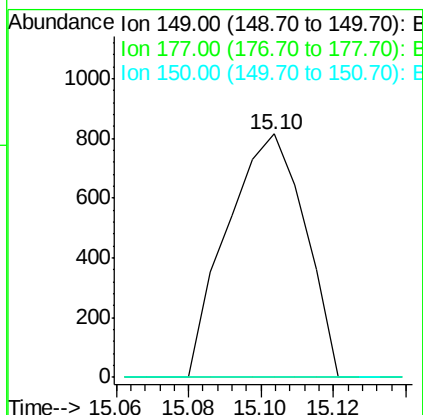

#58
Fluorene
Concen: 0.07 ng/ul
RT: 15.27 min Scan# 2156
Delta R.T. -0.06 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51

Tgt Ion:166 Resp: 1884
Ion Ratio Lower Upper
166 100
165 0.0 77.5 116.3#
167 33.5 10.8 16.2#



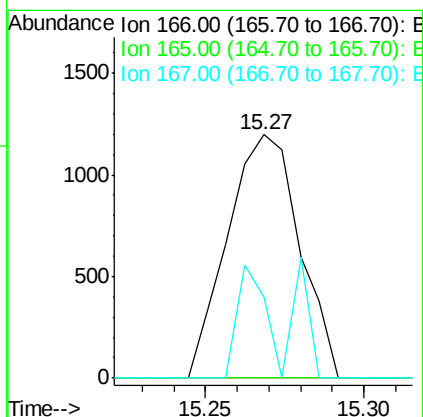



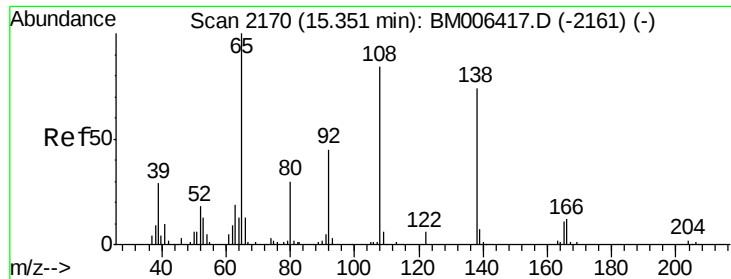

#60
 4-Nitroaniline
 Concen: 0.05 ng/ul
 RT: 15.39 min Scan# 2177
 Delta R.T. 0.04 min
 Lab File: BM006425.D
 Acq: 15 Jul 2016 03:51




Instrument :
 BNA_M
 ClientSampleId :
 BDJ68


Tgt Ion:138 Resp: 311
 Ion Ratio Lower Upper
 138 100
 92 286.5 43.4 65.0#
 108 4004.8 79.9 119.9#

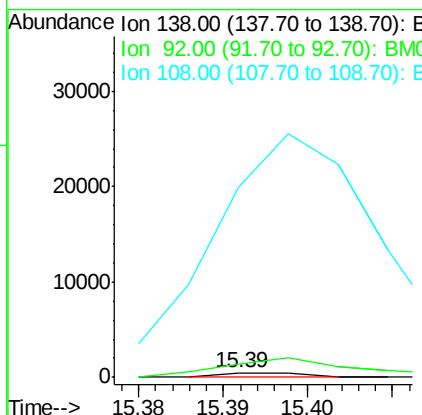

#63
 4,6-Dinitro-2-methylphenol
 Concen: 0.14 ng/ul
 RT: 15.40 min Scan# 2178
 Delta R.T. -0.02 min
 Lab File: BM006425.D
 Acq: 15 Jul 2016 03:51

Tgt Ion:198 Resp: 690
 Ion Ratio Lower Upper
 198 100
 182 366.0 3.0 4.6#
 77 1382.7 24.2 36.2#

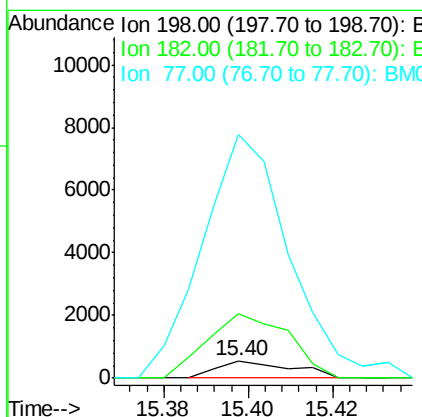

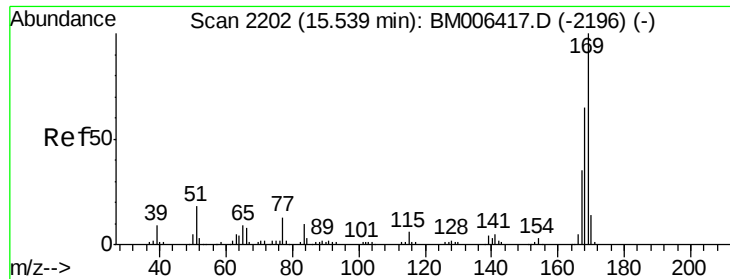

#64

N-Nitrosodiphenylamine

Concen: 0.07 ng/ul

RT: 15.40 min Scan# 2179

Delta R.T. -0.14 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68


Tgt Ion:169 Resp: 1530

Ion Ratio Lower Upper

169 100

168 0.0 52.9 79.3#




167 64.7 28.7 43.1#

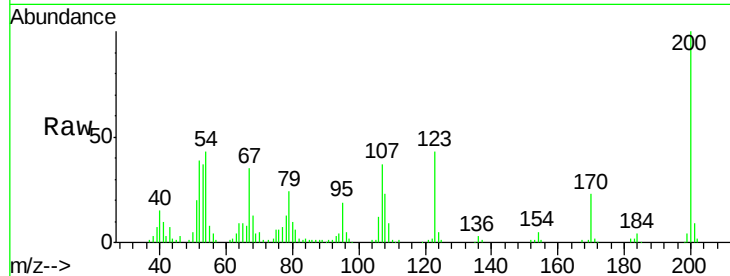

Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

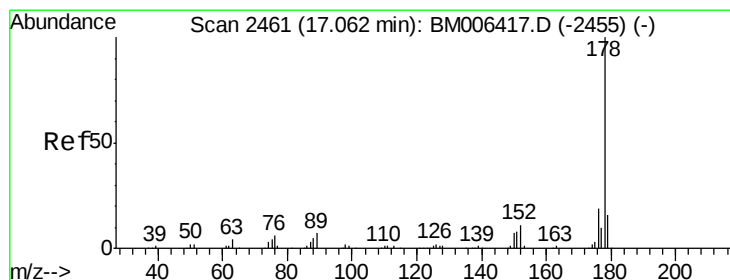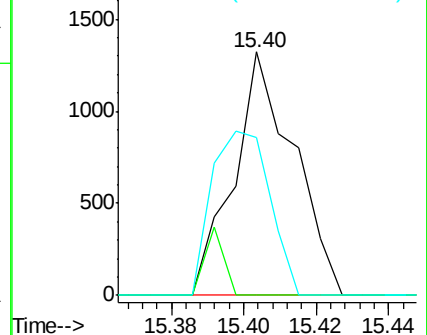

#69

Phenanthrene

Concen: 0.01 ng/ul

RT: 17.06 min Scan# 2461

Delta R.T. -0.00 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion:178 Resp: 619

Ion Ratio Lower Upper

178 100

179 0.0 11.9 17.9#



176 0.0 15.2 22.8#

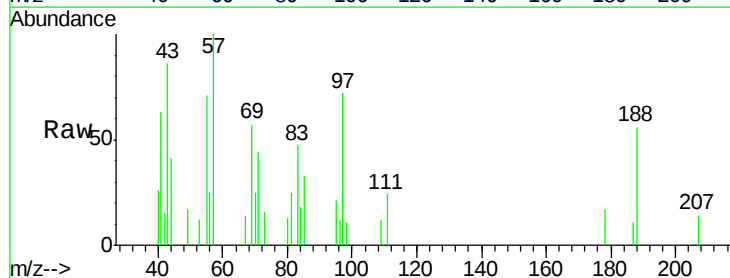


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

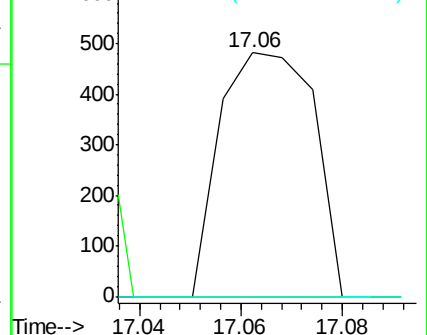

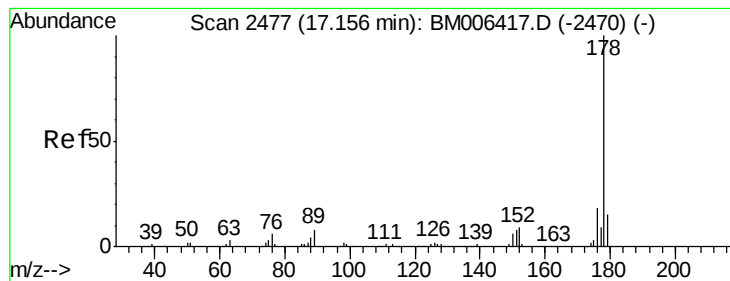

#71

Anthracene

Concen: 0.01 ng/ul

RT: 17.06 min Scan# 2461

Delta R.T. -0.09 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68


Tgt Ion:178 Resp: 619

Ion Ratio Lower Upper

178 100

179 0.0 12.0 18.0#




176 0.0 15.0 22.6#

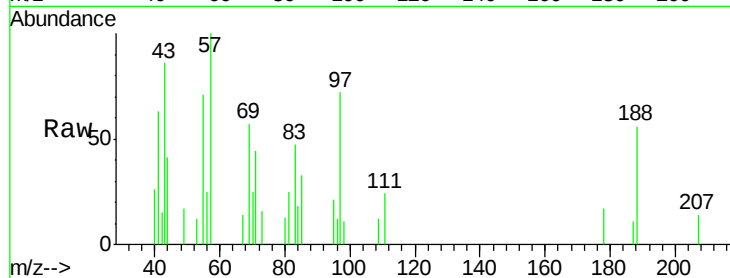

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

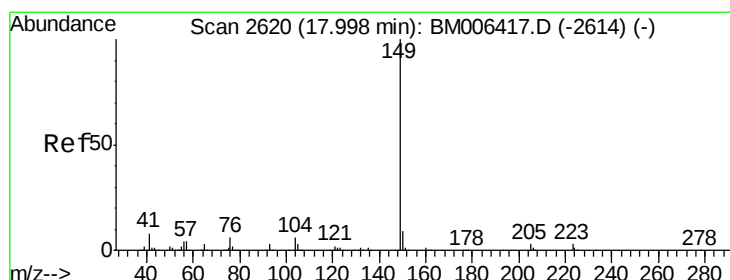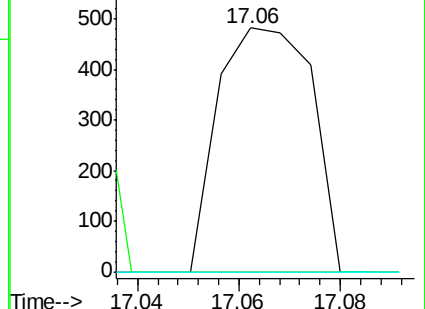

#73

Di-n-butylphthalate

Concen: 0.09 ng/ul

RT: 17.99 min Scan# 2619

Delta R.T. -0.01 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion:149 Resp: 4587

Ion Ratio Lower Upper

149 100

150 11.4 7.1 10.7#



104 10.3 4.4 6.6#

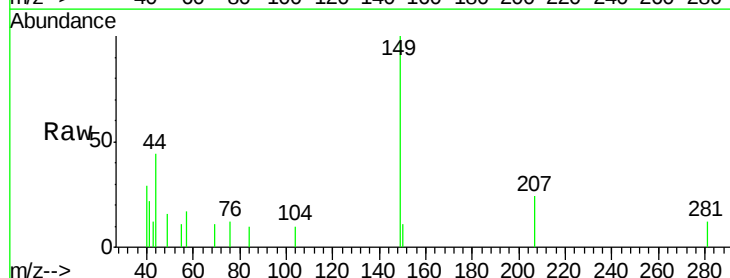


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

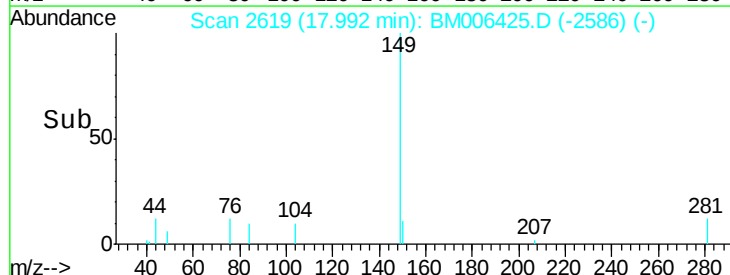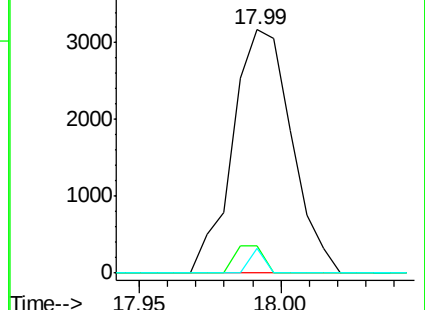



#74

Fluoranthene

Concen: 0.01 ng/ul

RT: 19.09 min Scan# 2805

Delta R.T. -0.00 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68


Tgt Ion:202 Resp: 614

Ion Ratio Lower Upper

202 100

101 0.0 8.6 12.8#

100 0.0 6.4 9.6#

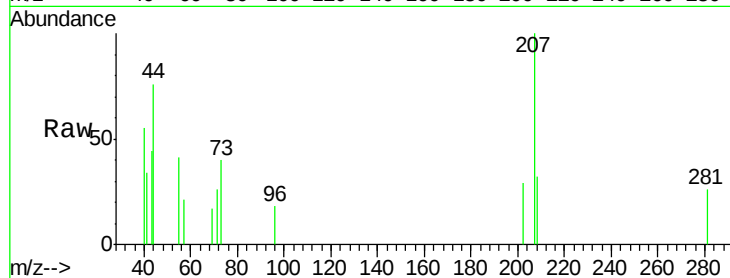


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

Time--> 19.06 19.08 19.10



Time--> 19.06 19.08 19.10

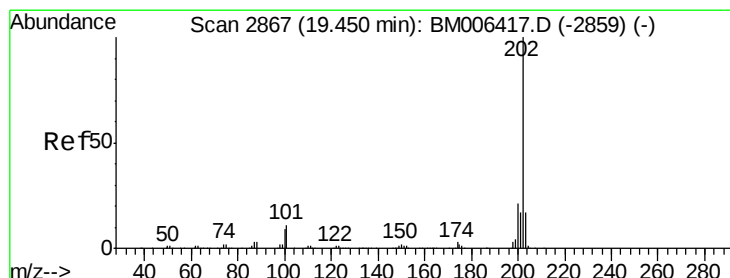

#77

Pyrene

Concen: 0.04 ng/ul

RT: 19.42 min Scan# 2862

Delta R.T. -0.03 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion:202 Resp: 2222

Ion Ratio Lower Upper

202 100

101 155.0 10.0 15.0#

100 1207.7 7.9 11.9#

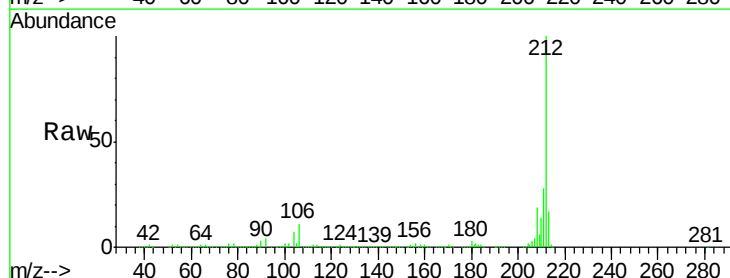


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

Time--> 19.40 19.42 19.44







Time--> 19.40 19.42 19.44



#78
Butylbenzylphthalate
Concen: 0.01 ng/ul
RT: 20.36 min Scan# 3021
Delta R.T. -0.01 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51




Instrument :
BNA_M
ClientSampleId :
BDJ68


Tgt Ion:149 Resp: 289
Ion Ratio Lower Upper
149 100
91 80.4 60.9 91.3
206 0.0 17.2 25.8#

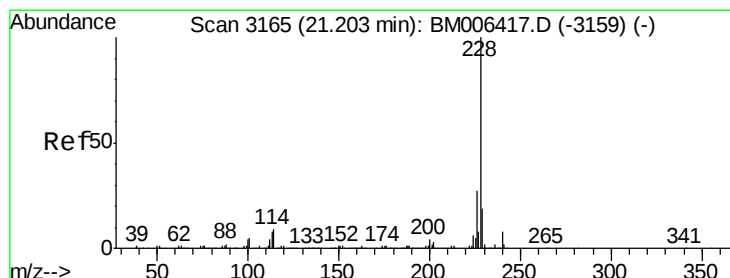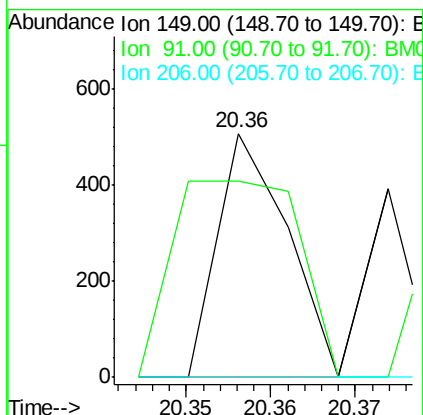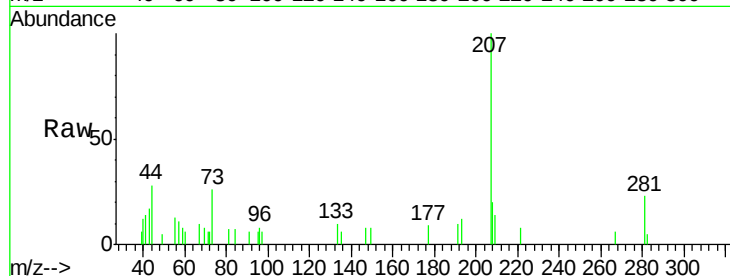

#80
Benzo(a)anthracene
Concen: 0.06 ng/ul
RT: 21.21 min Scan# 3167
Delta R.T. 0.01 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51

Tgt Ion:228 Resp: 3699
Ion Ratio Lower Upper
228 100
229 35.8 15.6 23.4#
226 0.0 21.4 32.2#


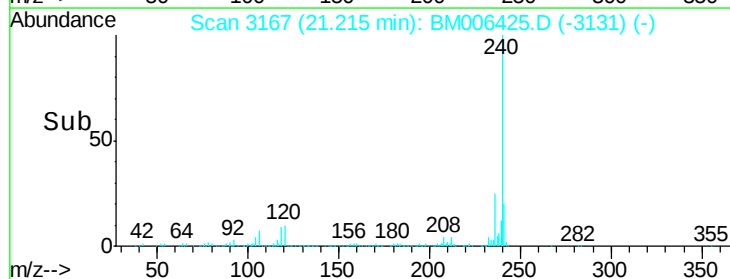
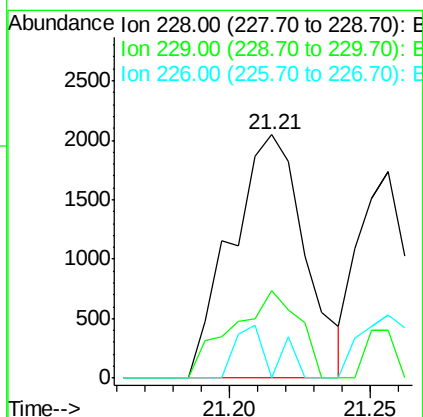
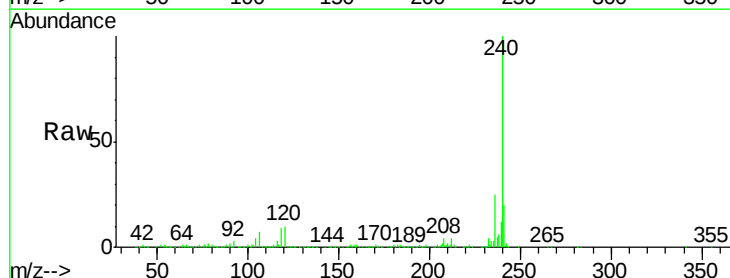




#81
Bis(2-ethylhexyl)phthalate
Concen: 0.12 ng/ul
RT: 21.14 min Scan# 3154
Delta R.T. -0.00 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51




Instrument :
BNA_M
ClientSampleId :
BDJ68


Tgt Ion:149 Resp: 4267
Ion Ratio Lower Upper
149 100
167 28.8 22.2 33.2
279 0.0 3.1 4.7#

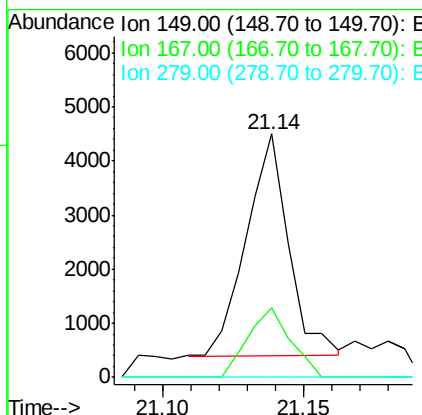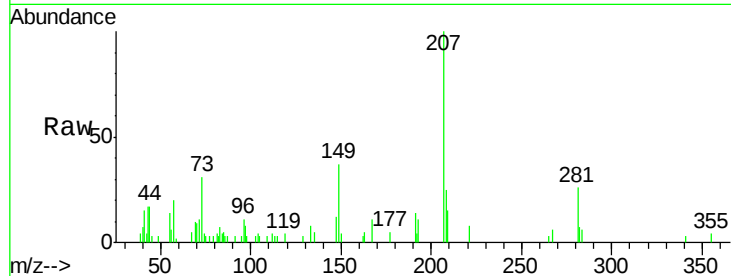

#82
Chrysene
Concen: 0.04 ng/ul
RT: 21.26 min Scan# 3174
Delta R.T. -0.00 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51

Tgt Ion:228 Resp: 2031
Ion Ratio Lower Upper
228 100
226 30.4 23.3 34.9
229 23.4 15.8 23.8

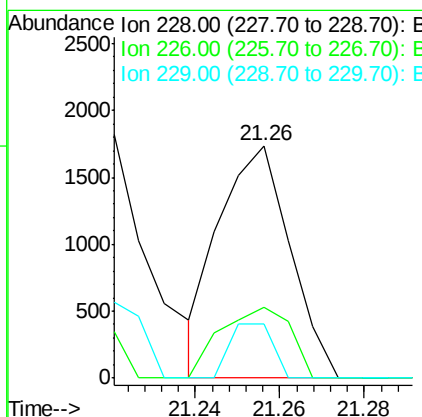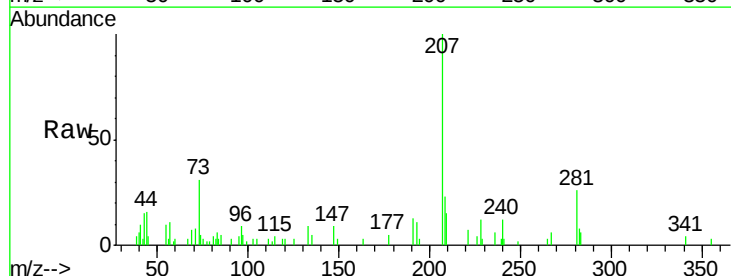

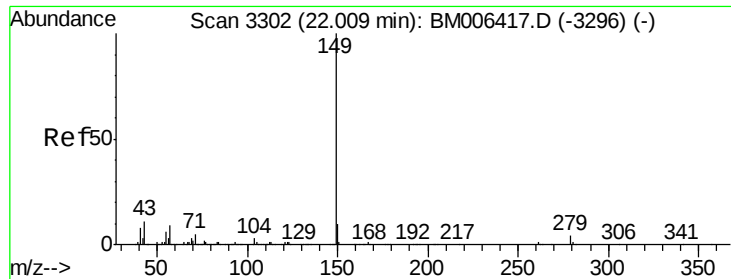

#84

Di-n-octyl phthalate

Concen: 0.01 ng/ul

RT: 22.00 min Scan# 3301

Delta R.T. -0.01 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampleId :

BDJ68


Tgt Ion:149 Resp: 404

Ion Ratio Lower Upper

149 100

167 0.0 1.4 2.0#




43 221.9 9.1 13.7#

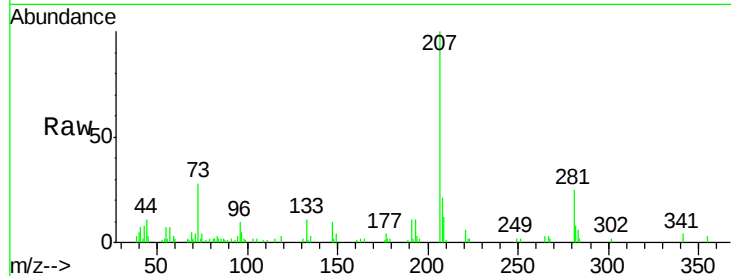

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 43.00 (42.70 to 43.70): BM

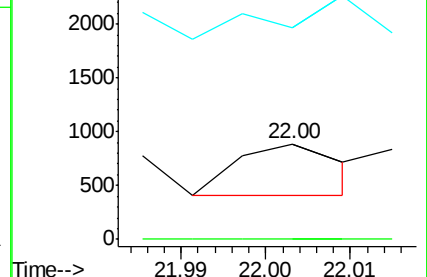

#85

Benzo(b)fluoranthene

Concen: 0.02 ng/ul

RT: 22.76 min Scan# 3430

Delta R.T. -0.00 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion:252 Resp: 1266

Ion Ratio Lower Upper

252 100

253 74.3 17.4 26.2#



125 94.3 6.7 10.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



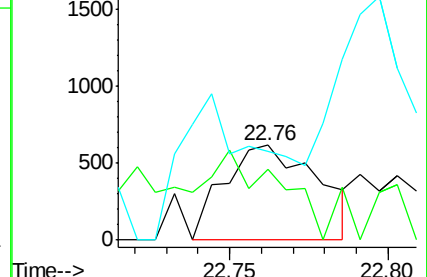





#86
Benzo(k)fluoranthene
Concen: 0.00 ng/ul
RT: 22.79 min Scan# 3435
Delta R.T. -0.02 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51

Instrument :
BNA_M
ClientSampleId :
BDJ68

Tgt Ion: 252 Resp: 56
Ion Ratio Lower Upper
252 100
253 0.0 17.3 25.9#
125 344.1 7.0 10.4#

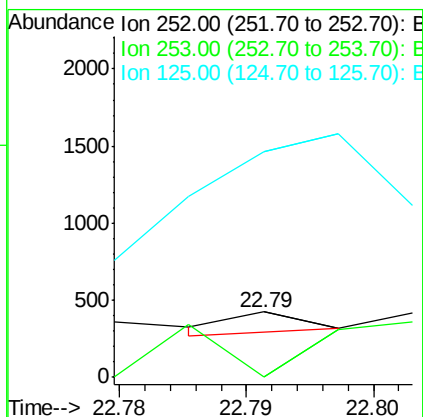

#88
Benzo(a)pyrene
Concen: 0.00 ng/ul
RT: 23.33 min Scan# 3527
Delta R.T. 0.01 min
Lab File: BM006425.D
Acq: 15 Jul 2016 03:51

Tgt Ion: 252 Resp: 235
Ion Ratio Lower Upper
252 100
253 91.0 17.4 26.2#
125 91.9 7.6 11.4#

